

Sequence Name: C:\HPCHEM\1\SEQUENCE\DEC0501.S
 Comment: 208
 Operator: GALOS
 Data Path: C:\HPCHEM\1\DATA\dec0501\
 Pre-Seq Cmd:
 Post-Seq Cmd:


Method Sections To Run On A Barcode Mismatch
 (X) Full Method (X) Inject Anyway
 () Reprocessing Only () Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP	NP112701	
2 Sample	2	26682	NP112701	gc/ms unknown 11/7
3 Sample	3	26712	NP112701	gc/ms unknown 11/7
4 Sample	4	26710	NP112701	gc/ms unknown 11/7
5 Sample	5	26711	NP112701	gc/ms unknown 11/7
6 Sample	6	26831	NP112701	gc/ms unknown 11/7
7 Sample	7	26319	NP112701	gc/ms unknown 11/3
8 Sample	8	LB	NP112701	gc/ms unknown 11/13
9 Sample	9	27015	NP112701	gc/ms unknown 11/13
10 Sample	10	27055	NP112701	gc/ms unknown 11/13
11 Sample	11	27111	NP112701	gc/ms unknown 11/13
12 Sample	12	27110	NP112701	gc/ms unknown 11/13
13 Sample	13	27113	NP112701	gc/ms unknown 11/13
14 Sample	14	27112	NP112701	gc/ms unknown 11/13
15 Sample	15	27056	NP112701	gc/ms unknown 11/13
16 Sample	16	27013	NP112701	gc/ms unknown 11/13
17 Sample	17	27014	NP112701	gc/ms unknown 11/13
18				

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC0401\DFTPP.D
 Acq On : 4 Dec 2001 10:05 am
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table

Vial: 1
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

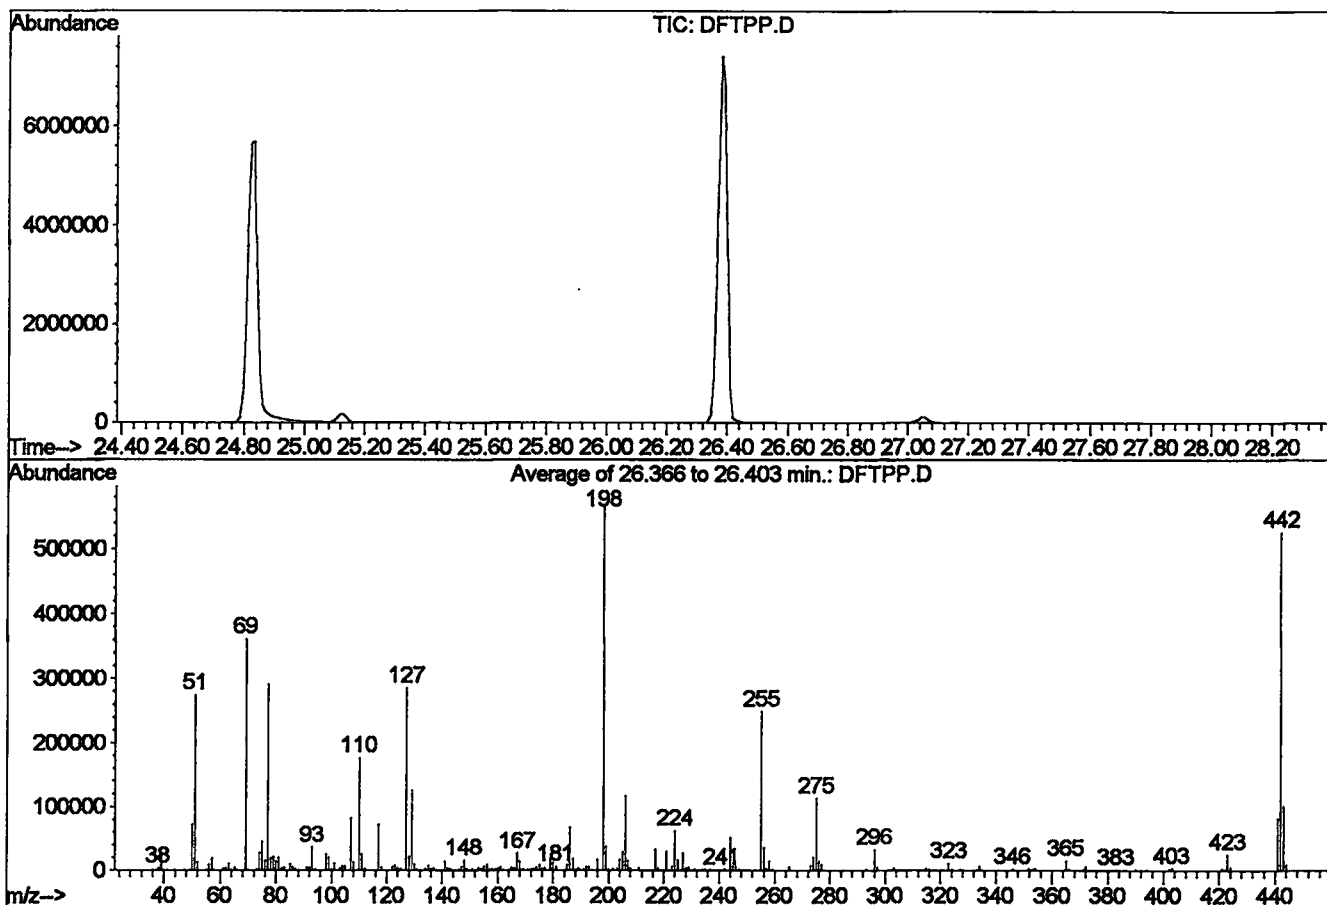

Spectrum Information: Average of 26.366 to 26.403 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	48.4	274683	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	63.5	361011	PASS
70	69	0.00	2	0.4	1426	PASS
127	198	40	60	50.3	285632	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	568102	PASS
199	198	5	9	6.7	37910	PASS
275	198	10	30	20.1	114288	PASS
365	198	1	99	2.7	15455	PASS
441	443	1	99	80.0	81184	PASS
442	198	40	110	92.6	526042	PASS
443	442	17	23	19.3	101418	PASS

DFTPP.D NP112701.M Tue Dec 04 11:16:24 2001

DFTPP

Data File : C:\HPCHEM\1\DATA\dec0601\DFTPP.D

Acq On : 6 Dec 2001 10:10 am

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)


Title : 208 625/TCLP calibration table

Vial: 1

Operator: GALOS

Inst : GC/MS Ins

Multiplr: 1.00

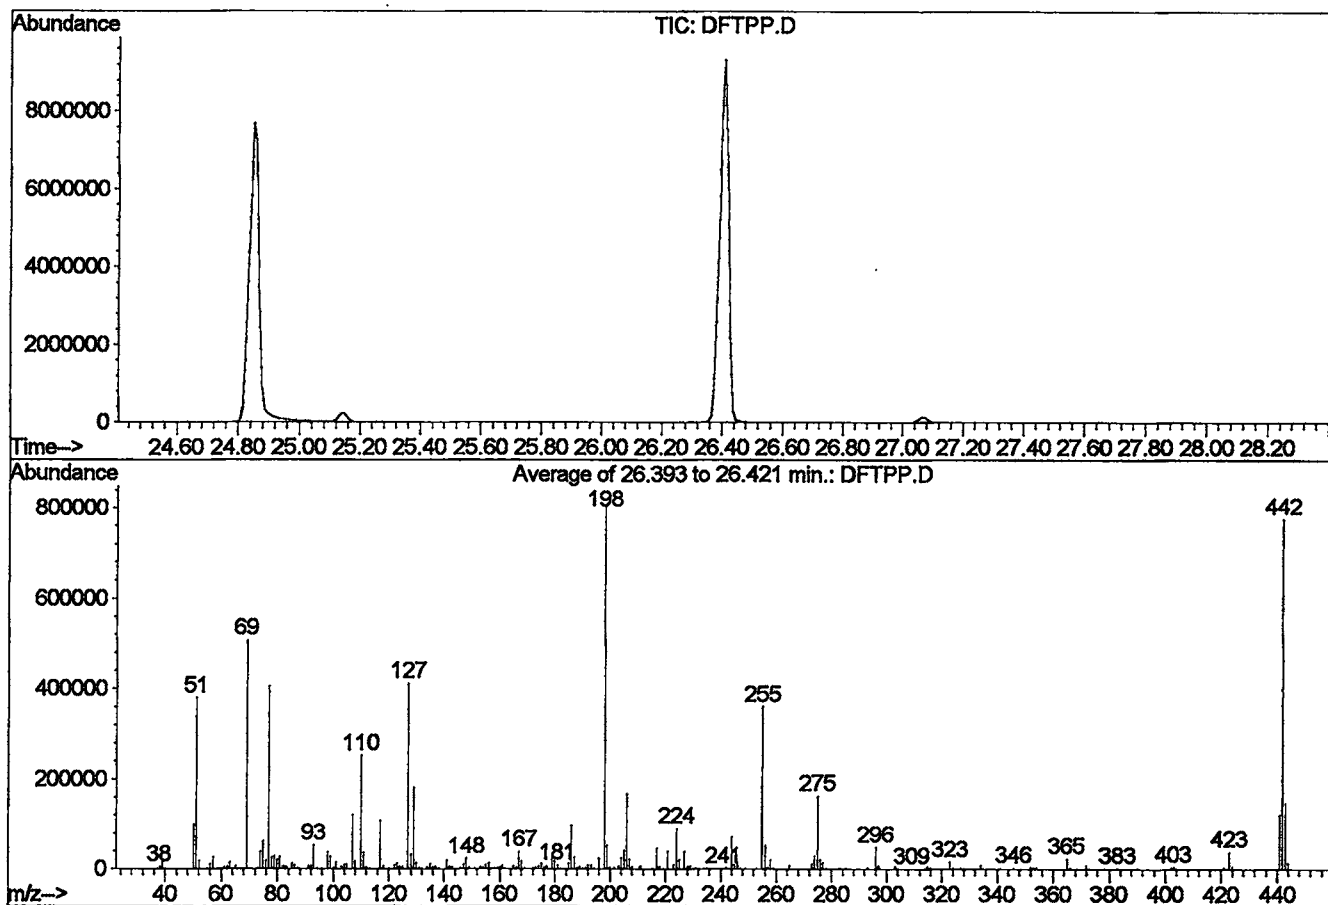

Spectrum Information: Average of 26.393 to 26.421 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	47.1	380256	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	62.9	508320	PASS
70	69	0.00	2	0.4	2228	PASS
127	198	40	60	50.9	411472	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	807888	PASS
199	198	5	9	6.6	53002	PASS
275	198	10	30	20.2	163528	PASS
365	198	1	99	2.8	22694	PASS
441	443	1	99	82.0	121282	PASS
442	198	40	110	96.1	776368	PASS
443	442	17	23	19.0	147890	PASS


DFTPP.D NP112701.M

Thu Dec 06 10:46:17 2001

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC0501\DFTPP.D
 Acq On : 5 Dec 2001 8:46 am
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table

Vial: 1
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

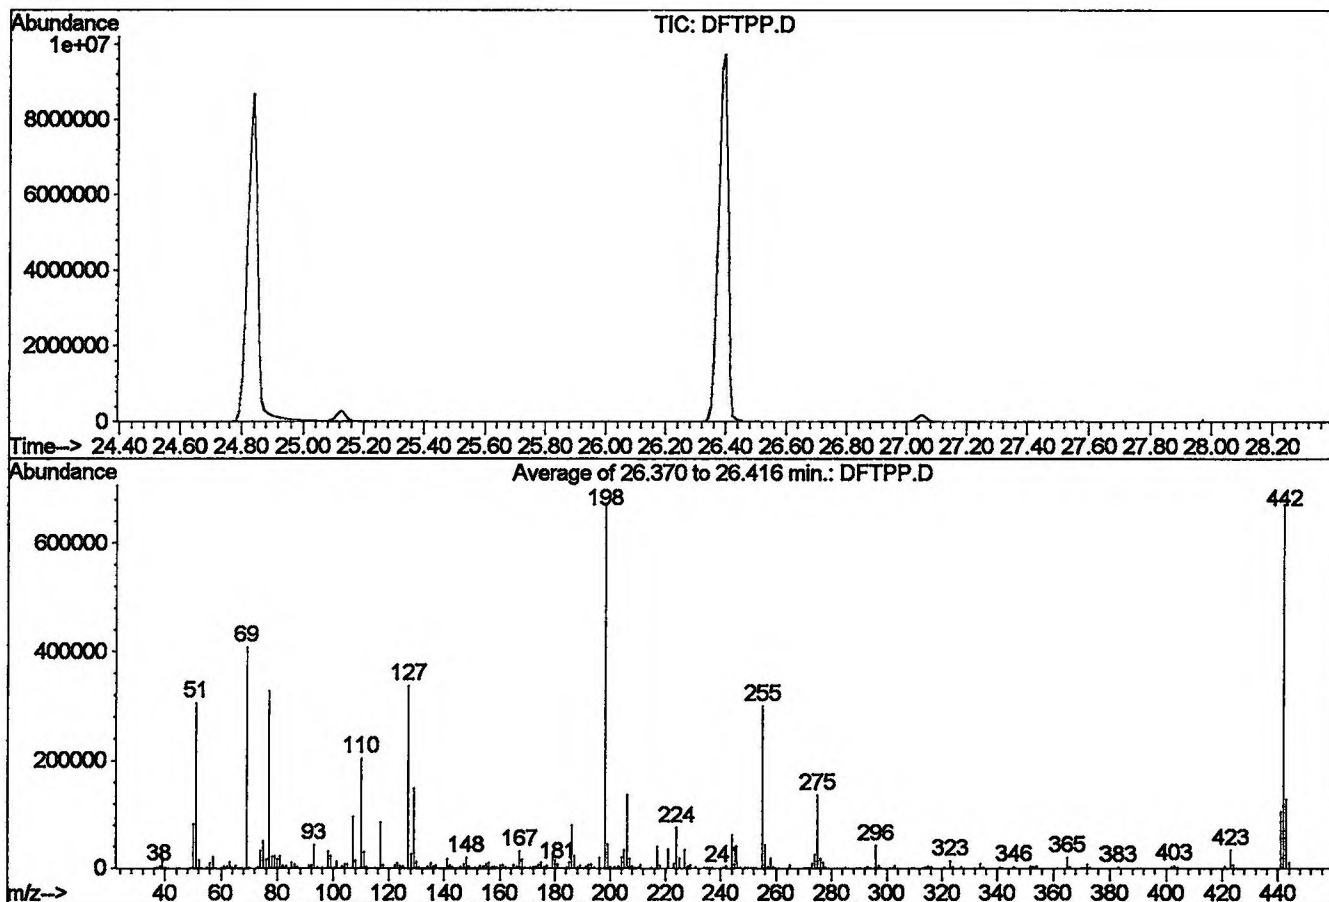

Spectrum Information: Average of 26.370 to 26.416 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	45.4	305979	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	60.7	408881	PASS
70	69	0.00	2	0.4	1589	PASS
127	198	40	60	50.1	337435	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	673916	PASS
199	198	5	9	6.5	43946	PASS
275	198	10	30	20.4	137168	PASS
365	198	1	99	2.9	19581	PASS
441	443	1	99	81.2	106161	PASS
442	198	40	110	99.8	672341	PASS
443	442	17	23	19.4	130693	PASS