

Method 508

GCMS

Date Extracted 11/9/01

Page

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH = 7	Count
	<u>LB</u>	<u>500ml</u>		<u>1ml</u>			<u>2ml</u>			
	<u>Ref chL+Ref</u>									
	<u>Ref TOX</u>									
	<u>S chL</u>				<u>1ml</u>					
	<u>SD chL</u>									
	<u>S TOX</u>									
	<u>SD TOX</u>									
<u>27013</u>	<u>S Prot</u>									
<u>27013</u>	<u>SD Prot</u>									
	<u>PRL 1254</u>									
<u>✓</u>	<u>27013 ✓</u>									<u>1</u>
<u>✓</u>	<u>27014 ✓</u>									<u>2</u>
<u>✓</u>	<u>27015 ✓</u>									<u>3</u>
<u>✓</u>	<u>27032 ✓</u>									<u>4</u>
<u>✓</u>	<u>27055 ✓</u>									<u>5</u>
<u>✓</u>	<u>27056 ✓</u>									<u>6</u>
<u>✓</u>	<u>27110 ✓</u>									<u>7</u>
<u>✓</u>	<u>27111 ✓</u>									<u>8</u>
<u>✓</u>	<u>27112 ✓</u>									<u>9</u>
<u>✓</u>	<u>27113 ✓</u>									<u>10</u>
Remarks										
Reviewed by, <u>SPB 2/19/02</u>										
drip rate must be between 5-15 ml/min for liq-liq extractors										
drip rate -										
Extraction type - <u>Sep funnel</u>		Solv. lot# <u>V42617</u>	NaCl lot# <u>V11599</u>		Na2SO4 lot# <u>V32603</u>					
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE	<u>TOX: 1992</u>	<u>chL: 1993</u>	<u>Prot: 20026</u>							
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE	<u>1839b</u>									
LPC										
ENDRIN/DDT										

Analyst ml/AJ/cm/E
revision 4/12/01

Verified by

Reviewed by DN
Date 12/11/01

Sequence Name: C:\HPCHEM\1\SEQUENCE\DEC0501.S
Comment: 208
Operator: GALOS
Data Path: C:\HPCHEM\1\DATA\dec0501\
Pre-Seq Cmd:
Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
(X) Full Method (X) Inject Anyway
() Reprocessing Only () Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP112701	
2	Sample	2	26682	NP112701	gc/ms unknown 11/7
3	Sample	3	26712	NP112701	gc/ms unknown 11/7
4	Sample	4	26710	NP112701	gc/ms unknown 11/7
5	Sample	5	26711	NP112701	gc/ms unknown 11/7
6	Sample	6	26831	NP112701	gc/ms unknown 11/7
7	Sample	7	26319	NP112701	gc/ms unknown 11/3
8	Sample	8	LB	NP112701	gc/ms unknown 11/13
9	Sample	9	27015	NP112701	gc/ms unknown 11/13
10	Sample	10	27055	NP112701	gc/ms unknown 11/13
11	Sample	11	27111	NP112701	gc/ms unknown 11/13
12	Sample	12	27110	NP112701	gc/ms unknown 11/13
13	Sample	13	27113	NP112701	gc/ms unknown 11/13
14	Sample	14	27112	NP112701	gc/ms unknown 11/13
15	Sample	15	27056	NP112701	gc/ms unknown 11/13
16	Sample	16	27013	NP112701	gc/ms unknown 11/13
17	Sample	17	27014	NP112701	gc/ms unknown 11/13
18					

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC0501\DFTPP.D

Acq On : 5 Dec 2001 8:46 am

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)


Title : 208 625/TCLP calibration table

Vial: 1

Operator: GALOS

Inst : GC/MS Ins

Multiplr: 1.00

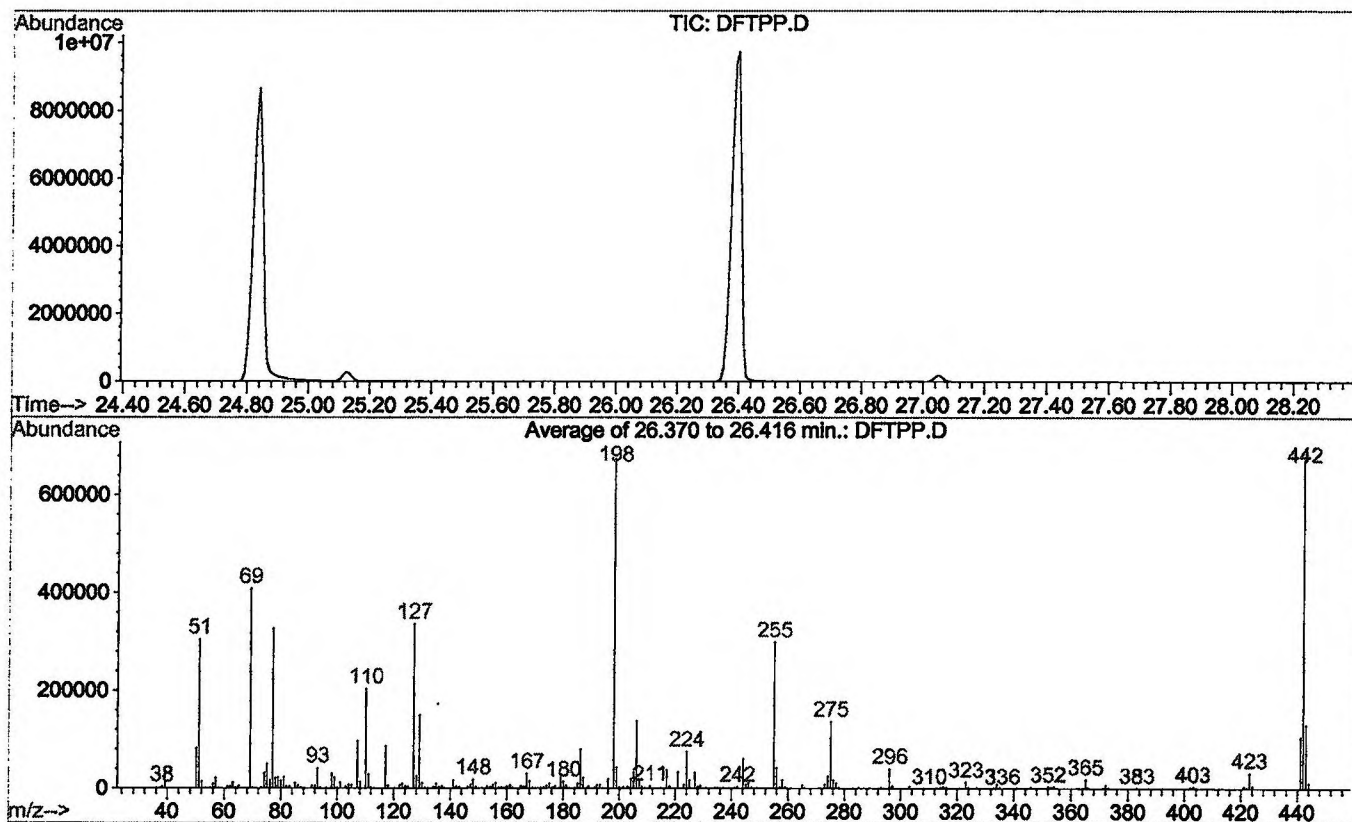

Spectrum Information: Average of 26.370 to 26.416 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	45.4	305979	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	60.7	408881	PASS
70	69	0.00	2	0.4	1589	PASS
127	198	40	60	50.1	337435	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	673916	PASS
199	198	5	9	6.5	43946	PASS
275	198	10	30	20.4	137168	PASS
365	198	1	99	2.9	19581	PASS
441	443	1	99	81.2	106161	PASS
442	198	40	110	99.8	672341	PASS
443	442	17	23	19.4	130693	PASS