

Date _____

Method 508Date Extracted 11/13/01Page

(cont)


Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
	27143 SOL	1mL					2mL		7	2		
	27144 SOL									3		
	27145 SOL									4		
	27146 SOL									5		
	27188 ✓									6		
	27189 ✓									7		
	27190 ✓									8		
	27191 ✓									9		
	27192 ✓									10		
Remarks												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type <u>Sol funnel</u>		Solv. lot# <u>V42817</u>		NaCl lot# <u>V11599</u>		Na2SO4 lot# <u>V32603</u>						
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE	<u>TOX: 1839.5</u>											
MDL/MDRF	<u>CHL: 2108</u>											
Q. CHECK	<u>PEST: 20606</u>											
INT. STD.												
SURROGATE	<u>1839.5</u>											
LPC												
ENDRIN/DDT												

Analyst ML/AD/CM/E
revision 4/12/01Verified by Reviewed by
Date

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC1001\DFTPP.D
 Acq On : 10 Dec 2001 9:25 am
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table

Vial: 1
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

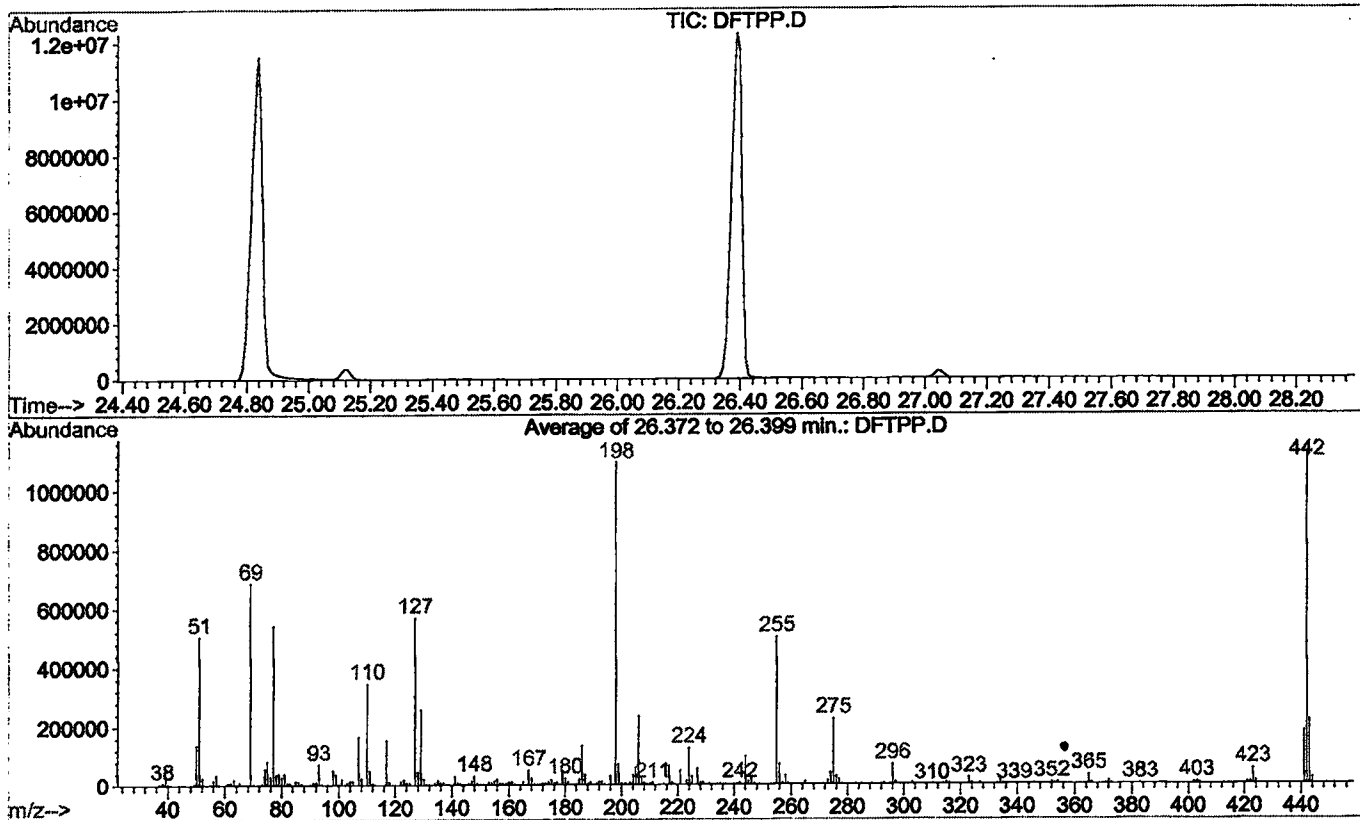

Spectrum Information: Average of 26.372 to 26.399 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	46.0	505280	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	62.5	686544	PASS
70	69	0.00	2	0.4	3010	PASS
127	198	40	60	52.0	570448	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	1097616	PASS
199	198	5	9	6.7	73408	PASS
275	198	10	30	20.6	226304	PASS
365	198	1	99	3.1	33818	PASS
441	443	1	99	82.3	181316	PASS
442	198	40	110	101.9	1118512	PASS
443	442	17	23	19.7	220204	PASS

Sequence Name: C:\HPCHEM\1\SEQUENCE\DEC0601.S

Comment: 208

Operator: GALOS

Data Path: C:\HPCHEM\1\DATA\dec0701\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP	NP112701	
2 Sample	34	27010	NP112701	gc/ms unknown
3 Sample	2	LB	NP112701	gc/ms unknown 11/6
4 Sample	3	26478	NP112701	gc/ms unknown 11/6
5 Sample	4	26537	NP112701	gc/ms unknown 11/6
6 Sample	5	26475	NP112701	gc/ms unknown 11/6
7 Sample	6	26476	NP112701	gc/ms unknown 11/6
8 Sample	7	26533	NP112701	gc/ms unknown 11/6
9 Sample	8	26532	NP112701	gc/ms unknown 11/6
10 Sample	9	26534	NP112701	gc/ms unknown 11/6
11 Sample	10	26535	NP112701	gc/ms unknown 11/6
12 Sample	11	26536	NP112701	gc/ms unknown 11/6
13 Sample	12	LBB	NP112701	gc/ms unknown 11/13
14 Sample	13	27545	NP112701	gc/ms unknown 11/13
15 Sample	14	27116	NP112701	gc/ms unknown 11/13
16 Sample	15	26830	NP112701	gc/ms unknown 11/13
17 Sample	16	27190	NP112701	gc/ms unknown 11/13
18 Sample	17	27191	NP112701	gc/ms unknown 11/13
19 Sample	18	27117	NP112701	gc/ms unknown 11/13
20 Sample	19	27118	NP112701	gc/ms unknown 11/13
21 Sample	20	27142	NP112701	gc/ms unknown 11/13
22 Sample	21	27141	NP112701	gc/ms unknown 11/13
23 Sample	22	27141A <i>sm</i>	NP112701	gc/ms unknown 11/13
24 Sample	23	27188	NP112701	gc/ms unknown 11/13
25 Sample	24	27115	NP112701	gc/ms unknown 11/13
26 Sample	25	27143	NP112701	gc/ms unknown 11/13
27 Sample	26	27114	NP112701	gc/ms unknown 11/13
28 Sample	27	27146	NP112701	gc/ms unknown 11/13
29 Sample	28	27140	NP112701	gc/ms unknown 11/13
30 Sample	29	27189	NP112701	gc/ms unknown 11/13
31 Sample	30	27192	NP112701	gc/ms unknown 11/13
32 Sample	31	27490	NP112701	gc/ms unknown 11/13
33 Sample	32	27491	NP112701	gc/ms unknown 11/13
34 Sample	33	27491A	NP112701	gc/ms unknown 11/13
35 Sample	35	27390	NP112701	gc/ms unknown 11/13
36 Sample	36	27391	NP112701	gc/ms unknown 11/13
37 Sample	37	27393	NP112701	gc/ms unknown 11/13
38 Sample	38	27392	NP112701	gc/ms unknown 11/13
39 Sample	39	27394	NP112701	gc/ms unknown 11/13
40 Sample	40	27395	NP112701	gc/ms unknown 11/13

report
↓