

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 12/11/2001 Time: 16:38:24

Sample: AD27114
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 12/11/01 16:37 Ended: 12/11/01 16:37 Analyst: MG
 Page: 1

	Component Name	Viol	Result	MDL
1	Other unknown compounds		see comment	
2	Surr_2,4-DDD			5.0

Comments for Sample AD27114 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 12-11-2001 Time: 16:38:29

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0701\27114.D
 Acq On : 8 Dec 2001 4:54 pm
 Sample : gc/ms unknown 11/13
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Dec 10 10:02 2001

Vial: 26
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table
 Last Update : Wed Nov 28 15:33:44 2001
 Response via : Initial Calibration
 DataAcq Meth : NP112701

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.87	152	774684	20.00	ng/uL	-0.06
19) Naphthalene-d8	15.49	136	2908617	20.00	ng/uL	-0.06
31) Acenaphthene-d10	20.76	164	1364125	20.00	ng/uL	-0.06
49) Phenanthrene-d10	25.17	188	1988028	20.00	ng/uL	-0.07
59) Chrysene-d12	33.17	240	1288097	20.00	ng/uL	-0.07
68) Perylene-d12	37.26	264	883476	20.00	ng/uL	-0.07

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ng/uL	
Spiked Amount	75.000	Range 18 - 42	Recovery	=	0.00%#	
5) Phenol-d5	0.00	99	0	0.00	ng/uL	
Spiked Amount	75.000	Range 19 - 32	Recovery	=	0.00%#	
6) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/uL	
Spiked Amount	75.000	Range 34 - 84	Recovery	=	0.00%#	
7) 1,2-Dichlorobenzene-d4	12.20	152	342	0.01	ng/uL	-0.26
Spiked Amount	50.000	Range 26 - 73	Recovery	=	0.02%#	
20) Nitrobenzene-d5	0.00	82	0	0.00	ng/uL	
Spiked Amount	50.000	Range 55 - 98	Recovery	=	0.00%#	
32) 2-Fluorobiphenyl	18.92	172	1137	0.01	ng/uL	0.08
Spiked Amount	50.000	Range 42 - 78	Recovery	=	0.02%#	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng/uL	
Spiked Amount	75.000	Range 45 - 96	Recovery	=	0.00%#	
62) Terphenyl-d14	0.00	244	0	0.00	ng/uL	
Spiked Amount	50.000	Range 58 - 98	Recovery	=	0.00%#	

Target Compounds

				Qvalue
2) Pyridine	0.00	79	0	N.D.
3) N-nitrosodimethylamine	0.00	74	0	N.D.
8) Phenol	0.00	94	0	N.D.
9) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
10) 2-Chlorophenol	0.00	128	0	N.D.
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.
14) 2-Methylphenol	0.00	108	0	N.D.
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
16) 3&4-Methylphenol	0.00	108	0	N.D.

(#) = qualifier out of range (m) = manual integration

27114.D NP112701.M Mon Dec 10 12:56:21 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0701\27114.D

Vial: 26

Acq On : 8 Dec 2001 4:54 pm

Operator: GALOS

Sample : gc/ms unknown 11/13

Inst : GC/MS Ins

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 10 10:02 2001

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

Last Update : Wed Nov 28 15:33:44 2001

Response via : Initial Calibration

DataAcq Meth : NP112701

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
17) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.		
18) Hexachloroethane	0.00	117	0	N.D.		
21) Nitrobenzene	0.00	77	0	N.D.		
22) Isophorone	0.00	82	0	N.D.		
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	0.00	128	0	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
45) Diethylphthalate	0.00	149	0	N.D.		
46) 4-Chlorophenylphenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	169	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	0.00	178	0	N.D.		
56) Anthracene	0.00	178	0	N.D.		
57) Di-n-butylphthalate	27.16	149	2087	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		

(#)=qualifier out of range (m)=manual integration

27114.D NP112701.M Mon Dec 10 12:56:23 2001

Page 2

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0701\27114.D

Vial: 26

Acq On : 8 Dec 2001 4:54 pm

Operator: GALOS

Sample : gc/ms unknown 11/13

Inst : GC/MS Ins

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 10 10:02 2001

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

Last Update : Wed Nov 28 15:33:44 2001

Response via : Initial Calibration

DataAcq Meth : NP112701

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.17	228	2027	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.44	149	7857	N.D.		
67) Chrysene	33.17	228	2027	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.26	252	2735	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenzo(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

27114.D NP112701.M Mon Dec 10 12:56:24 2001

Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC0701\27114.D
 Acq On : 8 Dec 2001 4:54 pm
 Sample : gc/ms unknown 11/13
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Dec 10 10:02 2001

Vial: 26
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

Quant Results File: NP112701.RES

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table
 Last Update : Wed Nov 28 15:33:44 2001
 Response via : Initial Calibration

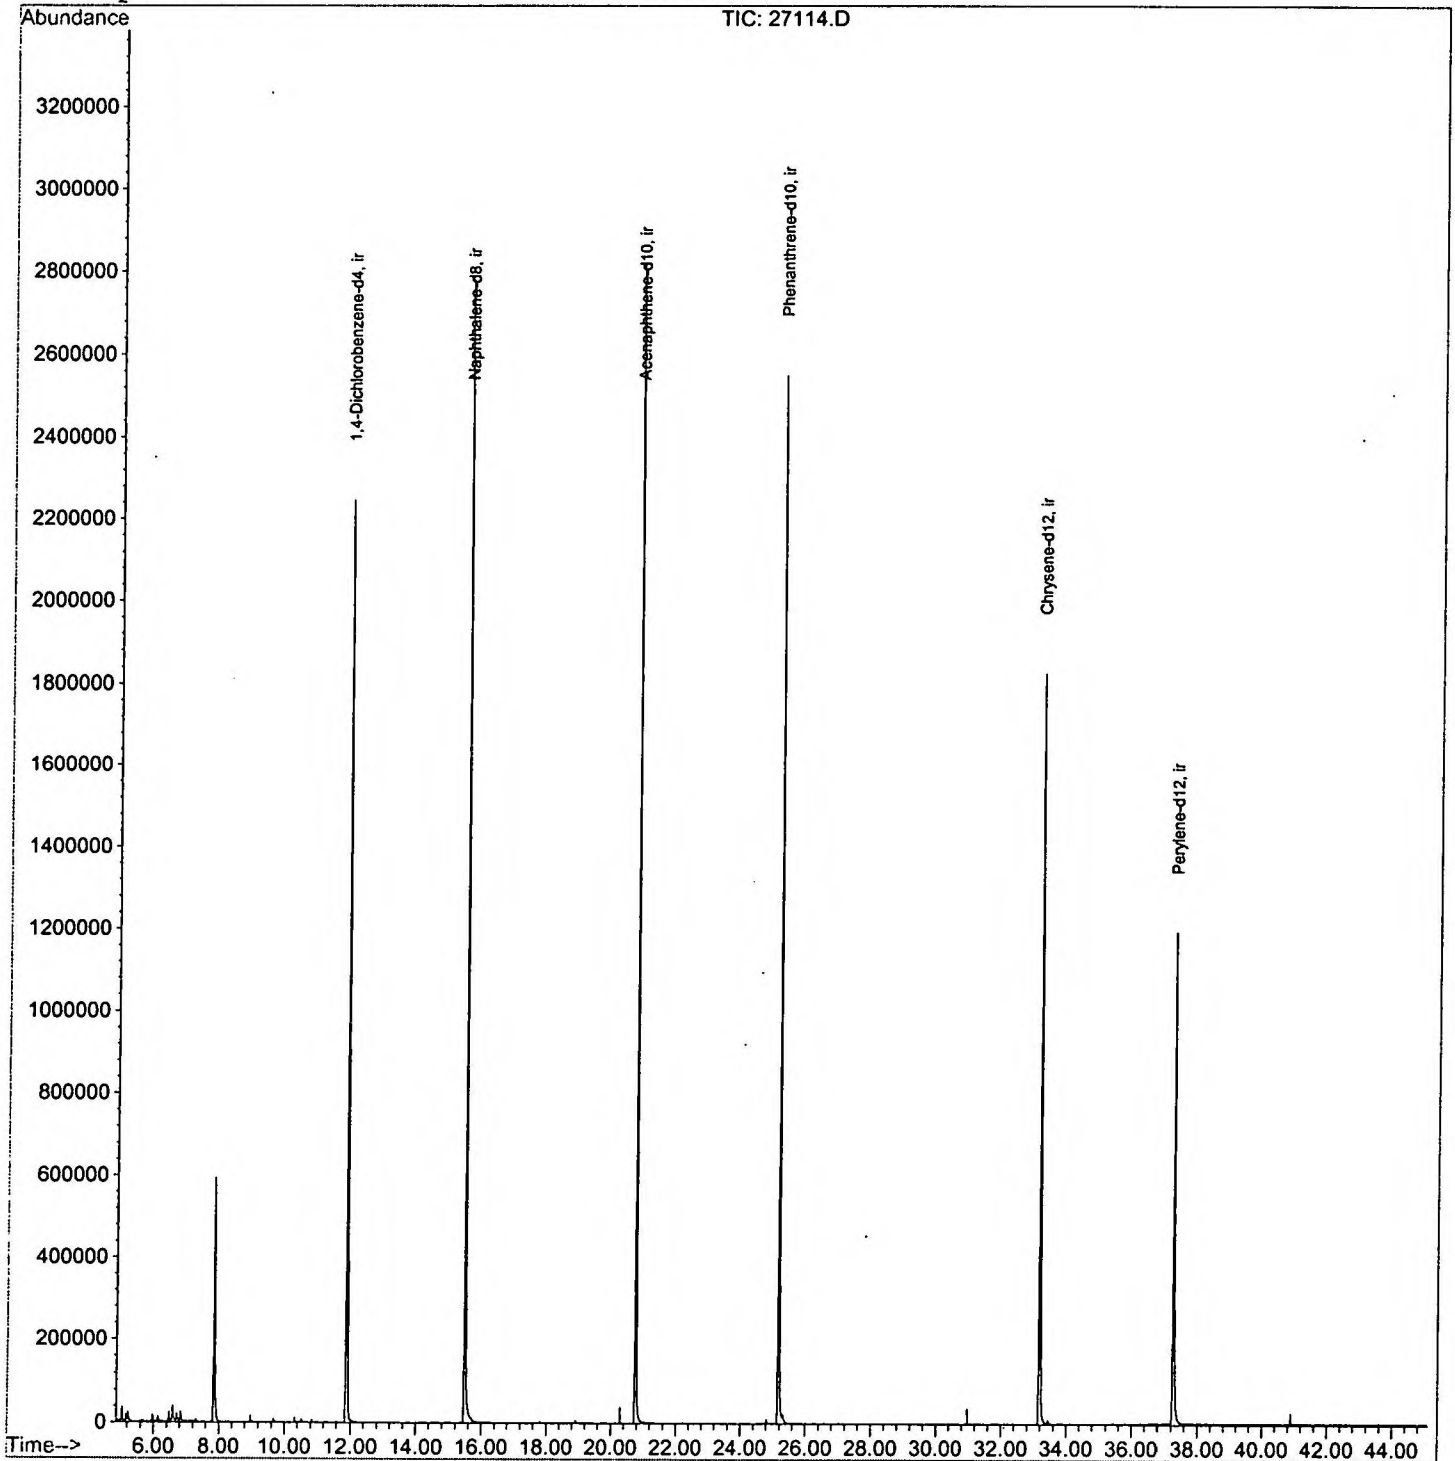

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC0701\27114.D

Vial: 26

Acq On : 8 Dec 2001 4:54 pm

Operator: GALOS

Sample : gc/ms unknown 11/13

Inst : GC/MS Ins

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	5.032	16	21	25	rVB	34106	62123	1.03%	0.199%
2	6.582	185	190	200	rVV	40019	94039	1.56%	0.302%
3	6.829	212	217	226	rBV	24954	63380	1.05%	0.203%
4	7.838	323	327	345	rBV	592962	1293944	21.44%	4.149%
5	11.873	762	767	780	rBV	2245151	4751478	78.73%	15.235%
6	15.486	1155	1161	1180	rBV	2780743	5919410	98.08%	18.979%
7	20.759	1730	1736	1754	rBV	2819407	6035100	100.00%	19.350%
8	25.169	2211	2217	2230	rBV2	2549458	5577898	92.42%	17.884%
9	25.316	2230	2233	2242	rVB	21303	62695	1.04%	0.201%
10	33.175	3084	3090	3109	rBV2	1825419	4086130	67.71%	13.101%
11	37.265	3528	3536	3558	rBV2	1192277	3242719	53.73%	10.397%


Sum of corrected areas: 31188916

27114.D NP112701.M

Tue Dec 11 15:11:18 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC0701\27114.D
 Operator : GALOS
 Acquired : 8 Dec 2001 4:54 pm using AcqMethod NP112701
 Instrument : GC/MS Ins
 Sample Name: gc/ms unknown 11/13
 Misc Info :
 Vial Number: 26
 Quant File :NP112701.RES (RTE Integrator)

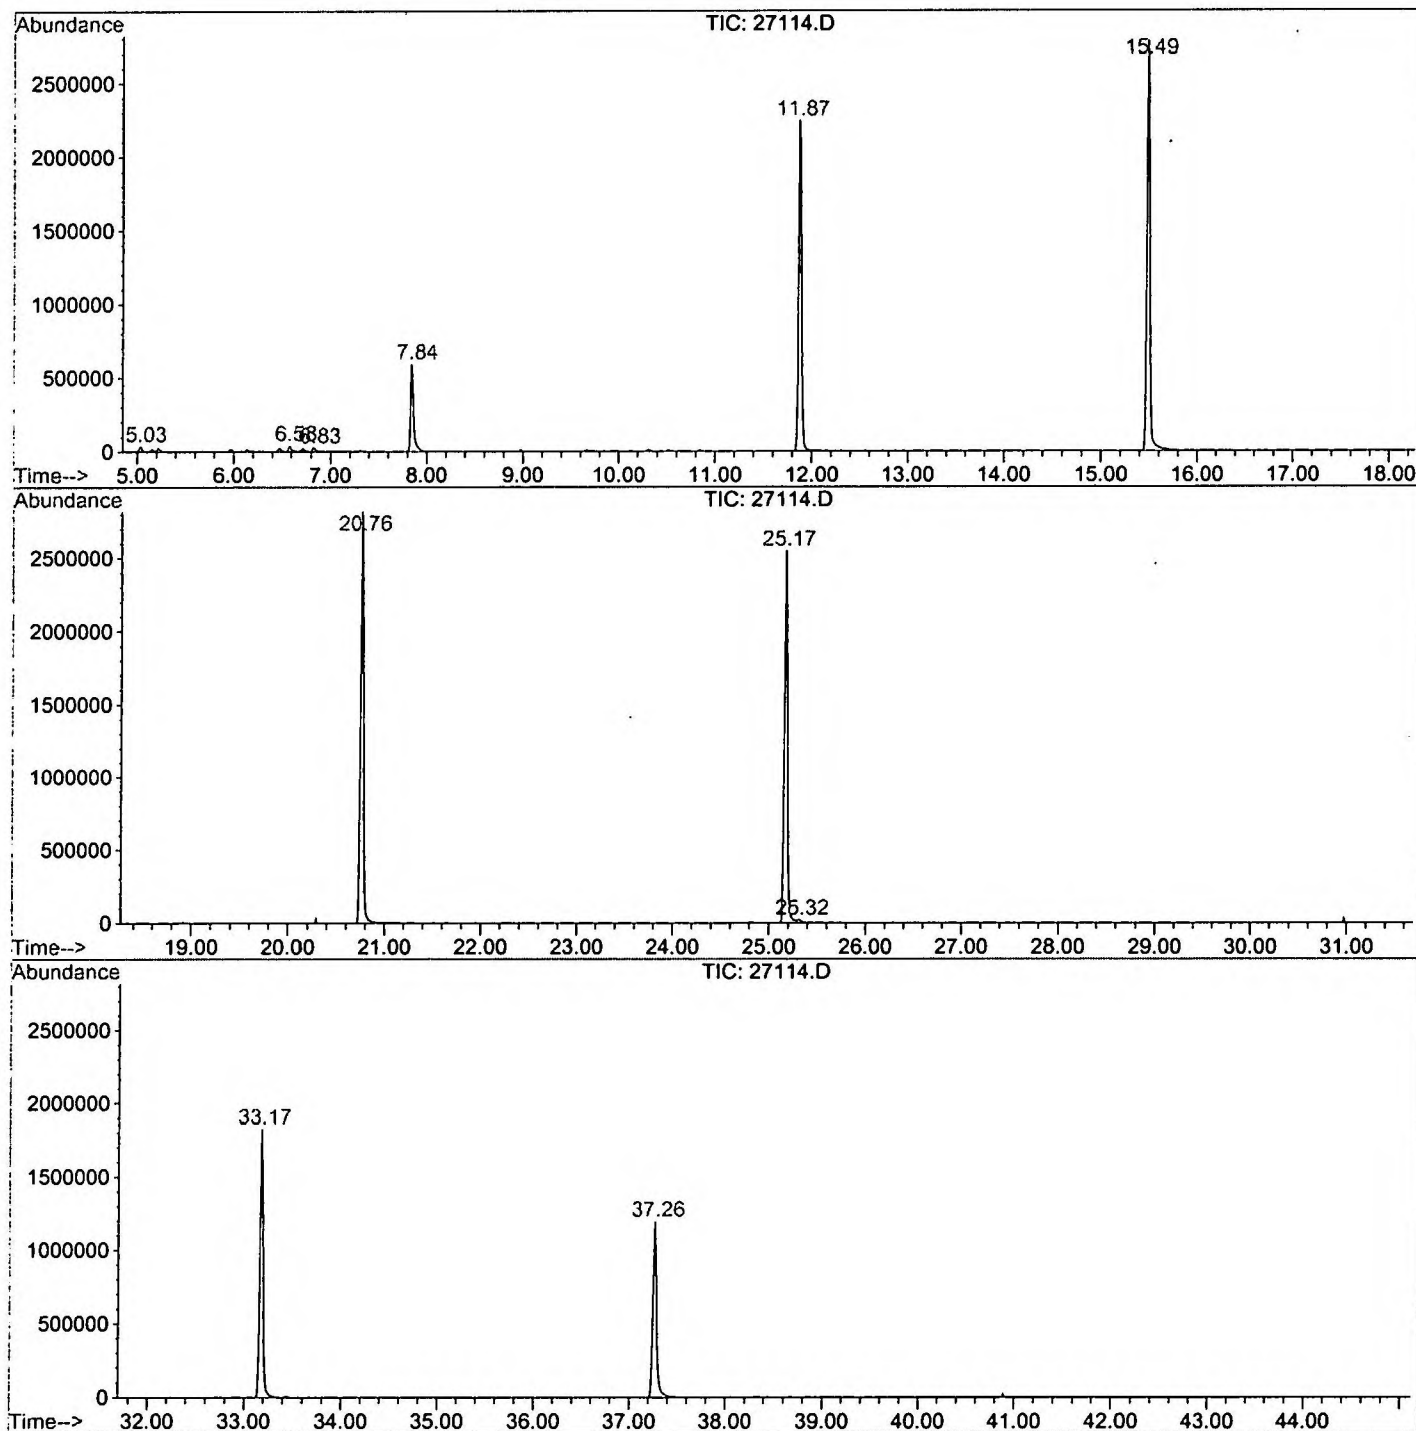

27114.D NP112701.M

Tue Dec 11 15:11:20 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC0701\27114.D
Acq On : 8 Dec 2001 4:54 pm
Sample : gc/ms unknown 11/13
Misc :
MS Integration Params: LSCINT.P










Vial: 26
Operator: GALOS
Inst : GC/MS Ins
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
Title : 208 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.84	5.45 ng/uL	1293940	1,4-Dichlorobenzene-d4	11.87

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78
2			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
3			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
4			Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	33

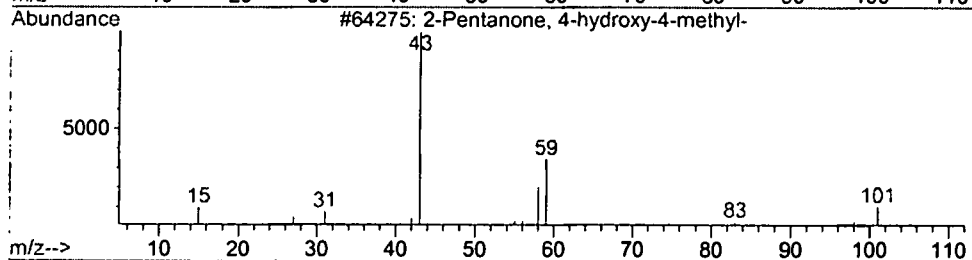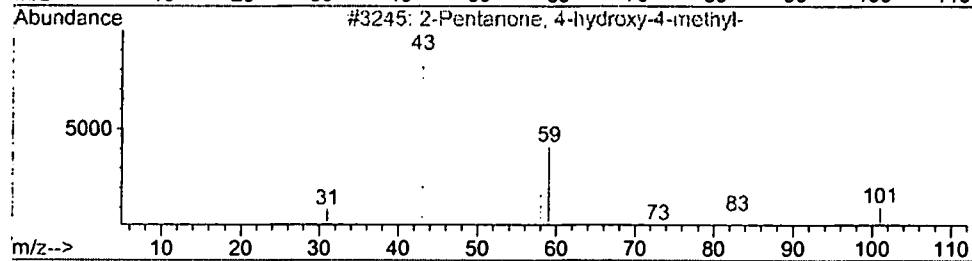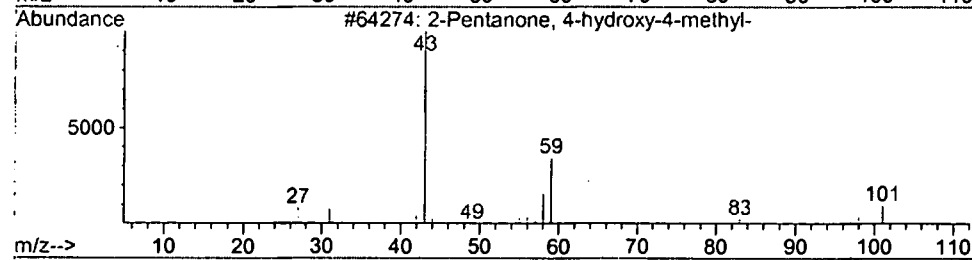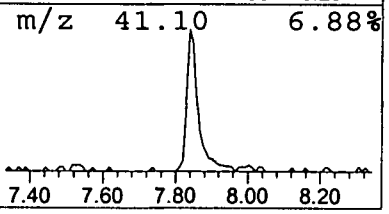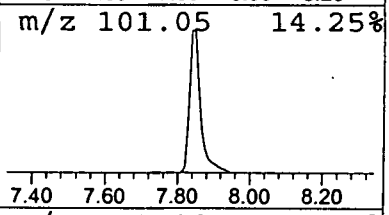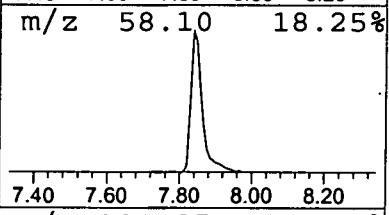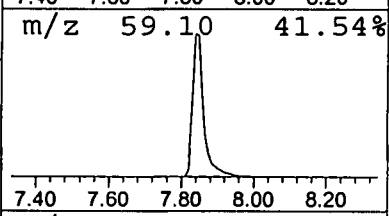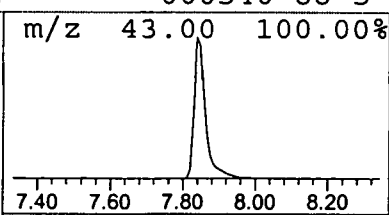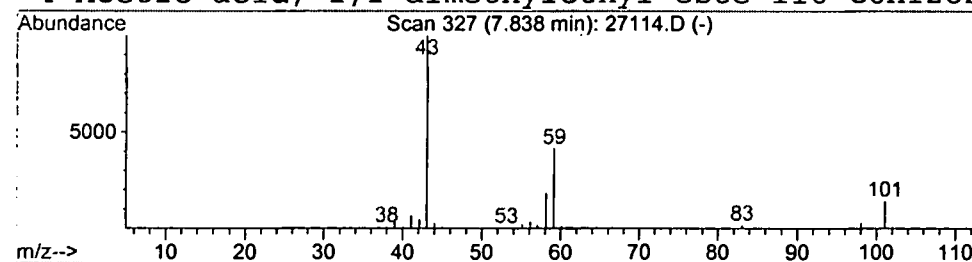

Tentatively Identified Compound (LSC) summary

Operator ID: GALOS Date Acquired: 8 Dec 2001 4:54 pm
Data File: C:\HPCHEM\1\DATA\DEC0701\27114.D
Name: gc/ms unknown 11/13
Misc:
Method: C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
Title: 208 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	7.84	5.4	ng/uL	1293940	ISTD01	11.87	4751480	20.0

27114.D NP112701.M Tue Dec 11 15:11:24 2001