

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC1201\DFTPP4.D

Acq On : 12 Dec 2001 3:19 pm

Sample :

Misc :

Vial: 1

Operator: GALOS


Inst : GC/MS Ins

Multiplr: 1.00

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

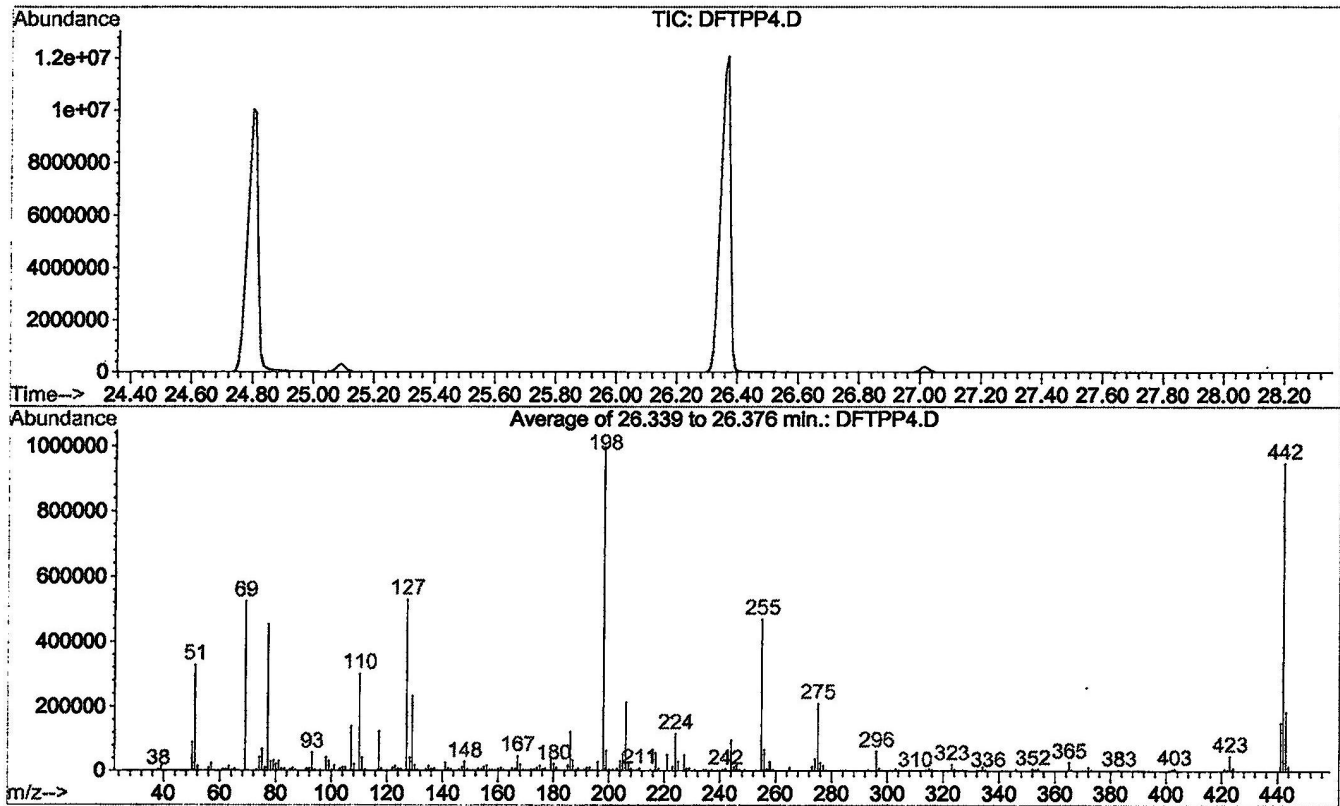

Spectrum Information: Average of 26.339 to 26.376 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	33.1	329549	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.7	525056	PASS
70	69	0.00	2	0.4	2159	PASS
127	198	40	60	53.2	529997	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	996672	PASS
199	198	5	9	6.6	65458	PASS
275	198	10	30	21.1	210376	PASS
365	198	1	99	2.8	28266	PASS
441	443	1	99	82.3	151688	PASS
442	198	40	110	95.1	947827	PASS
443	442	17	23	19.5	184400	PASS

DFTPP4.D NP112701.M

Fri Dec 14 09:15:42 2001