

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 12/19/2001 Time: 10:07:26

Sample: AD27194
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 12/19/01 10:07 Ended: 12/19/01 10:07 Analyst: MG
 Page: 1

	Component Name	Viol	Result	MDL
1	Other unknown compounds		see comment	
2	Surr_2,4-DDD			5.0

Comments for Sample AD27194 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 12-19-2001 Time: 10:07:32

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1201\27194.D
 Acq On : 13 Dec 2001 12:23 am
 Sample : gc/ms unknown 11/14
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Dec 14 9:33 2001

Vial: 11
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table
 Last Update : Wed Nov 28 15:33:44 2001
 Response via : Initial Calibration
 DataAcq Meth : NP112701

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	11.85	152	1013996	20.00	ng/uL	-0.09
19) Naphthalene-d8	15.45	136	4014020	20.00	ng/uL	-0.10
31) Acenaphthene-d10	20.72	164	1736027	20.00	ng/uL	-0.10
49) Phenanthrene-d10	25.13	188	2657399m	20.00	ng/uL	-0.11
59) Chrysene-d12	33.14	240	1852304	20.00	ng/uL	-0.11
68) Perylene-d12	37.21	264	1337391	20.00	ng/uL	-0.13

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ng/uL	
Spiked Amount	75.000	Range 18 - 42	Recovery	=	0.00%#	
5) Phenol-d5	0.00	99	0	0.00	ng/uL	
Spiked Amount	75.000	Range 19 - 32	Recovery	=	0.00%#	
6) 2-Chlorophenol-d4	11.84	132	737	0.01	ng/uL	0.41
Spiked Amount	75.000	Range 34 - 84	Recovery	=	0.01%#	
7) 1,2-Dichlorobenzene-d4	0.00	152	0	0.00	ng/uL	
Spiked Amount	50.000	Range 26 - 73	Recovery	=	0.00%#	
20) Nitrobenzene-d5	0.00	82	0	0.00	ng/uL	
Spiked Amount	50.000	Range 55 - 98	Recovery	=	0.00%#	
32) 2-Fluorobiphenyl	18.88	172	1821	0.02	ng/uL	0.05
Spiked Amount	50.000	Range 42 - 78	Recovery	=	0.04%#	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng/uL	
Spiked Amount	75.000	Range 45 - 96	Recovery	=	0.00%#	
62) Terphenyl-d14	0.00	244	0	0.00	ng/uL	
Spiked Amount	50.000	Range 58 - 98	Recovery	=	0.00%#	

Target Compounds

				Qvalue
2) Pyridine	0.00	79	0	N.D.
3) N-nitrosodimethylamine	0.00	74	0	N.D.
8) Phenol	0.00	94	0	N.D.
9) bis(2-Chloroethyl) ether	0.00	93	0	N.D.
10) 2-Chlorophenol	0.00	128	0	N.D.
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.
14) 2-Methylphenol	0.00	108	0	N.D.
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
16) 3&4-Methylphenol	0.00	108	0	N.D.

(#) = qualifier out of range (m) = manual integration

27194.D NP112701.M Fri Dec 14 10:00:13 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1201\27194.D
 Acq On : 13 Dec 2001 12:23 am
 Sample : gc/ms unknown 11/14
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Dec 14 9:33 2001

Vial: 11
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table
 Last Update : Wed Nov 28 15:33:44 2001
 Response via : Initial Calibration
 DataAcq Meth : NP112701

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
17) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.		
18) Hexachloroethane	0.00	117	0	N.D.		
21) Nitrobenzene	0.00	77	0	N.D.		
22) Isophorone	0.00	82	0	N.D.		
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	15.49	128	342	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
45) Diethylphthalate	0.00	149	0	N.D.		
46) 4-Chlorophenylphenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	169	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	0.00	178	0	N.D.		
56) Anthracene	0.00	178	0	N.D.		
57) Di-n-butylphthalate	0.00	149	0	N.D.	d	
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		

(#) = qualifier out of range (m) = manual integration

27194.D NP112701.M Fri Dec 14 10:00:15 2001

Page 2

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1201\27194.D
Acq On : 13 Dec 2001 12:23 am
Sample : gc/ms unknown 11/14
Misc :
MS Integration Params: RTEINT.P
Quant Time: Dec 14 9:33 2001

Vial: 11
Operator: GALOS
Inst : GC/MS Ins
Multiplr: 1.00

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
Title : 208 625/TCLP calibration table
Last Update : Wed Nov 28 15:33:44 2001
Response via : Initial Calibration
DataAcq Meth : NP112701

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.14	228	3850	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.40	149	16346	N.D.		
67) Chrysene	33.14	228	3850	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.21	252	4330	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

27194.D NP112701.M Fri Dec 14 10:00:16 2001

Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC1201\27194.D
Acq On : 13 Dec 2001 12:23 am
Sample : gc/ms unknown 11/14
Misc :
MS Integration Params: RTEINT.P
Quant Time: Dec 14 9:33 2001

Vial: 11
Operator: GALOS
Inst : GC/MS Ins
Multiplr: 1.00

Quant Results File: NP112701.RES

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
Title : 208 625/TCLP calibration table
Last Update : Fri Dec 14 09:15:17 2001
Response via : Initial Calibration

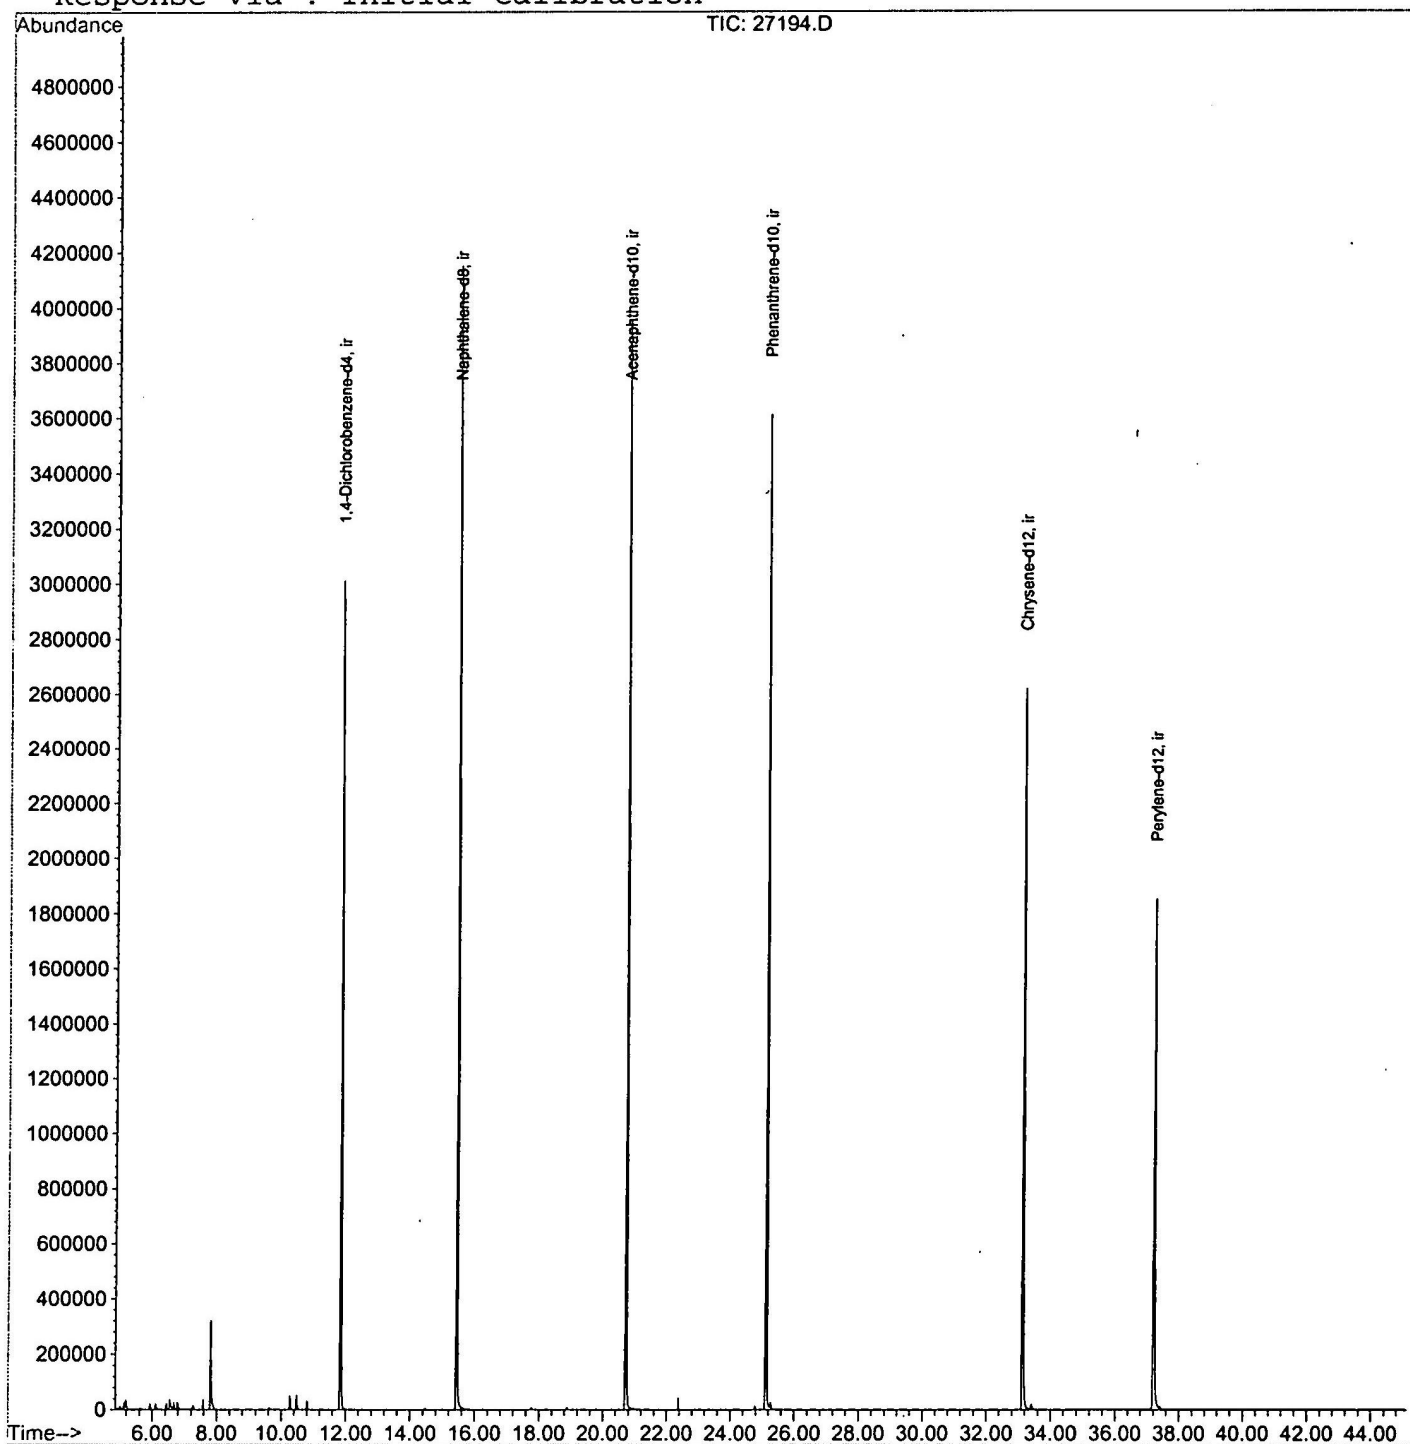

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC1201\27194.D
 Acq On : 13 Dec 2001 12:23 am
 Sample : gc/ms unknown 11/14
 Misc :
 MS Integration Params: LSCINT.P

Vial: 11
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.810	320	324	339	rBV	320254	688081	8.51%	1.655%
2	10.277	589	593	597	rBV	50730	96931	1.20%	0.233%
3	10.488	609	616	622	rBV	52899	106304	1.31%	0.256%
4	11.836	758	763	776	rBV	3010847	6256591	77.35%	15.053%
5	15.449	1151	1157	1174	rBV	4151987	8088492	100.00%	19.460%
6	20.722	1726	1732	1748	rBV	3955812	7839302	96.92%	18.861%
7	25.133	2206	2213	2225	rBV2	3611761	7444154	92.03%	17.910%
8	33.138	3079	3086	3107	rBV2	2620459	5995099	74.12%	14.424%
9	37.219	3523	3531	3551	rBV2	1849996	5048892	62.42%	12.147%

Sum of corrected areas: 41563846

27194.D NP112701.M Fri Dec 14 10:07:23 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC1201\27194.D
 Operator : GALOS
 Acquired : 13 Dec 2001 12:23 am using AcqMethod NP112701
 Instrument : GC/MS Ins
 Sample Name: gc/ms unknown 11/14
 Misc Info :
 Vial Number: 11
 Quant File :NP112701.RES (RTE Integrator)

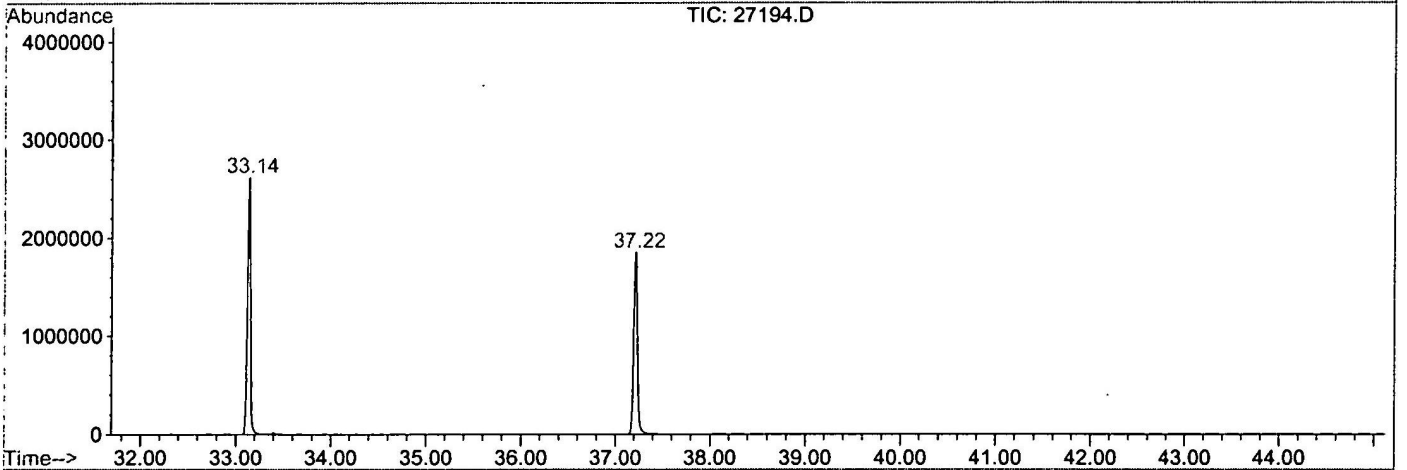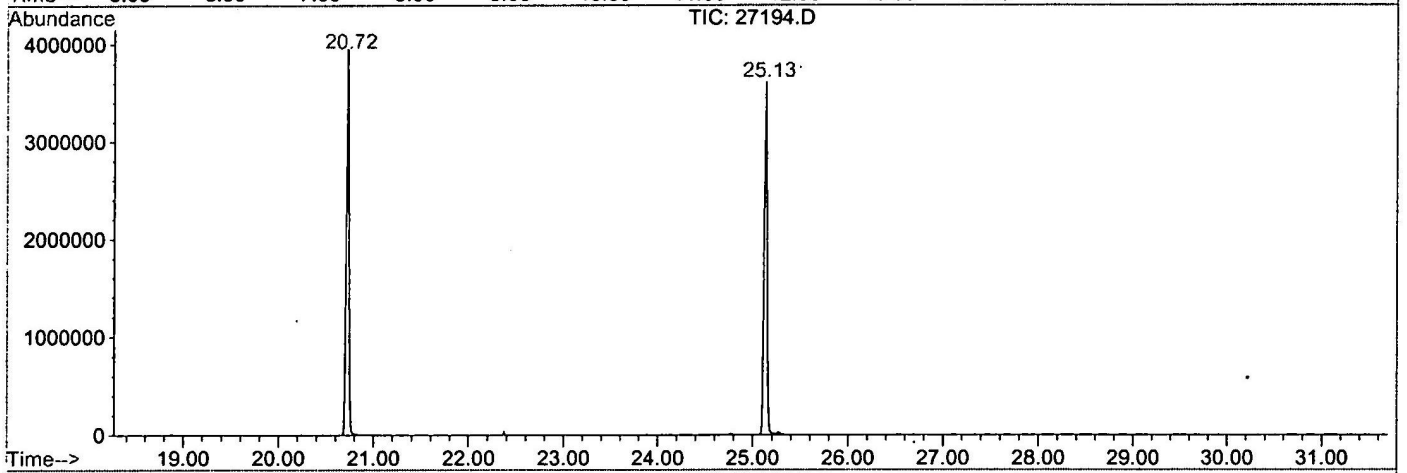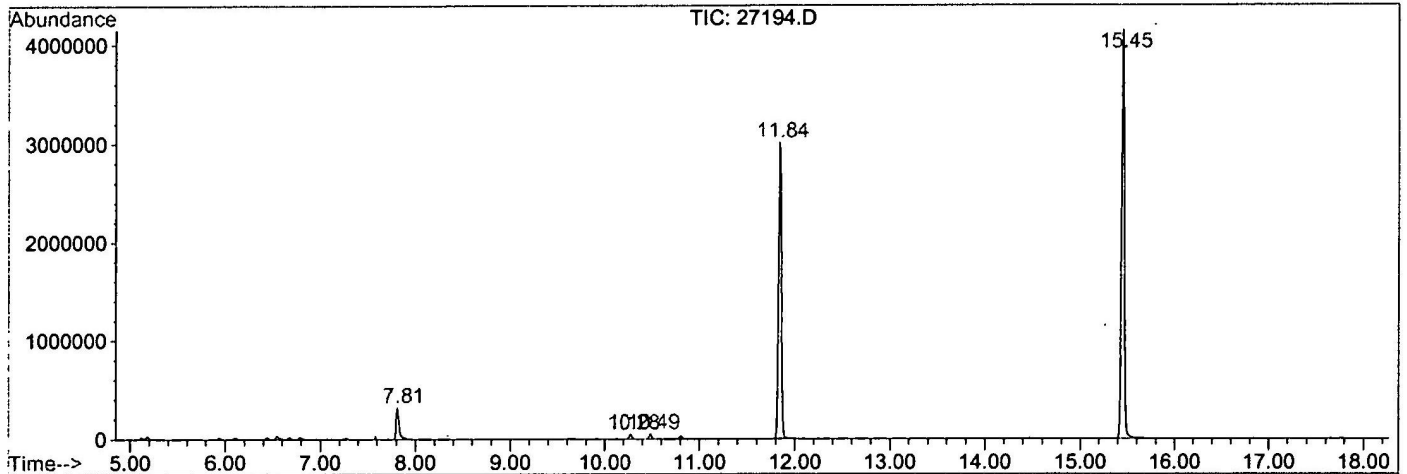

27194.D NP112701.M

Fri Dec 14 10:07:26 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC1201\27194.D
Acq On : 13 Dec 2001 12:23 am
Sample : gc/ms unknown 11/14
Misc :
MS Integration Params: LSCINT.P









Vial: 11
Operator: GALOS
Inst : GC/MS Ins
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
Title : 208 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.81	2.20 ng/uL	688081	1,4-Dichlorobenzene-d4	11.85

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	83
2		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
3		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	43
4		5-Hexen-2-one	98	C6H10O	000109-49-9	9

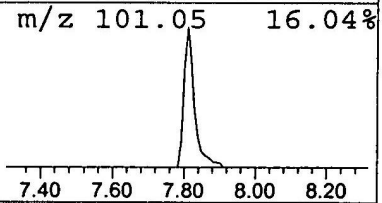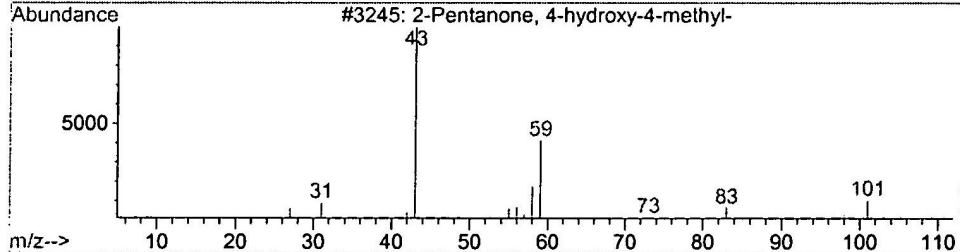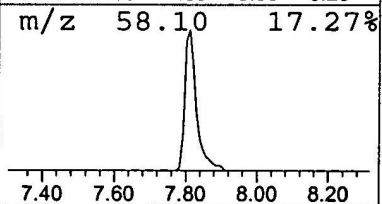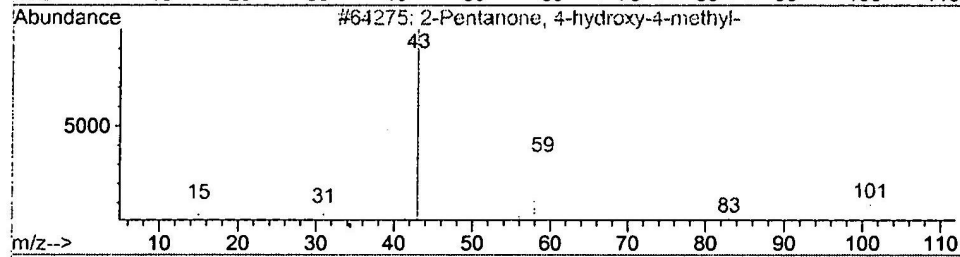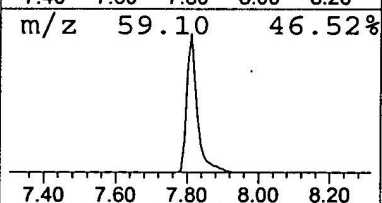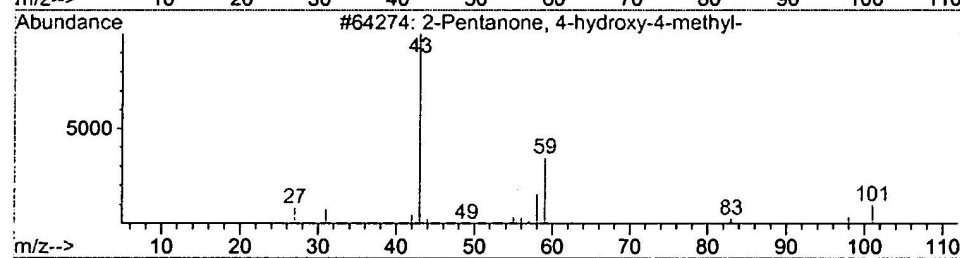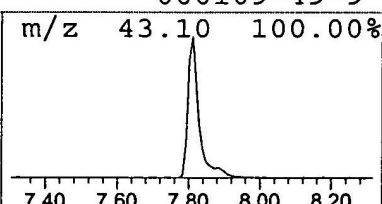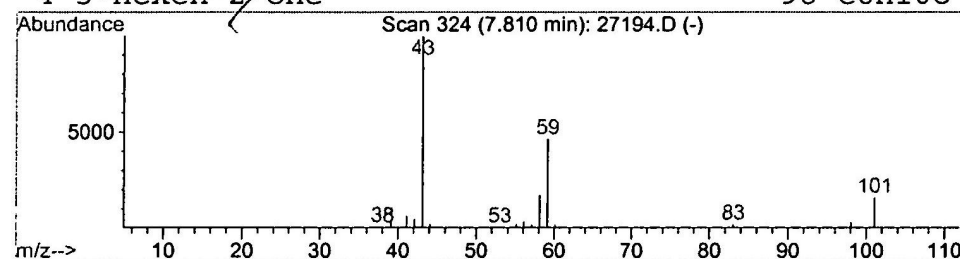

Tentatively Identified Compound (LSC) summary

Operator ID: GALOS Date Acquired: 13 Dec 2001 12:23 am
 Data File: C:\HPCHEM\1\DATA\DEC1201\27194.D
 Name: gc/ms unknown 11/14
 Misc:
 Method: C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title: 208 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
----- 2-Pentanone , 4-hydro	7.81	2.2	ng/uL	688081	ISTD01	11.85	6256590	20.0
27194.D NP112701.M			Fri Dec 14 10:07:30 2001					