

User: Galos, Marie
Westchester Dept. of Labs & Research
Date: 12/19/2001 Time: 13:02:52

Sample: AD27390
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 12/19/01 13:02 Ended: 12/19/01 13:02 Analyst: MG
Page: 1

	Component Name	Viol	Result	MDL
1	Other unknown compounds		see comment	
2	Surr_2,4-DDD			5.0

Comments for Sample AD27390 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 12-19-2001 Time: 13:02:58

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1301\27390.D
 Acq On : 13 Dec 2001 9:17 pm
 Sample : gcms unknown 11/14
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Dec 14 9:11 2001

Vial: 13
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table
 Last Update : Wed Nov 28 15:33:44 2001
 Response via : Initial Calibration
 DataAcq Meth : NP112701

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.86	152	911122	20.00	ng/uL	-0.08
19) Naphthalene-d8	15.47	136	3667876	20.00	ng/uL	-0.08
31) Acenaphthene-d10	20.75	164	1602363	20.00	ng/uL	-0.08
49) Phenanthrene-d10	25.15	188	2324290m	20.00	ng/uL	-0.10
59) Chrysene-d12	33.15	240	1477475	20.00	ng/uL	-0.10
68) Perylene-d12	37.23	264	1050043	20.00	ng/uL	-0.10

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ng/uL	
Spiked Amount	75.000	Range 18 - 42	Recovery	=	0.00%#	
5) Phenol-d5	0.00	99	0	0.00	ng/uL	
Spiked Amount	75.000	Range 19 - 32	Recovery	=	0.00%#	
6) 2-Chlorophenol-d4	11.86	132	730	0.01	ng/uL	0.44
Spiked Amount	75.000	Range 34 - 84	Recovery	=	0.01%#	
7) 1,2-Dichlorobenzene-d4	12.08	152	1274	0.03	ng/uL	-0.38
Spiked Amount	50.000	Range 26 - 73	Recovery	=	0.06%#	
20) Nitrobenzene-d5	0.00	82	0	0.00	ng/uL	
Spiked Amount	50.000	Range 55 - 98	Recovery	=	0.00%#	
32) 2-Fluorobiphenyl	18.89	172	1134	0.01	ng/uL	0.06
Spiked Amount	50.000	Range 42 - 78	Recovery	=	0.02%#	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng/uL	
Spiked Amount	75.000	Range 45 - 96	Recovery	=	0.00%#	
62) Terphenyl-d14	0.00	244	0	0.00	ng/uL	
Spiked Amount	50.000	Range 58 - 98	Recovery	=	0.00%#	

Target Compounds

				Qvalue
2) Pyridine	0.00	79	0	N.D.
3) N-nitrosodimethylamine	0.00	74	0	N.D.
8) Phenol	0.00	94	0	N.D.
9) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
10) 2-Chlorophenol	0.00	128	0	N.D.
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.
14) 2-Methylphenol	0.00	108	0	N.D.
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
16) 3&4-Methylphenol	0.00	108	0	N.D.

(#) = qualifier out of range (m) = manual integration

27390.D NP112701.M Fri Dec 14 12:15:53 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1301\27390.D
 Acq On : 13 Dec 2001 9:17 pm
 Sample : gcms unknown 11/14
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Dec 14 9:11 2001

Vial: 13
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table
 Last Update : Wed Nov 28 15:33:44 2001
 Response via : Initial Calibration
 DataAcq Meth : NP112701

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
17) N-Nitrosodi-n-propylamine	13.12	70	561	N.D.	
18) Hexachloroethane	0.00	117	0	N.D.	
21) Nitrobenzene	0.00	77	0	N.D.	
22) Isophorone	0.00	82	0	N.D.	
23) 2-Nitrophenol	0.00	139	0	N.D.	
24) 2,4-Dimethylphenol	0.00	107	0	N.D.	
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
26) 2,4-Dichlorophenol	0.00	162	0	N.D.	
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
28) Naphthalene	0.00	128	0	N.D.	
29) Hexachlorobutadiene	0.00	225	0	N.D.	
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.	
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.	
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.	
37) 2-Chloronaphthalene	0.00	162	0	N.D.	
38) Dimethylphthalate	0.00	163	0	N.D.	
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
40) Acenaphthylene	0.00	152	0	N.D.	
41) Acenaphthene	0.00	153	0	N.D.	
42) 2,4-Dinitrophenol	0.00	184	0	N.D.	
43) 4-Nitrophenol	0.00	65	0	N.D.	
44) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
45) Diethylphthalate	0.00	149	0	N.D.	
46) 4-Chlorophenylphenylether	0.00	204	0	N.D.	
47) Fluorene	0.00	166	0	N.D.	
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.	
51) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
53) Hexachlorobenzene	0.00	284	0	N.D.	
54) Pentachlorophenol	0.00	266	0	N.D.	
55) Phenanthrene	0.00	178	0	N.D.	
56) Anthracene	0.00	178	0	N.D.	
57) Di-n-butylphthalate	0.00	149	0	N.D.	d
58) Fluoranthene	0.00	202	0	N.D.	
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.	

(#) = qualifier out of range (m) = manual integration

27390.D NP112701.M Fri Dec 14 12:15:55 2001

Page 2

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1301\27390.D

Vial: 13

Acq On : 13 Dec 2001 9:17 pm

Operator: GALOS

Sample : gcms unknown 11/14

Inst : GC/MS Ins

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 14 9:11 2001

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

Last Update : Wed Nov 28 15:33:44 2001

Response via : Initial Calibration

DataAcq Meth : NP112701

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.15	228	2753	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.41	149	334	N.D.		
67) Chrysene	33.15	228	2753	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.23	252	3317	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

27390.D NP112701.M

Fri Dec 14 12:15:56 2001

Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC1301\27390.D
 Acq On : 13 Dec 2001 9:17 pm
 Sample : gcms unknown 11/14
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Dec 14 9:11 2001

Vial: 13
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

Quant Results File: NP112701.RES

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table
 Last Update : Fri Dec 14 09:15:17 2001
 Response via : Initial Calibration

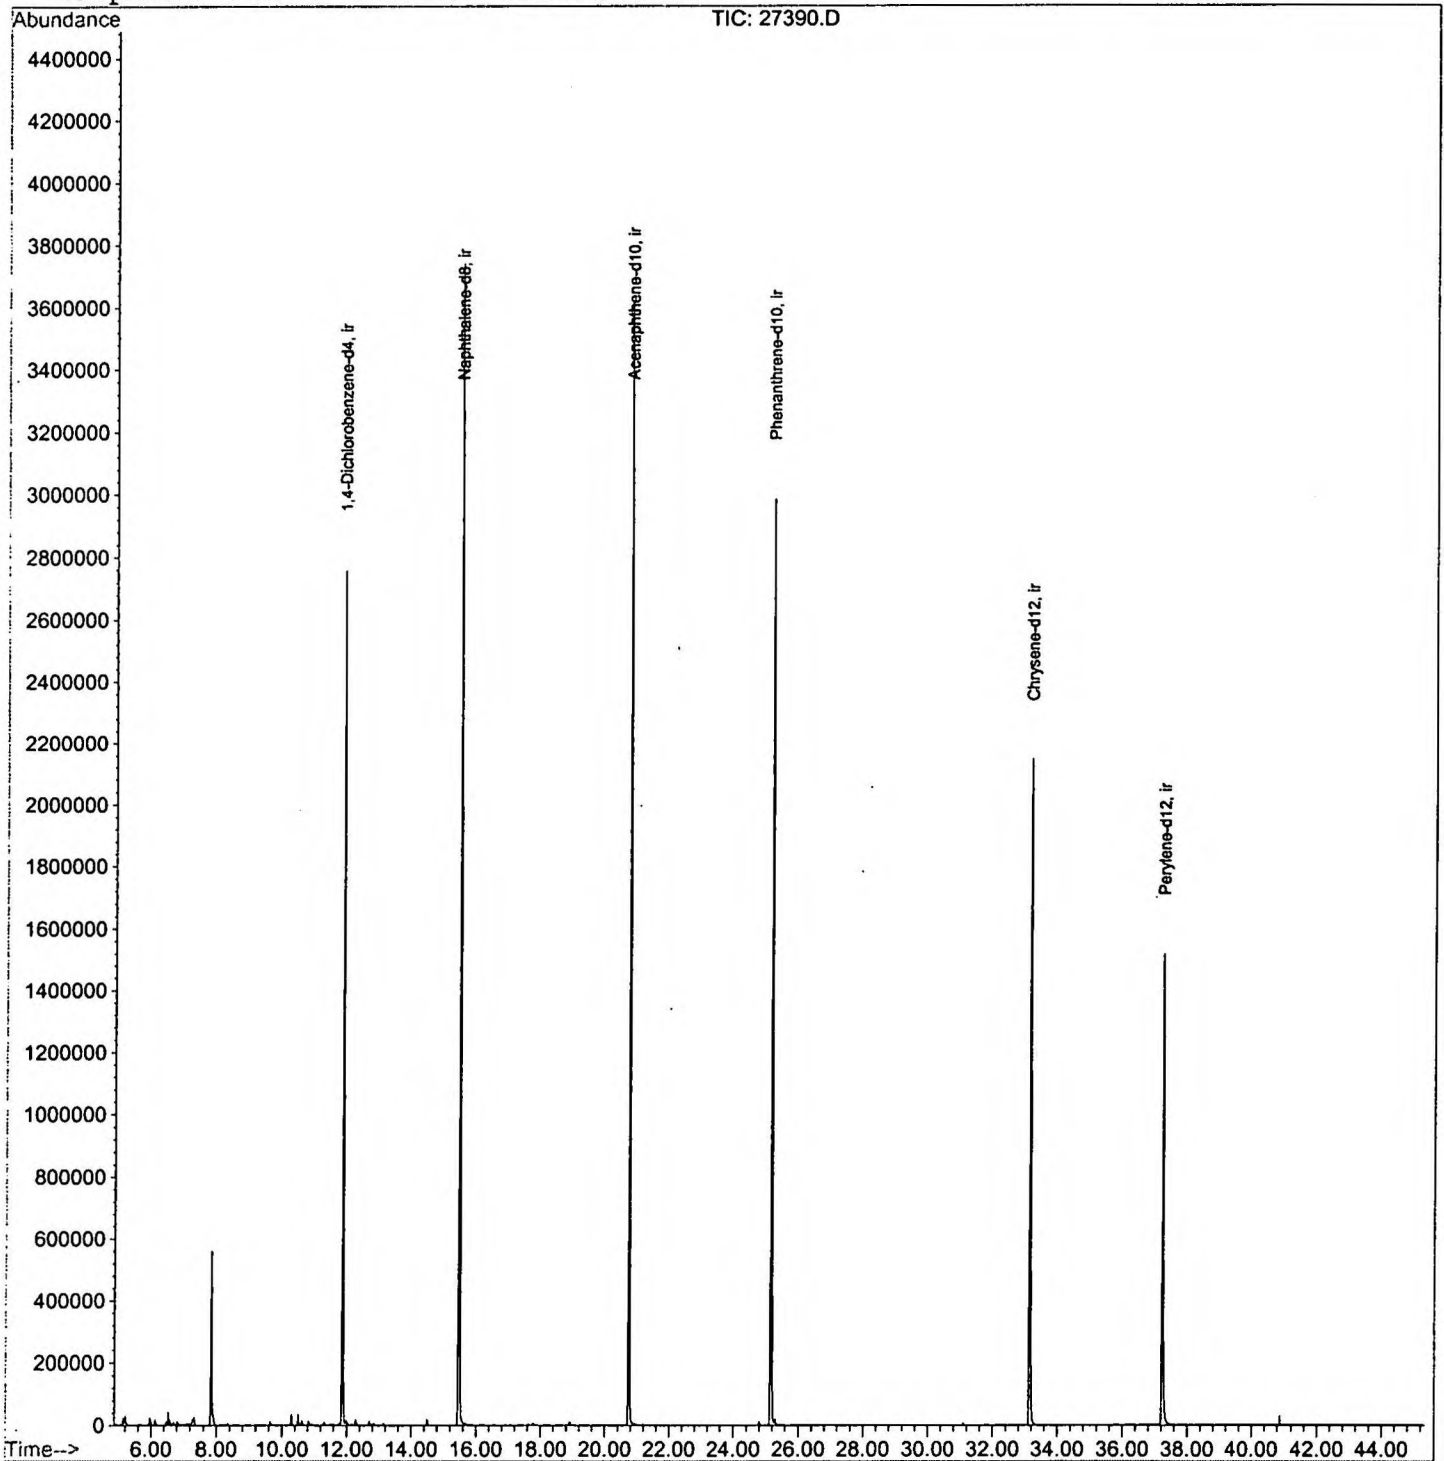

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC1301\27390.D

Vial: 13

Acq On : 13 Dec 2001 9:17 pm

Operator: GALOS

Sample : gcms unknown 11/14

Inst : GC/MS Ins

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.824	321	325	342	rBV	560805	1242371	16.78%	3.405%
2	11.859	760	765	776	rBV	2751801	5609989	75.78%	15.375%
3	15.472	1153	1159	1177	rBV	3740843	7403323	100.00%	20.290%
4	20.745	1728	1734	1747	rBV	3622237	7141501	96.46%	19.573%
5	25.156	2208	2215	2226	rBV2	2986361	6509133	87.92%	17.840%
6	33.152	3080	3087	3107	rBV2	2146389	4690564	63.36%	12.855%
7	37.233	3525	3532	3554	rBV	1514087	3890195	52.55%	10.662%




Sum of corrected areas: 36487076

27390.D NP112701.M

Fri Dec 14 12:38:31 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC1301\27390.D
 Operator : GALOS
 Acquired : 13 Dec 2001 9:17 pm using AcqMethod NP112701
 Instrument : GC/MS Ins
 Sample Name: gcms unknown 11/14
 Misc Info :
 Vial Number: 13
 Quant File :NP112701.RES (RTE Integrator)

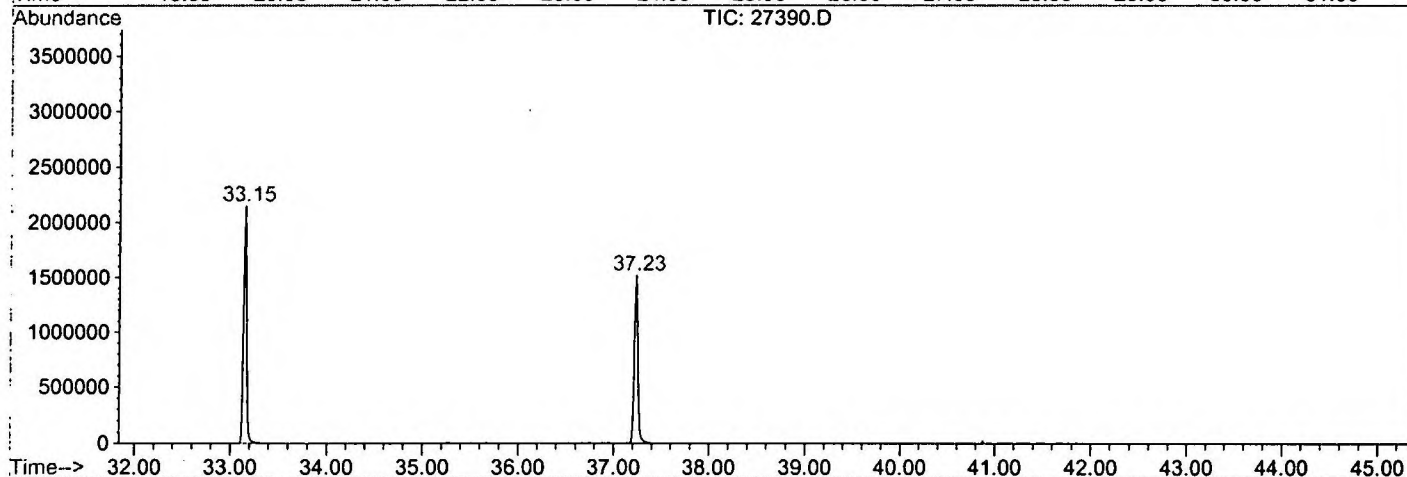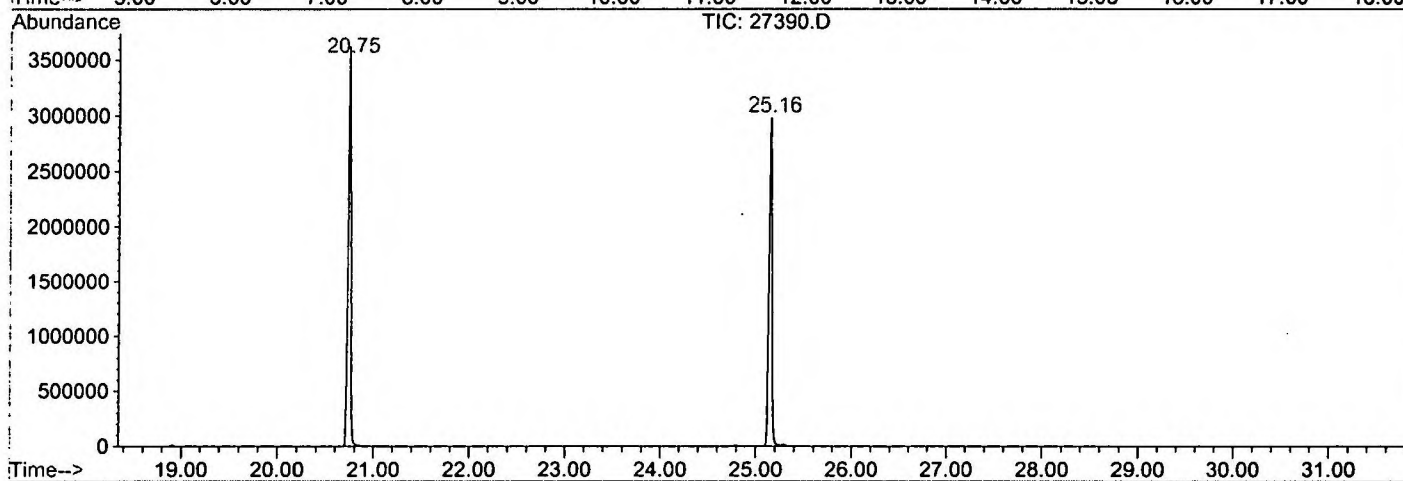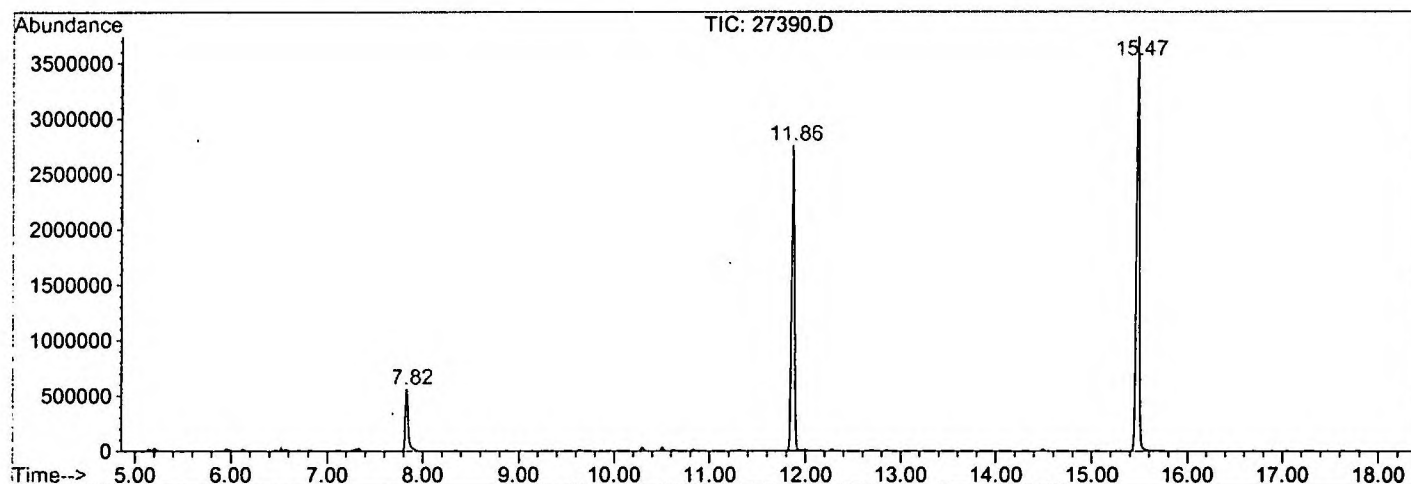

27390.D NP112701.M

Fri Dec 14 12:38:34 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC1301\27390.D
 Acq On : 13 Dec 2001 9:17 pm
 Sample : gcms unknown 11/14
 Misc :
 MS Integration Params: LSCINT.P










Vial: 13
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.82	4.43 ng/uL	1242370	1,4-Dichlorobenzene-d4	11.86

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
3			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45
4			Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	36

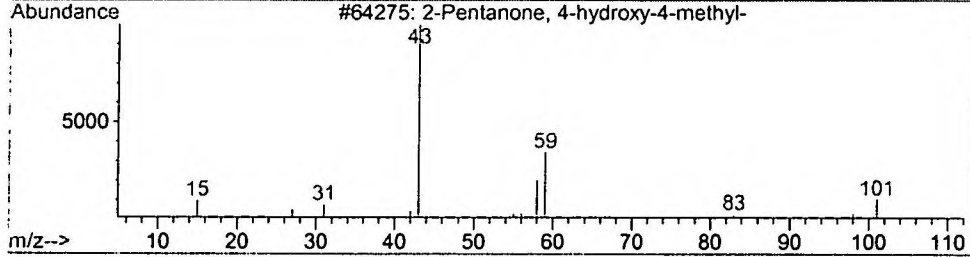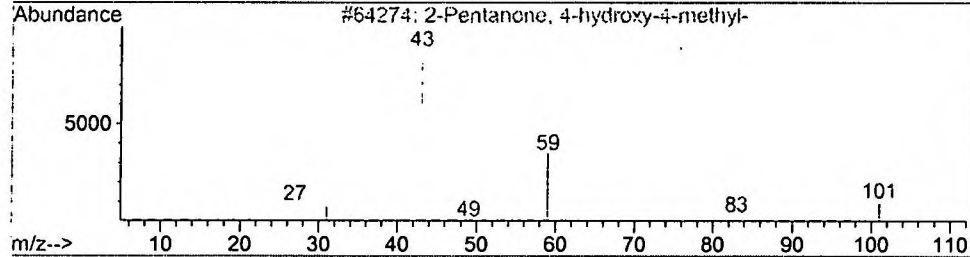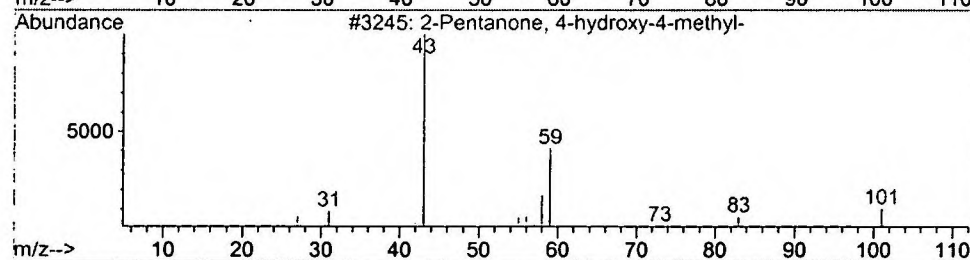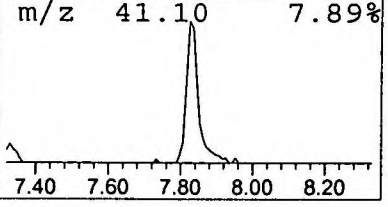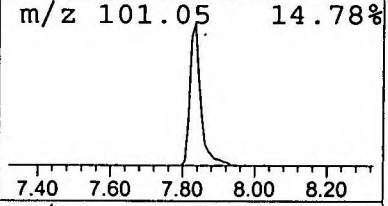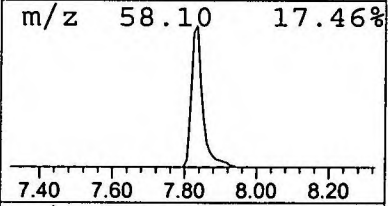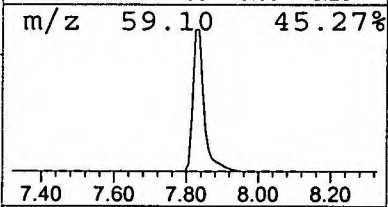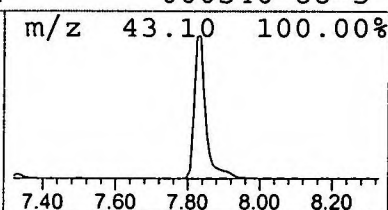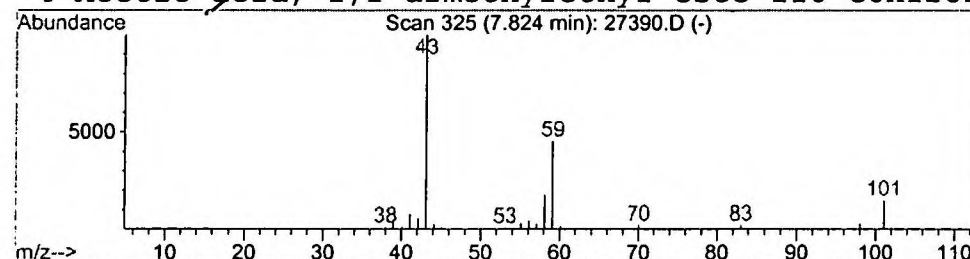

Tentatively Identified Compound (LSC) summary

Operator ID: GALOS Date Acquired: 13 Dec 2001 9:17 pm
 Data File: C:\HPCHEM\1\DATA\DEC1301\27390.D
 Name: gcms unknown 11/14
 Misc:
 Method: C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title: 208 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
----- 2-Pentanone , 4-hydro	7.82	4.4	ng/uL	1242370	ISTD01	11.86	5609990	20.0
27390.D NP112701.M	Fri Dec 14 12:38:38 2001							