

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 12/19/2001 Time: 11:22:46

Sample: AD27394
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 12/19/01 10:47 Ended: 12/19/01 10:47 Analyst: MG
 Page: 1

	Component Name	Viol	Result	MDL
1	Other unknown compounds		see comment	
2	Surr_2,4-DDD			5.0

Comments for Sample AD27394 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Galos, Marie

Date: 12-19-2001 Time: 11:22:53

A scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 12/19/2001 Time: 11:24:24

Sample: AD27395
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 12/19/01 10:45 Ended: 12/19/01 10:45 Analyst: MG
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	MDL
1	Other unknown compounds		see comment	
2	Surr_2,4-DDD	LSPEC	< MDL	5.0

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1301\27394.D
 Acq On : 14 Dec 2001 12:55 am
 Sample : gcms unknown 11/14
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Dec 14 9:12 2001

Vial: 17
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table
 Last Update : Wed Nov 28 15:33:44 2001
 Response via : Initial Calibration
 DataAcq Meth : NP112701

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.86	152	1031651	20.00	ng/uL	-0.07
19) Naphthalene-d8	15.47	136	4195433	20.00	ng/uL	-0.08
31) Acenaphthene-d10	20.74	164	1832613m	20.00	ng/uL	-0.08
49) Phenanthrene-d10	25.15	188	2754058m	20.00	ng/uL	-0.09
59) Chrysene-d12	33.15	240	1866890	20.00	ng/uL	-0.10
68) Perylene-d12	37.23	264	1355332	20.00	ng/uL	-0.11

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ng/uL	
Spiked Amount	75.000	Range 18 - 42	Recovery	=	0.00%#	
5) Phenol-d5	0.00	99	0	0.00	ng/uL	
Spiked Amount	75.000	Range 19 - 32	Recovery	=	0.00%#	
6) 2-Chlorophenol-d4	11.86	132	1080	0.01	ng/uL	0.43
Spiked Amount	75.000	Range 34 - 84	Recovery	=	0.01%#	
7) 1,2-Dichlorobenzene-d4	12.10	152	917	0.02	ng/uL	-0.36
Spiked Amount	50.000	Range 26 - 73	Recovery	=	0.04%#	
20) Nitrobenzene-d5	0.00	82	0	0.00	ng/uL	
Spiked Amount	50.000	Range 55 - 98	Recovery	=	0.00%#	
32) 2-Fluorobiphenyl	0.00	172	0d	0.00	ng/uL	
Spiked Amount	50.000	Range 42 - 78	Recovery	=	0.00%#	
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng/uL	
Spiked Amount	75.000	Range 45 - 96	Recovery	=	0.00%#	
62) Terphenyl-d14	0.00	244	0	0.00	ng/uL	
Spiked Amount	50.000	Range 58 - 98	Recovery	=	0.00%#	

Target Compounds

				Qvalue
2) Pyridine	0.00	79	0	N.D.
3) N-nitrosodimethylamine	0.00	74	0	N.D.
8) Phenol	0.00	94	0	N.D.
9) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
10) 2-Chlorophenol	0.00	128	0	N.D.
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.
14) 2-Methylphenol	0.00	108	0	N.D.
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
16) 3&4-Methylphenol	0.00	108	0	N.D.

(#) = qualifier out of range (m) = manual integration

27394.D NP112701.M Fri Dec 14 12:24:52 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1301\27394.D

Vial: 17

Acq On : 14 Dec 2001 12:55 am

Operator: GALOS

Sample : gcms unknown 11/14

Inst : GC/MS Ins

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 14 9:12 2001

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

Last Update : Wed Nov 28 15:33:44 2001

Response via : Initial Calibration

DataAcq Meth : NP112701

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
17) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.		
18) Hexachloroethane	0.00	117	0	N.D.		
21) Nitrobenzene	0.00	77	0	N.D.		
22) Isophorone	0.00	82	0	N.D.		
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	0.00	128	0	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.	d	
44) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
45) Diethylphthalate	0.00	149	0	N.D.		
46) 4-Chlorophenylphenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	169	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	25.22	178	388	N.D.		
56) Anthracene	25.22	178	388	N.D.		
57) Di-n-butylphthalate	27.14	149	14230	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		

(#)=qualifier out of range (m)=manual integration

27394.D NP112701.M Fri Dec 14 12:24:54 2001

Page 2

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1301\27394.D

Vial: 17

Acq On : 14 Dec 2001 12:55 am

Operator: GALOS

Sample : gcms unknown 11/14

Inst : GC/MS Ins

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 14 9:12 2001

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

Last Update : Wed Nov 28 15:33:44 2001

Response via : Initial Calibration

DataAcq Meth : NP112701

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
61) Benzidine	0.00	184	0	N.D.		
63) Pyrene	0.00	202	0	N.D.		
64) Butylbenzylphthalate	0.00	149	0	N.D.		
65) Benzo(a)anthracene	33.15	228	3691	N.D.		
66) Bis(2-ethylhexyl)phthalate	33.41	149	23416	N.D.		
67) Chrysene	33.15	228	3691	N.D.		
69) Di-n-Octylphthalate	0.00	149	0	N.D.		
70) Benzo(b)fluoranthene	0.00	252	0	N.D.		
71) Benzo(k)fluoranthene	0.00	252	0	N.D.		
72) Benzo(a)pyrene	37.24	252	4453	N.D.		
73) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
74) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
75) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

27394.D NP112701.M Fri Dec 14 12:24:55 2001

Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC1301\27394.D
 Acq On : 14 Dec 2001 12:55 am
 Sample : gcms unknown 11/14
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Dec 14 9:12 2001

Vial: 17
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

Quant Results File: NP112701.RES

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table
 Last Update : Fri Dec 14 09:15:17 2001
 Response via : Initial Calibration

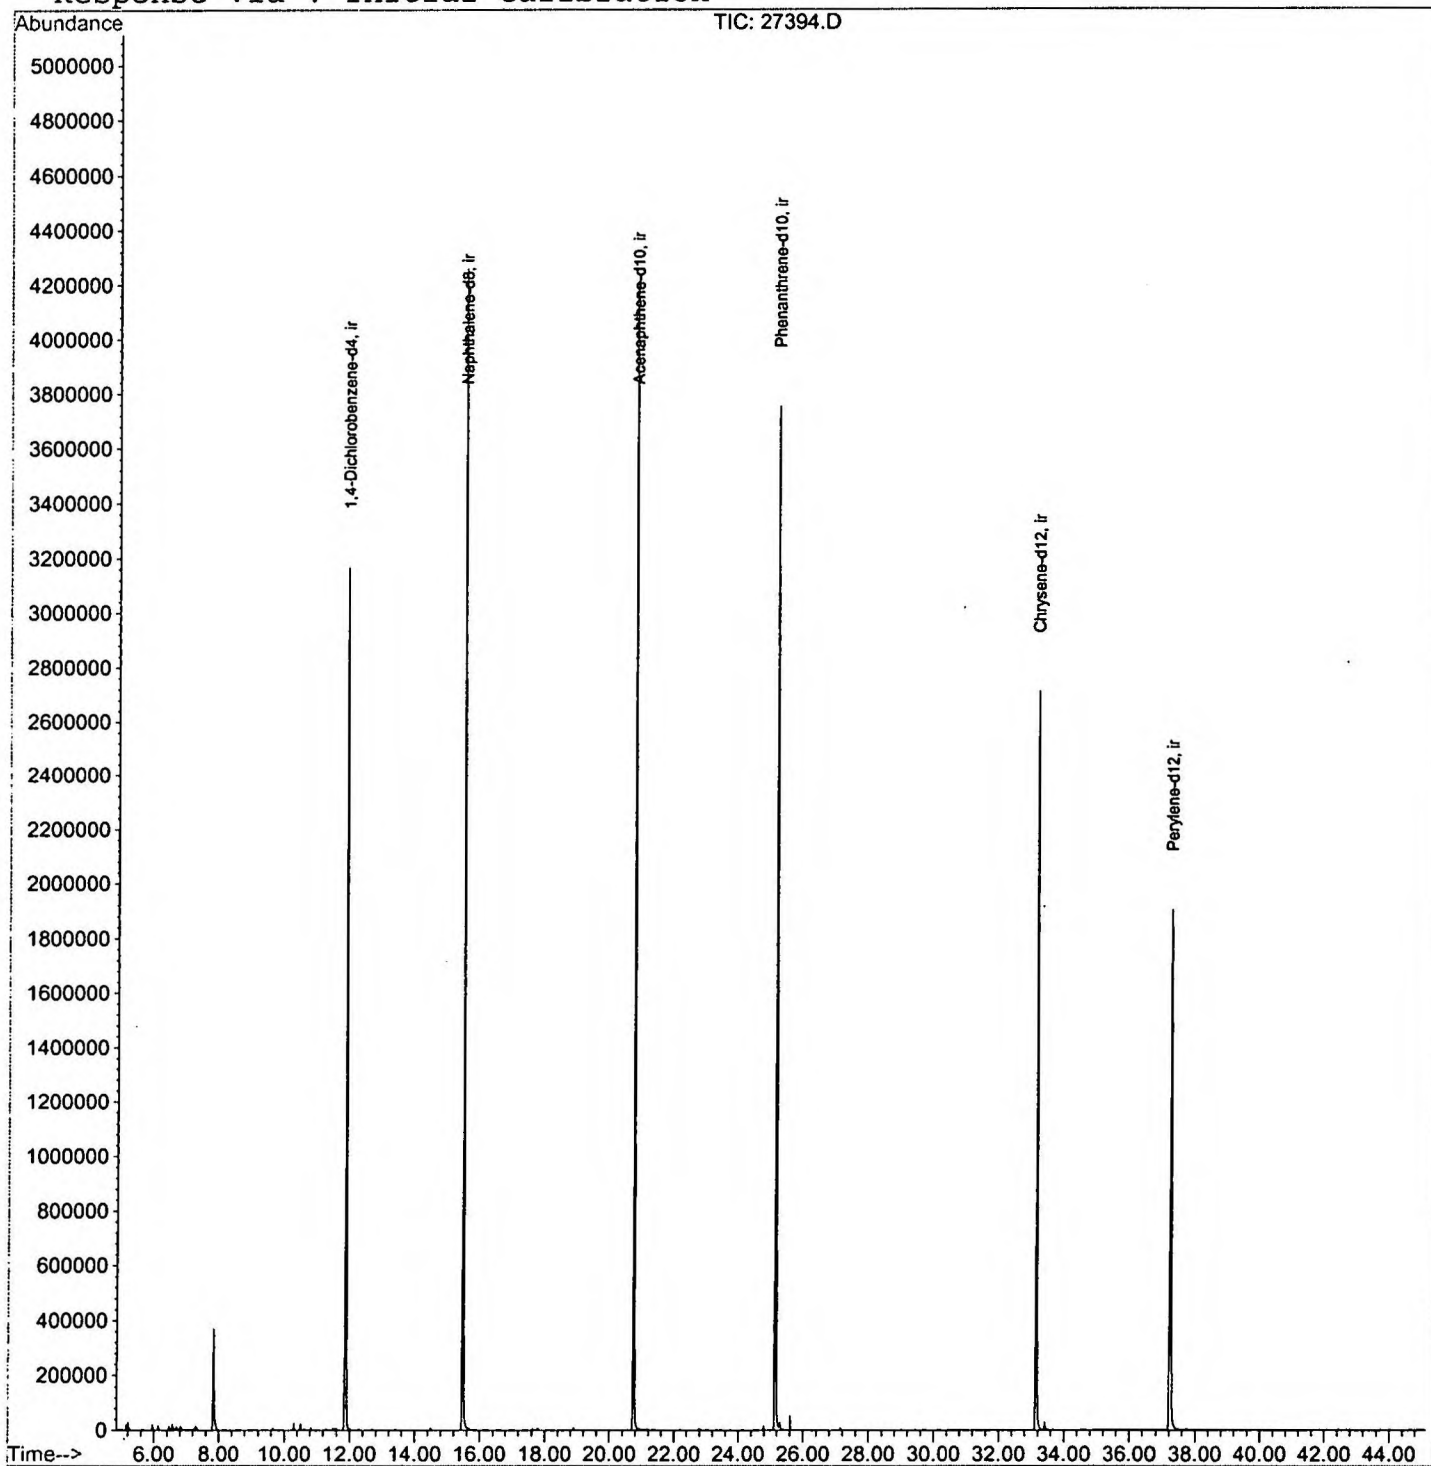

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC1301\27394.D
 Acq On : 14 Dec 2001 12:55 am
 Sample : gcms unknown 11/14
 Misc :
 MS Integration Params: LSCINT.P

Vial: 17
 Operator: GALOS
 Inst : GC/MS Ins
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title : 208 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.830	322	326	341	rBV	370389	788163	9.32%	1.846%
2	11.865	760	766	777	rVB	3162048	6390138	75.59%	14.968%
3	15.469	1153	1159	1177	rBV	4259918	8454064	100.00%	19.802%
4	20.741	1728	1734	1750	rBV	4212904	8305378	98.24%	19.454%
5	25.152	2208	2215	2226	rBV2	3754739	7748443	91.65%	18.149%
6	33.148	3081	3087	3103	rBV2	2711925	5946099	70.33%	13.928%
7	37.229	3524	3532	3552	rBV2	1902491	5060264	59.86%	11.853%

Sum of corrected areas: 42692549

27394.D NP112701.M Fri Dec 14 12:39:53 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC1301\27394.D
 Operator : GALOS
 Acquired : 14 Dec 2001 12:55 am using AcqMethod NP112701
 Instrument : GC/MS Ins
 Sample Name: gcms unknown 11/14
 Misc Info :
 Vial Number: 17
 Quant File :NP112701.RES (RTE Integrator)

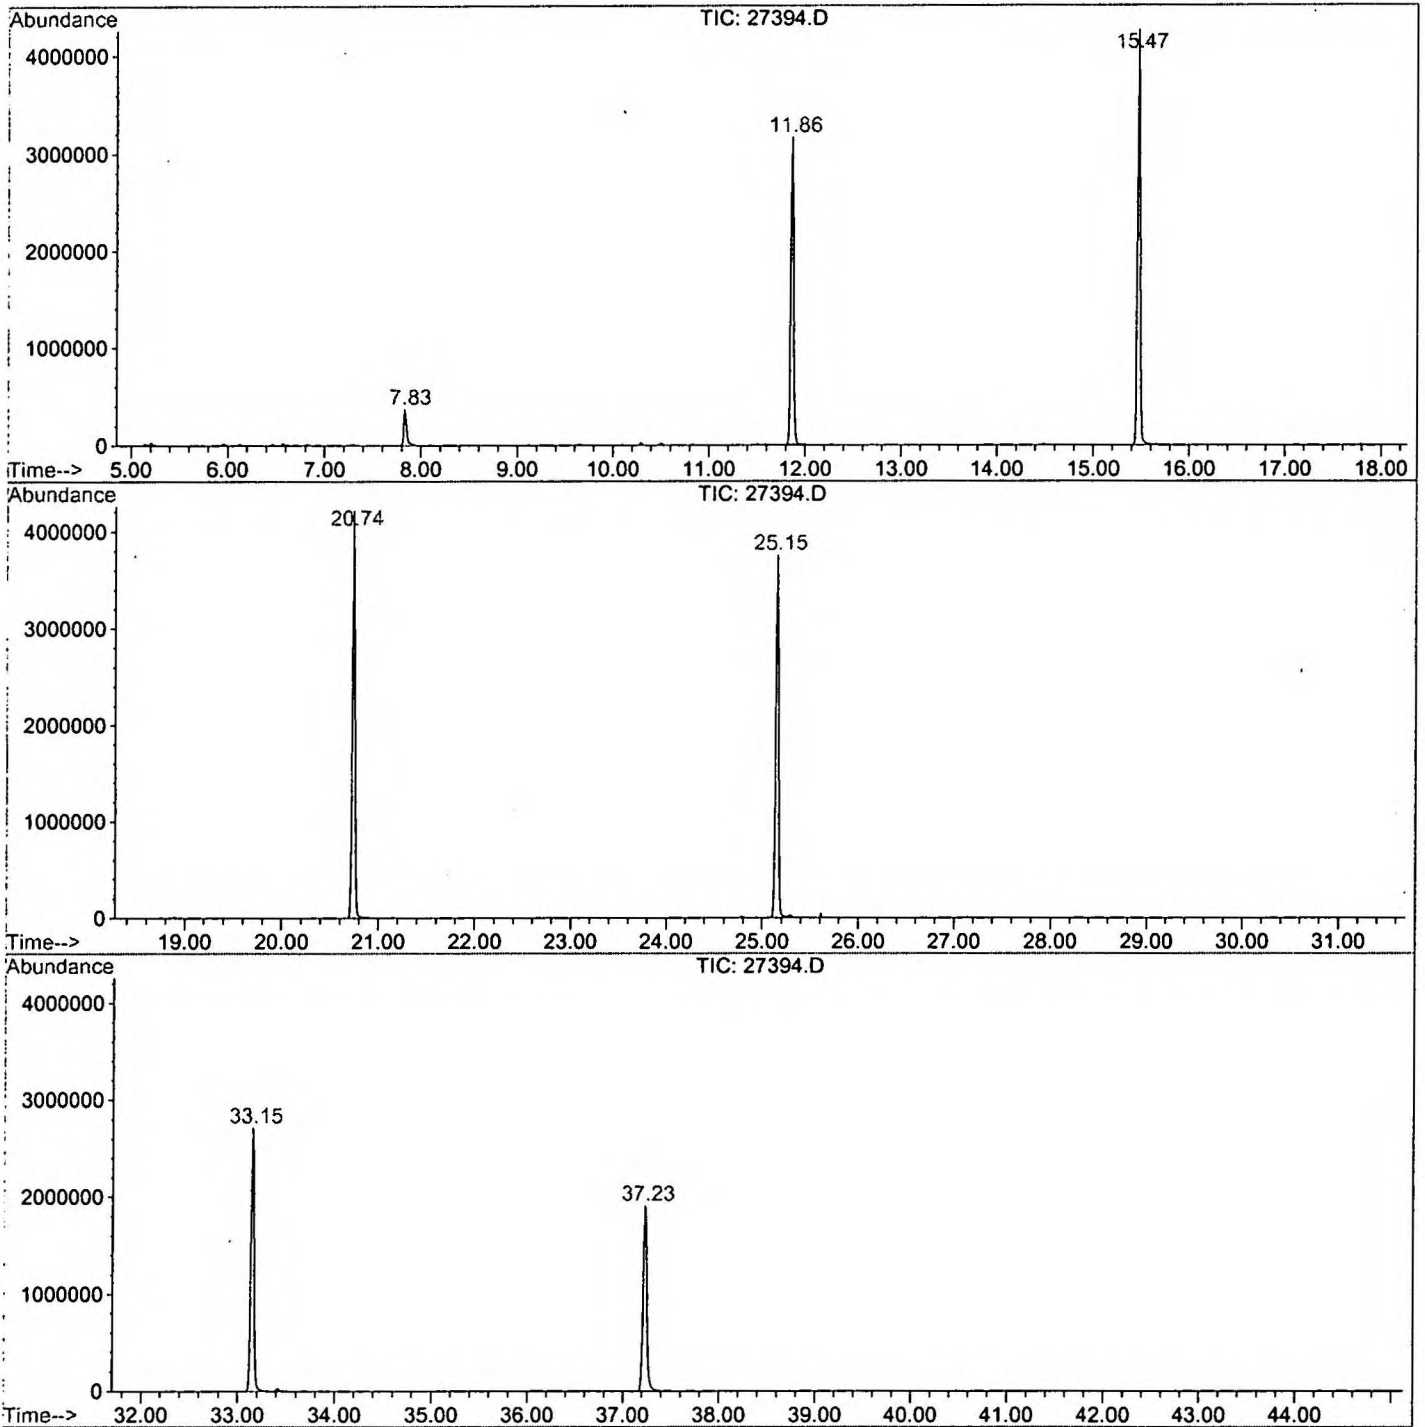

27394.D NP112701.M

Fri Dec 14 12:39:56 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC1301\27394.D
Acq On : 14 Dec 2001 12:55 am
Sample : gcms unknown 11/14
Misc :
MS Integration Params: LSCINT.P


Vial: 17
Operator: GALOS
Inst : GC/MS Ins
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
Title : 208 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.83	2.47 ng/uL	788163	1,4-Dichlorobenzene-d4	11.86

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
3			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	43
4			Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	28

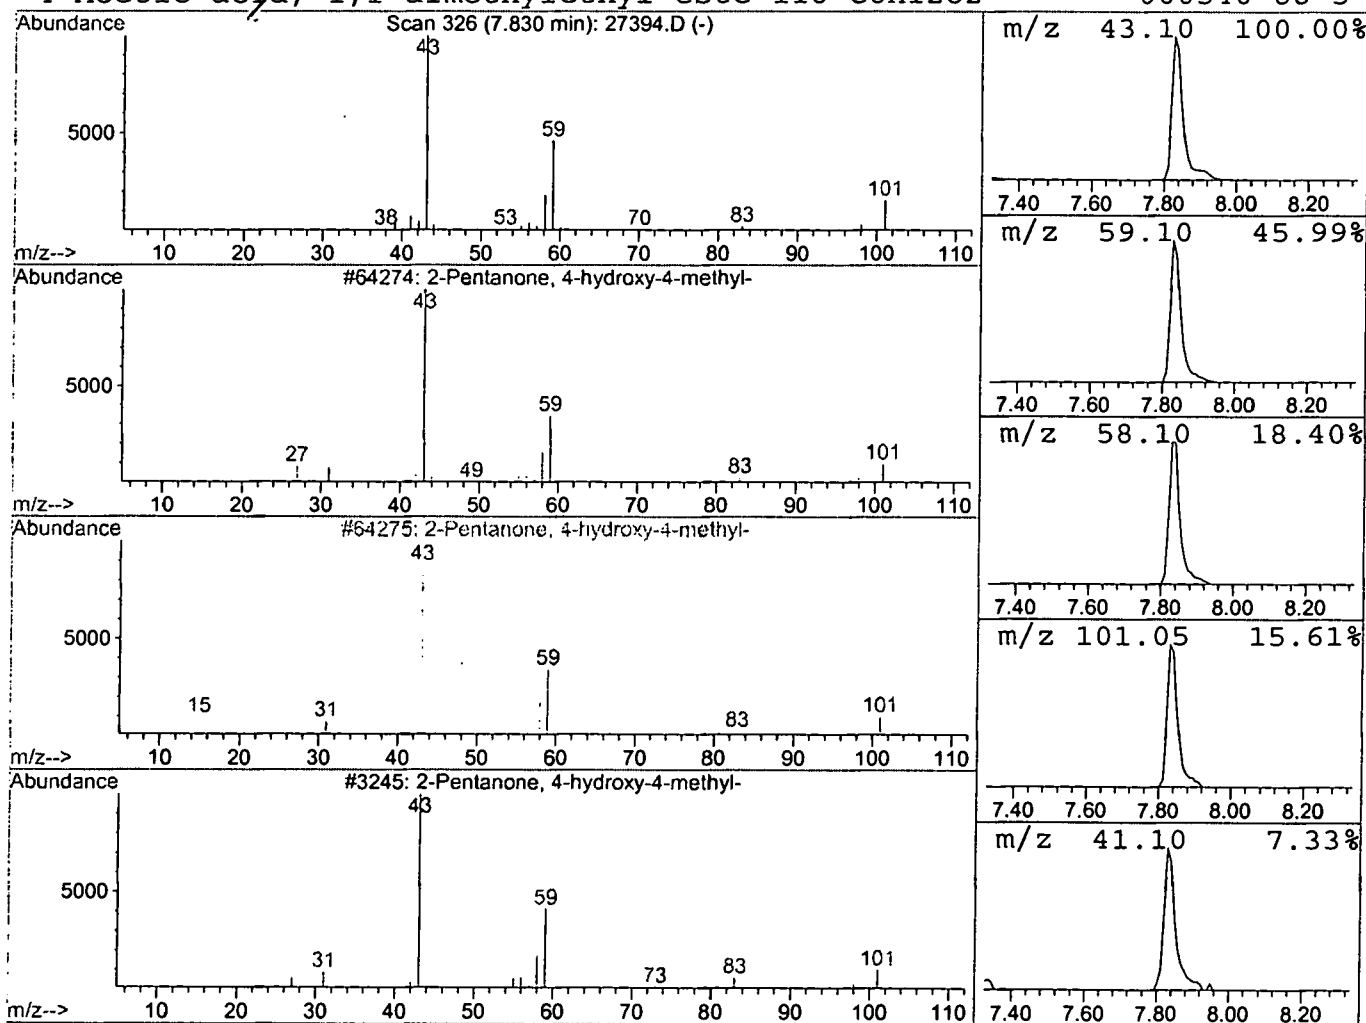

Tentatively Identified Compound (LSC) summary

Operator ID: GALOS Date Acquired: 14 Dec 2001 12:55 am
Data File: C:\HPCHEM\1\DATA\DEC1301\27394.D
Name: gcms unknown 11/14
Misc:
Method: C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
Title: 208 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	7.83	2.5	ng/uL	788163	ISTD01	11.86	6390140	20.0

27394.D NP112701.M Fri Dec 14 12:40:00 2001