

Page

(Cont)

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
	27780	500 mL	500	1 mL			2 mL		= 7	1
	27781		↓							2
	27782		↓							3
/	✓ 27817	- ✓								4
/	✓ 27818	- ✓								5
/	✓ 27819	- ✓								6
/	✓ 27823	- ✓								7
/	✓ 27826	- ✓								8
/	✓ 27828	- ✓								9
/	✓ 27831	- ✓								10
Remarks										
27776 - 27782 Rochland County samples.										
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -										
Extraction type - Sep funnel Solv. lot# V43 E07 NaCl lot# V11599 Na2SO4 lot# V30603										
STANDARD INT STD LOG#										
CALIBRATION										
REF/SPIKE tox: 2109 chl: 2108 Pest: 2062										
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE 1839 b										
LPC										
ENDRIN/DDT										

Analyst ML/AN/EH/LF
revision 4/12/01

Verified by

Reviewed by _____
Date _____

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC1801\DFTPP1.D

Vial: 1

Acq On : 19 Dec 2001 8:42 am

Operator: 209 GALOS

Sample :

Inst : GC/MS 209


Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

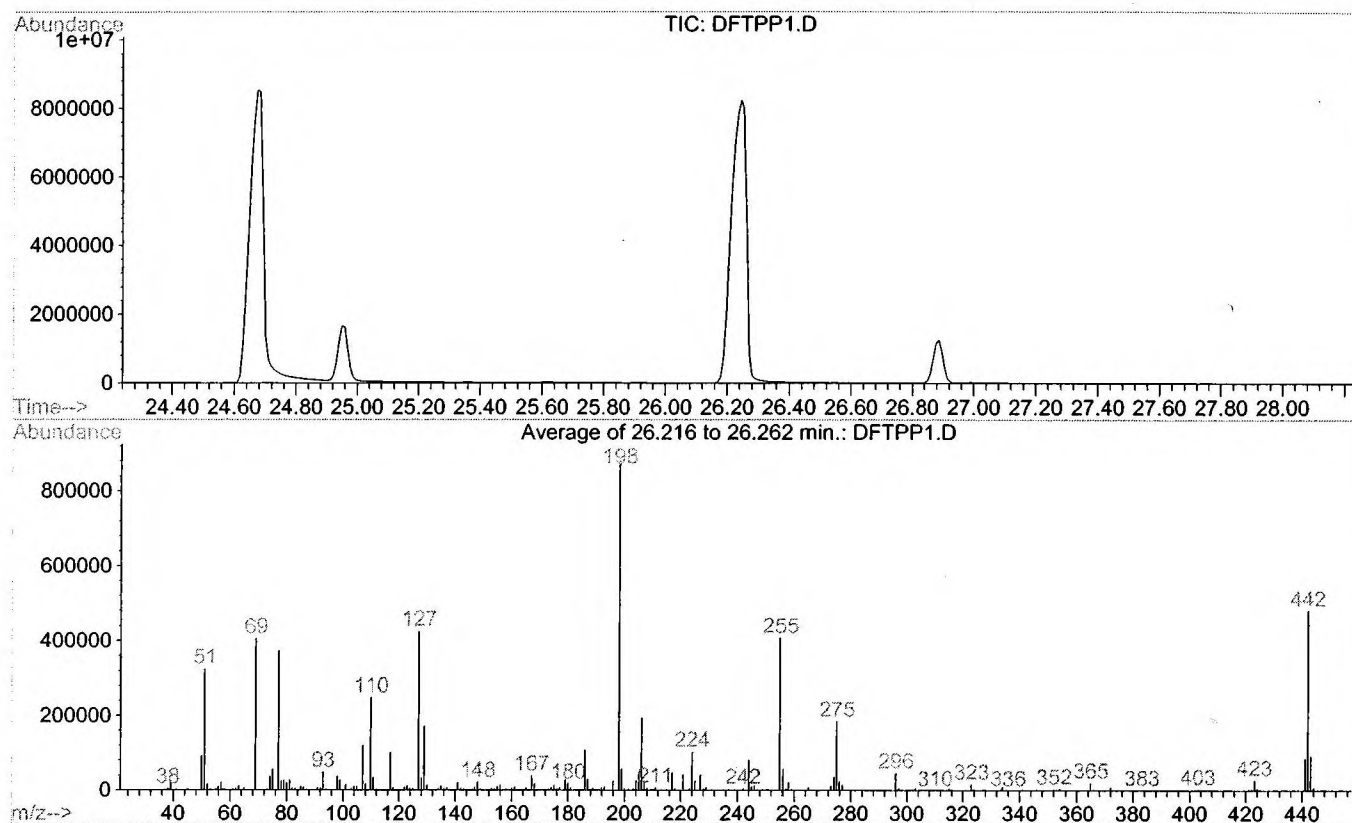

Spectrum Information: Average of 26.216 to 26.262 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.9	325045	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.2	406955	PASS
70	69	0.00	2	0.0	56	PASS
127	198	40	60	48.4	426496	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	881184	PASS
199	198	5	9	6.6	58321	PASS
275	198	10	30	21.1	185931	PASS
365	198	1	100	2.5	21764	PASS
441	443	0.01	100	92.7	86832	PASS
442	198	40	110	54.7	481835	PASS
443	442	17	23	19.4	93632	PASS