

Jser: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 01/03/2002 Time: 10:12:03

Sample: AD27823
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 1/3/02 10:10 Ended: 1/3/02 10:10 Analyst: MG
 Page: 1

	Component Name	Viol	Result	MDL
1	Other unknown compounds		see comment	
2	Surr_2,4-DDD			5.0

Comments for Sample AD27823 - Analysis \$GCMS

Westchester Dept. of Labs & Research

Analyst: Galos, Marie

Date: 01-03-2002 Time: 10:12:17

Scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1901\27823.D

Vial: 31

Acq On : 19 Dec 2001 8:32 pm

Operator: 209 GALOS

Sample : gc/msunknown 11/19

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Dec 19 21:21 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 14 12:19:30 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.66	152	736907	20.00	ug/l	-0.04
10) Naphthalene-d8	15.28	136	2805814	20.00	ug/l	-0.03
17) Acenaphthene-d10	20.55	164	1378974	20.00	ug/l	-0.03
29) Phenanthrene-d10	24.97	188	2050212	20.00	ug/l	-0.02
38) Chrysene-d12	33.01	240	1330149	20.00	ug/l	-0.02
44) Perylene-d12	37.10	264	859057	20.00	ug/l	-0.02

System Monitoring Compounds

37) 2,4-DDD	0.00	235	0	0.00 ug/mL
Spiked Amount	5.000		Recovery	= 0.00%

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	12.88	77	101	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	15.33	128	201	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	20.96	165	432	N.D.
25) Diethylphthalate	0.00	149	0	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#)=qualifier out of range (m)=manual integration

27823.D GCMS1126.M Mon Dec 31 11:14:13 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1901\27823.D

Vial: 31

Acq On : 19 Dec 2001 8:32 pm

Operator: 209 GALOS

Sample : gc/msunknown 11/19

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Dec 19 21:21 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 14 12:19:30 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.05	178	118 /	N.D.		
34) Anthracene	25.05	178	118 /	N.D.		
35) Di-n-butylphthalate	27.04	149	1506 /	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0 /	N.D.		
41) Benzo(a)anthracene	33.01	228	3497	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.29	149	2478 /	N.D.		
43) Chrysene	33.01	228	3497 /	N.D.		
45) Di-n-Octylphthalate	35.04	149	111	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.10	252	3236 /	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

27823.D GCMS1126.M Mon Dec 31 11:14:17 2001

Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC1901\27823.D

Acq On : 19 Dec 2001 8:32 pm

Sample : gc/msunknown 11/19

Misc :

MS Integration Params: GOOFY.P

Quant Time: Dec 19 21:21 2001

Vial: 31

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00


Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

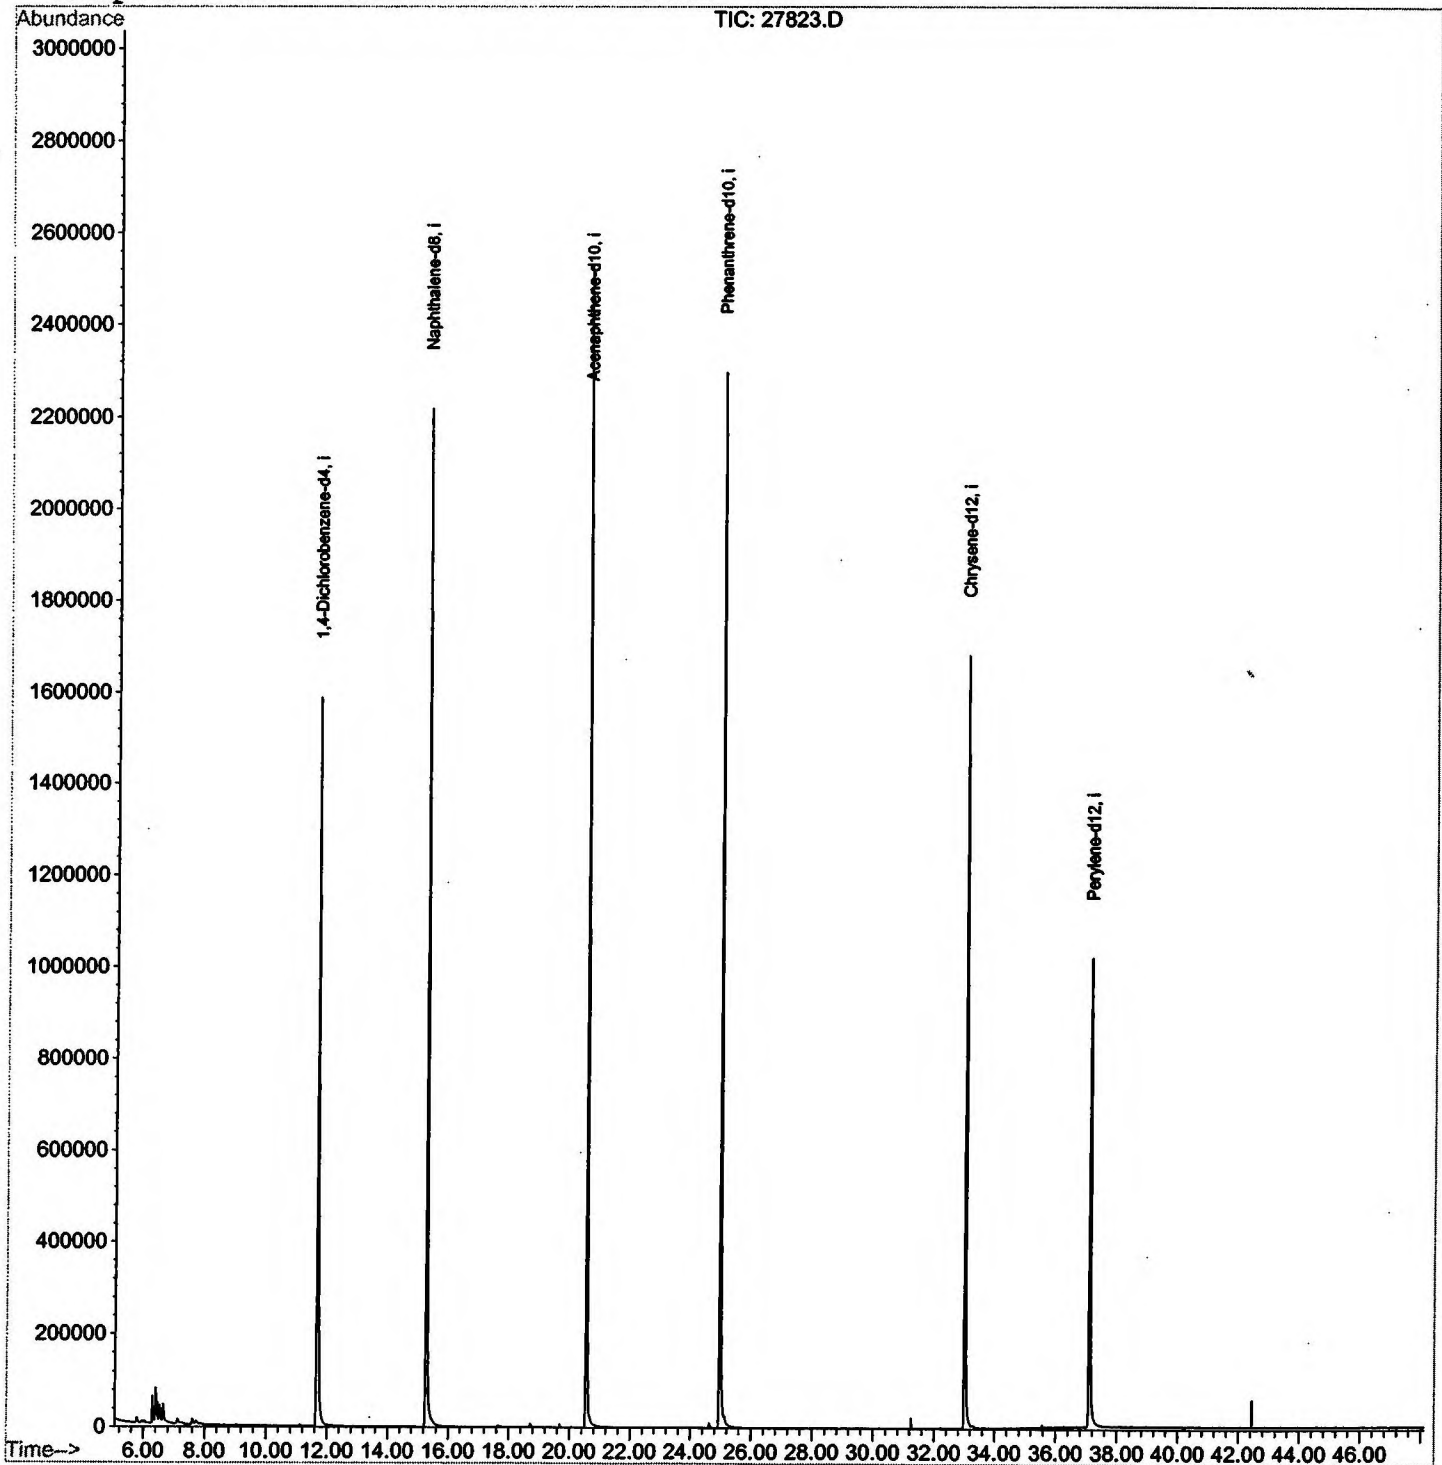

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC1901\27823.D

Vial: 31

Acq On : 19 Dec 2001 8:32 pm

Operator: 209 GALOS

Sample : gc/msunknown 11/19

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	6.290	132	136	143	rBV	58495	128884	2.21%	0.449%
2	6.391	144	147	153	rBV	70707	185631	3.18%	0.646%
3	6.529	158	162	171	rVV	38047	108186	1.86%	0.377%
4	6.639	171	174	191	rVB2	39178	120958	2.07%	0.421%
5	11.661	716	721	747	rBV	1586385	4253283	72.94%	14.804%
6	15.269	1109	1114	1133	rBV	2217153	5410366	92.78%	18.832%
7	20.547	1683	1689	1710	rBV	2530251	5831232	100.00%	20.297%
8	24.972	2165	2171	2185	rBV2	2297734	5392100	92.47%	18.768%
9	33.014	3040	3047	3070	rBV2	1680883	4176082	71.62%	14.536%
10	37.109	3485	3493	3517	rBV2	1016677	3123115	53.56%	10.871%


Sum of corrected areas: 28729837

27823.D GCMS1126.M

Wed Jan 02 12:07:47 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC1901\27823.D
 Operator : 209 GALOS
 Acquired : 19 Dec 2001 8:32 pm using AcqMethod GCMS1126
 Instrument : GC/MS 209
 Sample Name: gc/msunknown 11/19
 Misc Info :
 Vial Number: 31
 Quant File :GCMS1126.RES (RTE Integrator)

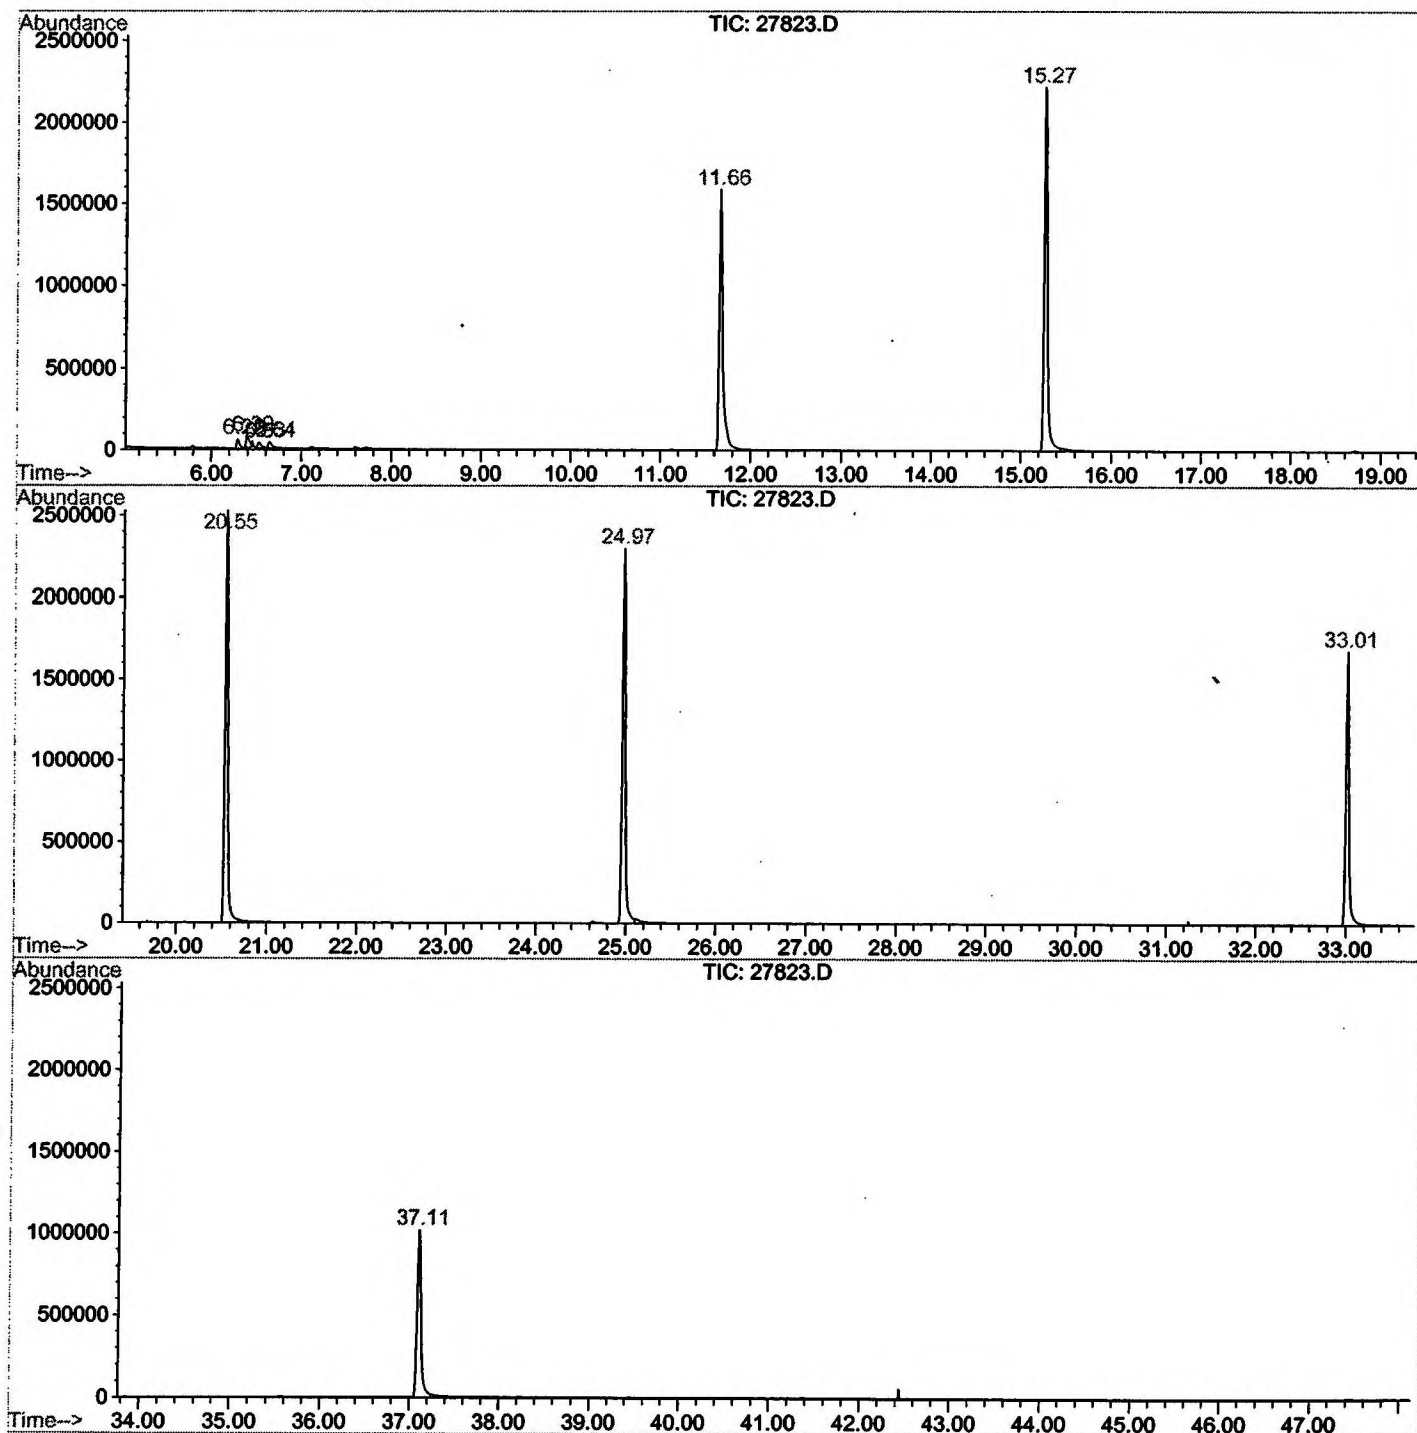

27823.D GCMS1126.M

Wed Jan 02 12:07:52 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC1901\27823.D
Acq On : 19 Dec 2001 8:32 pm
Sample : gc/msunknown 11/19
Misc :
MS Integration Params: LSCINT.P









Vial: 31
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 3-Hexanone Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.29	0.61 ug/l	128884	1,4-Dichlorobenzene-d4	11.66

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Hexanone			100	C6H12O	000589-38-8	91
2	3-Pentanone, 2-methyl-			100	C6H12O	000565-69-5	43
3	3(2H)-Furanone, dihydro-2-methyl-			100	C5H8O2	003188-00-9	38
4	Butane, 2,2-dimethyl-			86	C6H14	000075-83-2	33

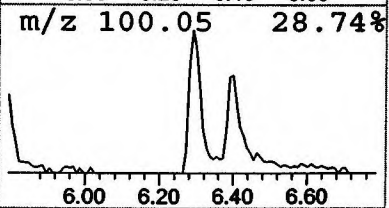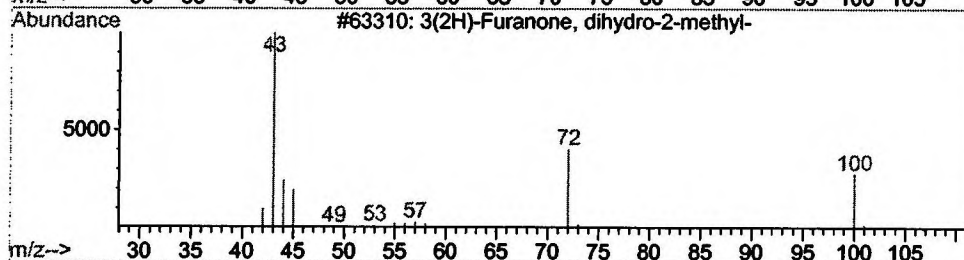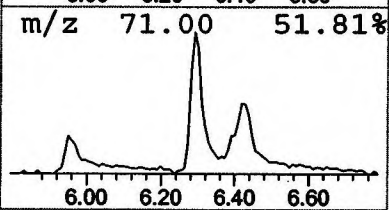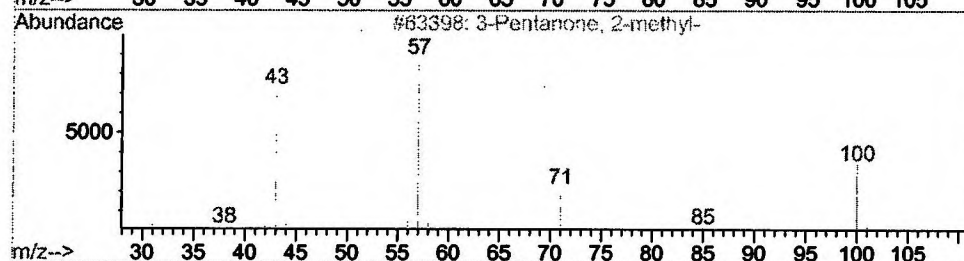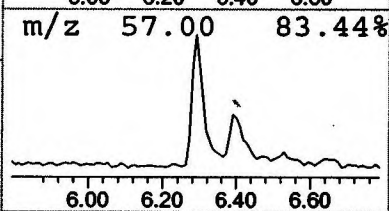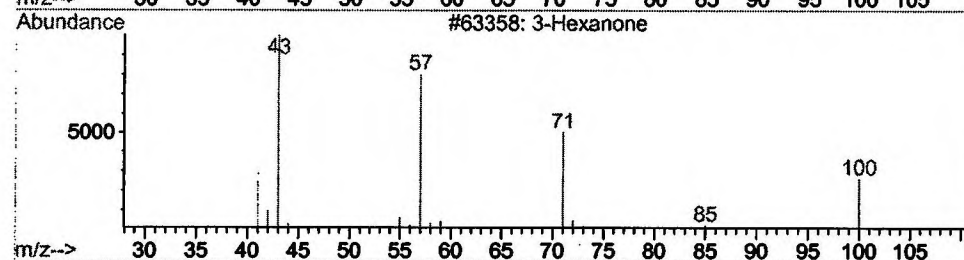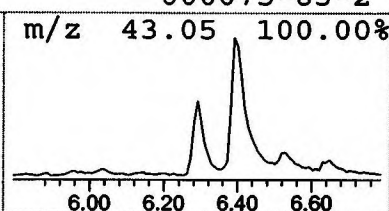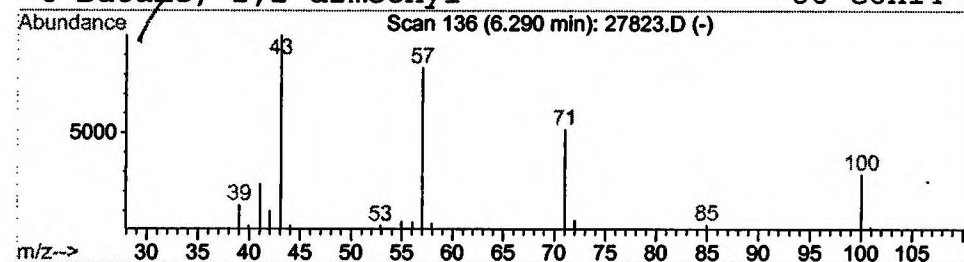

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC1901\27823.D

Acq On : 19 Dec 2001 8:32 pm

Sample : gc/msunknown 11/19

Misc :

MS Integration Params: LSCINT.P

Vial: 31

Operator: 209 GALOS

Inst. : GC/MS 209

Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table










Library : C:\DATABASE\NBS75K.L

Peak Number 2 2-Hexanone

Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.39	0.87 ug/l	185631	1,4-Dichlorobenzene-d4	11.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Hexanone	100	C6H12O	000591-78-6	91
2		2-Hexanone, 4-hydroxy-3-propyl-	158	C9H18O2	062338-17-4	64
3		2-Hexanone, 4-hydroxy-5-methyl-3-pr	172	C10H20O2	061141-74-0	59
4		Oxirane, 2-methyl-2-(1-methylethyl)	100	C6H12O	072221-03-5	50

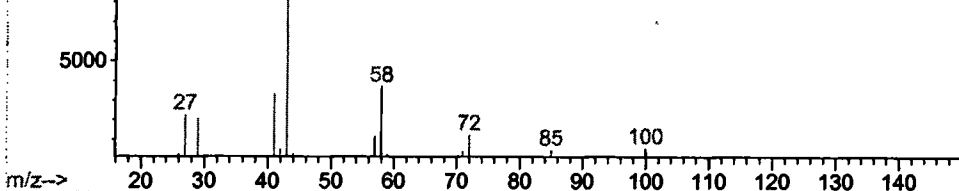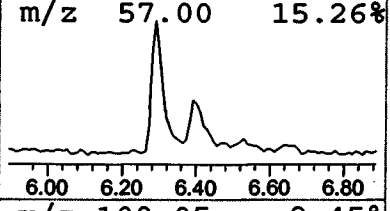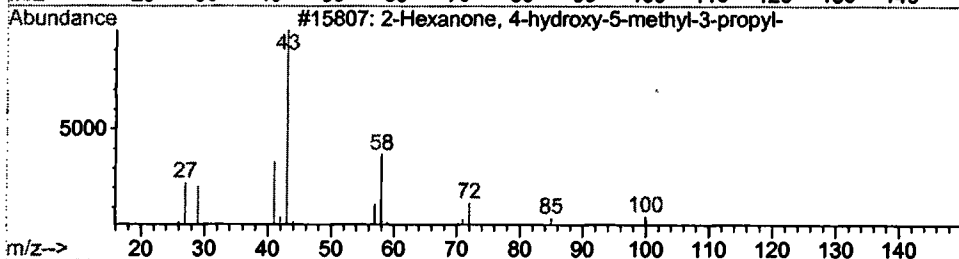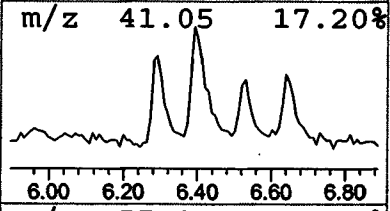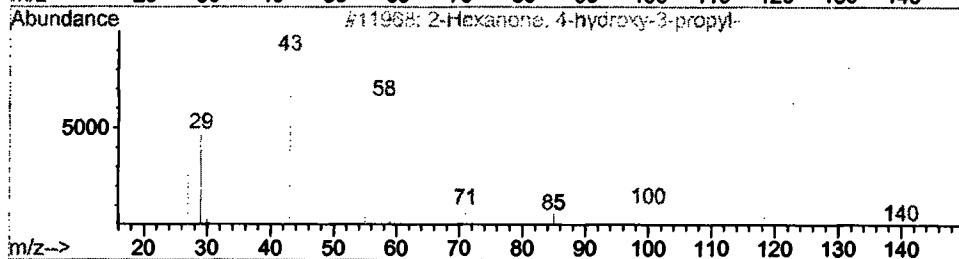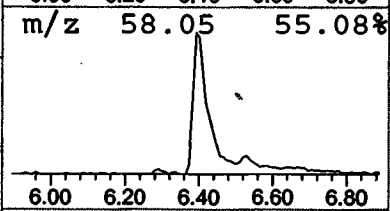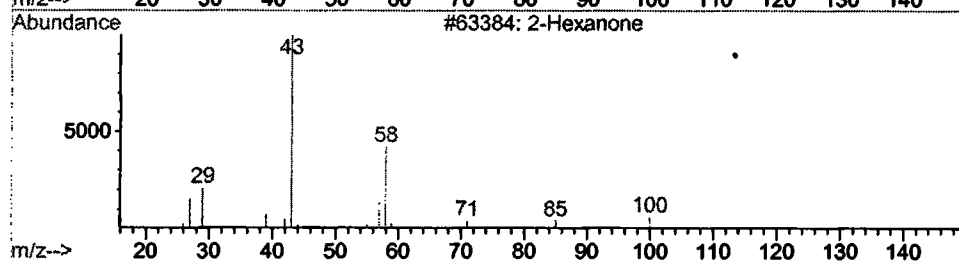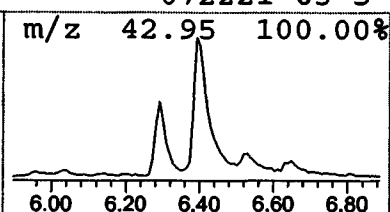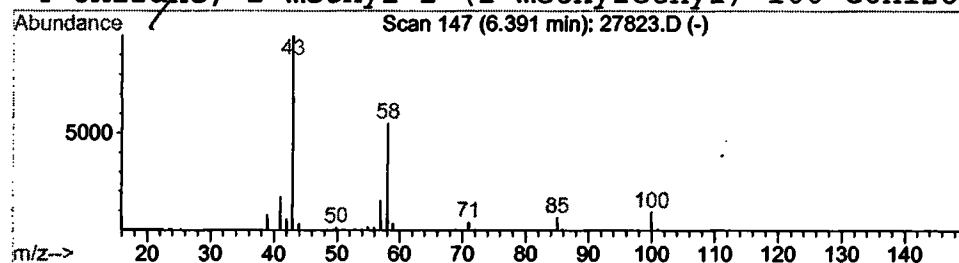

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC1901\27823.D
Acq On : 19 Dec 2001 8:32 pm
Sample : gc/msunknown 11/19
Misc :
MS Integration Params: LSCINT.P










Vial: 31
Operator: 209 GALOS
Inst. : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 3 3-Hexanol Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.53	0.51 ug/l	108186	1,4-Dichlorobenzene-d4	11.66

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Hexanol	102	C6H14O	000623-37-0	90
2			3-Pentanol, 2-methyl-	102	C6H14O	000565-67-3	50
3			3-Pentanol	88	C5H12O	000584-02-1	42
4			Amylene Hydrate	88	C5H12O	000075-85-4	39

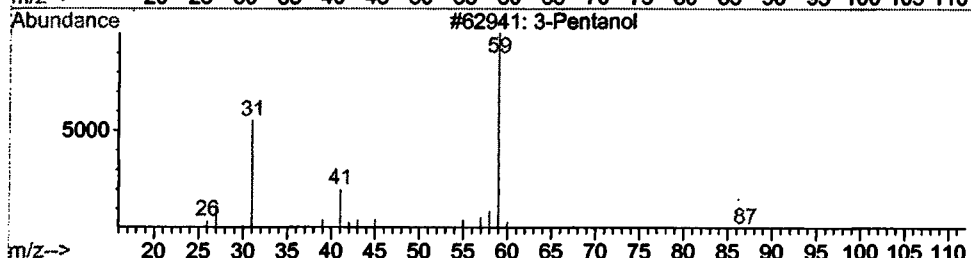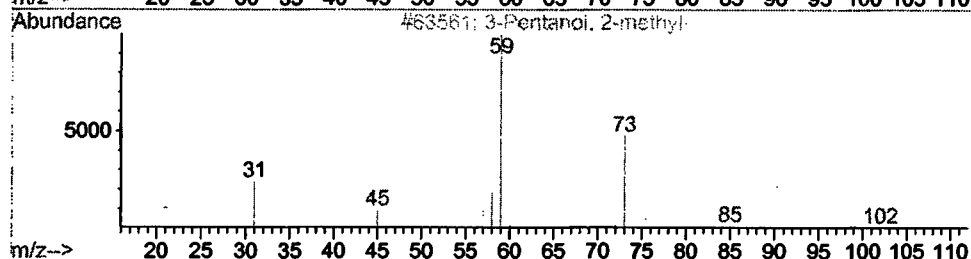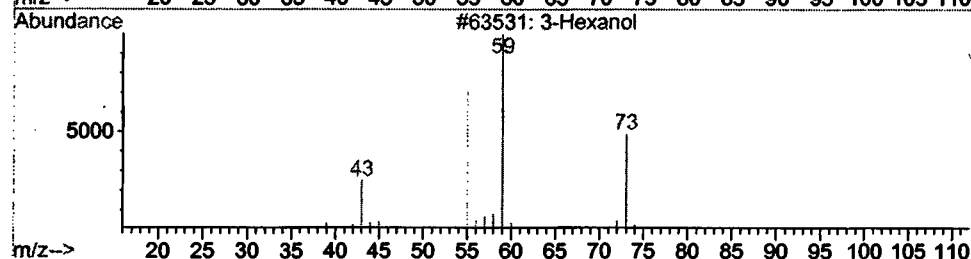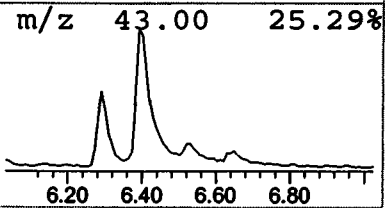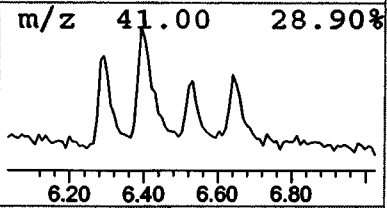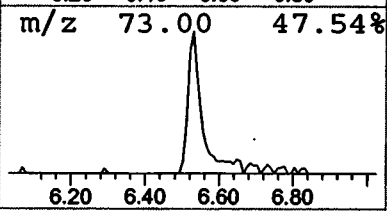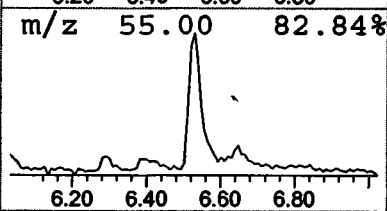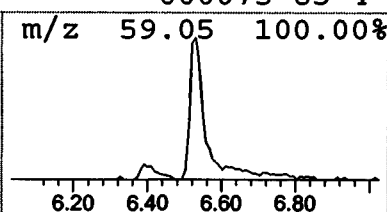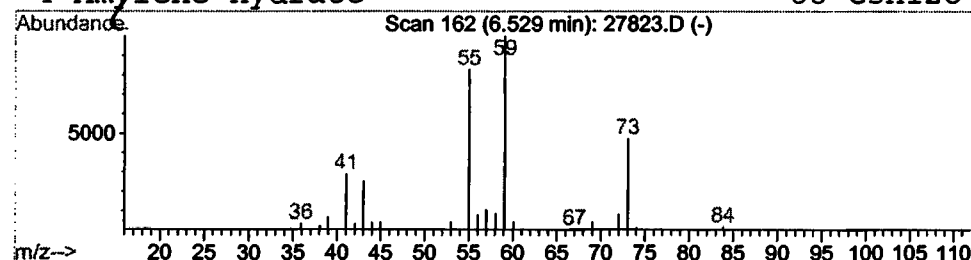

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC1901\27823.D
 Acq.On : 19 Dec 2001 8:32 pm
 Sample : gc/msunknown 11/19
 Misc :
 MS Integration Params: LSCINT.P


Vial: 31
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 4 2-Hexanol Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.64	0.57 ug/l	120958	1,4-Dichlorobenzene-d4	11.66

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Hexanol	102	C6H14O	000626-93-7	74
2	2-Pentanol, 4-methyl-	102	C6H14O	000108-11-2	64
3	2-Hexanol, (S)-	102	C6H14O	052019-78-0	64
4	2-Butanol	74	C4H10O	000078-92-2	50

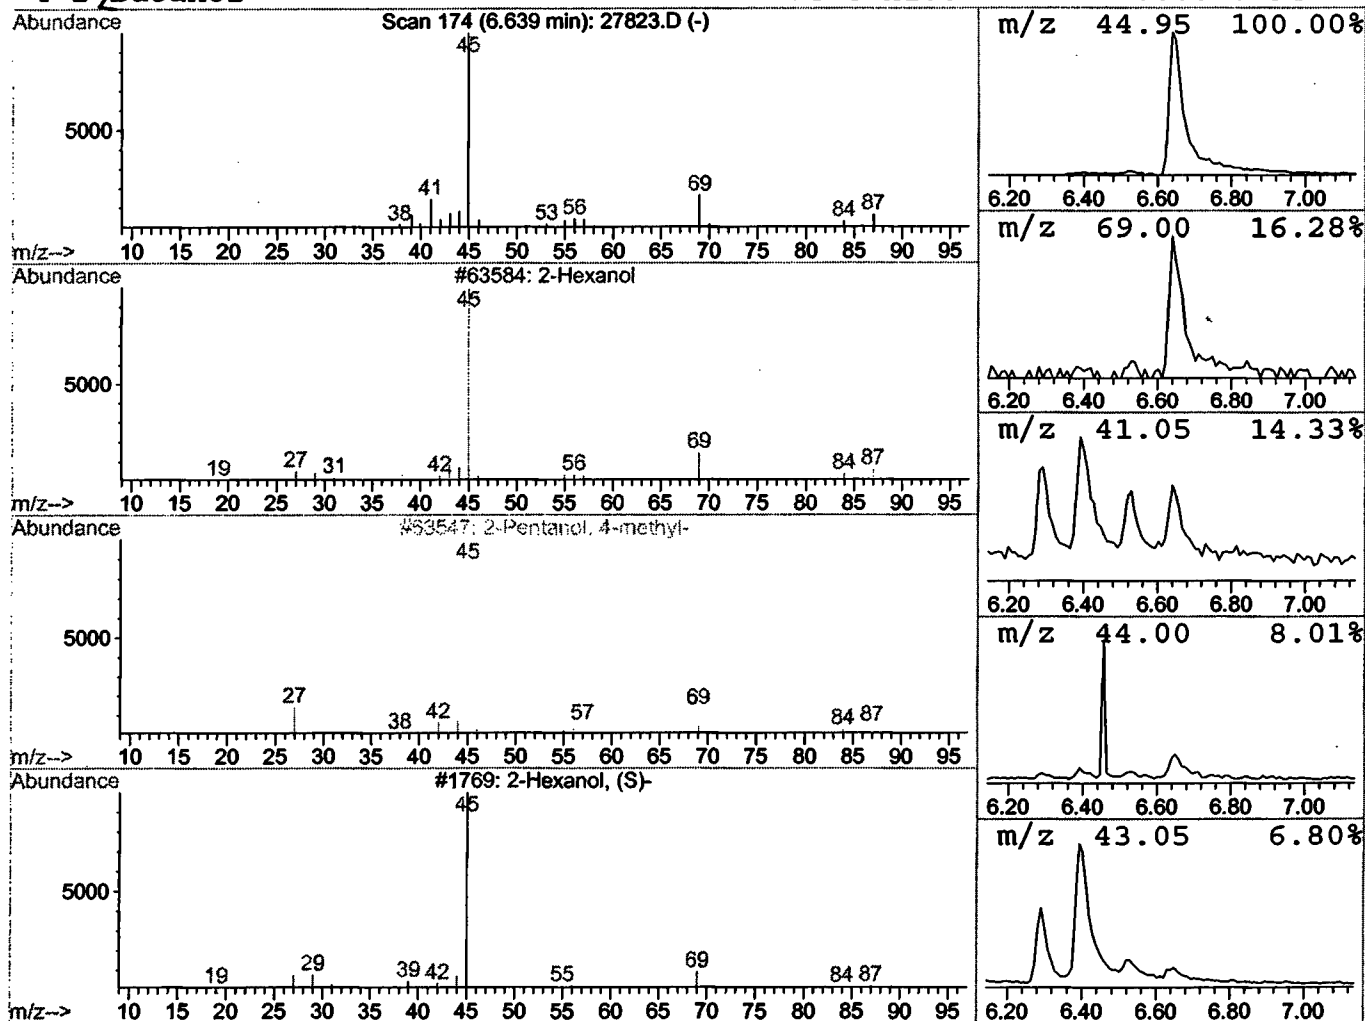

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 19 Dec 2001 8:32 pm
Data File: C:\HPCHEM\1\DATA\DEC1901\27823.D
Name: gc/msunknown 11/19
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
3-Hexanone	6.29	0.6	ug/l	128884	ISTD01	11.66	4253280	20.0
2-Hexanone	6.39	0.9	ug/l	185631	ISTD01	11.66	4253280	20.0
3-Hexanol	6.53	0.5	ug/l	108186	ISTD01	11.66	4253280	20.0
2-Hexanol	6.64	0.6	ug/l	120958	ISTD01	11.66	4253280	20.0

27823.D GCMS1126.M Wed Jan 02 12:08:14 2002