

Comments for Sample AD28157 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 11-29-2001 Time: 10:04:33

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.
Recoveries for 14 of the 44 compounds in the LCS Standard were outside of their acceptance ranges. The recovery for the Surrogate Standard in this sample was 86%.

NOT DLP

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 11/29/2001 Time: 10:04:06

Sample: AD28157
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 11/29/01 10:03 Ended: 11/29/01 10:03 Analyst: DLV
 Page: 1

	Component Name	Vol	Result
1	Other unknown compounds		.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV2601\28157.D

Vial: 16

Acq On : 27 Nov 2001 1:22 am

Operator: 209 GALOS

Sample : 11/20 scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 28 8:26 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Tue Nov 27 12:20:14 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Nothing present

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	11.69	152	788018	20.00	ug/l	0.00
15) Naphthalene-d8	15.30	136	2980167	20.00	ug/l	0.00
26) Acenaphthene-d10	20.57	164	1445584	20.00	ug/l	0.00
42) Phenanthrene-d10	24.99	188	1961149	20.00	ug/l	0.00
53) Chrysene-d12	33.03	240	980312	20.00	ug/l	0.00
59) Perylene-d12	37.12	264	677652	20.00	ug/l	0.00

System Monitoring Compounds

52) 2,4-DDD	30.07	235	100917	4.32	ug/mL	0.00
Spiked Amount	5.000		Recovery	=	86.40%	

Target Compounds

					Qvalue
2) Pyridine	0.00	79	0	N.D.	
3) N-nitroso-dimethyl amine	5.17	74	538	N.D.	
4) Phenol	0.00	94	0	N.D.	
5) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
6) 2-Chlorophenol	0.00	128	0	N.D.	
7) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
8) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
9) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
10) 2-Methylphenol	0.00	108	0	N.D.	
11) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
12) 3&4-Methylphenol	0.00	108	0	N.D.	
13) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
14) Hexachloroethane	0.00	117	0	N.D.	
16) Nitrobenzene	0.00	77	0	N.D.	
17) Isophorone	0.00	82	0	N.D.	
18) 2-Nitrophenol	0.00	139	0	N.D.	
19) 2,4-Dimethylphenol	0.00	107	0	N.D.	
20) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
21) 2,4-Dichlorophenol	0.00	162	0	N.D.	
22) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
23) Naphthalene	15.35	128	1216	N.D.	
24) Hexachlorobutadiene	0.00	225	0	N.D.	
25) 4-Chloro-3-methylphenol	0.00	107	0	N.D.	
27) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
28) 2,4,6-Trichlorophenol	0.00	196	0	N.D.	
29) 2,4,5-Trichlorophenol	0.00	196	0	N.D.	
30) 2-Chloronaphthalene	0.00	162	0	N.D.	
31) Dimethylphthalate	0.00	163	0	N.D.	
32) 2,6-Dinitrotoluene	0.00	165	0	N.D.	

(#) = qualifier out of range (m) = manual integration

28157.D GCMS1126.M Wed Nov 28 08:30:04 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV2601\28157.D
 Acq On : 27 Nov 2001 1:22 am
 Sample : 11/20 scan
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 28 8:26 2001

Vial: 16
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue Nov 27 12:20:14 2001
 Response via : Initial Calibration
 DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) Acenaphthylene	0.00	152	0	N.D.		
34) Acenaphthene	0.00	153	0	N.D.		
35) 2,4-Dinitrophenol	0.00	184	0	N.D.		
36) 4-Nitrophenol	0.00	65	0	N.D.		
37) 2,4-Dinitrotoluene	21.01	165	198	N.D.		
38) Diethylphthalate	22.09	149	807	N.D.		
39) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
40) Fluorene	0.00	166	0	N.D.		
41) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
43) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
44) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
45) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
46) Hexachlorobenzene	0.00	284	0	N.D.		
47) Pentachlorophenol	0.00	266	0	N.D.		
48) Phenanthrene	25.07	178	194	N.D.		
49) Anthracene	25.07	178	194	N.D.		
50) Di-n-butylphthalate	27.00	149	4289	N.D.		
51) Fluoranthene	0.00	202	0	N.D.		
54) Pyrene	0.00	202	0	N.D.		
55) Butylbenzylphthalate	0.00	149	0	N.D.		
56) Benzo(a)anthracene	33.03	228	2783	N.D.		
57) Bis(2-ethylhexyl)phthalate	33.30	149	9265	N.D.		
58) Chrysene	33.10	228	1190	N.D.		
60) Di-n-Octylphthalate	35.05	149	5992	N.D.		
61) Benzo(b)fluoranthene	36.06	252	3887	N.D.		
62) Benzo(k)fluoranthene	36.13	252	4484	N.D.		
63) Benzo(a)pyrene	36.95	252	3113	N.D.		
64) Indeno(1,2,3-cd)pyrene	40.84	276	2291	N.D.		
65) Dibenz(a,h)anthracene	40.88	278	1557	N.D.		
66) Benzo(g,h,i)perylene	41.89	276	2720	N.D.		

(#) = qualifier out of range (m) = manual integration

28157.D GCMS1126.M Wed Nov 28 08:30:08 2001

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\NOV2601\28157.D
Acq On : 27 Nov 2001 1:22 am
Sample : 11/20 scan
Misc :
MS Integration Params: RTEINT.P
Quant Time: Nov 28 8:26 2001

Vial: 16
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Tue Nov 27 12:20:14 2001
Response via : Initial Calibration

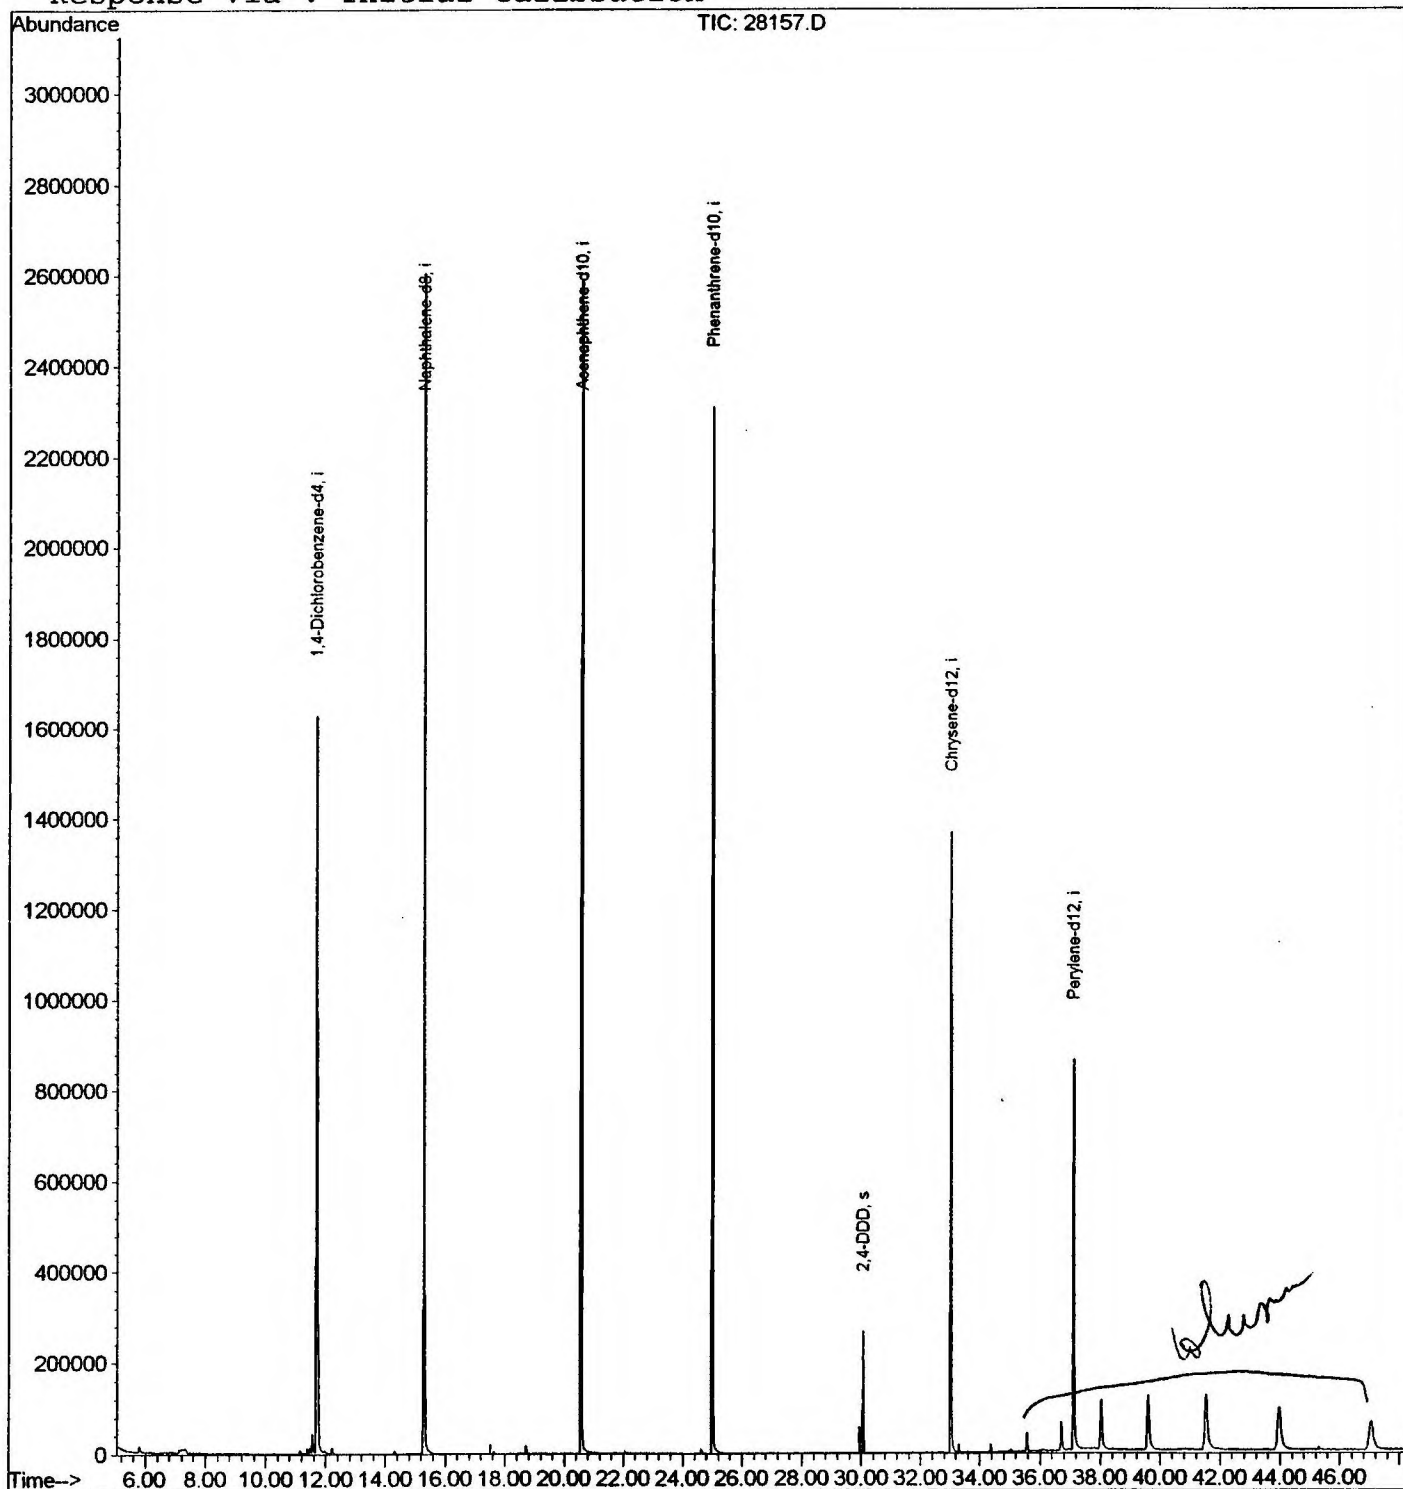

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\NOV2601\28157.D
 Acq On : 27 Nov 2001 1:22 am
 Sample : 11/20 scan
 Misc :
 MS Integration Params: LSCINT.P

Vial: 16
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	11.563	706	710	719	rVV	41686	102803	1.81%	0.343%
2	11.691	719	724	745	rBV	1623811	4152334	73.01%	13.863%
3	15.299	1111	1117	1135	rBV	2604178	5487091	96.48%	18.319%
4	20.569	1685	1691	1710	rBV	2588732	5687176	100.00%	18.987%
5	24.993	2167	2173	2187	rBV	2307772	4896342	86.09%	16.347%
6	30.070	2721	2726	2733	rBV	265009	522314	9.18%	1.744%
7	33.026	3041	3048	3067	rBV	1367167	3098082	54.47%	10.343%
8	35.578	3320	3326	3332	rBV2	40479	99702	1.75%	0.333%
9	36.726	3445	3451	3459	rBV	62264	189339	3.33%	0.632%
10	37.121	3486	3494	3511	rBV	858633	2421287	42.57%	8.084%
11	38.029	3584	3593	3609	rBV	109267	453735	7.98%	1.515%
12	39.599	3753	3764	3789	rBV2	120750	631710	11.11%	2.109%
13	41.546	3962	3976	4001	rBV	120941	838903	14.75%	2.801%
14	43.978	4224	4241	4264	rBV3	92208	776451	13.65%	2.592%
15	47.054	4557	4576	4600	rBV6	60825	595757	10.48%	1.989%




Sum of corrected areas: 29953026

28157.D GCMS1126.M

Wed Nov 28 09:13:35 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\NOV2601\28157.D
 Operator : 209 GALOS
 Acquired : 27 Nov 2001 1:22 am using AcqMethod NP103001
 Instrument : GC/MS 209
 Sample Name: 11/20 scan
 Misc Info :
 Vial Number: 16
 Quant File : GCMS1126.RES (RTE Integrator)

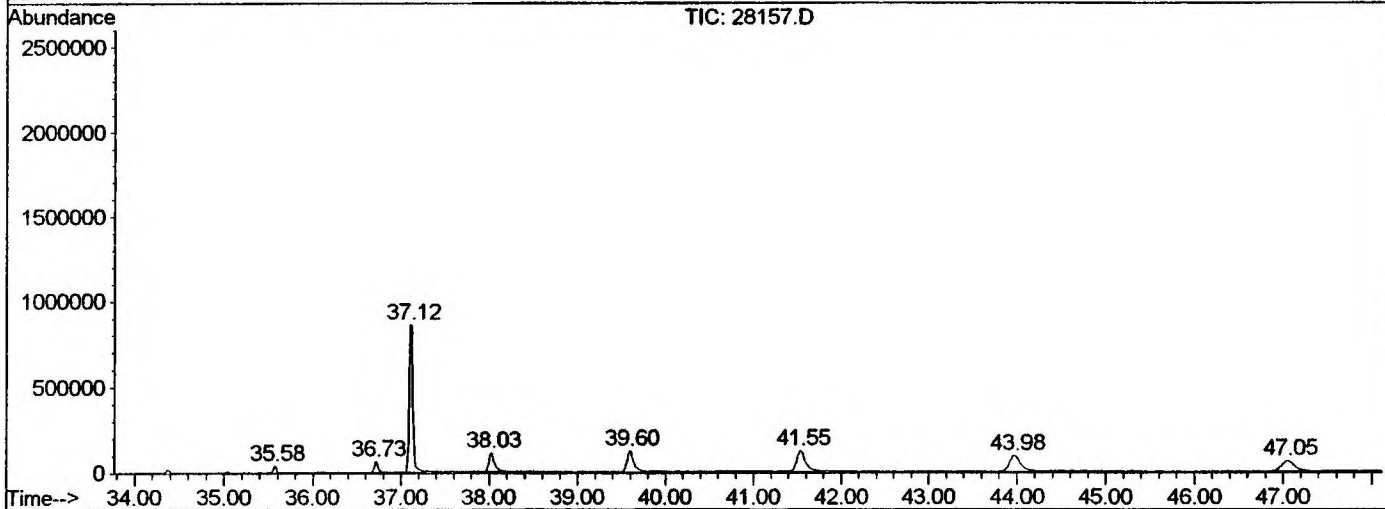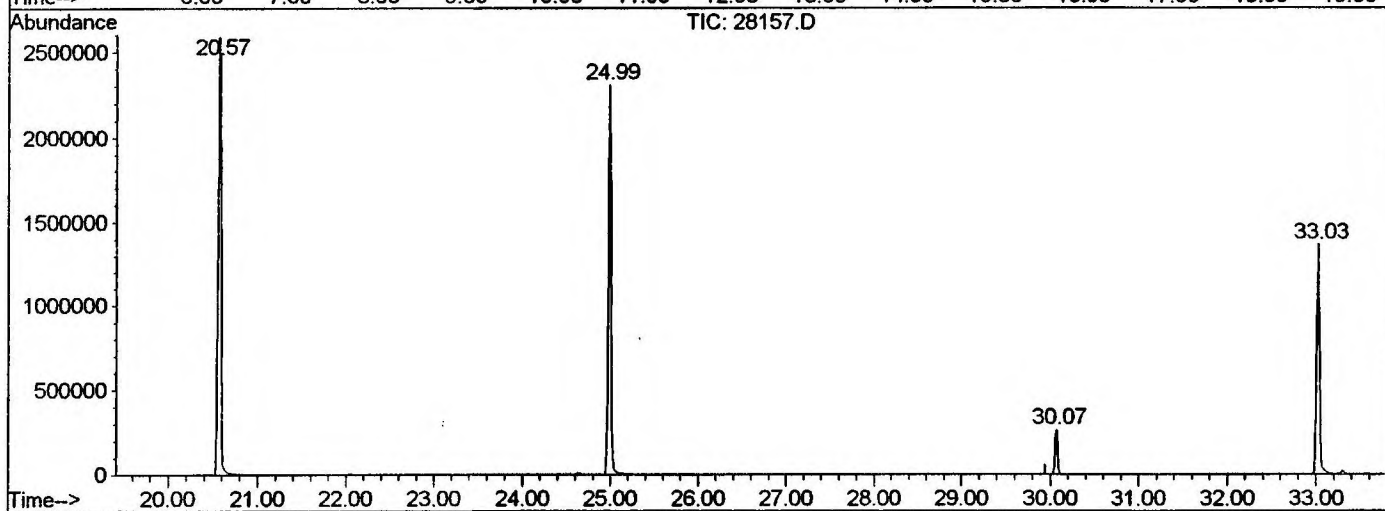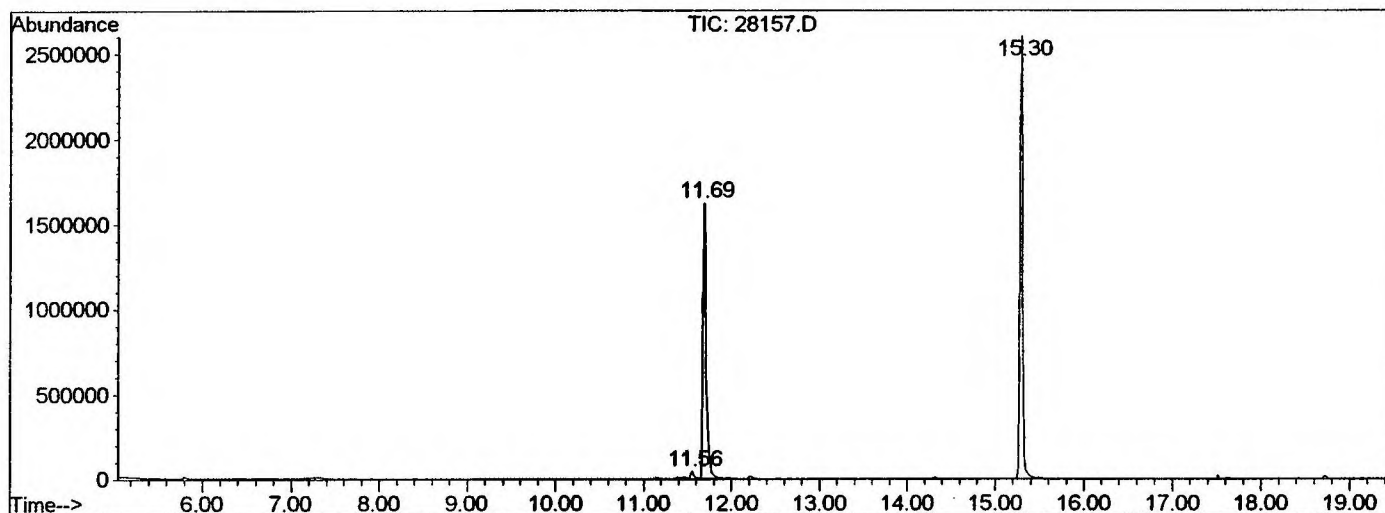

28157.D GCMS1126.M Wed Nov 28 09:13:37 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV2601\28157.D
 Acq On : 27 Nov 2001 1:22 am
 Sample : 11/20 scan
 Misc :
 MS Integration Params: LSCINT.P


Vial: 16
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 1,4-Dichlorobenzene-d4 Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.56	0.50 ug/l	102803	1,4-Dichlorobenzene-d4	11.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,4-Dichlorobenzene-d4	150	C6Cl2D4	003855-82-1	50
2		Benzene-1,2,3,4-d4-, 5,6-dichloro-	150	C6Cl2D4	002199-69-1	36
3		Biphenylene	152	C12H8	000259-79-0	9
4		Vanillin	152	C8H8O3	000121-33-5	9

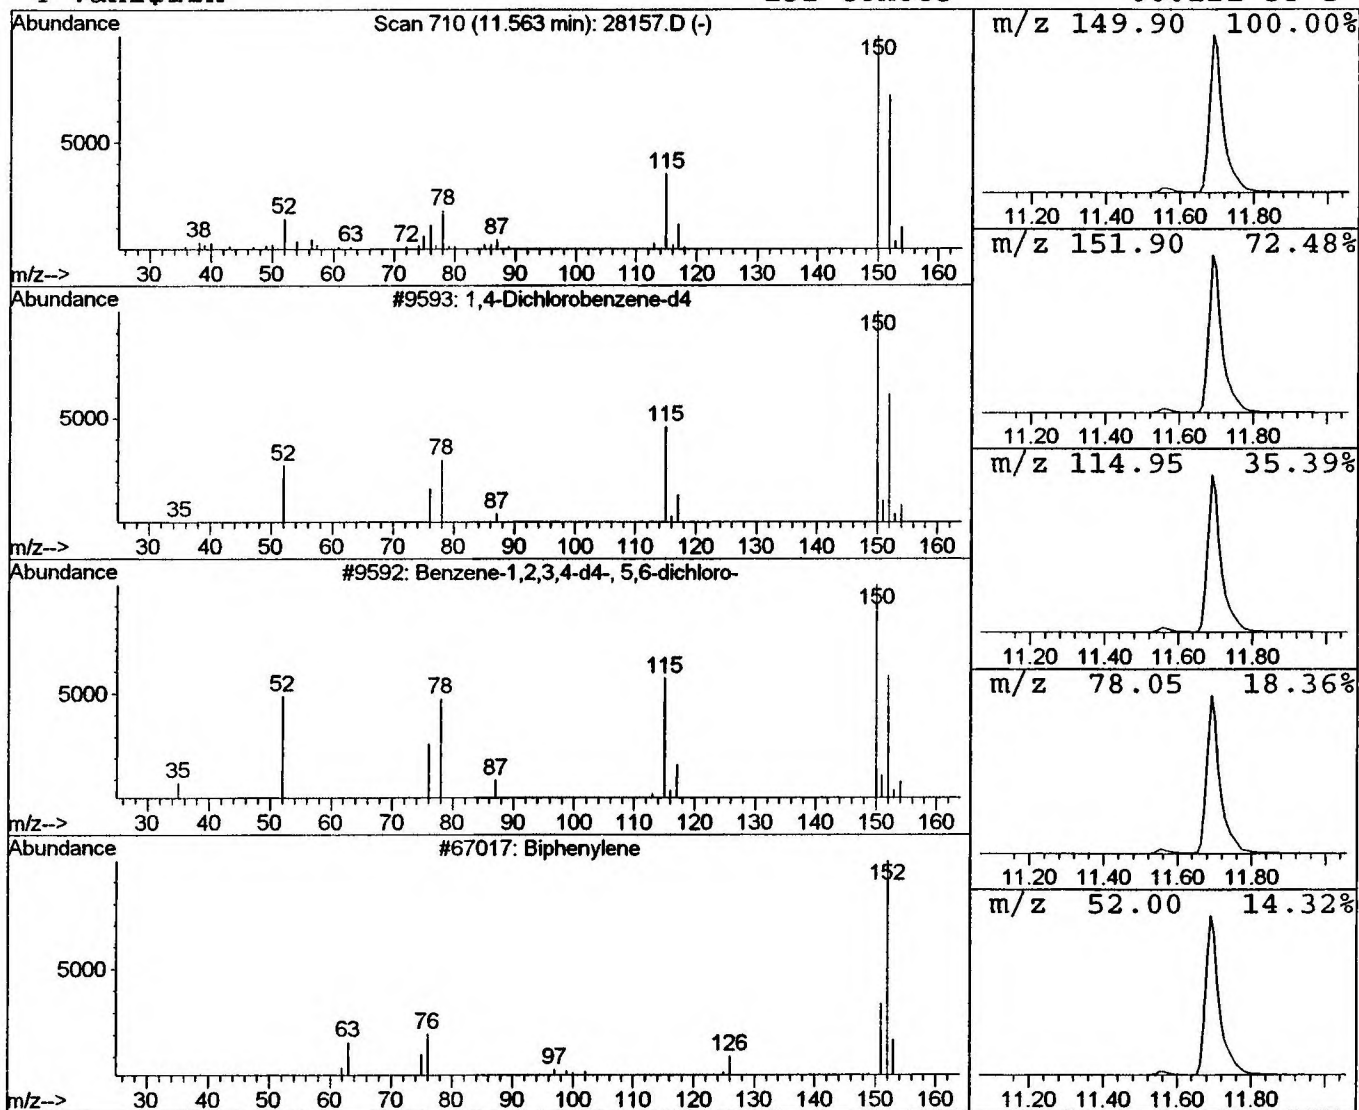

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV2601\28157.D
Acq On : 27 Nov 2001 1:22 am
Sample : 11/20 scan
Misc :
MS Integration Params: LSCINT.P


Vial: 16
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 2 1-Monolinoleoylglycerol trimet Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
35.58	0.82 ug/l	99702	Perylene-d12	37.12

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Monolinoleoylglycerol trimethylsi	498	C27H54O4Si2	054284-45-6	36
2			1,1,1,5,7,7,7-Heptamethyl-3,3-bis(t	444	C13H40O5Si6	038147-00-1	12
3			Silaname, N-[2,6-dimethyl-4-[(tri	281	C14H27NOSi2	072088-09-6	11
4			3-Trimethylsilyloxystearic acid, tr	444	C24H52O3Si2	000000-00-0	9

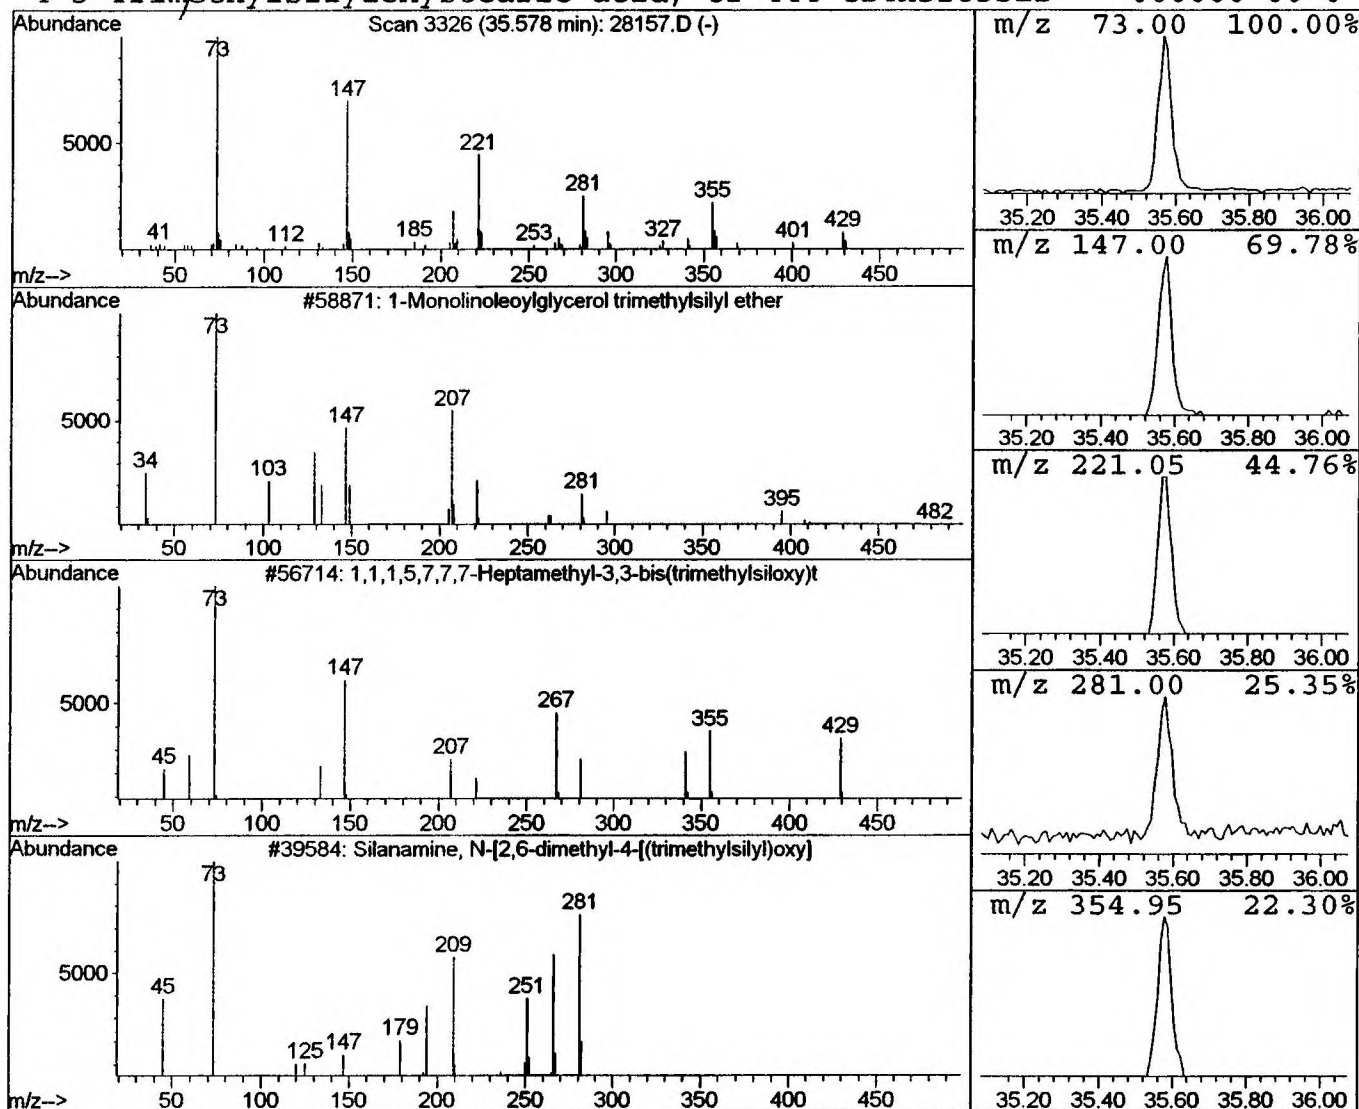

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV2601\28157.D
 Acq On : 27 Nov 2001 1:22 am
 Sample : 11/20 scan
 Misc :
 MS Integration Params: LSCINT.P


Vial: 16
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 3 Mercaptoacetic acid, bis(trimethy Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
36.73	1.56 ug/l	189339	Perylene-d12	37.12

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Mercaptoacetic acid, bis(trimethyls	236	C8H20O2SSi2	006398-62-5	17
2		Silanamine, N-[2,6-dimethyl-4-[(tri	281	C14H27NOSi2	072088-09-6	14
3		3-Isopropoxy-1,1,1,7,7,7-hexamethyl	576	C18H52O7Si7	071579-69-6	12
4		Tris(trimethylsilyl)borate	278	C9H27BO3Si3	004325-85-3	12

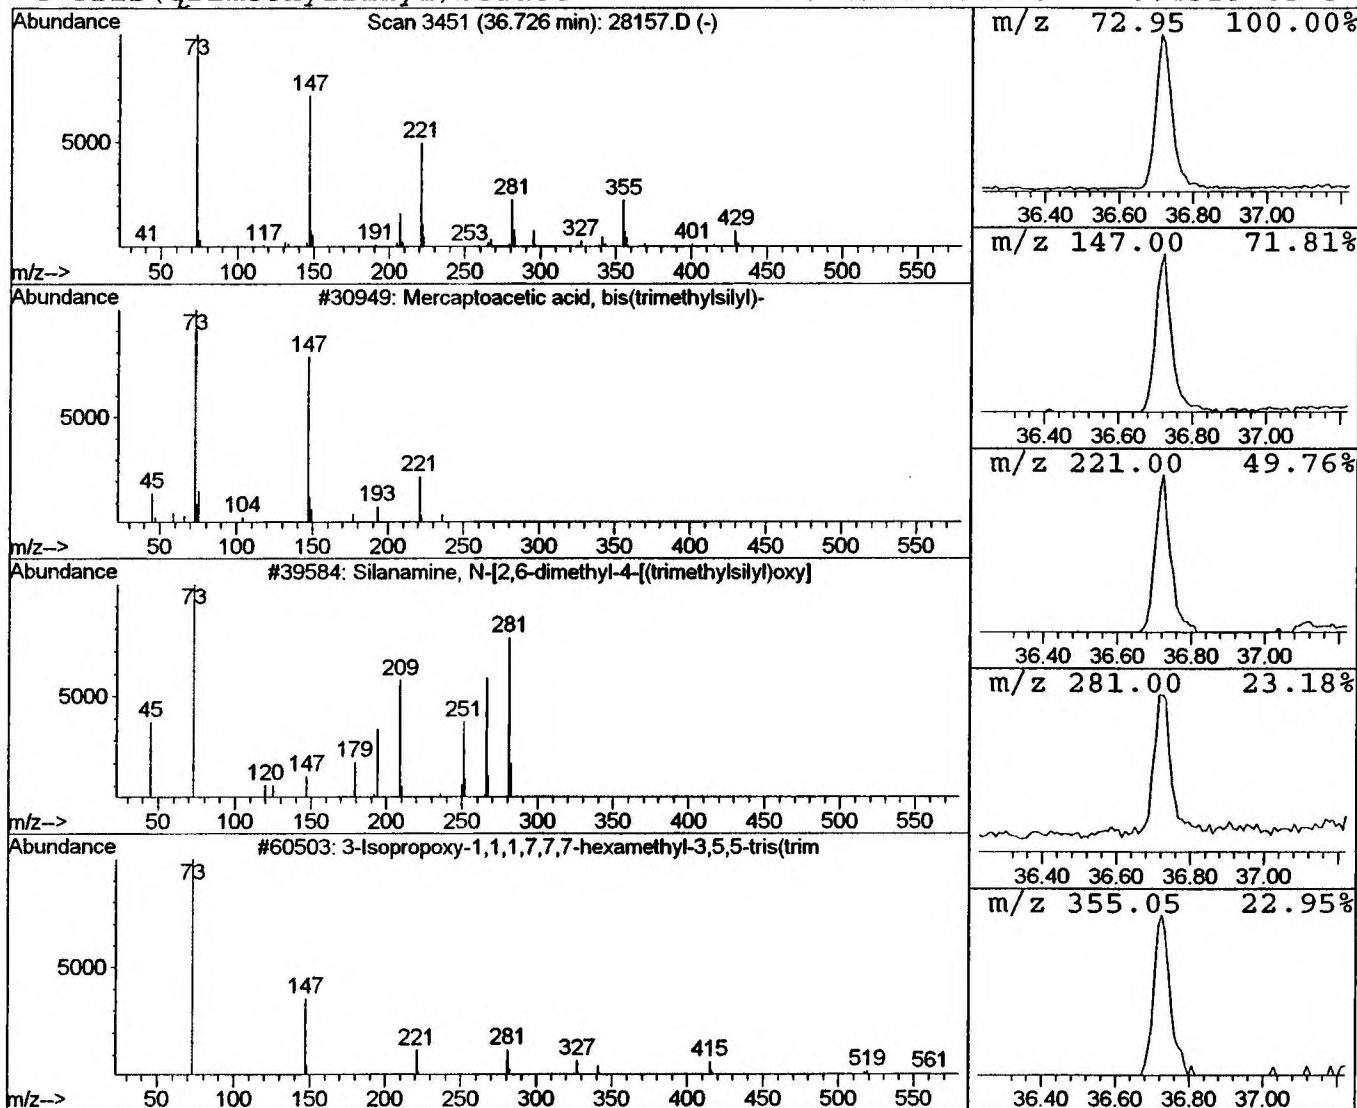

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV2601\28157.D
Acq On : 27 Nov 2001 1:22 am
Sample : 11/20 scan
Misc :
MS Integration Params: LSCINT.P


Vial: 16
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 4 1-Monolinoleoylglycerol trimet Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
38.03	3.75 ug/l	453735	Perylene-d12	37.12

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Monolinoleoylglycerol trimethylsi	498	C27H54O4Si2	054284-45-6	23
2			1,1,1,5,7,7,7-Heptamethyl-3,3-bis(t	444	C13H40O5Si6	038147-00-1	17
3			1,2-Benzenedicarboxylic acid, bis(t	310	C14H22O4Si2	002078-22-0	12
4			Benzoic acid, 2,5-bis(trimethylsilo	370	C16H30O4Si3	003618-20-0	10

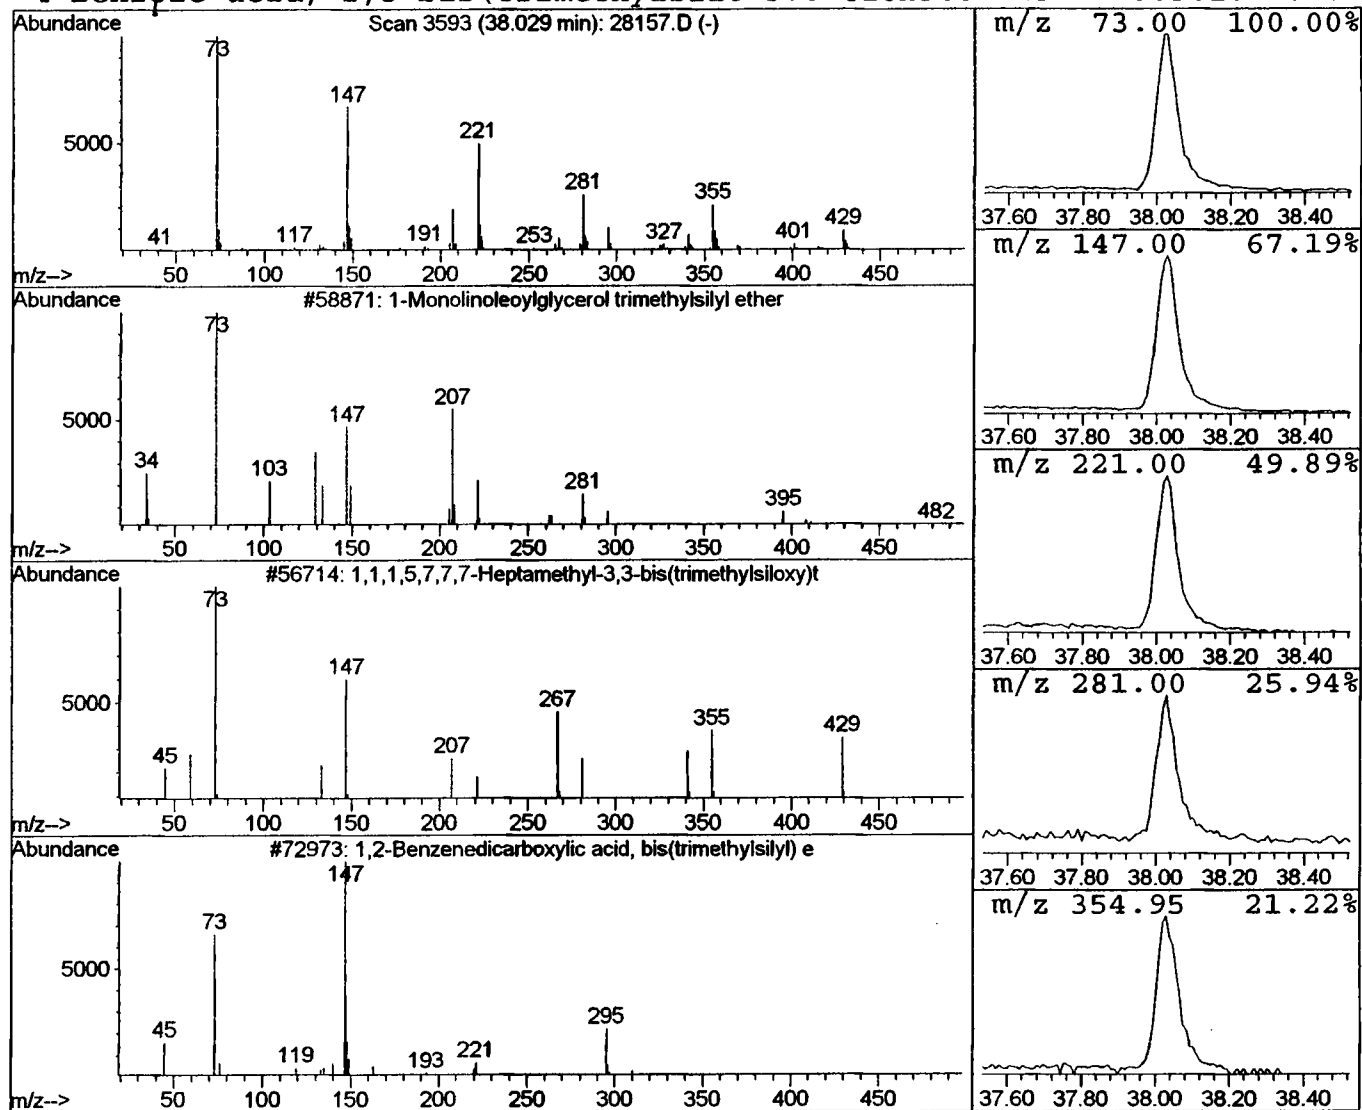

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV2601\28157.D
 Acq On : 27 Nov 2001 1:22 am
 Sample : 11/20 scan
 Misc :
 MS Integration Params: LSCINT.P


Vial: 16
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 5 1,2-Benzenedicarboxylic acid, Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
39.60	5.22 ug/l	631710	Perylene-d12	37.12

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,2-Benzenedicarboxylic acid, bis(t	310	C14H22O4Si2	002078-22-0	27
2			Trisiloxane, 1,1,1,5,5,5-hexamethyl	384	C12H36O4Si5	003555-47-3	25
3			1,1,1,5,7,7,7-Heptamethyl-3,3-bis(t	444	C13H40O5Si6	038147-00-1	25
4			N-Benzhydrylidene-1-(2,4,6-trimethy	343	C24H25NO	089839-57-6	22

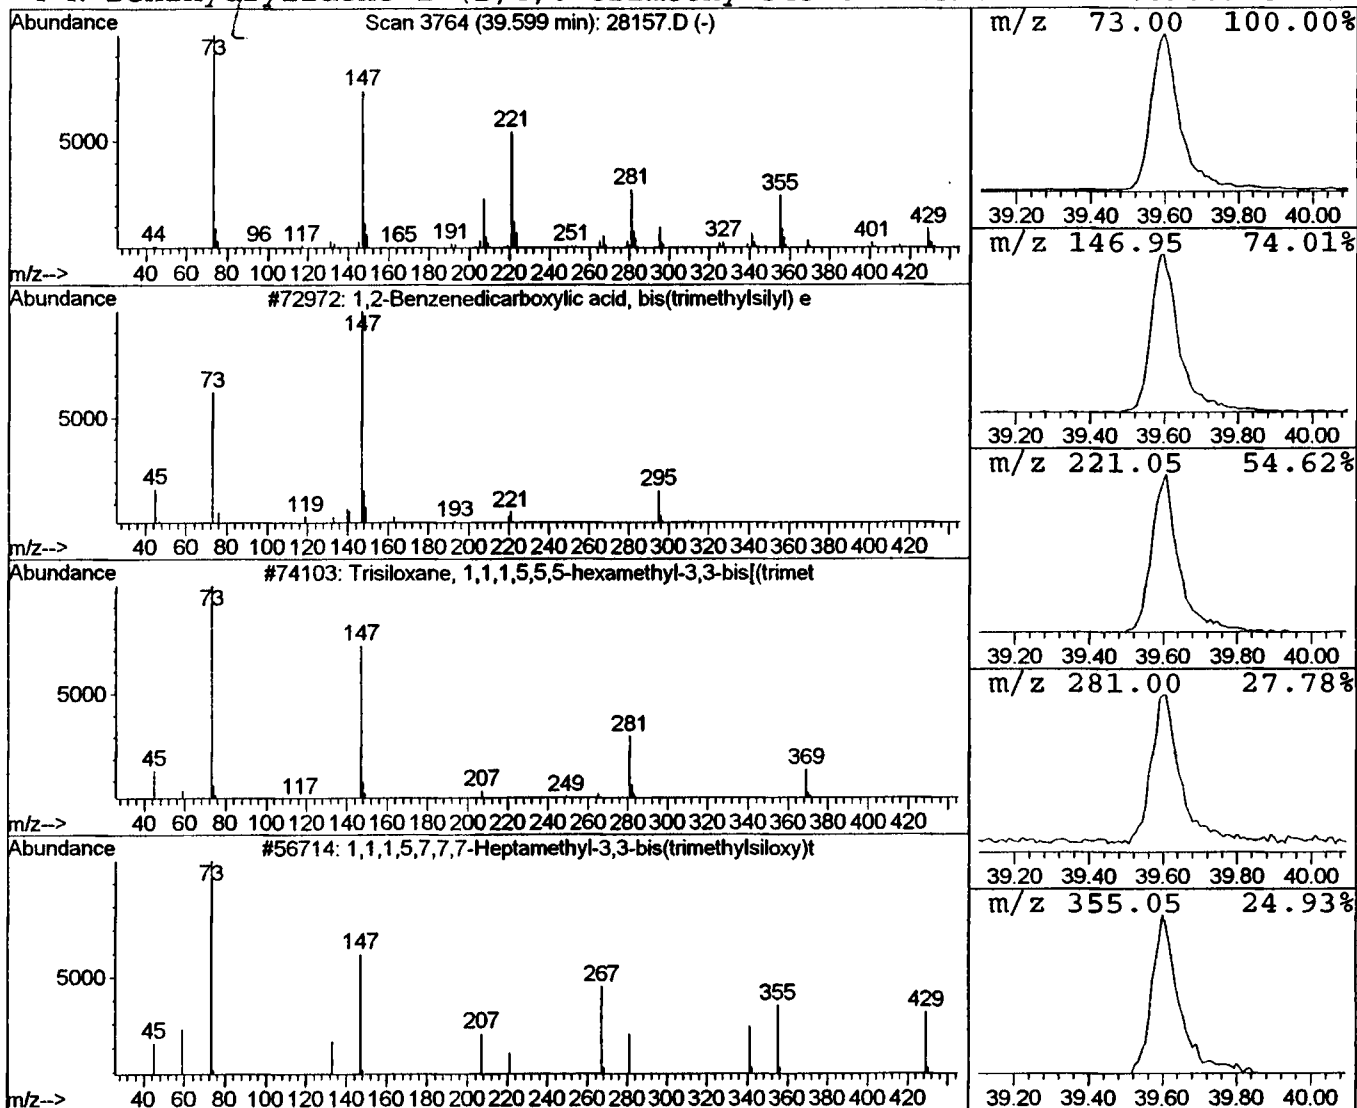

Library Search Compound Report


Data File : C:\HPCHEM\1\DATA\NOV2601\28157.D
Acq On : 27 Nov 2001 1:22 am
Sample : 11/20 scan
Misc :
MS Integration Params: LSCINT.P

Vial: 16
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 6 3,6-Dioxa-2,4,5,7-tetrasilaoct Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
41.55	6.93 ug/l	838903	Perylene-d12	37.12	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	3,6-Dioxo-2,4,5,7-tetrasilaoctane,	294	C10H30O2Si4	004342-25-0	25
2	1,3-Benzodioxole, 5-[3-acetaminopro	221	C12H15NO3	000000-00-0	22
3	Trisiloxane, octamethyl-	236	C8H24O2Si3	000107-51-7	12
4	1,2-Benzenedicarboxylic acid, bis(t	310	C14H22O4Si2	002078-22-0	12

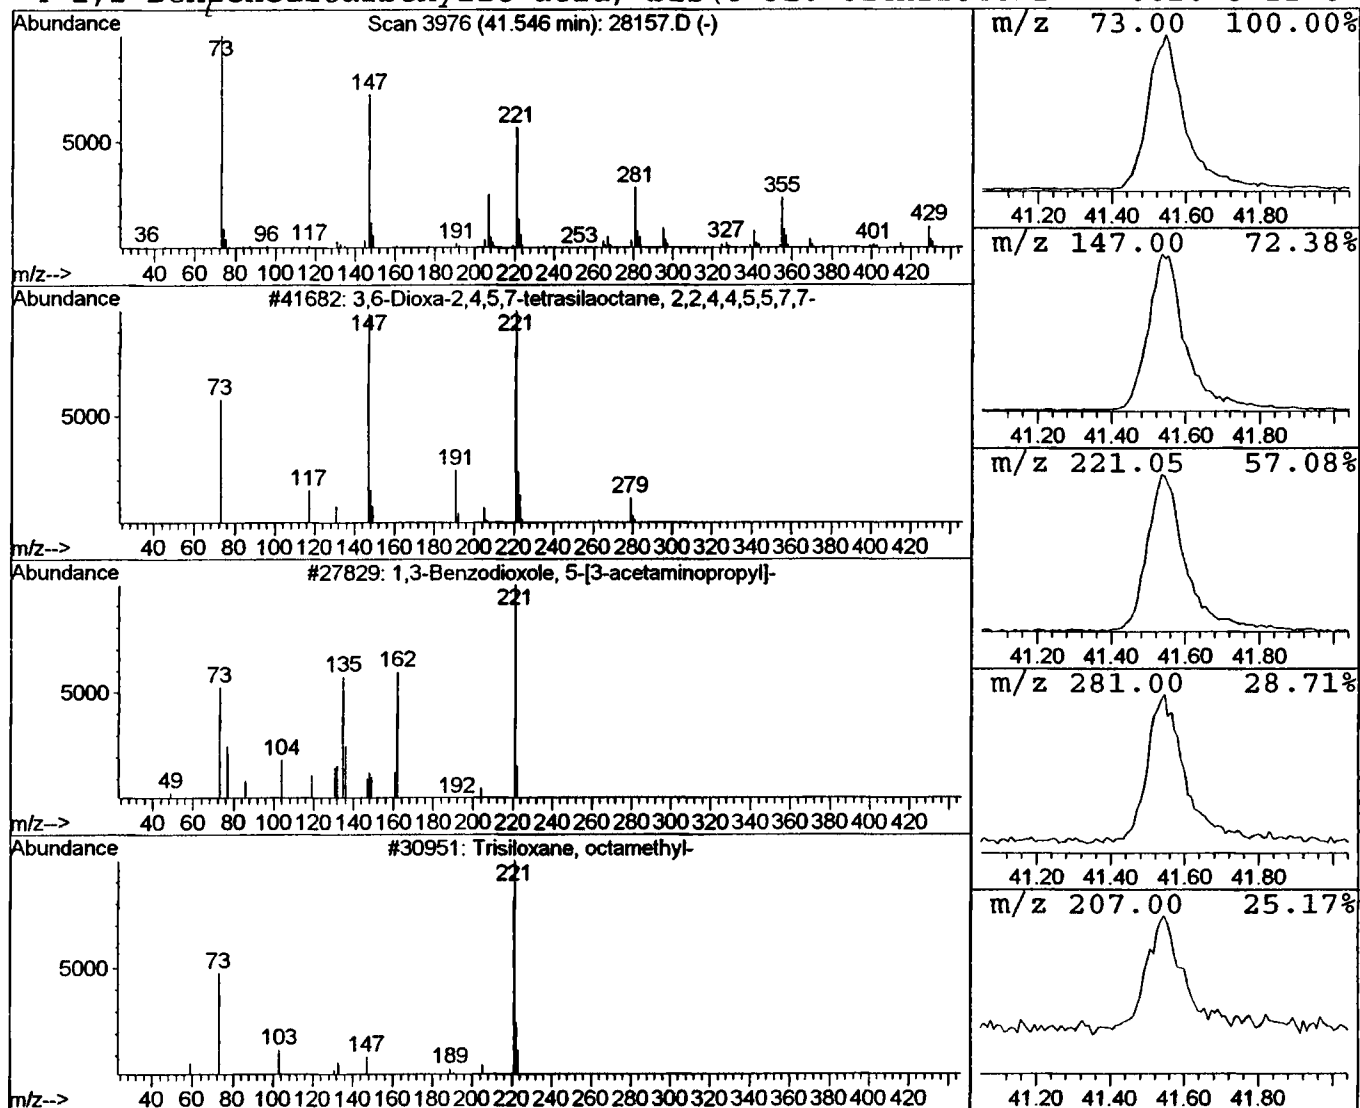

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV2601\28157.D
Acq On : 27 Nov 2001 1:22 am
Sample : 11/20 scan
Misc :
MS Integration Params: LSCINT.P


Vial: 16
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 7 3,6-Dioxa-2,4,5,7-tetrasilaoct Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
43.98	6.41 ug/l	776451	Perylene-d12	37.12

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3,6-Dioxa-2,4,5,7-tetrasilaoctane,	294	C10H30O2Si4	004342-25-0	25
2			Ethanedioic acid, bis(trimethylsilyl	234	C8H18O4Si2	018294-04-7	22
3			1,2-Benzenedicarboxylic acid, bis(t	310	C14H22O4Si2	002078-22-0	17
4			Mercaptoacetic acid, bis(trimethyls	236	C8H20O2SSi2	006398-62-5	12

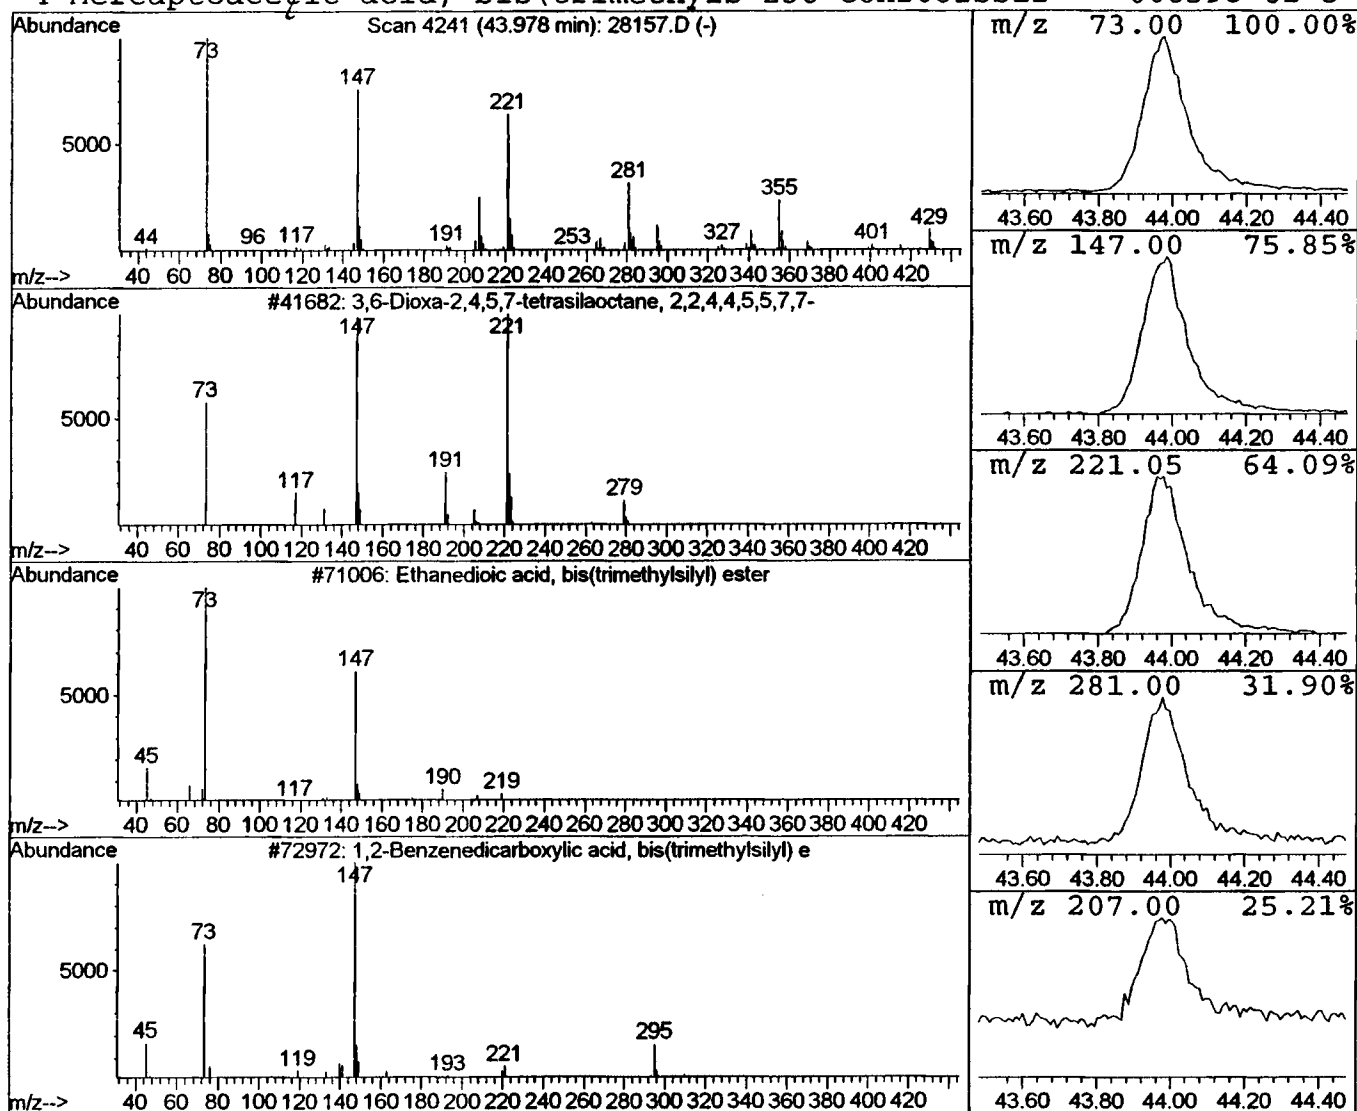

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV2601\28157.D
Acq On : 27 Nov 2001 1:22 am
Sample : 11/20 scan
Misc :
MS Integration Params: LSCINT.P


Vial: 16
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 8 Trisiloxane, 1,1,1,5,5,5-hexam Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
47.05	4.92 ug/l	595757	Perylene-d12	37.12

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trisiloxane, 1,1,1,5,5,5-hexamethyl	384	C12H36O4Si5	003555-47-3	25
2			1,2-Benzenedicarboxylic acid, bis(t	310	C14H22O4Si2	002078-22-0	22
3			3,6-Dioxo-2,4,5,7-tetrasilaoctane,	294	C10H30O2Si4	004342-25-0	17
4			Tris(trimethylsilyl)borate	278	C9H27BO3Si3	004325-85-3	10

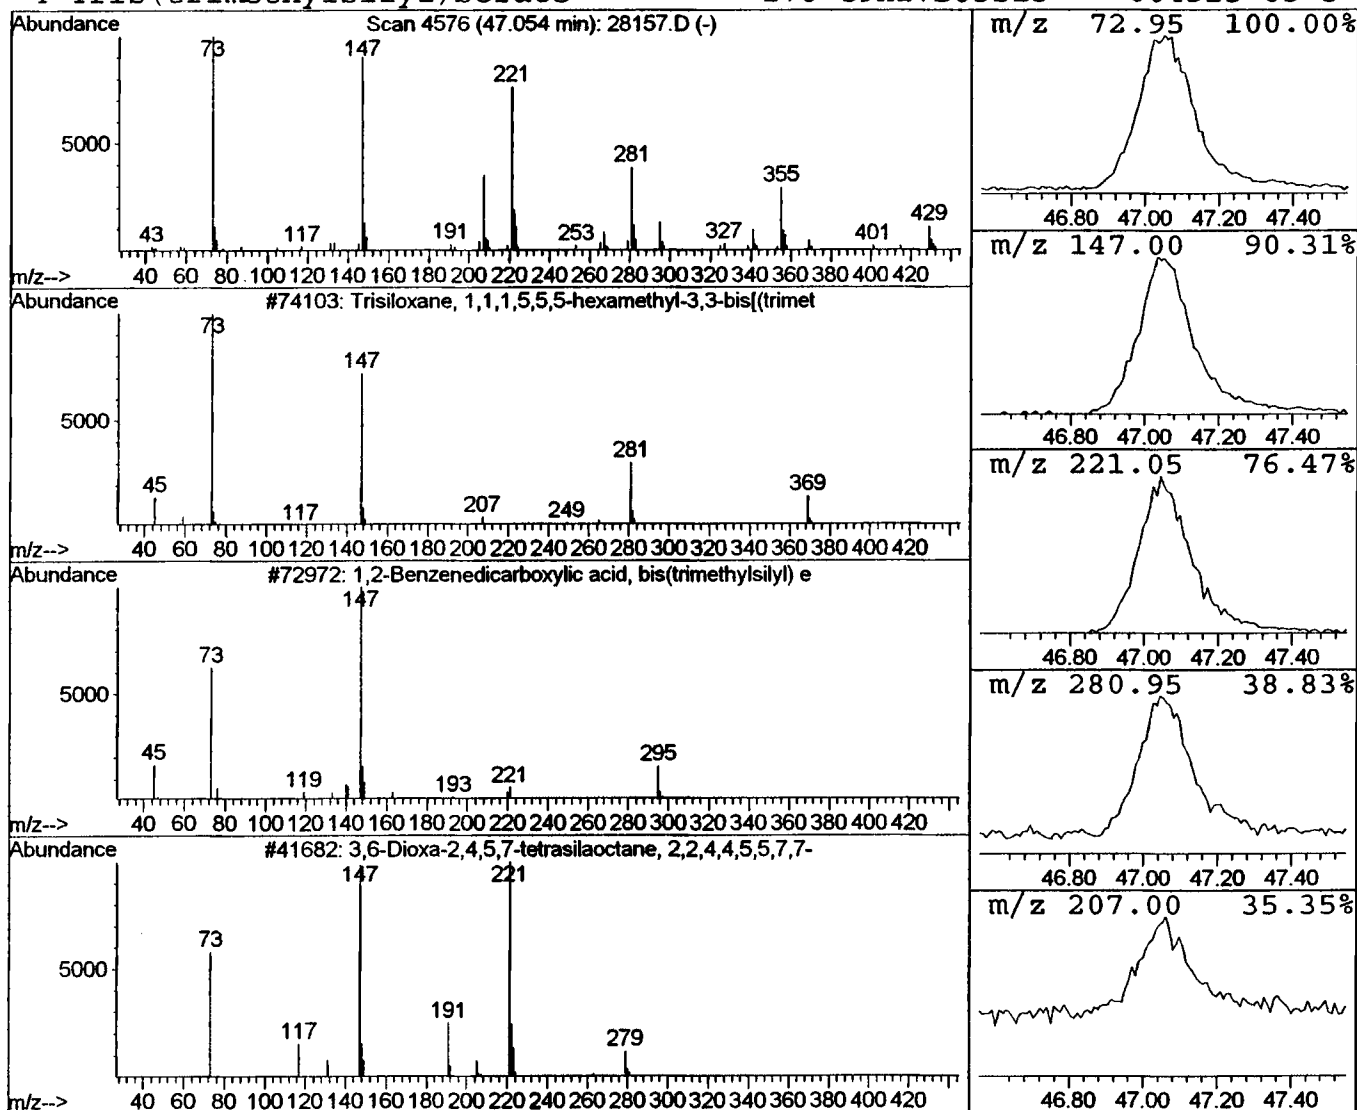

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 27 Nov 2001 1:22 am
 Data File: C:\HPCHEM\1\DATA\NOV2601\28157.D
 Name: 11/20 scan
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc Units	Area	IntStd	ISRT	ISArea	ISConc
1,4-Dichlorobenzene-	11.56	0.5 ug/l	102803	ISTD01	11.69	4152330	20.0
1-Monolinoleoylglyce	35.58	0.8 ug/l	99702	ISTD06	37.12	2421290	20.0
Mercaptoacetic acid,	36.73	1.6 ug/l	189339	ISTD06	37.12	2421290	20.0
1-Monolinoleoylglyce	38.03	3.7 ug/l	453735	ISTD06	37.12	2421290	20.0
1,2-Benzenedicarboxy	39.60	5.2 ug/l	631710	ISTD06	37.12	2421290	20.0
3,6-Dioxa-2,4,5,7-te	41.55	6.9 ug/l	838903	ISTD06	37.12	2421290	20.0
3,6-Dioxa-2,4,5,7-te	43.98	6.4 ug/l	776451	ISTD06	37.12	2421290	20.0
Trisiloxane, 1,1,1,5	47.05	4.9 ug/l	595757	ISTD06	37.12	2421290	20.0

28157.D GCMS1126.M Wed Nov 28 09:13:57 2001