

Comments for Sample AD28265 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 11-29-2001 Time: 10:42:29



The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Recoveries for 14 of the 44 compounds in the LCS Standard were outside of their acceptance ranges. The recovery for the Surrogate Standard in this sample was 45%.

NOT DET

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 11/29/2001 Time: 10:40:56

Sample: AD28265
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 11/29/01 10:40 Ended: 11/29/01 10:40 Analyst: DLV
 Page: 1

	Component Name	Viol	Result
1	Other unknown compounds		

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV2601\28265.D
 Acq On : 27 Nov 2001 5:17 am
 Sample : 11/20 scan
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Nov 28 11:26 2001

Vial: 20
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Tue Nov 27 12:20:14 2001
 Response via : Initial Calibration
 DataAcq Meth : NP103001

Nothing

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.70	152	743762	20.00	ug/l	0.00
15) Naphthalene-d8	15.30	136	2814485	20.00	ug/l	-0.01
26) Acenaphthene-d10	20.57	164	1346778	20.00	ug/l	0.00
42) Phenanthrene-d10	24.99	188	1808146	20.00	ug/l	0.00
53) Chrysene-d12	33.02	240	821692	20.00	ug/l	-0.01
59) Perylene-d12	37.12	264	520050	20.00	ug/l	0.00

System Monitoring Compounds

52) 2,4-DDD	30.07	235	48857	2.27	ug/mL	0.00
Spiked Amount	5.000		Recovery	=	45.40%	

Target Compounds

2) Pyridine	0.00	79	0	N.D.		
3) N-nitroso-dimethyl amine	5.20	74	182	N.D.		
4) Phenol	0.00	94	0	N.D.		
5) bis(2-Chloroethyl)ether	0.00	93	0	N.D.		
6) 2-Chlorophenol	0.00	128	0	N.D.		
7) 1,3-Dichlorobenzene	0.00	146	0	N.D.		
8) 1,4-Dichlorobenzene	0.00	146	0	N.D.		
9) 1,2-Dichlorobenzene	0.00	146	0	N.D.		
10) 2-Methylphenol	0.00	108	0	N.D.		
11) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.		
12) 3&4-Methylphenol	0.00	108	0	N.D.		
13) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
14) Hexachloroethane	0.00	117	0	N.D.		
16) Nitrobenzene	0.00	77	0	N.D.		
17) Isophorone	0.00	82	0	N.D.		
18) 2-Nitrophenol	0.00	139	0	N.D.		
19) 2,4-Dimethylphenol	0.00	107	0	N.D.		
20) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
21) 2,4-Dichlorophenol	0.00	162	0	N.D.		
22) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
23) Naphthalene	15.36	128	452	N.D.		
24) Hexachlorobutadiene	0.00	225	0	N.D.		
25) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
27) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
28) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
29) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
30) 2-Chloronaphthalene	0.00	162	0	N.D.		
31) Dimethylphthalate	0.00	163	0	N.D.		
32) 2,6-Dinitrotoluene	0.00	165	0	N.D.		

Qvalue

(#) = qualifier out of range (m) = manual integration

28265.D GCMS1126.M Wed Nov 28 11:27:38 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\NOV2601\28265.D

Vial: 20

Acq On : 27 Nov 2001 5:17 am

Operator: 209 GALOS

Sample : 11/20 scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Nov 28 11:26 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Tue Nov 27 12:20:14 2001

Response via : Initial Calibration

DataAcq Meth : NP103001

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) Acenaphthylene	0.00	152	0	N.D.		
34) Acenaphthene	0.00	153	0	N.D.		
35) 2,4-Dinitrophenol	0.00	184	0	N.D.		
36) 4-Nitrophenol	0.00	65	0	N.D.		
37) 2,4-Dinitrotoluene	20.87	165	864	N.D.		
38) Diethylphthalate	22.09	149	1480	N.D.		
39) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
40) Fluorene	0.00	166	0	N.D.		
41) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
43) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
44) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
45) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
46) Hexachlorobenzene	0.00	284	0	N.D.		
47) Pentachlorophenol	0.00	266	0	N.D.		
48) Phenanthrene	24.99	178	513	N.D.		
49) Anthracene	24.99	178	513	N.D.		
50) Di-n-butylphthalate	27.00	149	1550	N.D.		
51) Fluoranthene	0.00	202	0	N.D.		
54) Pyrene	0.00	202	0	N.D.		
55) Butylbenzylphthalate	0.00	149	0	N.D.		
56) Benzo(a)anthracene	33.02	228	1812	N.D.		
57) Bis(2-ethylhexyl)phthalate	33.31	149	1056	N.D.		
58) Chrysene	33.02	228	1812	N.D.		
60) Di-n-Octylphthalate	0.00	149	0	N.D.		
61) Benzo(b)fluoranthene	36.09	252	294	N.D.		
62) Benzo(k)fluoranthene	36.09	252	394	N.D.		
63) Benzo(a)pyrene	37.11	252	1898	N.D.		
64) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
65) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
66) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

28265.D GCMS1126.M Wed Nov 28 11:27:41 2001

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\NOV2601\28265.D
Acq On : 27 Nov 2001 5:17 am
Sample : 11/20 scan
Misc :
MS Integration Params: RTEINT.P
Quant Time: Nov 28 11:26 2001

Vial: 20
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Tue Nov 27 12:20:14 2001
Response via : Initial Calibration

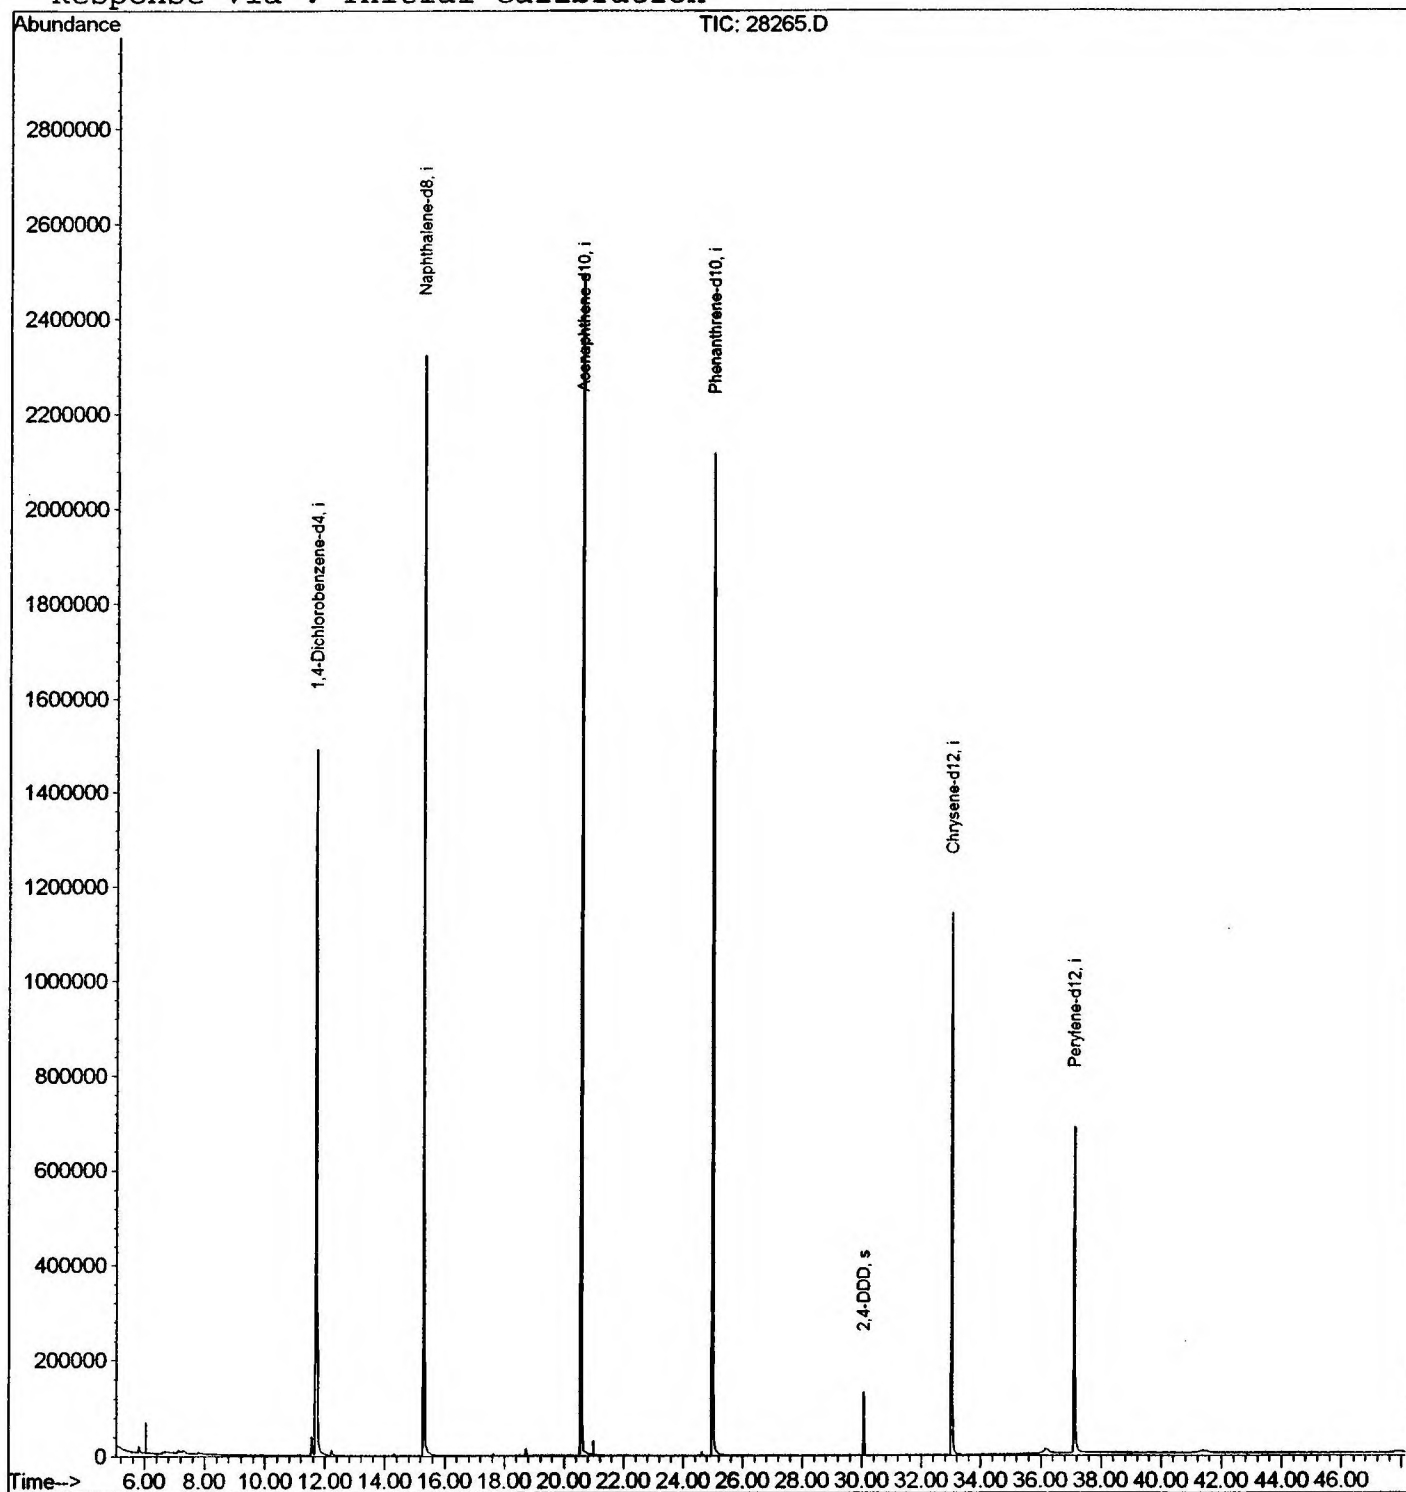

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\NOV2601\28265.D

Vial: 20

Acq On : 27 Nov 2001 5:17 am

Operator: 209 GALOS

Sample : 11/20 scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	11.560	706	710	720	rBV	38490	99884	1.89%	0.423%
2	11.697	720	725	743	rBV	1490741	3826608	72.53%	16.219%
3	15.296	1112	1117	1135	rBV	2322234	5130944	97.26%	21.747%
4	20.575	1686	1692	1704	rBV	2494324	5275677	100.00%	22.360%
5	24.990	2167	2173	2188	rBV2	2115957	4531793	85.90%	19.207%
6	30.067	2722	2726	2734	rVB	131632	260142	4.93%	1.103%
7	33.023	3042	3048	3064	rBV2	1140816	2589939	49.09%	10.977%
8	37.118	3486	3494	3515	rBV	683034	1878921	35.61%	7.964%




Sum of corrected areas: 23593908

28265.D GCMS1126.M

Wed Nov 28 11:29:11 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\NOV2601\28265.D
 Operator : 209 GALOS
 Acquired : 27 Nov 2001 5:17 am using AcqMethod NP103001
 Instrument : GC/MS 209
 Sample Name: 11/20 scan
 Misc Info :
 Vial Number: 20
 Quant File :GCMS1126.RES (RTE Integrator)

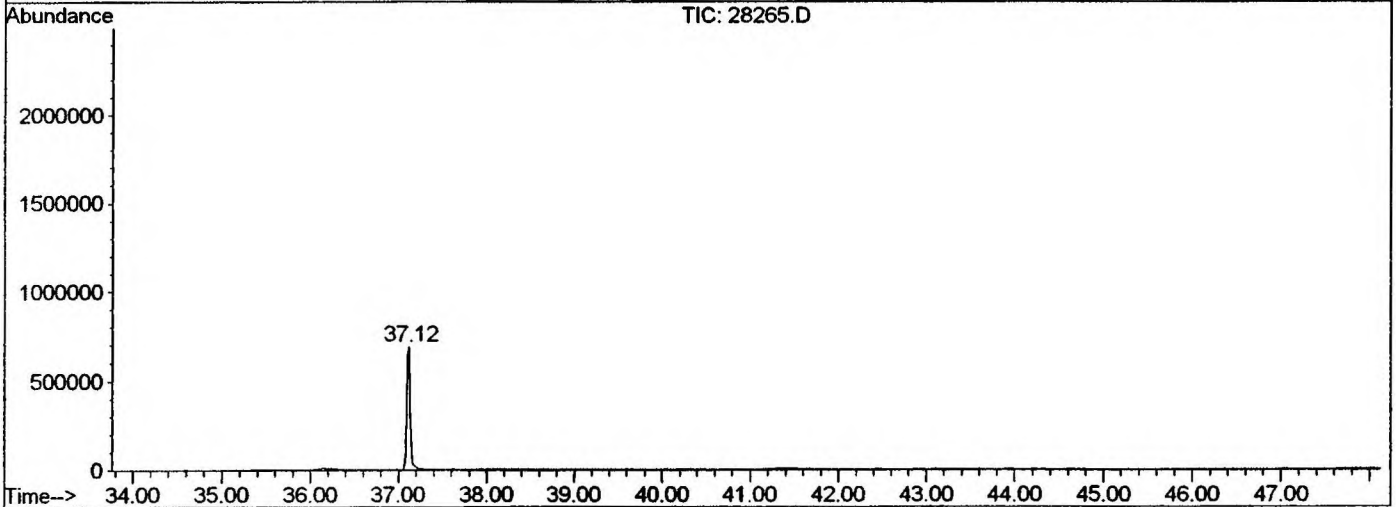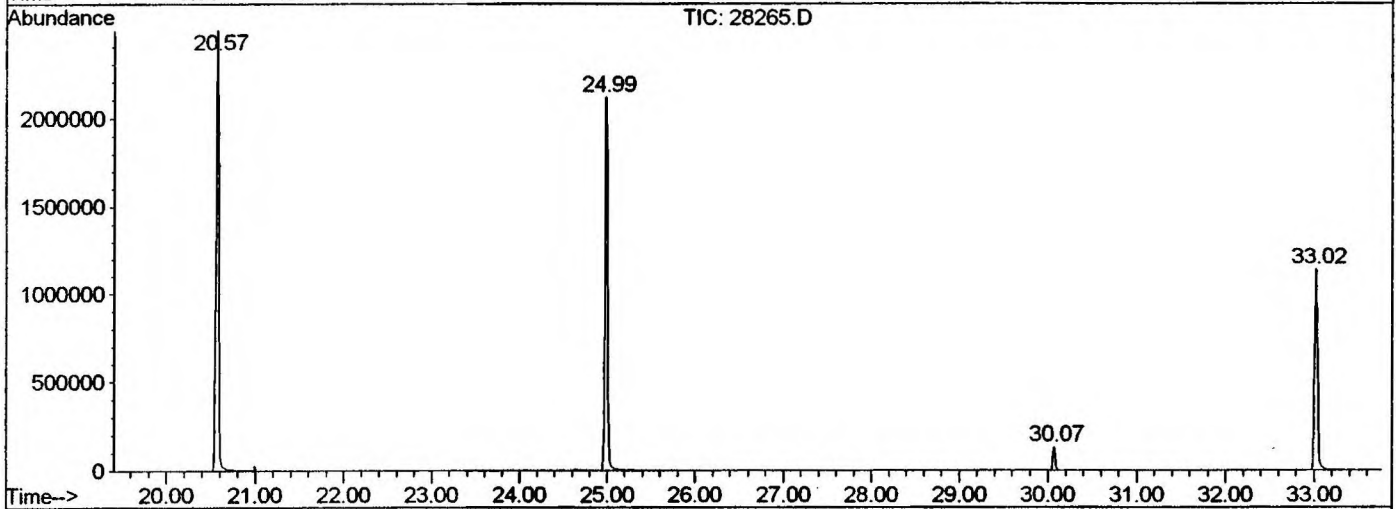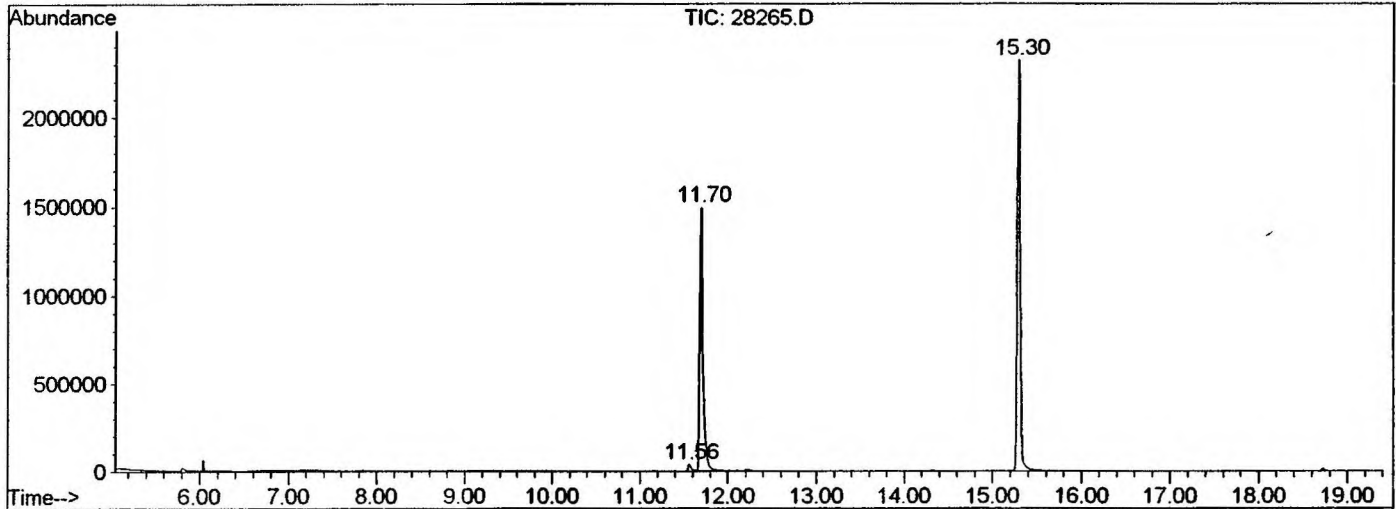

28265.D GCMS1126.M Wed Nov 28 11:29:13 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\NOV2601\28265.D
 Acq On : 27 Nov 2001 5:17 am
 Sample : 11/20 scan
 Misc :
 MS Integration Params: LSCINT.P


Vial: 20
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 1,4-Dichlorobenzene-d4 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.56	0.52 ug/l	99884	1,4-Dichlorobenzene-d4	11.70

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,4-Dichlorobenzene-d4	150	C6Cl2D4	003855-82-1	64
2		Benzene-1,2,3,4-d4-, 5,6-dichloro-	150	C6Cl2D4	002199-69-1	37
3		Benzaldehyde, 2-hydroxy-3-methoxy-	152	C8H8O3	000148-53-8	10
4		Benzenamine, N-methyl-4-nitro-	152	C7H8N2O2	000100-15-2	9

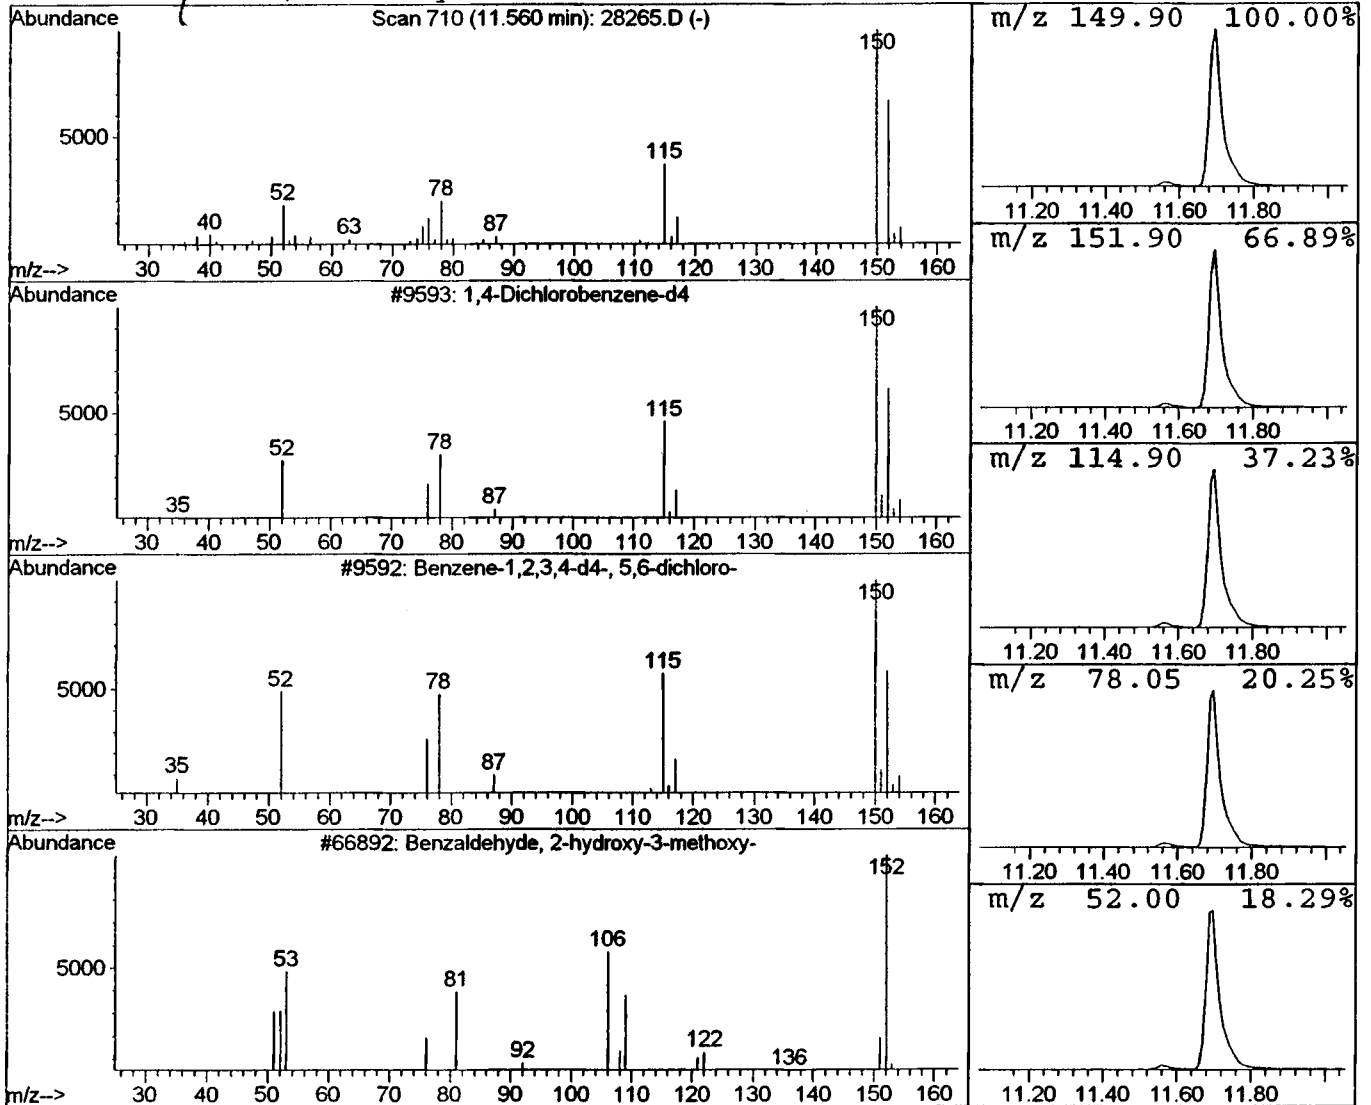

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 27 Nov 2001 5:17 am
 Data File: C:\HPCHEM\1\DATA\NOV2601\28265.D
 Name: 11/20 scan
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
1,4-Dichlorobenzene-	11.56	0.5	ug/l	99884	ISTD01	11.70	3826610	20.0
28265.D GCMS1126.M	Wed Nov 28 11:29:18 2001							