

GC/MS unknown by 508

Method 508Date Extracted 20 Nov 01

Page _____

Alternate Method

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH = 7	Count
	2B ✓	500mL		1mL		1mL				
	REF				1/2 mL					
	28143									1
	28145									2
	28147									3
	28153									4
	28149									5
	28151									6
	28155									7
	28157									8
	28159									9
	28161									10
	28141									11
	28163									12
	28265 ✓									13
	28325									14
	28326 ✓									15
	28327 ✓									16
	28334 ✓									17
	28335 ✓									18
	28230 ✓									19
	28229 ✓									20
Remarks										
1/2 mL of Ref 91759 added to "Ref"										
drip rate must be between 5-15 ml/min for liq-liq extractors										
Extraction type: <u>Sep funnel</u> Solv. lot# <u>V43 E07</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V32603</u>										
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE	<u>91759</u>									
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE	<u>24 000</u>									
LPC										
ENDRIN/DDT										

Analyst

LF/RW

on 4/12/01

Verified by _____

Reviewed by DWDate 11/12

DFTPP

Data File : M:\INSTRU~1\209\DATA\NOV2601\DFTPP.D

Acq On : 26 Nov 2001 10:40 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

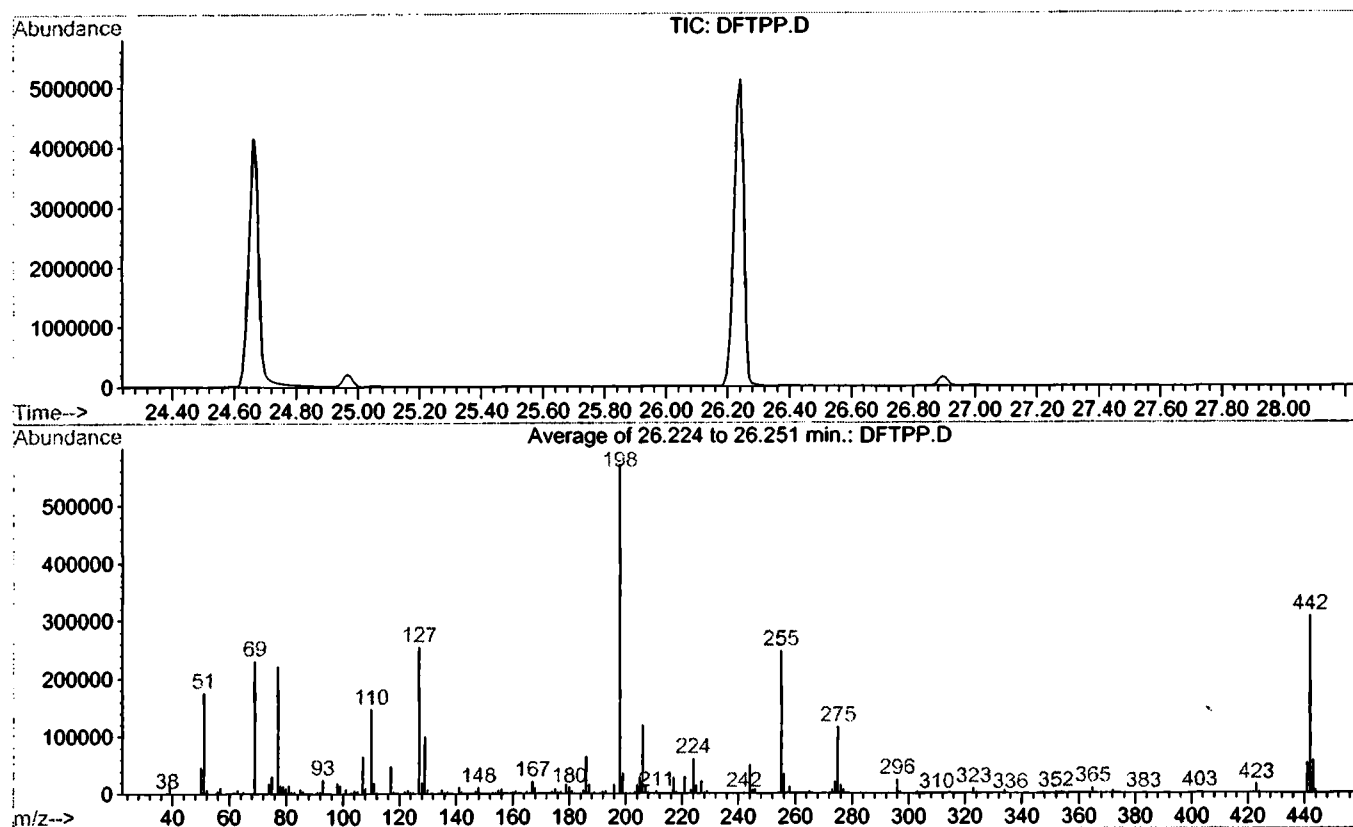

Spectrum Information: Average of 26.224 to 26.251 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	30.8	175908	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.5	231312	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	44.7	254976	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	570816	PASS
199	198	5	9	6.6	37502	PASS
275	198	10	30	20.3	115872	PASS
365	198	1	100	1.8	10464	PASS
441	443	0.01	100	92.0	54000	PASS
442	198	40	110	53.7	306592	PASS
443	442	17	23	19.1	58668	PASS

DFTPP.D GCMS1126.M

Wed Jan 09 14:19:11 2002