

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV2601.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\nov2601\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

(X) Full Method

(X) Inject Anyway

() Reprocessing Only

() Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP	NP103001	
2 Sample	2	CAL5	NP103001	calib mix
3 Sample	3	CAL10	NP103001	calib mix
4 Sample	4	CAL25	NP103001	calib mix
5 Sample	5	CAL40	NP103001	calib mix
6 Sample	6	CAL80	NP103001	calib mix
7 Sample	7	CAL100	NP103001	calib mix
8 Sample	8	LB	NP103001	10/22
9 Sample	9	LBA	NP103001	11/20 lab blk scan
10 Sample	10	28145	NP103001	11/20 scan
11 Sample	11	28155	NP103001	11/20 scan
12 Sample	12	28141	NP103001	11/20 scan
13 Sample	13	28147	NP103001	11/20 scan
14 Sample	14	28143	NP103001	11/20 scan
15 Sample	15	28149	NP103001	11/20 scan
16 Sample	16	28157	NP103001	11/20 scan
17 Sample	17	28153	NP103001	11/20 scan
18 Sample	18	28151	NP103001	11/20 scan
19 Sample	19	28161	NP103001	11/20 scan
20 Sample	20	28265	NP103001	11/20 scan
21 Sample	21	28159	NP103001	11/20 scan
22 Sample	22	REF	NP103001	11/20 scan
23 Sample	23	LBB	NP103001	11/21 scan
24 Sample	1	DFTPP1	NP103001	
25 Sample	2	24DDD	NP103001	gc/ms scan surrogate 5 ug/ml
26 Sample	24	28269	NP103001	11/21 scan
27 Sample	25	28267	NP103001	11/21 scan
28 Sample	26	28271	NP103001	11/21 scan
29 Sample	27	28273	NP103001	11/21 scan
30 Sample	28	28277	NP103001	11/21 scan
31 Sample	29	28473	NP103001	11/21 scan
32 Sample	30	REFA	NP103001	11/21 scan
33 Sample	2	CAL40A	NP103001	calib
34 Sample	3	28141A	NP103001	11/20 re injected
35 Sample	4	LBC	NP103001	11/23 scan
36 Sample	5	28473A	NP103001	11/23 scan
37 Sample	6	28477	NP103001	11/23 scan
38 Sample	7	28479	NP103001	11/23 scan
39 Sample	8	REFB	NP103001	11/23 scan
40 Sample	9	LBD	NP103001	11/24 scan
41 Sample	10	28682	NP103001	11/24 scan
42 Sample	11	28680	NP103001	11/24 scan
43 Sample	12	REFC	NP103001	11/24 scan

re injected

Last Modified: Wed Nov 28 11:41:43 2001

Page: 1

Sequence Name: C:\HPCHEM\1\SEQUENCE\NOV2701.S
 Comment: INST 209; 30Mx0.25umX0.50
 Operator: 209 GALOS
 Data Path: C:\HPCHEM\1\data\nov2701\
 Pre-Seq Cmd:
 Post-Seq Cmd:

Method Sections To Run On A Barcode Mismatch
 (X) Full Method (X) Inject Anyway
 () Reprocessing Only () Don't Inject


Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP2	NP103001	
2	Sample	16	28335	NP103001	11/20 scan
3	Sample	17	28326	NP103001	11/20 scan
4	Sample	18	28230	NP103001	11/20 scan
5	Sample	19	28327	NP103001	11/20 scan
6	Sample	2	CALIB40✓	NP103001	
7	Sample	20	28470✓	NP103001	11/21 scan
8	Sample	21	28429✓	NP103001	11/21 scan
9	Sample	22	28432✓	NP103001	11/21 scan
10	Sample	23	28433✓	NP103001	11/21 scan
11	Sample	2	CALCHK	GCMS1126	25
12	Sample	24	28468	GCMS1126	11/21 scan
13	Sample	25	28431	GCMS1126	11/21 scan
14	Sample	26	28434	GCMS1126	11/21 scan
15	Sample	27	28427	GCMS1126	11/21 scan
16	Sample	28	28428	GCMS1126	11/21 scan
17	Sample	31	28469	GCMS1126	11/21 scan
18	Sample	32	28476	GCMS1126	11/21 scan ?
19	Sample	33	326	GCMS1126	11/21 scan ?
20	Sample	34	28591	GCMS1126	11/23 scan
21	Sample	35	28666	GCMS1126	11/23 scan
22	Sample	36	28593	GCMS1126	11/23 scan
23	Sample	37	28595	GCMS1126	11/23 scan
24	Sample	38	28475	GCMS1126	11/23 scan
25	Sample	39	28600	GCMS1126	11/23 scan
26	Sample	40	28596	GCMS1126	11/23 scan
27	Sample	41	28652	GCMS1126	11/23 scan
28	Sample	42	28665	GCMS1126	11/23 scan
29	Sample	43	28599	GCMS1126	11/23 scan
30	Sample	44	28668	GCMS1126	11/23 scan
31	Sample	45	28667	GCMS1126	11/23 scan
32	Sample	46	28597	GCMS1126	11/23 scan
33	Sample	47	28598	GCMS1126	11/23 scan
34	Sample	48	28649	GCMS1126	11/23 scan
35	Sample	49	28651	GCMS1126	11/23 scan
36	Sample	51	LBD	NP103001	lb 11/2 gc/ms
37	Sample	52	LBE	NP103001	lb 11/2 gc/ms
38	Sample	53	26079	NP103001	11/2 gc/ms
39	Sample	54	26707	NP103001	11/2 gc/ms
40	Sample	55	26208	NP103001	11/2 gc/ms
41	Sample	56	26206	NP103001	11/2 gc/ms
42	Sample	57	26251	NP103001	11/2 gc/ms
43	Sample	58	26080	NP103001	11/2 gc/ms

do not scan
run

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV2601\DFTPP1.D
 Acq On : 27 Nov 2001 9:12 am
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

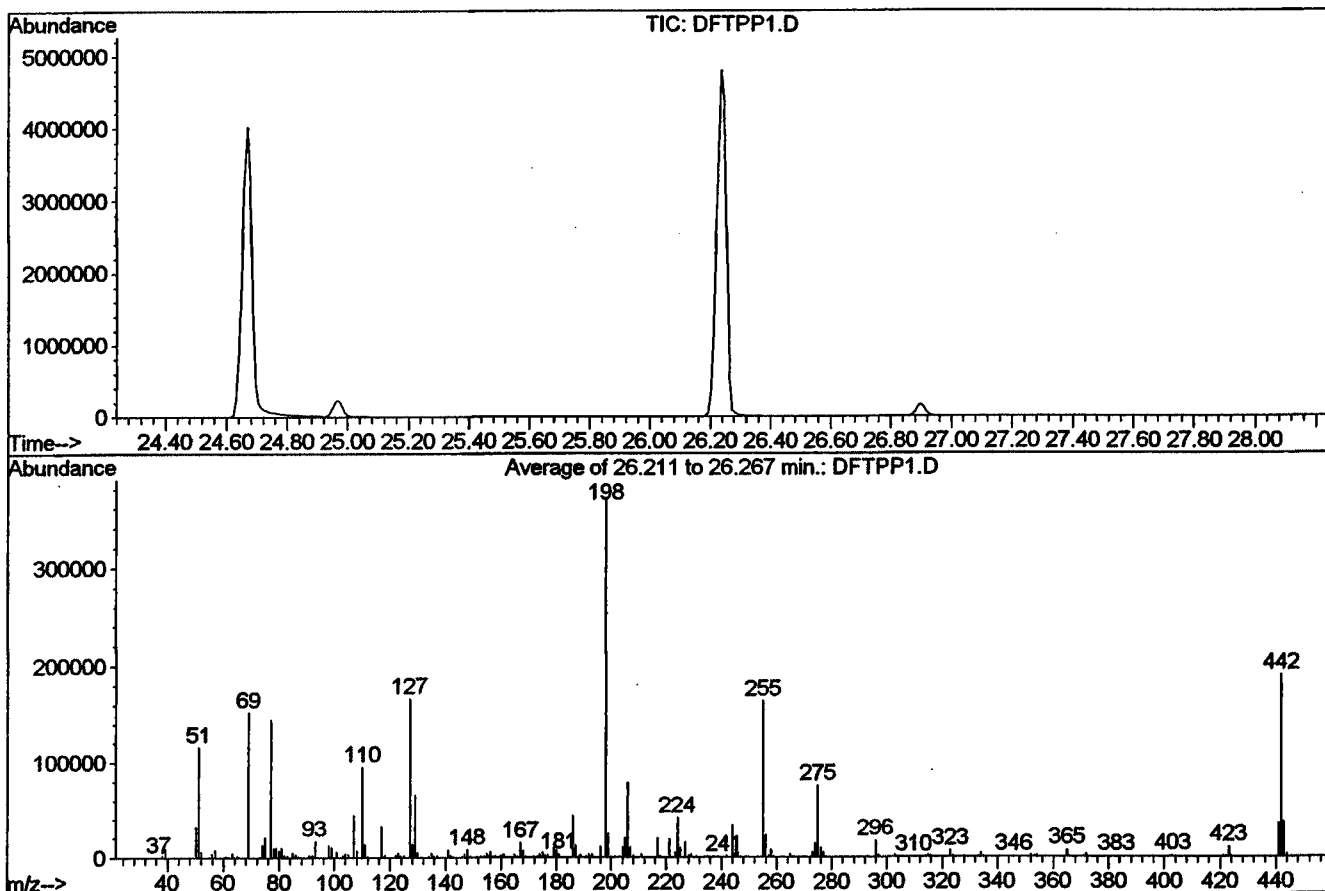


Spectrum Information: Average of 26.211 to 26.267 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	31.3	116050	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.1	152552	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	44.9	166397	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	370960	PASS
199	198	5	9	6.7	24825	PASS
275	198	10	30	20.4	75709	PASS
365	198	1	100	1.9	7199	PASS
441	443	0.01	100	94.7	34579	PASS
442	198	40	110	51.3	190205	PASS
443	442	17	23	19.2	36518	PASS

DFTPP

Data File : C:\HPCHEM\1\DATA\NOV2601\DFTPP2.D
 Acq On : 28 Nov 2001 7:56 am
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

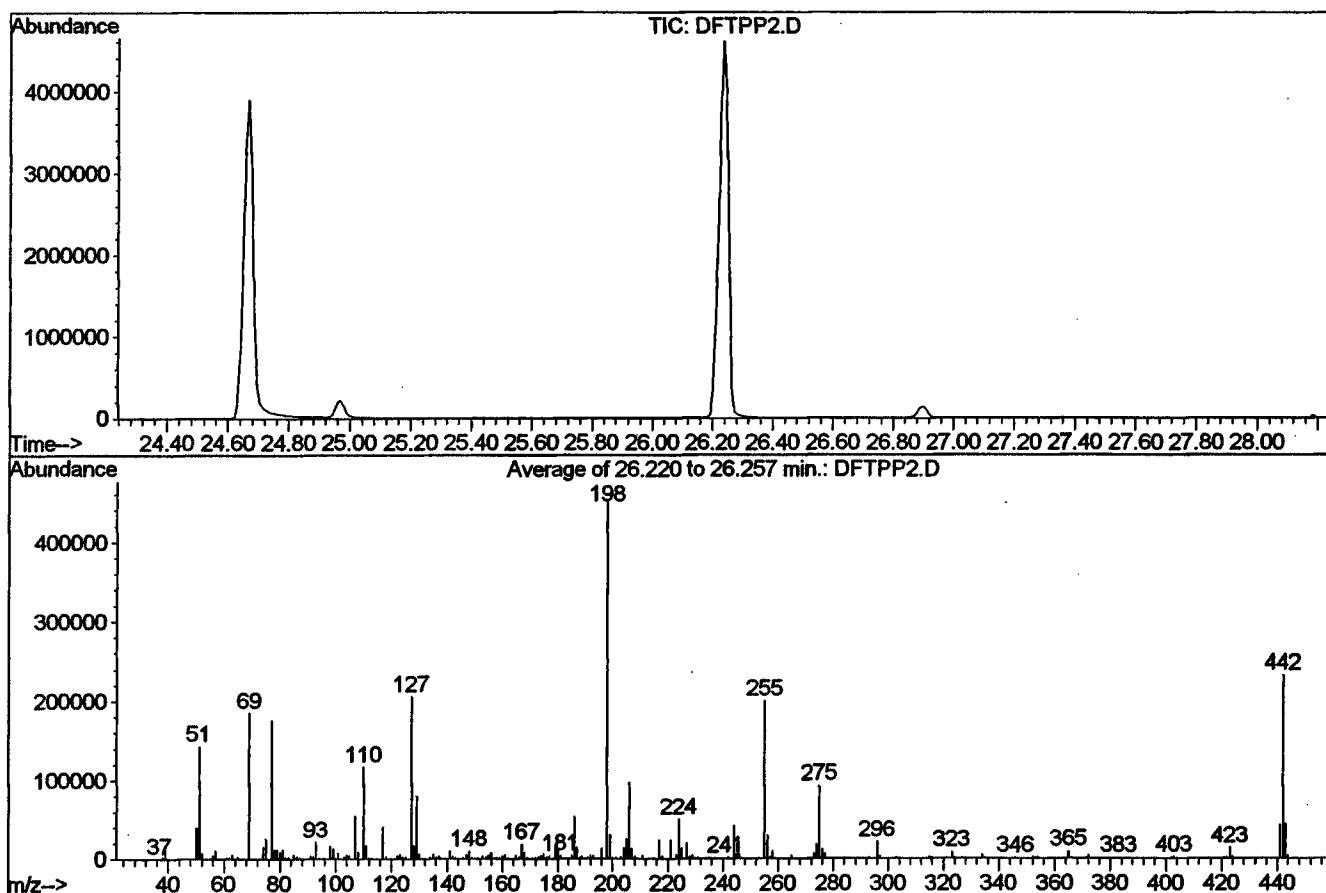

Spectrum Information: Average of 26.220 to 26.257 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	31.6	143211	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.9	185373	PASS
70	69	0.00	2	0.1	238	PASS
127	198	40	60	45.5	206224	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	453350	PASS
199	198	5	9	6.7	30319	PASS
275	198	10	30	20.6	93314	PASS
365	198	1	100	2.0	8943	PASS
441	443	0.01	100	94.9	41813	PASS
442	198	40	110	51.3	232346	PASS
443	442	17	23	19.0	44070	PASS