

Method 508

Date Extracted 11-29-01

Page

Rem

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
✓	L B ✓	500ml		1ml			2ml		7	0		
	Ref chl	111								0		
	Ref TOX	111								0		
	Ref pest									0		
28048	S chl									0		
28048	S D chl									0		
27984	S TOX									0		
27984	S D TOX									0		
27985	S pest									0		
27985	S D pest									0		
	PR L 1254									0		
✓	27984									1		
✓	27985									2		
✓	27986									3		
✓	28043									4		
✓	28044									5		
✓	28045									6		
✓	28046									7		
✓	28047									8		
✓	28048									9		
✓	28049									10		
✓	27775									11		
Remarks 27775 Re-EXTRACTED Reviewed by, <i>DB 5/11/02</i>												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -												
Extraction type -		Solv.lot#		NaCl lot#		Na2SO4 lot#						
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE												
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE												
LPC												
ENDRIN/DDT												

Analyst AD

Review

DN 1/29/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\DEC1901.S

Line Type	Vial	DataFile	Method	Sample Name
44 Sample	10 27954	NP112701	gcms	unknown 11/20
45 Sample	11 27955	NP112701	gcms	unknown 11/20
46 Sample	12 27956	NP112701	gcms	unknown 11/20
47 Sample	13 27957	NP112701	gcms	unknown 11/20
48 Sample	23 LBC	NP112701	gcms	unknown 11/21
49 Sample	24 27775	NP112701	gcms	unknown 11/21
50 Sample	25 27984	NP112701	gcms	unknown 11/21
51 Sample	26 27985	NP112701	gcms	unknown 11/21
52 Sample	27 27986	NP112701	gcms	unknown 11/21
53 Sample	28 28043	NP112701	gcms	unknown 11/21
54 Sample	29 28045	NP112701	gcms	unknown 11/21
55 Sample	30 28046	NP112701	gcms	unknown 11/21
56 Sample	31 28047	NP112701	gcms	unknown 11/21
57 Sample	33 28048	NP112701	gcms	unknown 11/21
58 Sample	34 28049	NP112701	gcms	unknown 11/21
59 Sample	35 28044	NP112701	gcms	unknown 11/21

from
Dec 21/01

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC2101\DFTPP1.D

Acq On : 21 Dec 2001 3:10 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)


Title : 208 625/TCLP calibration table

Vial: 1

Operator: GALOS

Inst : GC/MS Ins

Multiplr: 1.00

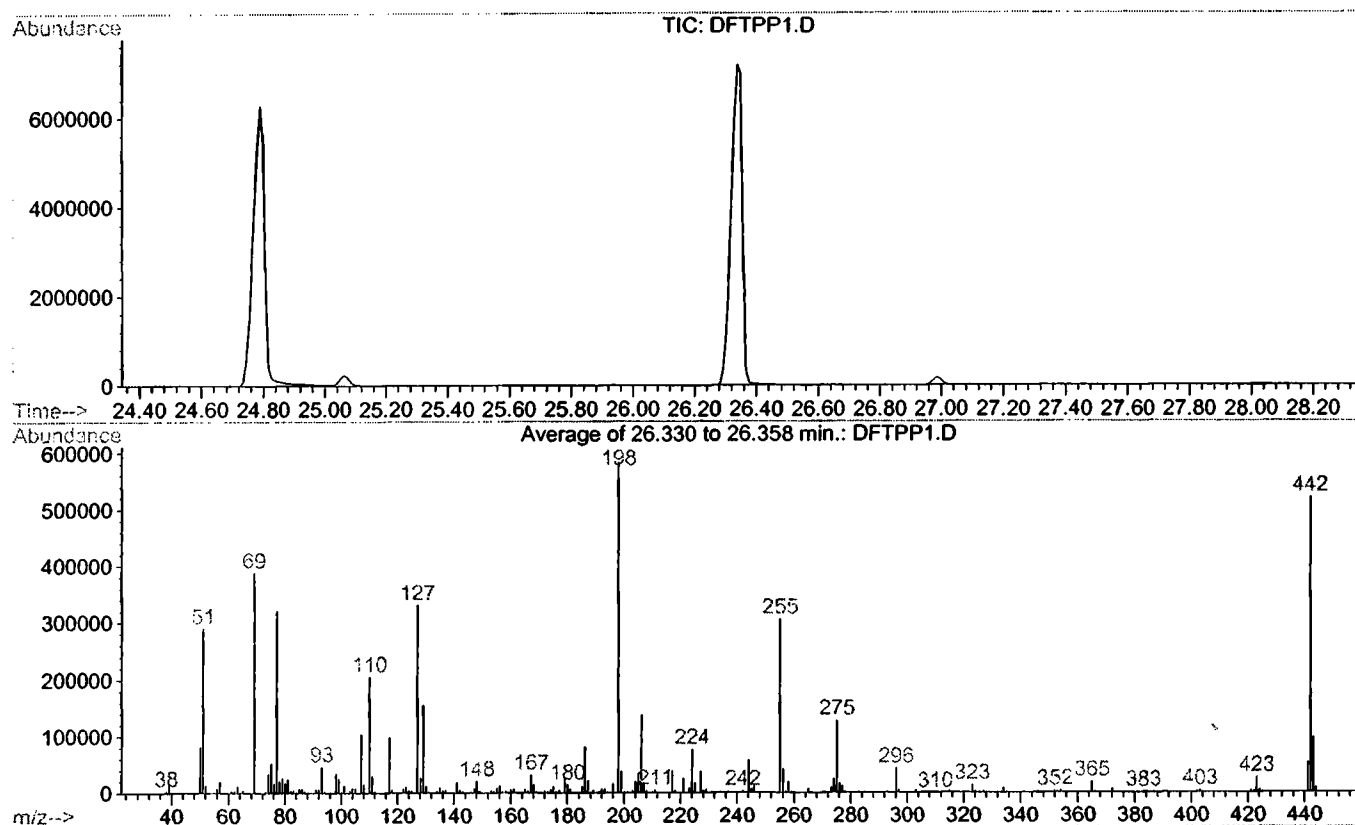

Spectrum Information: Average of 26.330 to 26.358 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	49.9	290600	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	66.8	389152	PASS
70	69	0.00	2	0.5	1883	PASS
127	198	40	60	57.0	331888	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	582416	PASS
199	198	5	9	6.6	38612	PASS
275	198	10	30	22.2	129300	PASS
365	198	1	99	3.4	19749	PASS
441	443	1	99	54.5	53750	PASS
442	198	40	110	89.4	520960	PASS
443	442	17	23	18.9	98614	PASS

DFTPP1.D NP112701.M

Thu Dec 27 08:13:00 2001