

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 01/02/2002 Time: 14:52:08

Sample: AD27984
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 1/2/02 14:50 Ended: 1/2/02 14:50 Analyst: MG
 Page: 1

	Component Name	Viol	Result	MDL
1	Other unknown compounds		see comment	
2	Surr_2,4-DDD			5.0

Comments for Sample AD27984 - Analysis \$GCMS

Vestchester Dept. of Labs & Research

User: Galos, Marie

Date: 01-02-2002 Time: 14:52:27

Scan of the extract prepared for the 508 analysis, from 35-550 amu using a mass spectrometer, does not reveal the presence of non-target compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1901\27984.D

Vial: 25

Acq On : 21 Dec 2001 5:51 am

Operator: GALOS

Sample : gcms unknown 11/21

Inst : GC/MS Ins

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 21 9:28 2001

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

Last Update : Wed Nov 28 15:33:44 2001

Response via : Initial Calibration

DataAcq Meth : NP112701

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	11.86	152	1085722	20.00	ng/uL	-0.08
19) Naphthalene-d8	15.47	136	4269621	20.00	ng/uL	-0.08
31) Acenaphthene-d10	20.74	164	1903285	20.00	ng/uL	-0.08
49) Phenanthrene-d10	25.16	188	2790400	20.00	ng/uL	-0.09
59) Chrysene-d12	33.16	240	1928221	20.00	ng/uL	-0.09
68) Perylene-d12	37.24	264	1026299	20.00	ng/uL	-0.10

System Monitoring Compounds

4) 2-Fluorophenol	0.00	112	0	0.00	ng/uL	
Spiked Amount	75.000	Range	18 - 42	Recovery	=	0.00%#
5) Phenol-d5	0.00	99	0	0.00	ng/uL	
Spiked Amount	75.000	Range	19 - 32	Recovery	=	0.00%#
6) 2-Chlorophenol-d4	11.86	132	682	0.01	ng/uL	0.44
Spiked Amount	75.000	Range	34 - 84	Recovery	=	0.01%#
7) 1,2-Dichlorobenzene-d4	12.09	152	1010	0.02	ng/uL	-0.37
Spiked Amount	50.000	Range	26 - 73	Recovery	=	0.04%#
20) Nitrobenzene-d5	0.00	82	0	0.00	ng/uL	
Spiked Amount	50.000	Range	55 - 98	Recovery	=	0.00%#
32) 2-Fluorobiphenyl	18.89	172	2322	0.02	ng/uL	0.06
Spiked Amount	50.000	Range	42 - 78	Recovery	=	0.04%#
33) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng/uL	
Spiked Amount	75.000	Range	45 - 96	Recovery	=	0.00%#
62) Terphenyl-d14	0.00	244	0	0.00	ng/uL	
Spiked Amount	50.000	Range	58 - 98	Recovery	=	0.00%#

Target Compounds

				Qvalue
2) Pyridine	0.00	79	0	N.D.
3) N-nitrosodimethylamine	0.00	74	0	N.D.
8) Phenol	0.00	94	0	N.D.
9) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
10) 2-Chlorophenol	0.00	128	0	N.D.
11) 1,3-Dichlorobenzene	0.00	146	0	N.D.
12) 1,4-Dichlorobenzene	0.00	146	0	N.D.
13) 1,2-Dichlorobenzene	0.00	146	0	N.D.
14) 2-Methylphenol	0.00	108	0	N.D.
15) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
16) 3&4-Methylphenol	0.00	108	0	N.D.

(#) = qualifier out of range (m) = manual integration

27984.D NP112701.M Fri Dec 21 09:35:02 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1901\27984.D

Vial: 25

Acq On : 21 Dec 2001 5:51 am

Operator: GALOS

Sample : gcms unknown 11/21

Inst : GC/MS Ins

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 21 9:28 2001

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

Last Update : Wed Nov 28 15:33:44 2001

Response via : Initial Calibration

DataAcq Meth : NP112701

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
17) N-Nitrosodi-n-propylamine	0.00	70	0	N.D.		
18) Hexachloroethane	0.00	117	0	N.D.		
21) Nitrobenzene	0.00	77	0	N.D.		
22) Isophorone	0.00	82	0	N.D.		
23) 2-Nitrophenol	0.00	139	0	N.D.		
24) 2,4-Dimethylphenol	0.00	107	0	N.D.		
25) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
26) 2,4-Dichlorophenol	0.00	162	0	N.D.		
27) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
28) Naphthalene	0.00	128	0	N.D.		
29) Hexachlorobutadiene	0.00	225	0	N.D.		
30) 4-Chloro-3-methylphenol	0.00	107	0	N.D.		
34) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
35) 2,4,6-Trichlorophenol	0.00	196	0	N.D.		
36) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
37) 2-Chloronaphthalene	0.00	162	0	N.D.		
38) Dimethylphthalate	0.00	163	0	N.D.		
39) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
40) Acenaphthylene	0.00	152	0	N.D.		
41) Acenaphthene	0.00	153	0	N.D.		
42) 2,4-Dinitrophenol	0.00	184	0	N.D.		
43) 4-Nitrophenol	0.00	65	0	N.D.		
44) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
45) Diethylphthalate	0.00	149	0	N.D.		
46) 4-Chlorophenylphenylether	0.00	204	0	N.D.		
47) Fluorene	0.00	166	0	N.D.		
48) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
50) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
51) N-Nitrosodiphenylamine	0.00	169	0	N.D.		
52) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
53) Hexachlorobenzene	0.00	284	0	N.D.		
54) Pentachlorophenol	0.00	266	0	N.D.		
55) Phenanthrene	25.15	178	617	N.D.		
56) Anthracene	25.15	178	617	N.D.		
57) Di-n-butylphthalate	27.15	149	11727	N.D.		
58) Fluoranthene	0.00	202	0	N.D.		
60) 3,3'-Dichlorobenzidine	0.00	252	0	N.D.		

(#)=qualifier out of range (m)=manual integration

27984.D NP112701.M Fri Dec 21 09:35:04 2001

Page 2

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1901\27984.D

Vial: 25

Acq On : 21 Dec 2001 5:51 am

Operator: GALOS

Sample : gcms unknown 11/21

Inst : GC/MS Ins

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 21 9:28 2001

Quant Results File: NP112701.RES

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

Last Update : Wed Nov 28 15:33:44 2001

Response via : Initial Calibration

DataAcq Meth : NP112701

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
61) Benzidine	0.00	184	0		N.D.	
63) Pyrene	0.00	202	0		N.D.	
64) Butylbenzylphthalate	0.00	149	0		N.D.	
65) Benzo(a)anthracene	33.16	228	4272		N.D.	
66) Bis(2-ethylhexyl)phthalate	33.41	149	3816		N.D.	
67) Chrysene	33.16	228	4272		N.D.	
69) Di-n-Octylphthalate	0.00	149	0		N.D.	
70) Benzo(b)fluoranthene	0.00	252	0		N.D.	
71) Benzo(k)fluoranthene	0.00	252	0		N.D.	
72) Benzo(a)pyrene	37.23	252	3622		N.D.	
73) Indeno(1,2,3-cd)pyrene	0.00	276	0		N.D.	
74) Dibenz(a,h)anthracene	0.00	278	0		N.D.	
75) Benzo(g,h,i)perylene	0.00	276	0		N.D.	

(#) = qualifier out of range (m) = manual integration

27984.D NP112701.M

Fri Dec 21 09:35:05 2001

Page 3


Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC1901\27984.D
Acq On : 21 Dec 2001 5:51 am
Sample : gcms unknown 11/21
Misc :
MS Integration Params: RTEINT.P
Quant Time: Dec 21 9:28 2001

Vial: 25
Operator: GALOS
Inst : GC/MS Ins
Multiplr: 1.00

Quant Results File: NP112701.RES

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
Title : 208 625/TCLP calibration table
Last Update : Wed Nov 28 15:33:44 2001
Response via : Initial Calibration

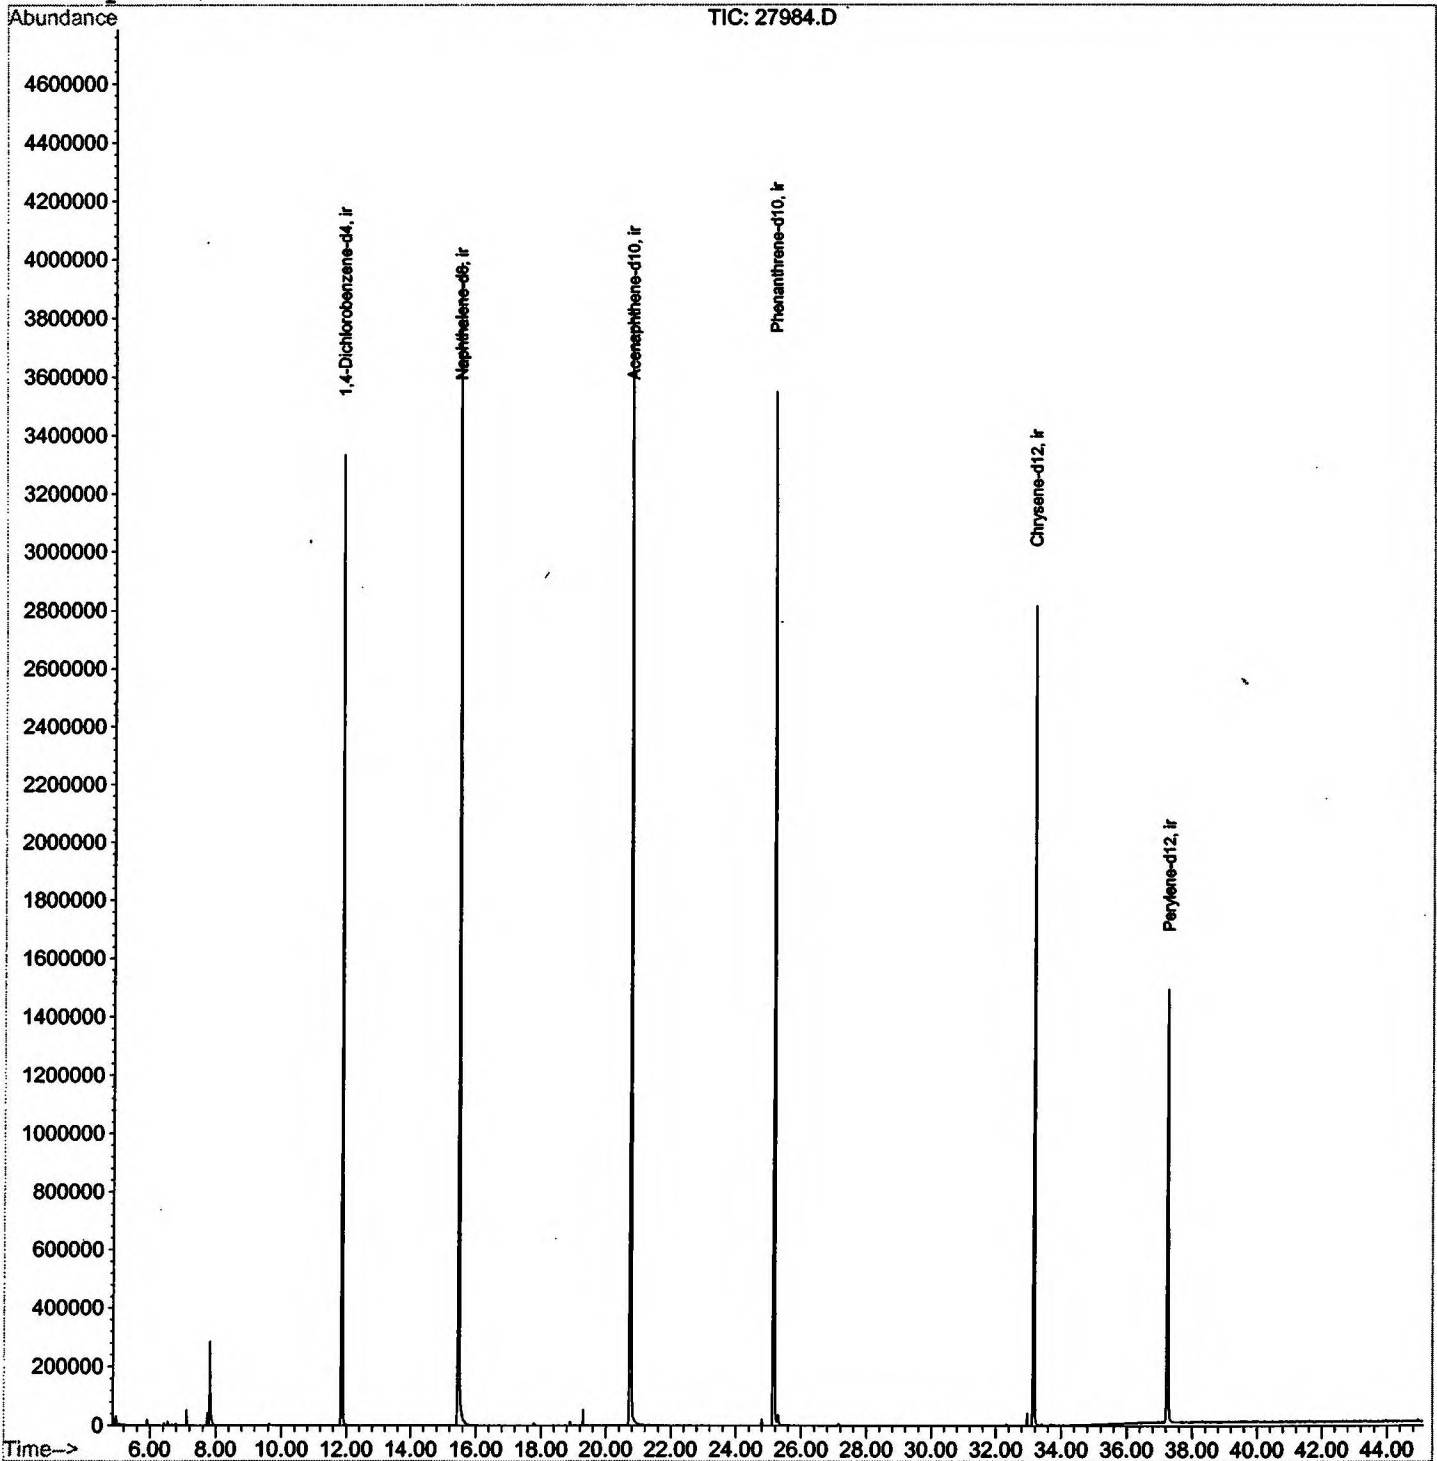

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC1901\27984.D

Vial: 25

Acq On : 21 Dec 2001 5:51 am

Operator: GALOS

Sample : gcms unknown 11/21

Inst : GC/MS Ins

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)

Title : 208 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.815	320	324	339	rVB	284387	585689	6.66%	1.356%
2	11.859	759	765	779	rBV	3334467	6743914	76.70%	15.616%
3	15.472	1153	1159	1177	rBV	3988370	8793080	100.00%	20.361%
4	20.745	1727	1734	1752	rBV	3825445	8519959	96.89%	19.729%
5	25.156	2208	2215	2226	rBV2	3549583	8036067	91.39%	18.608%
6	33.161	3081	3088	3101	rBV2	2812468	6471206	73.59%	14.985%
7	37.242	3525	3533	3544	rBV2	1477353	4035089	45.89%	9.344%




Sum of corrected areas: 43185004

27984.D NP112701.M

Fri Dec 28 09:30:16 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC1901\27984.D
Operator : GALOS
Acquired : 21 Dec 2001 5:51 am using AcqMethod NP112701
Instrument : GC/MS Ins
Sample Name: gcms unknown 11/21
Misc Info :
Vial Number: 25
Quant File :NP112701.RES (RTE Integrator)

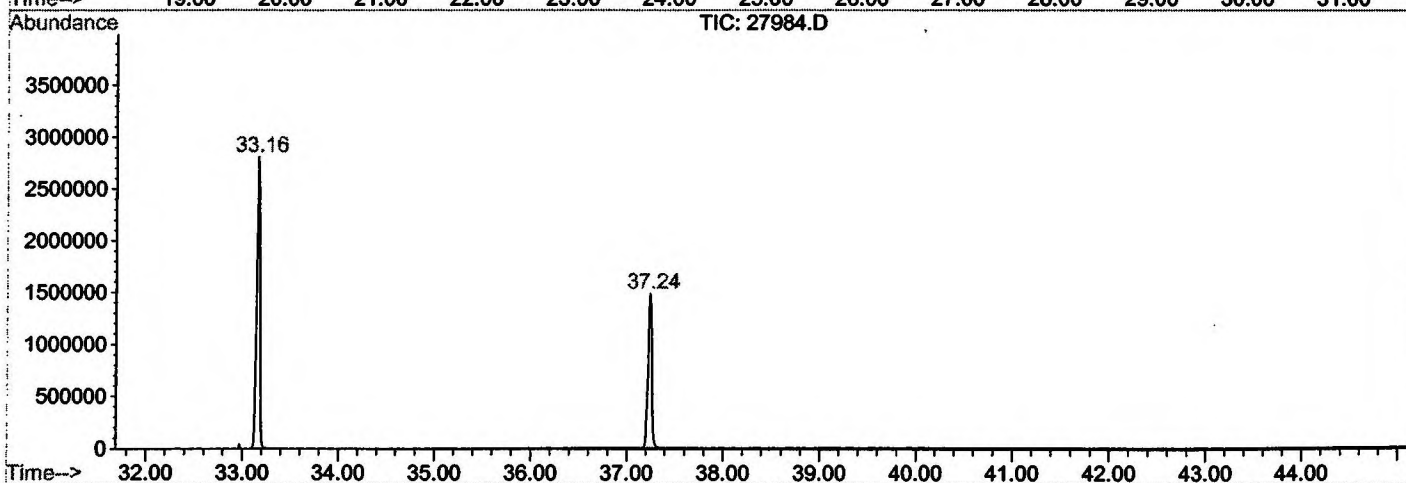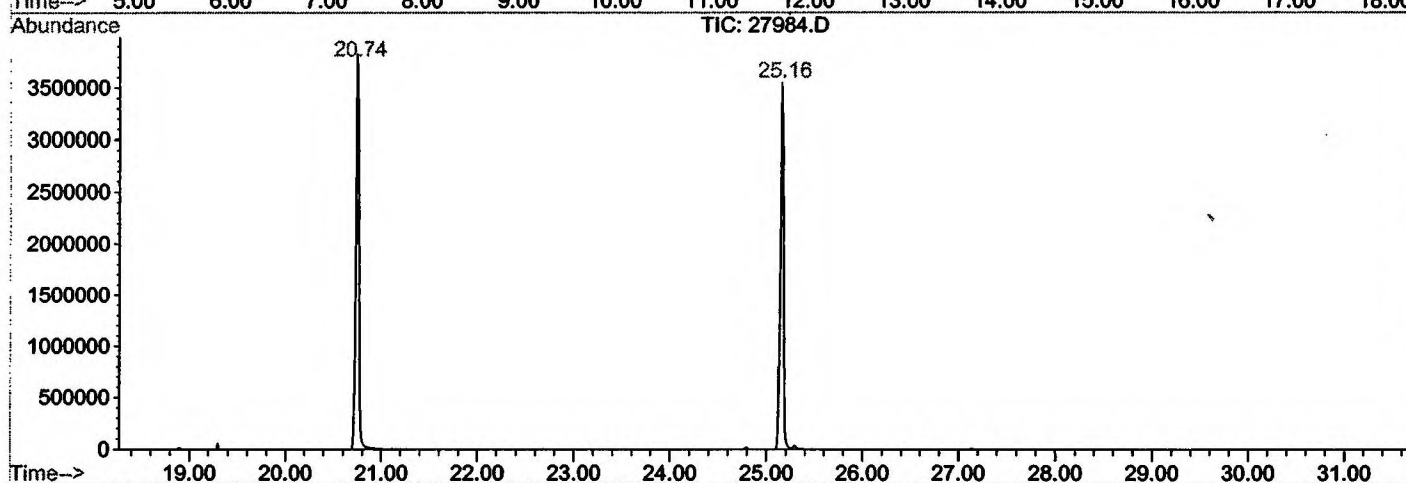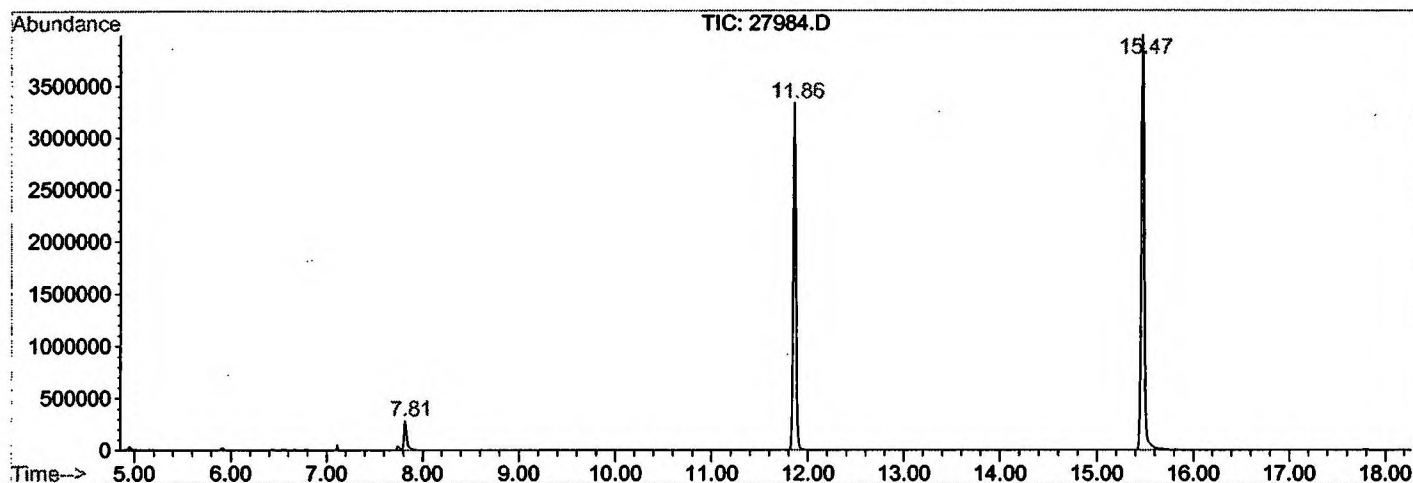

27984.D NP112701.M

Fri Dec 28 09:30:19 2001

Library Search Compound Report







Data File : C:\HPCHEM\1\DATA\DEC1901\27984.D
Acq On : 21 Dec 2001 5:51 am
Sample : gcms unknown 11/21
Misc :
MS Integration Params: LSCINT.P

Vial: 25
Operator: GALOS
Inst : GC/MS Ins
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
Title : 208 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methy Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
7.81	1.74 ng/uL	585689	1,4-Dichlorobenzene-d4	11.86	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	53
2	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	43
3	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	43
4	Acetic acid, 1,1-dimethylethyl este	116	C6H12O2	000540-88-5	28

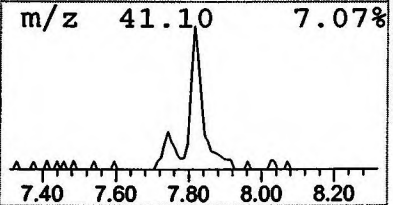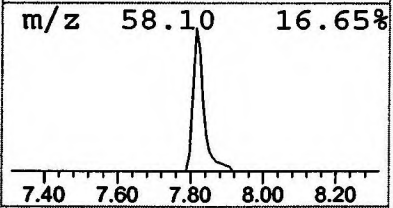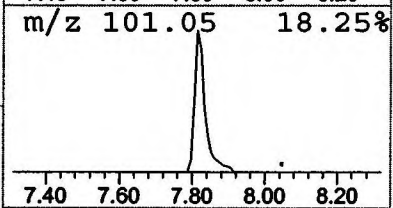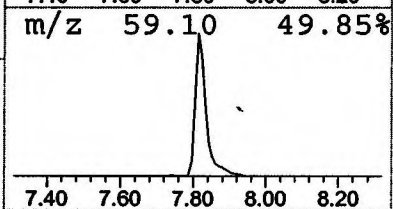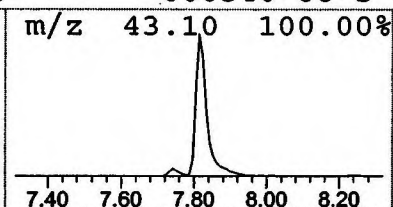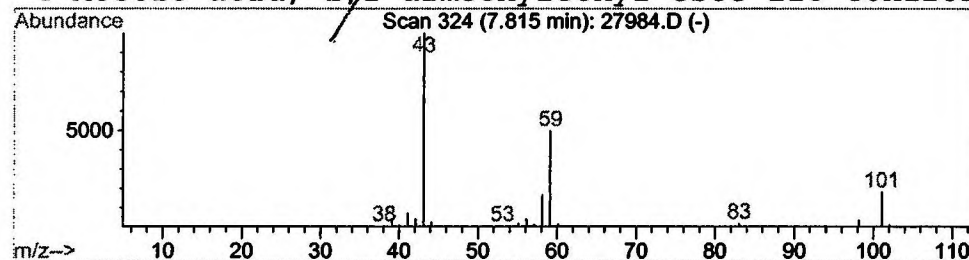

Tentatively Identified Compound (LSC) summary

Operator ID: GALOS Date Acquired: 21 Dec 2001 5:51 am
 Data File: C:\HPCHEM\1\DATA\DEC1901\27984.D
 Name: gcms unknown 11/21
 Misc:
 Method: C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)
 Title: 208 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc

2-Pentanone, 4-hydro	7.81	1.7	ng/uL	585689	ISTD01	11.86	6743910	20.0

27984.D NP112701.M Fri Dec 28 09:30:23 2001