

Method 508

Date Extracted 11-28-01

Page

GCM8

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
	L.B.	500 ml		1 ml			2 ml		7			
	Ref chl											
	Ref TOX											
	Ref pest											
28168	S chl											
28168	S D chl											
28166	S TOX											
28166	S D TOX											
	PRL 1260											
	✓ 28104									1		
	✓ 28105									2		
	✓ 28106									3		
	✓ 28107									4		
	✓ 28165									5		
	✓ 28166									6		
	✓ 28167									7		
	✓ 28168									8		
	✓ 28169									9		
	✓ 28170									10		
28167	S D Pest											
28167	S pest											
Reviewed by, <i>JB 5/11/02</i>												
Remarks												
drip rate must be between 5-15 ml/min for liq-liq extractors												
Extraction type - Solv.lot# NaCl lot# Na2SO4 lot#												
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE												
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE												
LPC												
ENDRIN/DDT												

Analyst *MD*
Revision 4/12/01

Verified by _____

Reviewed by *OW*
Date *1/4/02*

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC2101\DFTPP2.D

Acq On : 21 Dec 2001 7:44 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)


Title : 208 625/TCLP calibration table

Vial: 1

Operator: GALOS

Inst : GC/MS Ins

Multiplr: 1.00

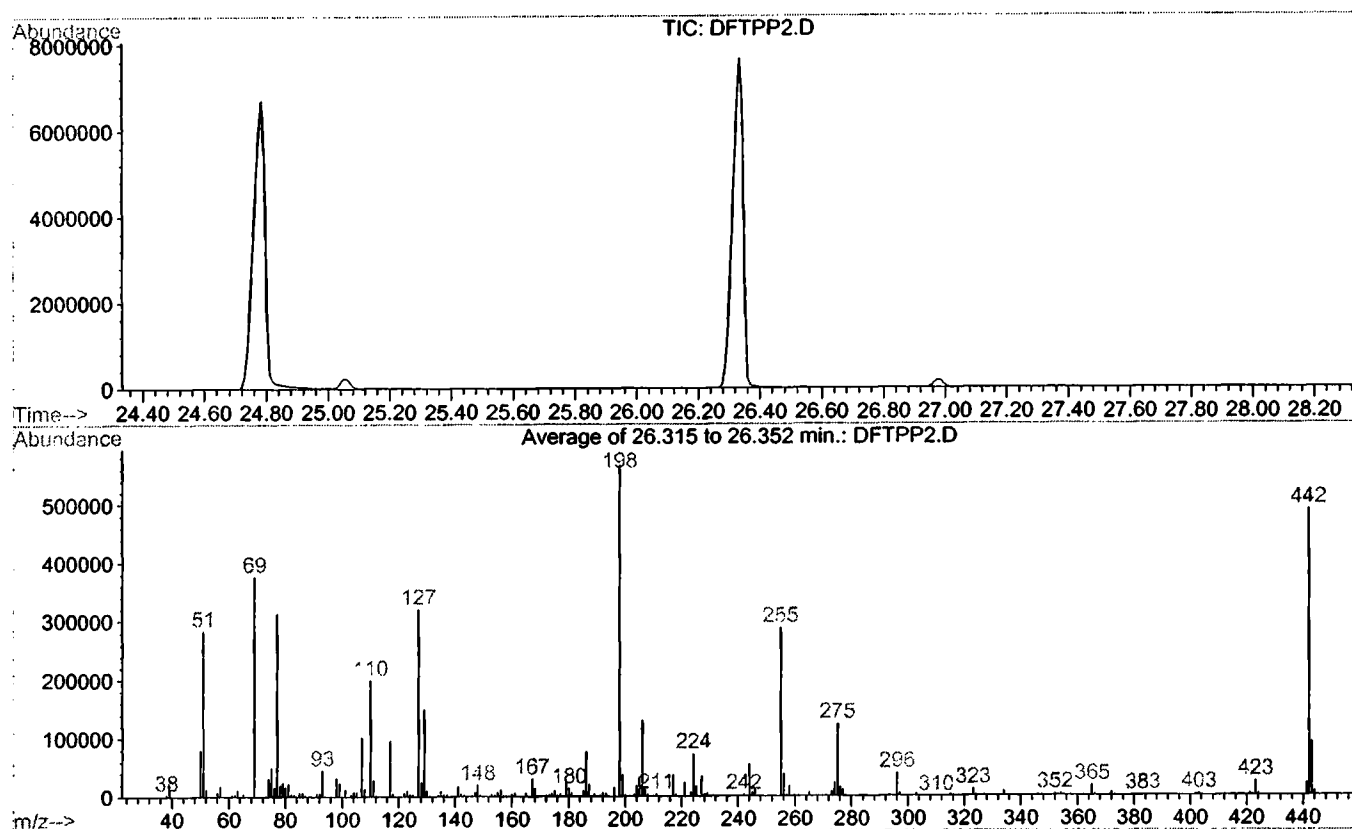

Spectrum Information: Average of 26.315 to 26.352 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	50.0	283450	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	66.5	376949	PASS
70	69	0.00	2	0.5	1865	PASS
127	198	40	60	56.7	321110	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	566579	PASS
199	198	5	9	6.6	37409	PASS
275	198	10	30	21.9	124242	PASS
365	198	1	99	3.2	18387	PASS
441	443	1	99	24.1	22450	PASS
442	198	40	110	86.5	489907	PASS
443	442	17	23	19.0	93128	PASS

DFTPP2.D NP112701.M

Thu Jan 03 08:38:16 2002