

Method 508 modifiedDate Extracted 11/24/01Page 1

36C MS - 15843

ref

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
LB		500 ml		1.0 ml			1 ml		7	
Ref					0.5 mL					
28669	✓									
28662	✓									
28691	✓									
28684	✓									
28690	✓									
28688	✓									
28664	✓									
28663	✓									
28695	✓									
28694	✓									
28692	✓									
28693	✓									
28682	✓ HPD									
28678	✓									
28680	✓ HPD									
28677	✓									
28267	re-extract									
28430	re-extract									
28471	re-extract									
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										
See 11/24/01										

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC0401\DFTPP1.D

Acq On : 4 Dec 2001 8:28 am

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP112601.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

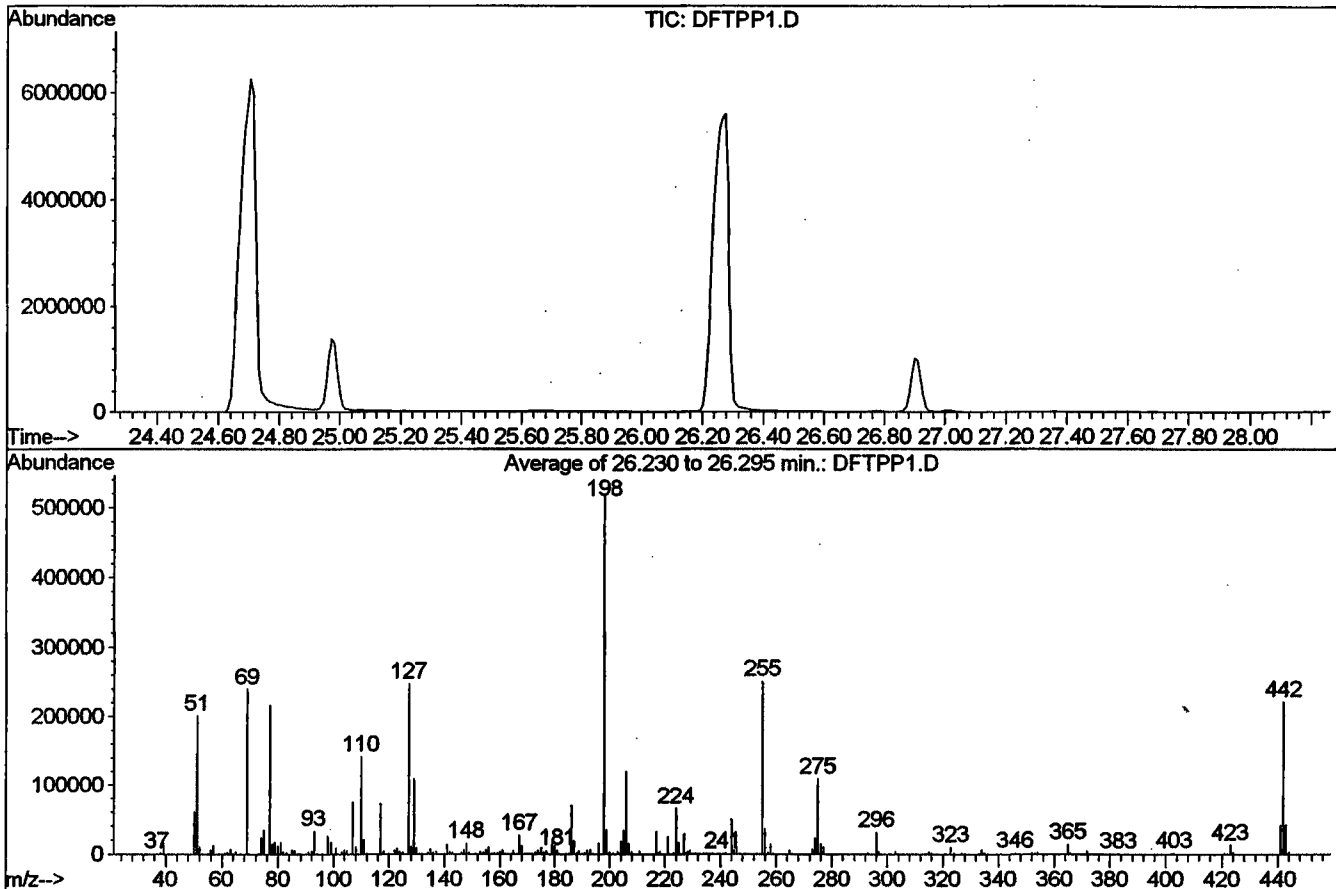

Spectrum Information: Average of 26.230 to 26.295 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	38.7	201281	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.2	239966	PASS
70	69	0.00	2	0.0	33	PASS
127	198	40	60	47.6	247474	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	519597	PASS
199	198	5	9	6.7	35018	PASS
275	198	10	30	21.1	109560	PASS
365	198	1	100	2.7	14224	PASS
441	443	0.01	100	96.5	41152	PASS
442	198	40	110	42.6	221456	PASS
443	442	17	23	19.3	42647	PASS

DFTPP1.D NP112601.M

Tue Dec 04 10:07:56 2001