

Comments for Sample AD28756 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 12-12-2001 Time: 09:39:48

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 12/12/2001 Time: 09:39:22

Sample: AD28756
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 12/12/01 09:38 Ended: 12/12/01 09:38 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds				
2					

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0501\28756.D

Vial: 20

Acq On : 6 Dec 2001 7:09 am

Operator: 209 GALOS

Sample : 11/26 gc/ms scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 6 7:58 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Nov 28 15:06:24 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	11.72	152	850353	20.00	ug/l	0.02
15) Naphthalene-d8	15.31	136	3224890	20.00	ug/l	0.00
26) Acenaphthene-d10	20.58	164	1534987	20.00	ug/l	0.00
42) Phenanthrene-d10	25.01	188	2207415	20.00	ug/l	0.02
53) Chrysene-d12	33.04	240	1368251	20.00	ug/l	0.00
59) Perylene-d12	37.14	264	875057	20.00	ug/l	0.02

System Monitoring Compounds

52) 2,4-DDD	30.09	235	113241	4.31	ug/mL	0.02
Spiked Amount	5.000		Recovery	=	86.20%	

Target Compounds

					Qvalue
2) Pyridine	0.00	79	0	N.D.	
3) N-nitroso-dimethyl amine	5.18	74	628	N.D.	
4) Phenol	0.00	94	0	N.D.	
5) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
6) 2-Chlorophenol	0.00	128	0	N.D.	
7) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
8) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
9) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
10) 2-Methylphenol	0.00	108	0	N.D.	
11) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
12) 3&4-Methylphenol	0.00	108	0	N.D.	
13) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
14) Hexachloroethane	0.00	117	0	N.D.	
16) Nitrobenzene	0.00	77	0	N.D.	
17) Isophorone	0.00	82	0	N.D.	
18) 2-Nitrophenol	0.00	139	0	N.D.	
19) 2,4-Dimethylphenol	0.00	107	0	N.D.	
20) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
21) 2,4-Dichlorophenol	0.00	162	0	N.D.	
22) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
23) Naphthalene	15.38	128	817	N.D.	
24) Hexachlorobutadiene	0.00	225	0	N.D.	
25) 4-Chloro-3-methylphenol	0.00	107	0	N.D.	
27) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
28) 2,4,6-Trichlorophenol	0.00	196	0	N.D.	

(#) = qualifier out of range (m) = manual integration

28756.D GCMS1126.M Fri Dec 07 14:29:46 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0501\28756.D

Vial: 20

Acq On : 6 Dec 2001 7:09 am

Operator: 209 GALOS

Sample : 11/26 gc/ms scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 6 7:58 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Nov 28 15:06:24 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
29) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
30) 2-Chloronaphthalene	0.00	162	0	N.D.		
31) Dimethylphthalate	0.00	163	0	N.D.		
32) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
33) Acenaphthylene	0.00	152	0	N.D.		
34) Acenaphthene	0.00	153	0	N.D.		
35) 2,4-Dinitrophenol	0.00	184	0	N.D.		
36) 4-Nitrophenol	0.00	65	0	N.D.		
37) 2,4-Dinitrotoluene	21.19	165	111	N.D.		
38) Diethylphthalate	22.11	149	816	N.D.		
39) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
40) Fluorene	0.00	166	0	N.D.		
41) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
43) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
44) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
45) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
46) Hexachlorobenzene	0.00	284	0	N.D.		
47) Pentachlorophenol	0.00	266	0	N.D.		
48) Phenanthrene	25.07	178	331	N.D.		
49) Anthracene	25.07	178	331	N.D.		
50) Di-n-butylphthalate	27.02	149	5700	N.D.		
51) Fluoranthene	0.00	202	0	N.D.		
54) Pyrene	0.00	202	0	N.D.		
55) Butylbenzylphthalate	0.00	149	0	N.D.		
56) Benzo(a)anthracene	33.04	228	3315	N.D.		
57) Bis(2-ethylhexyl)phthalate	33.32	149	7120	N.D.		
58) Chrysene	33.04	228	3315	N.D.		
60) Di-n-Octylphthalate	0.00	149	0	N.D.		
61) Benzo(b)fluoranthene	0.00	252	0	N.D.		
62) Benzo(k)fluoranthene	0.00	252	0	N.D.		
63) Benzo(a)pyrene	37.14	252	3257	N.D.		
64) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
65) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
66) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

28756.D GCMS1126.M Fri Dec 07 14:29:50 2001

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC0501\28756.D
Acq On : 6 Dec 2001 7:09 am
Sample : 11/26 gc/ms scan
Misc :
MS Integration Params: RTEINT.P
Quant Time: Dec 6 7:58 2001

Vial: 20
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Nov 28 15:06:24 2001
Response via : Initial Calibration

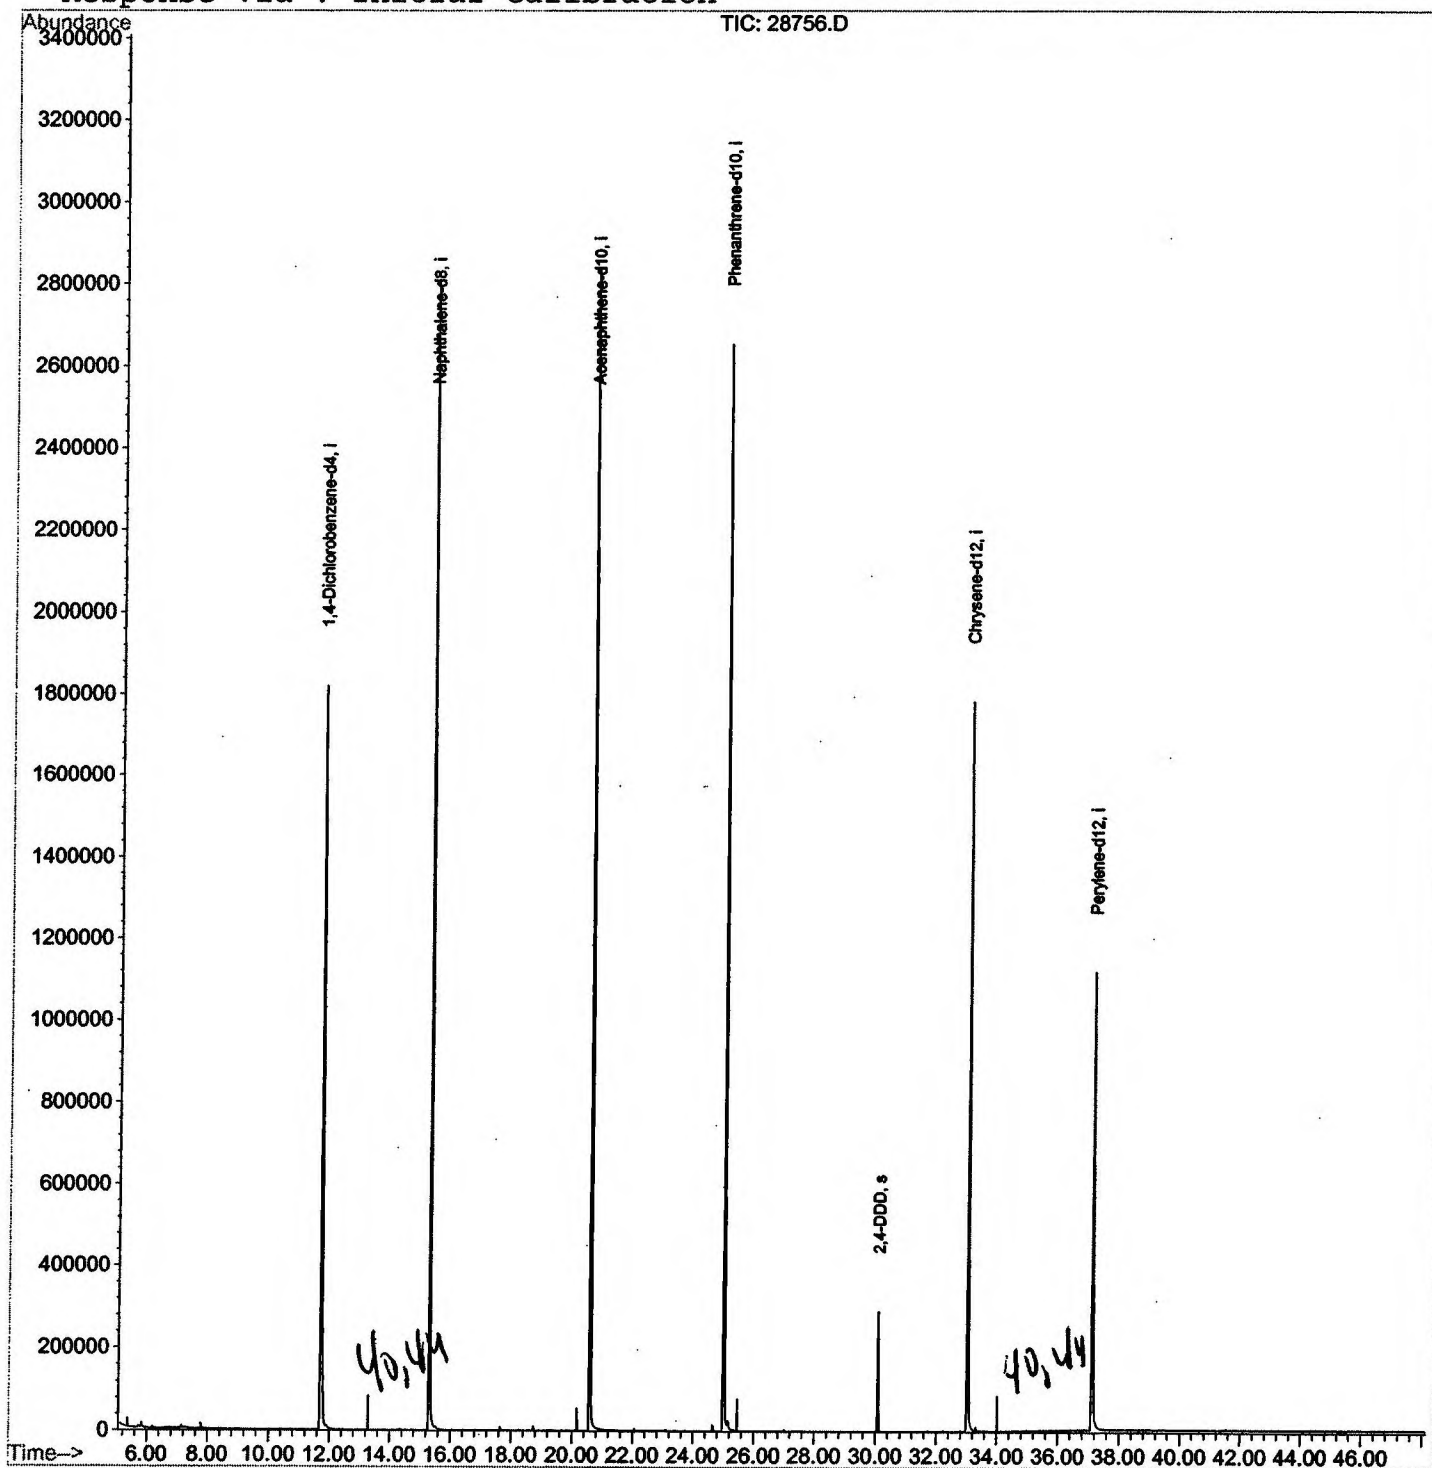

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC0501\28756.D

Acq On : 6 Dec 2001 7:09 am

Sample : 11/26 gc/ms scan

Misc :

MS Integration Params: LSCINT.P

Vial: 20

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	11.716	721	727	745	rBV	1818472	4562124	72.80%	14.819%
2	15.314	1113	1119	1137	rBV	2809763	6012643	95.95%	19.531%
3	20.584	1687	1693	1713	rBV	2838895	6266547	100.00%	20.356%
4	25.009	2168	2175	2187	rBV2	2652737	5837341	93.15%	18.961%
5	25.146	2187	2190	2201	rVB2	22738	77396	1.24%	0.251%
6	30.085	2722	2728	2736	rBV	288156	602458	9.61%	1.957%
7	33.041	3042	3050	3067	rBV2	1782099	4266288	68.08%	13.858%
8	37.136	3487	3496	3510	rBV2	1112693	3160575	50.44%	10.266%


Sum of corrected areas: 30785372

28756.D GCMS1126.M

Fri Dec 07 17:01:20 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC0501\28756.D
Operator : 209 GALOS
Acquired : 6 Dec 2001 7:09 am using AcqMethod GCMS1126
Instrument : GC/MS 209
Sample Name: 11/26 gc/ms scan
Misc Info :
Vial Number: 20
Quant File :GCMS1126.RES (RTE Integrator)

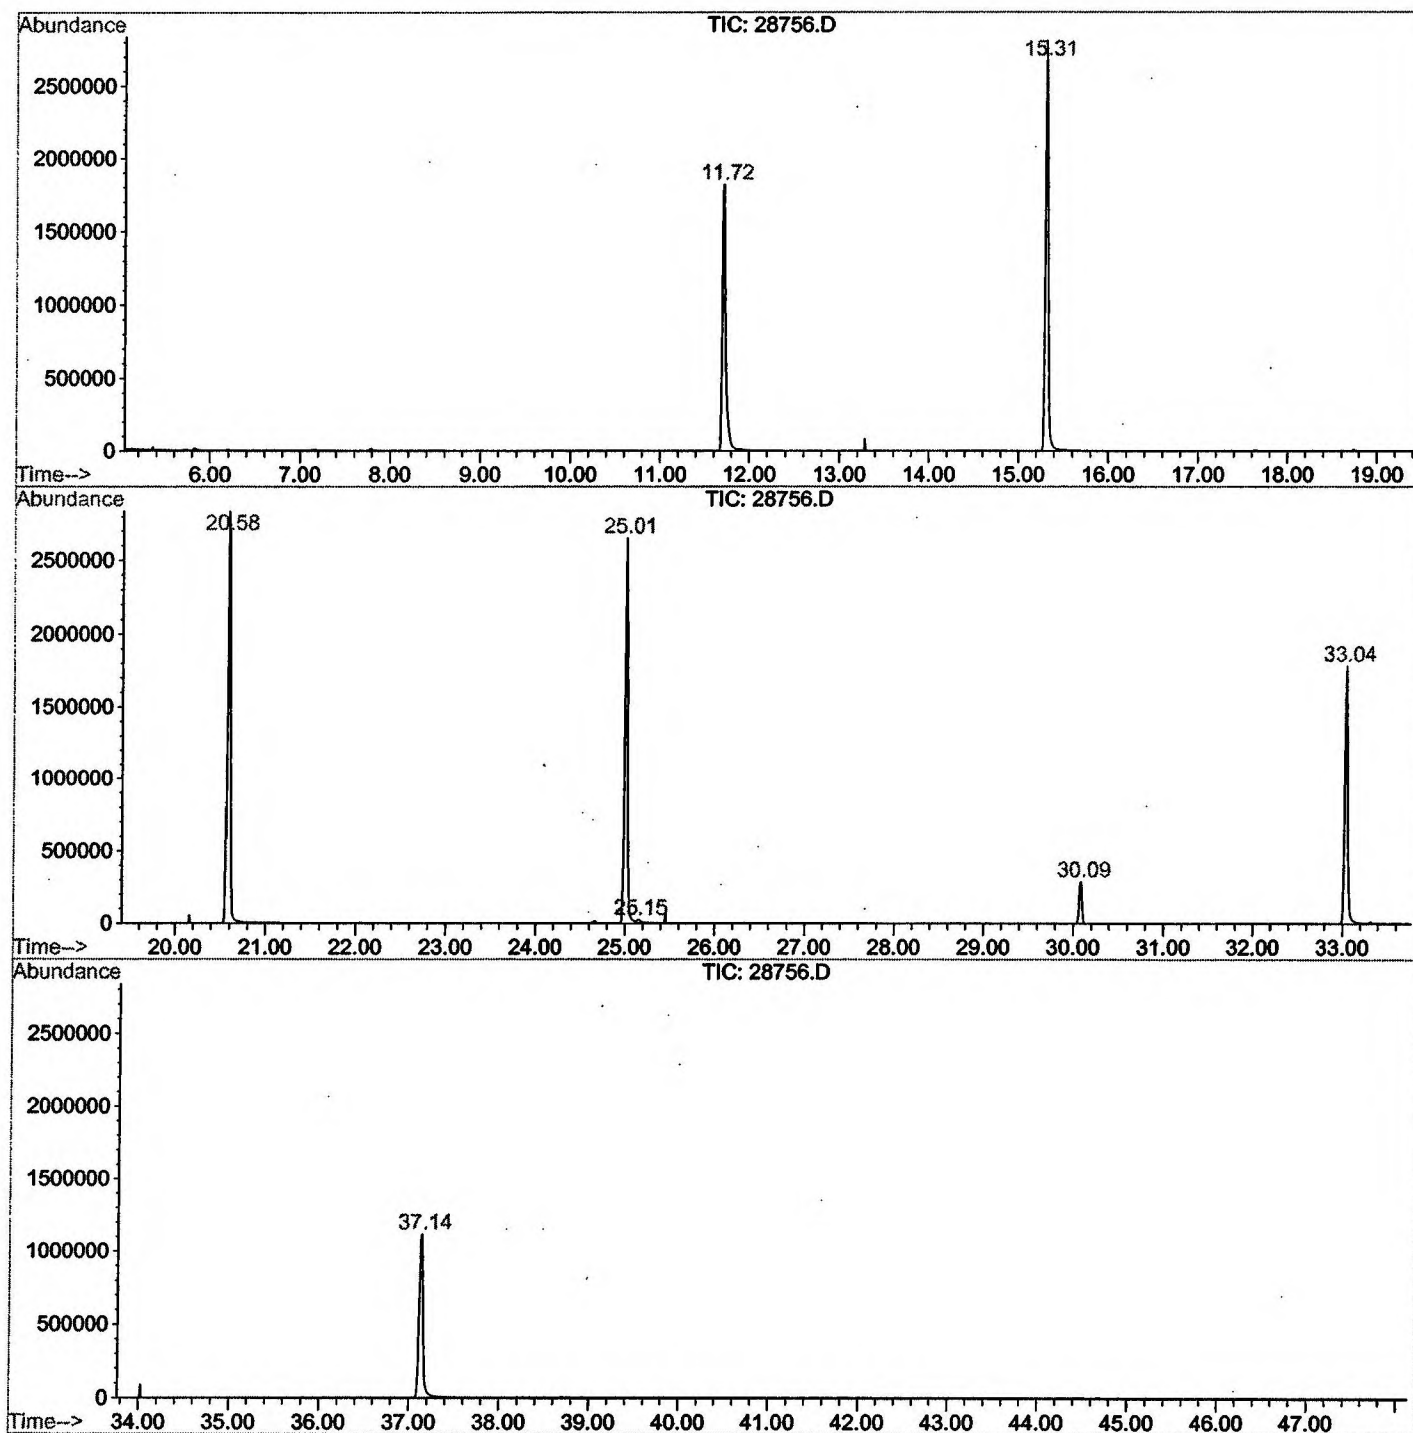

28756.D GCMS1126.M

Fri Dec 07 17:01:25 2001

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 6 Dec 2001 7:09 am
 Data File: C:\HPCHEM\1\DATA\DEC0501\28756.D
 Name: 11/26 gc/ms scan
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc

28756.D GCMS1126.M			Fri Dec 07 17:01:30 2001					