

Method 508 mod

Date Extracted 11/27/01

Page 1

ref

\$6CMS15952

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
✓ LB ✓		500 mL		1 mL	0.5 mL		1 mL		7			
✓ Ref ✓												
✓ 28800 ✓												
✓ 28801 ✓												
✓ 28802 ✓												
✓ 28855 ✓												
✓ 28856 ✓												
✓ 28857 ✓												
✓ 28858 ✓												
✓ 28859 ✓												
28263	re-extract											
28275												
28163												
not included in this batch												
Remarks 28855, 28857, and 28859 were very acidic → pH ≈ 1. Their pH was brought to 7 upon the addition of 11 mL 1M NaOH to each. Reviewed by, <u>JB 5/11/02</u> drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type <u>sep fun</u> Solv. lot# <u>V34E09</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V39400</u> STANDARD INT STD LOG# CALIBRATION REF/SPIKE <u>91759</u> MDL/MDRF Q. CHECK INT. STD. SURROGATE <u>6CMS 12601</u> LPC ENDRIN/DDT												

Analyst LF
Revision 4/12/01

Verified by _____

Reviewed by DN
Date 12/16/01

Sequence Name: C:\HPCHEM\1\SEQUENCE\DCE0601.S
 Comment: INST 209; 30Mx0.25umX0.50
 Operator: 209 GALOS
 Data Path: C:\HPCHEM\1\data\dec0601\
 Pre-Seq Cmd:
 Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP1	GCMS1126	
2 Sample	2	CAL25	GCMS1126	
3 Sample	10	REF	GCMS1126	11/24 gc/ms scan
4 Sample	5	28897	GCMS1126	11/28 gc/ms scan
5 Sample	6	28862	GCMS1126	11/28 gc/ms scan
6 Sample	7	28899	GCMS1126	11/28 gc/ms scan
7 Sample	8	28902	GCMS1126	11/28 gc/ms scan
8 Sample	23	28753A	GCMS1126	11/26 gc/ms scan
9 Sample	24	LBA —	GCMS1126	11/27 gc/ms scan
10 Sample	25	28263	GCMS1126	11/27 gc/ms scan
11 Sample	26	REFA	GCMS1126	11/27 gc/ms scan
12 Sample	27	28800	GCMS1126	11/27 gc/ms scan
13 Sample	28	28801	GCMS1126	11/27 gc/ms scan
14 Sample	29	28802	GCMS1126	11/27 gc/ms scan
15 Sample	30	28857	GCMS1126	11/27 gc/ms scan
16 Sample	31	28859	GCMS1126	11/27 gc/ms scan
17 Sample	32	28858	GCMS1126	11/27 gc/ms scan
18 Sample	33	28856	GCMS1126	11/27 gc/ms scan
19 Sample	34	28855	GCMS1126	11/27 gc/ms scan
20 Sample	35	LBB	GCMS1126	11/28 gc/ms scan
21 Sample	36	REFB	GCMS1126	11/28 gc/ms scan
22 Sample	37	28861	GCMS1126	11/28 gc/ms scan
23 Sample	38	28901	GCMS1126	11/28 gc/ms scan
24 Sample	1	DFTPP2	GCMS1126	
25 Sample	2	REFD	GCMS1126	11/24 ref
26 Sample	3	CAL40	GCMS1126	
27 Sample	4	28968	GCMS1126	11/28 gc/ms scan
28 Sample	5	28900	GCMS1126	11/28 gc/ms scan
29 Sample	6	28860	GCMS1126	11/28 gc/ms scan

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC0601\DFTPP2.D

Acq On : 7 Dec 2001 2:33 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

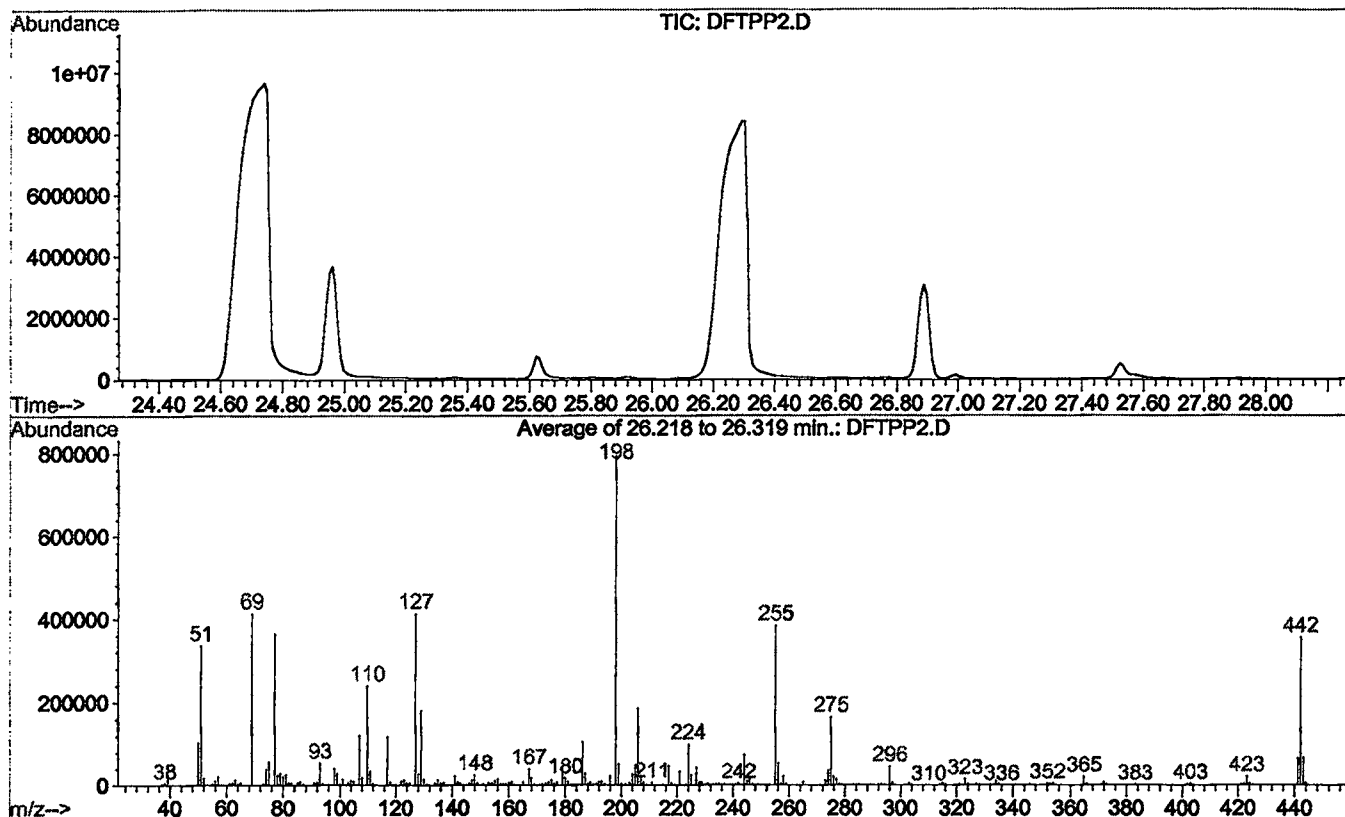

Spectrum Information: Average of 26.218 to 26.319 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	42.6	337569	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.2	414041	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	52.1	413209	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	792789	PASS
199	198	5	9	6.8	53550	PASS
275	198	10	30	20.9	165710	PASS
365	198	1	100	2.7	21493	PASS
441	443	0.01	100	97.5	66987	PASS
442	198	40	110	44.9	356043	PASS
443	442	17	23	19.3	68709	PASS