

Comments for Sample AD28800 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 12-16-2001 Time: 09:37:13

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Recoveries for 1 of the 43 compounds in the LCS Standard was above its acceptance range.

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 12/16/2001 Time: 09:37:53

Sample: AD28800
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 12/16/01 09:32 Ended: 12/16/01 09:32 Analyst: DLV
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr 2,4 DDD	TARGET	98%		5.0

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0601\28800.D

Vial: 27

Acq On : 7 Dec 2001 1:03 am

Operator: 209 GALOS

Sample : 11/27 gc/ms scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 11 11:24 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Nov 28 15:06:24 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.67	152	1005969	20.00	ug/l	-0.03
15) Naphthalene-d8	15.27	136	3768891	20.00	ug/l	-0.03
26) Acenaphthene-d10	20.55	164	1852414	20.00	ug/l	-0.02
42) Phenanthrene-d10	24.98	188	2773828	20.00	ug/l	-0.01
53) Chrysene-d12	33.01	240	1831914	20.00	ug/l	-0.02
59) Perylene-d12	37.11	264	1348466	20.00	ug/l	-0.01

System Monitoring Compounds

52) 2,4-DDD	30.06	235	161799	4.90	ug/mL	-0.01
Spiked Amount	5.000		Recovery	=	98.00%	

Target Compounds

					Qvalue
2) Pyridine	0.00	79	0	N.D.	
3) N-nitroso-dimethyl amine	5.21	74	366	N.D.	
4) Phenol	11.28	94	184	N.D.	
5) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
6) 2-Chlorophenol	0.00	128	0	N.D.	
7) 1,3-Dichlorobenzene	11.71	146	219	N.D.	
8) 1,4-Dichlorobenzene	11.71	146	219	N.D.	
9) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
10) 2-Methylphenol	0.00	108	0	N.D.	
11) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
12) 3&4-Methylphenol	0.00	108	0	N.D.	
13) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
14) Hexachloroethane	0.00	117	0	N.D.	
16) Nitrobenzene	0.00	77	0	N.D.	
17) Isophorone	0.00	82	0	N.D.	
18) 2-Nitrophenol	0.00	139	0	N.D.	
19) 2,4-Dimethylphenol	0.00	107	0	N.D.	
20) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
21) 2,4-Dichlorophenol	0.00	162	0	N.D.	
22) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
23) Naphthalene	15.33	128	2933	N.D.	
24) Hexachlorobutadiene	0.00	225	0	N.D.	
25) 4-Chloro-3-methylphenol	0.00	107	0	N.D.	
27) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
28) 2,4,6-Trichlorophenol	0.00	196	0	N.D.	

(#) = qualifier out of range (m) = manual integration

28800.D GCMS1126.M Tue Dec 11 14:38:42 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0601\28800.D

Vial: 27

Acq On : 7 Dec 2001 1:03 am

Operator: 209 GALOS

Sample : 11/27 gc/ms scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 11 11:24 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Nov 28 15:06:24 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
29) 2,4,5-Trichlorophenol	0.00	196	0	N.D.		
30) 2-Chloronaphthalene	0.00	162	0	N.D.		
31) Dimethylphthalate	0.00	163	0	N.D.		
32) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
33) Acenaphthylene	0.00	152	0	N.D.		
34) Acenaphthene	0.00	153	0	N.D.		
35) 2,4-Dinitrophenol	0.00	184	0	N.D.		
36) 4-Nitrophenol	21.03	65	377	N.D.		
37) 2,4-Dinitrotoluene	20.94	165	874	N.D.		
38) Diethylphthalate	22.08	149	3047	N.D.		
39) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
40) Fluorene	0.00	166	0	N.D.		
41) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
43) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.		
44) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
45) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
46) Hexachlorobenzene	0.00	284	0	N.D.		
47) Pentachlorophenol	0.00	266	0	N.D.		
48) Phenanthrene	25.04	178	527	N.D.		
49) Anthracene	25.04	178	527	N.D.		
50) Di-n-butylphthalate	26.99	149	9188	N.D.		
51) Fluoranthene	0.00	202	0	N.D.		
54) Pyrene	0.00	202	0	N.D.		
55) Butylbenzylphthalate	0.00	149	0	N.D.		
56) Benzo(a)anthracene	33.01	228	5506	N.D.		
57) Bis(2-ethylhexyl)phthalate	33.29	149	21722	N.D.		
58) Chrysene	33.01	228	5506	N.D.		
60) Di-n-Octylphthalate	0.00	149	0	N.D.		
61) Benzo(b)fluoranthene	36.05	252	752	N.D.		
62) Benzo(k)fluoranthene	36.05	252	752	N.D.		
63) Benzo(a)pyrene	36.92	252	242	N.D.		
64) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
65) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
66) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

28800.D GCMS1126.M Tue Dec 11 14:38:46 2001

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC0601\28800.D
 Acq On : 7 Dec 2001 1:03 am
 Sample : 11/27 gc/ms scan
 Misc :
 MS Integration Params: RTEINT.P
 Quant Time: Dec 11 11:24 2001

Vial: 27
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Nov 28 15:06:24 2001
 Response via : Initial Calibration

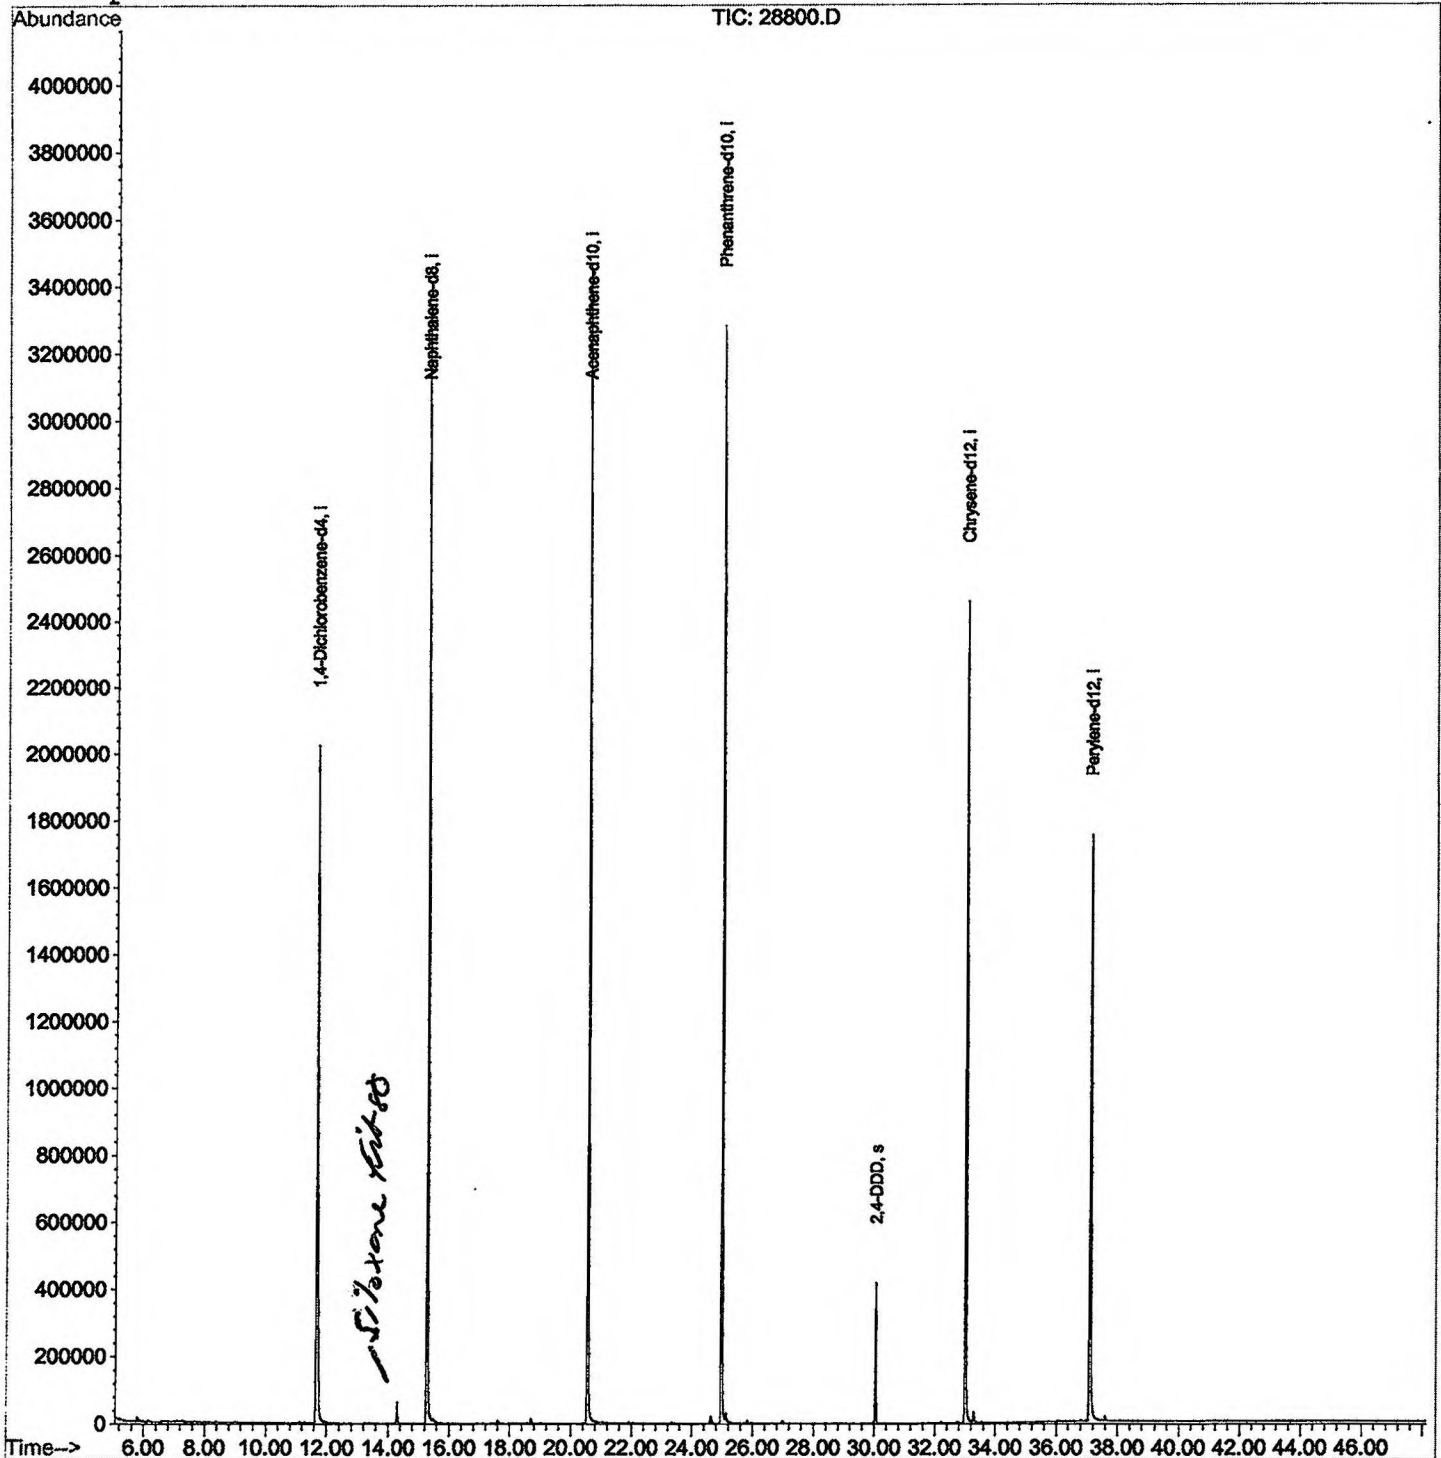

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC0601\28800.D

Vial: 27

Acq On : 7 Dec 2001 1:03 am

Operator: 209 GALOS

Sample : 11/27 gc/ms scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	11.667	716	721	740	rBV	2023753	5441420	72.06%	13.904%
2	14.302	1003	1008	1016	rVB	63700	122074	1.62%	0.312%
3	15.275	1108	1114	1132	rBV	3316804	7082995	93.81%	18.098%
4	20.554	1682	1689	1705	rBV	3468494	7550762	100.00%	19.293%
5	24.979	2164	2171	2183	rBV2	3282518	7285640	96.49%	18.616%
6	25.125	2183	2187	2202	rVB	29375	95464	1.26%	0.244%
7	30.046	2717	2723	2735	rBV	417880	861937	11.42%	2.202%
8	33.011	3039	3046	3062	rBV2	2455903	5762217	76.31%	14.723%
9	37.106	3484	3492	3511	rBV2	1747633	4933850	65.34%	12.607%


Sum of corrected areas: 39136359

28800.D GCMS1126.M

Wed Dec 12 11:32:50 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC0601\28800.D
Operator : 209 GALOS
Acquired : 7 Dec 2001 1:03 am using AcqMethod GCMS1126
Instrument : GC/MS 209
Sample Name: 11/27 gc/ms scan
Misc Info :
Vial Number: 27
Quant File :GCMS1126.RES (RTE Integrator)

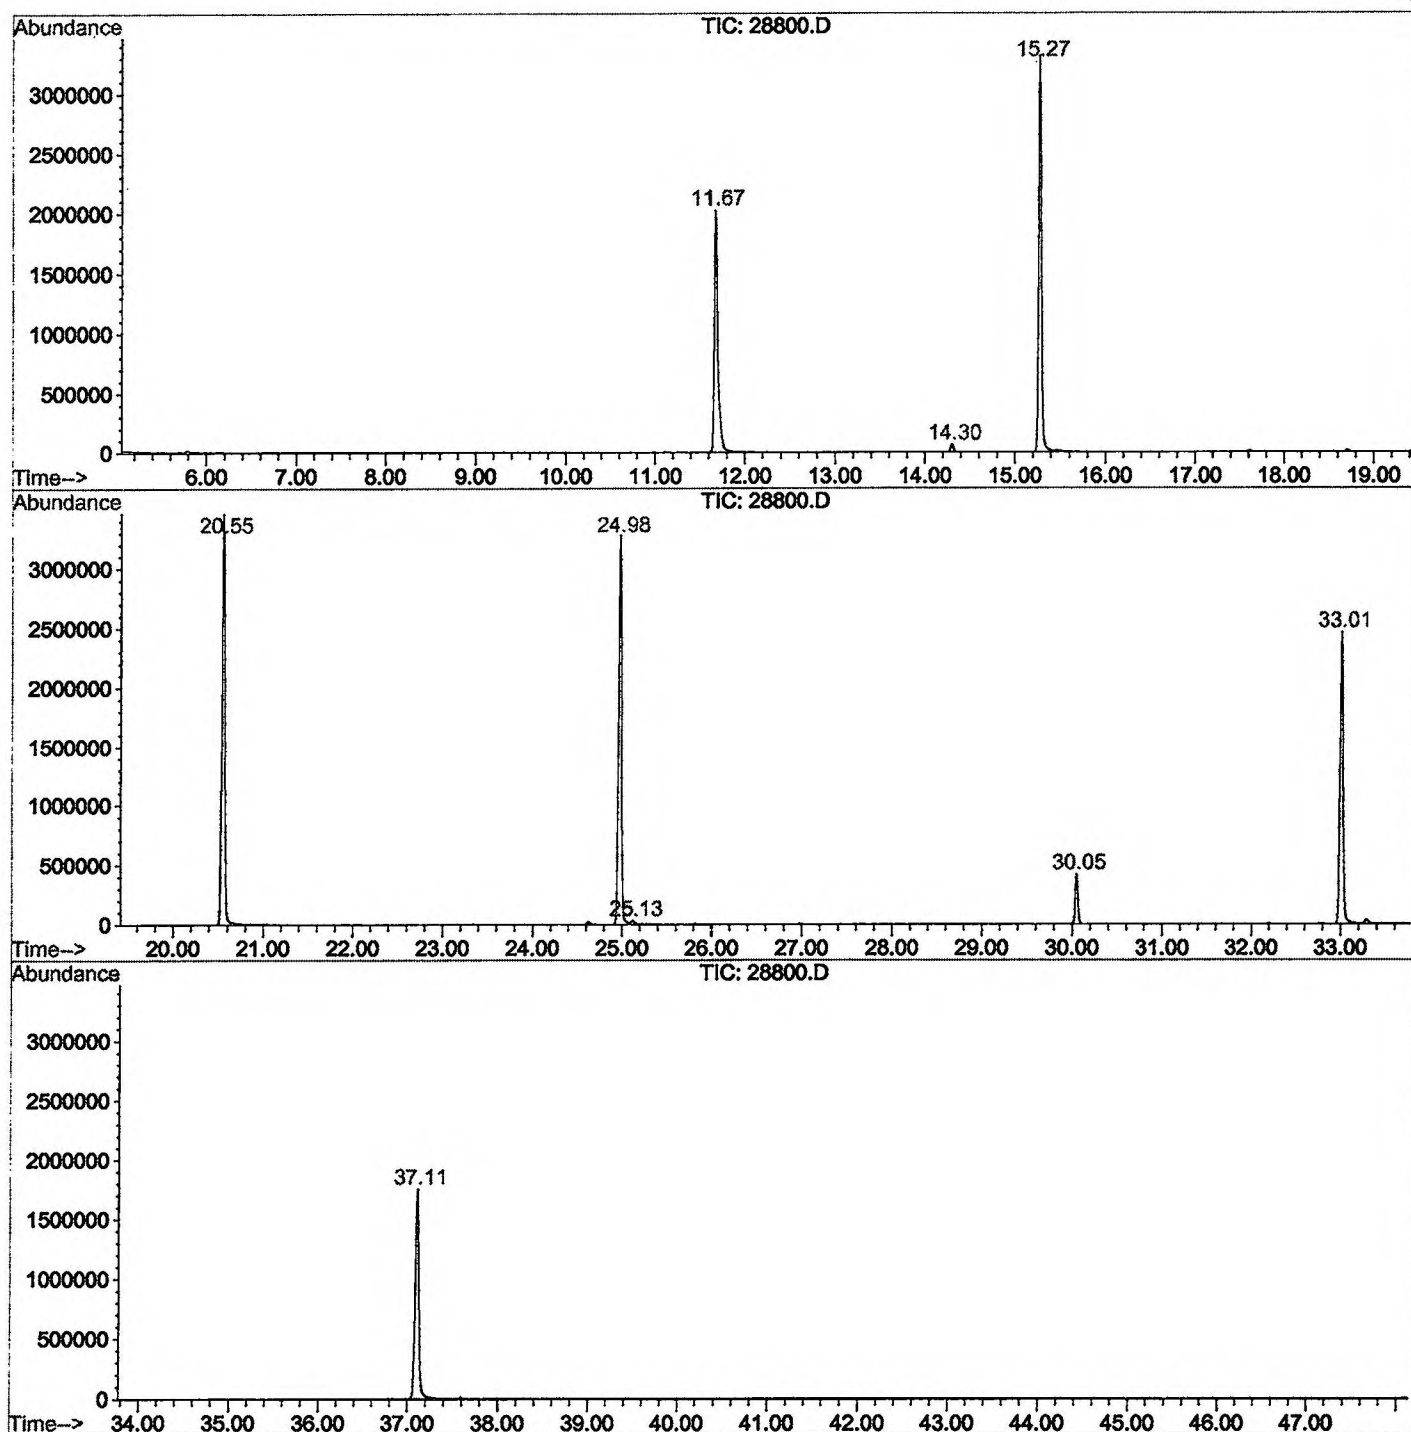

28800.D GCMS1126.M

Wed Dec 12 11:32:56 2001

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 7 Dec 2001 1:03 am
 Data File: C:\HPCHEM\1\DATA\DEC0601\28800.D
 Name: 11/27 gc/ms scan
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc

28800.D GCMS1126.M		Wed Dec 12	11:33:01	2001				