

Comments for Sample AD28801 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 12-16-2001 Time: 09:40:53

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds, except for the presence of bis(2-Ethylhexyl)phthalate at an estimated level of 0.37 ug/L. It is also present in the Laboratory BLank at 0.30 ug/L. Recoveries for 1 of the 43 compounds in the LCS Standard was above its acceptance range.

*collected 11/26
reported 12/15/01*

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 12/16/2001 Time: 09:41:53

Sample: AD28801
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 12/16/01 09:37 Ended: 12/16/01 09:37 Analyst: DLV
Result source: manual entry
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr. 2,4 DDD	TARGET	104%		5.0

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0601\28801.D

Vial: 28

Acq On : 7 Dec 2001 2:01 am

Operator: 209 GALOS

Sample : 11/27 gc/ms scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 11 11:25 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Nov 28 15:06:24 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	11.67	152	1007475	20.00	ug/l	-0.03
15) Naphthalene-d8	15.28	136	3829146	20.00	ug/l	-0.03
26) Acenaphthene-d10	20.56	164	1868000	20.00	ug/l	-0.02
42) Phenanthrene-d10	24.97	188	2781421	20.00	ug/l	-0.02
53) Chrysene-d12	33.01	240	1930958	20.00	ug/l	-0.02
59) Perylene-d12	37.10	264	1425461	20.00	ug/l	-0.02

System Monitoring Compounds

52) 2,4-DDD	30.05	235	171878	5.19	ug/mL	-0.02
Spiked Amount	5.000		Recovery	=	103.80%	

Target Compounds

				Qvalue
2) Pyridine	0.00	79	0	N.D.
3) N-nitroso-dimethyl amine	5.22	74	324	N.D.
4) Phenol	11.05	94	177	N.D.
5) bis(2-Chloroethyl) ether	0.00	93	0	N.D.
6) 2-Chlorophenol	0.00	128	0	N.D.
7) 1,3-Dichlorobenzene	0.00	146	0	N.D.
8) 1,4-Dichlorobenzene	0.00	146	0	N.D.
9) 1,2-Dichlorobenzene	0.00	146	0	N.D.
10) 2-Methylphenol	12.29	108	100	N.D.
11) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
12) 3&4-Methylphenol	0.00	108	0	N.D.
13) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
14) Hexachloroethane	0.00	117	0	N.D.
16) Nitrobenzene	0.00	77	0	N.D.
17) Isophorone	13.56	82	381	N.D.
18) 2-Nitrophenol	0.00	139	0	N.D.
19) 2,4-Dimethylphenol	0.00	107	0	N.D.
20) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.
21) 2,4-Dichlorophenol	0.00	162	0	N.D.
22) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
23) Naphthalene	15.32	128	1667	N.D.
24) Hexachlorobutadiene	0.00	225	0	N.D.
25) 4-Chloro-3-methylphenol	0.00	107	0	N.D.
27) Hexachlorocyclopentadiene	0.00	237	0	N.D.
28) 2,4,6-Trichlorophenol	0.00	196	0	N.D.

(#) = qualifier out of range (m) = manual integration

28801.D GCMS1126.M Tue Dec 11 14:39:35 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0601\28801.D

Vial: 28

Acq On : 7 Dec 2001 2:01 am

Operator: 209 GALOS

Sample : 11/27 gc/ms scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 11 11:25 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Nov 28 15:06:24 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
29) 2,4,5-Trichlorophenol	0.00	196	0	N.D.	
30) 2-Chloronaphthalene	0.00	162	0	N.D.	
31) Dimethylphthalate	0.00	163	0	N.D.	
32) 2,6-Dinitrotoluene	0.00	165	0	N.D. d	
33) Acenaphthylene	0.00	152	0	N.D.	
34) Acenaphthene	0.00	153	0	N.D.	
35) 2,4-Dinitrophenol	0.00	184	0	N.D.	
36) 4-Nitrophenol	0.00	65	0	N.D.	
37) 2,4-Dinitrotoluene	20.96	165	463	N.D.	
38) Diethylphthalate	22.07	149	2228	N.D.	
39) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
40) Fluorene	0.00	166	0	N.D.	
41) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
43) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.	
44) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
45) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
46) Hexachlorobenzene	0.00	284	0	N.D.	
47) Pentachlorophenol	0.00	266	0	N.D.	
48) Phenanthrene	25.05	178	265	N.D.	
49) Anthracene	25.05	178	265	N.D.	
50) Di-n-butylphthalate	26.98	149	22200	N.D.	
51) Fluoranthene	0.00	202	0	N.D.	
54) Pyrene	0.00	202	0	N.D.	
55) Butylbenzylphthalate	31.49	149	372	N.D.	
56) Benzo(a)anthracene	33.00	228	4909	N.D.	
57) Bis(2-ethylhexyl)phthalate	33.29	149	43041	0.37 ug/l	100
58) Chrysene	33.00	228	4909	N.D.	
60) Di-n-Octylphthalate	35.03	149	408	N.D.	
61) Benzo(b)fluoranthene	0.00	252	0	N.D.	
62) Benzo(k)fluoranthene	0.00	252	0	N.D.	
63) Benzo(a)pyrene	37.10	252	5760	N.D.	
64) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
65) Dibenzo(a,h)anthracene	0.00	278	0	N.D.	
66) Benzo(g,h,i)perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration

28801.D GCMS1126.M

Tue Dec 11 14:39:40 2001

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC0601\28801.D
Acq On : 7 Dec 2001 2:01 am
Sample : 11/27 gc/ms scan
Misc :
MS Integration Params: RTEINT.P
Quant Time: Dec 11 11:25 2001

Vial: 28
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Nov 28 15:06:24 2001
Response via : Initial Calibration

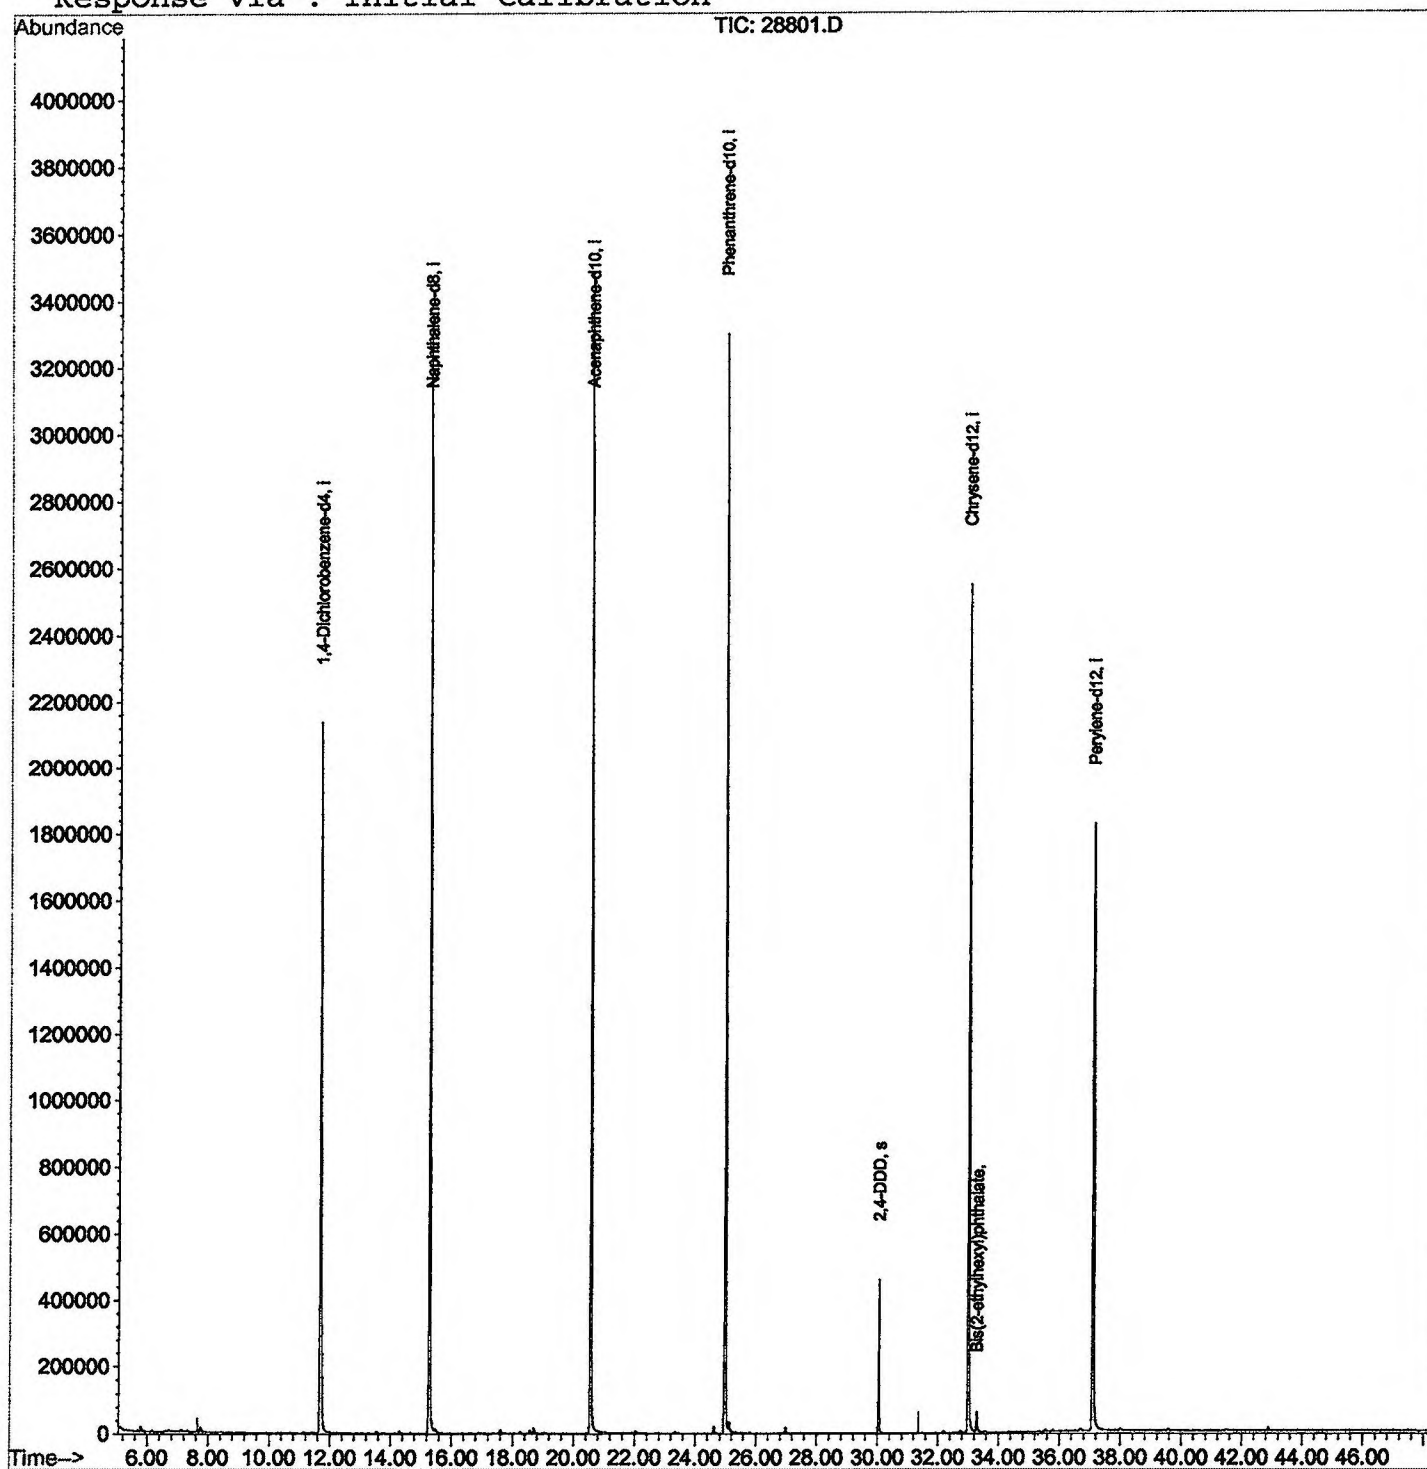

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC0601\28801.D

Vial: 28

Acq On : 7 Dec 2001 2:01 am

Operator: 209 GALOS

Sample : 11/27 gc/ms scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	11.669	717	722	750	rBV	2135635	5460505	72.47%	13.674%
2	15.277	1109	1115	1133	rBV	3335479	7176081	95.24%	17.970%
3	20.556	1683	1690	1698	rBV	3487094	7534500	100.00%	18.867%
4	24.972	2165	2171	2183	rBV2	3298541	7316228	97.10%	18.320%
5	25.118	2183	2187	2194	rVB2	29243	81264	1.08%	0.203%
6	30.048	2719	2724	2736	rBV	458791	916004	12.16%	2.294%
7	33.014	3038	3047	3071	rBV2	2545375	6102289	80.99%	15.281%
8	33.289	3072	3077	3089	rVB	59712	156604	2.08%	0.392%
9	37.108	3484	3493	3513	rBV	1820458	5191188	68.90%	12.999%


Sum of corrected areas: 39934663

28801.D GCMS1126.M

Wed Dec 12 11:33:18 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC0601\28801.D
Operator : 209 GALOS
Acquired : 7 Dec 2001 2:01 am using AcqMethod GCMS1126
Instrument : GC/MS 209
Sample Name: 11/27 gc/ms scan
Misc Info :
Vial Number: 28
Quant File :GCMS1126.RES (RTE Integrator)

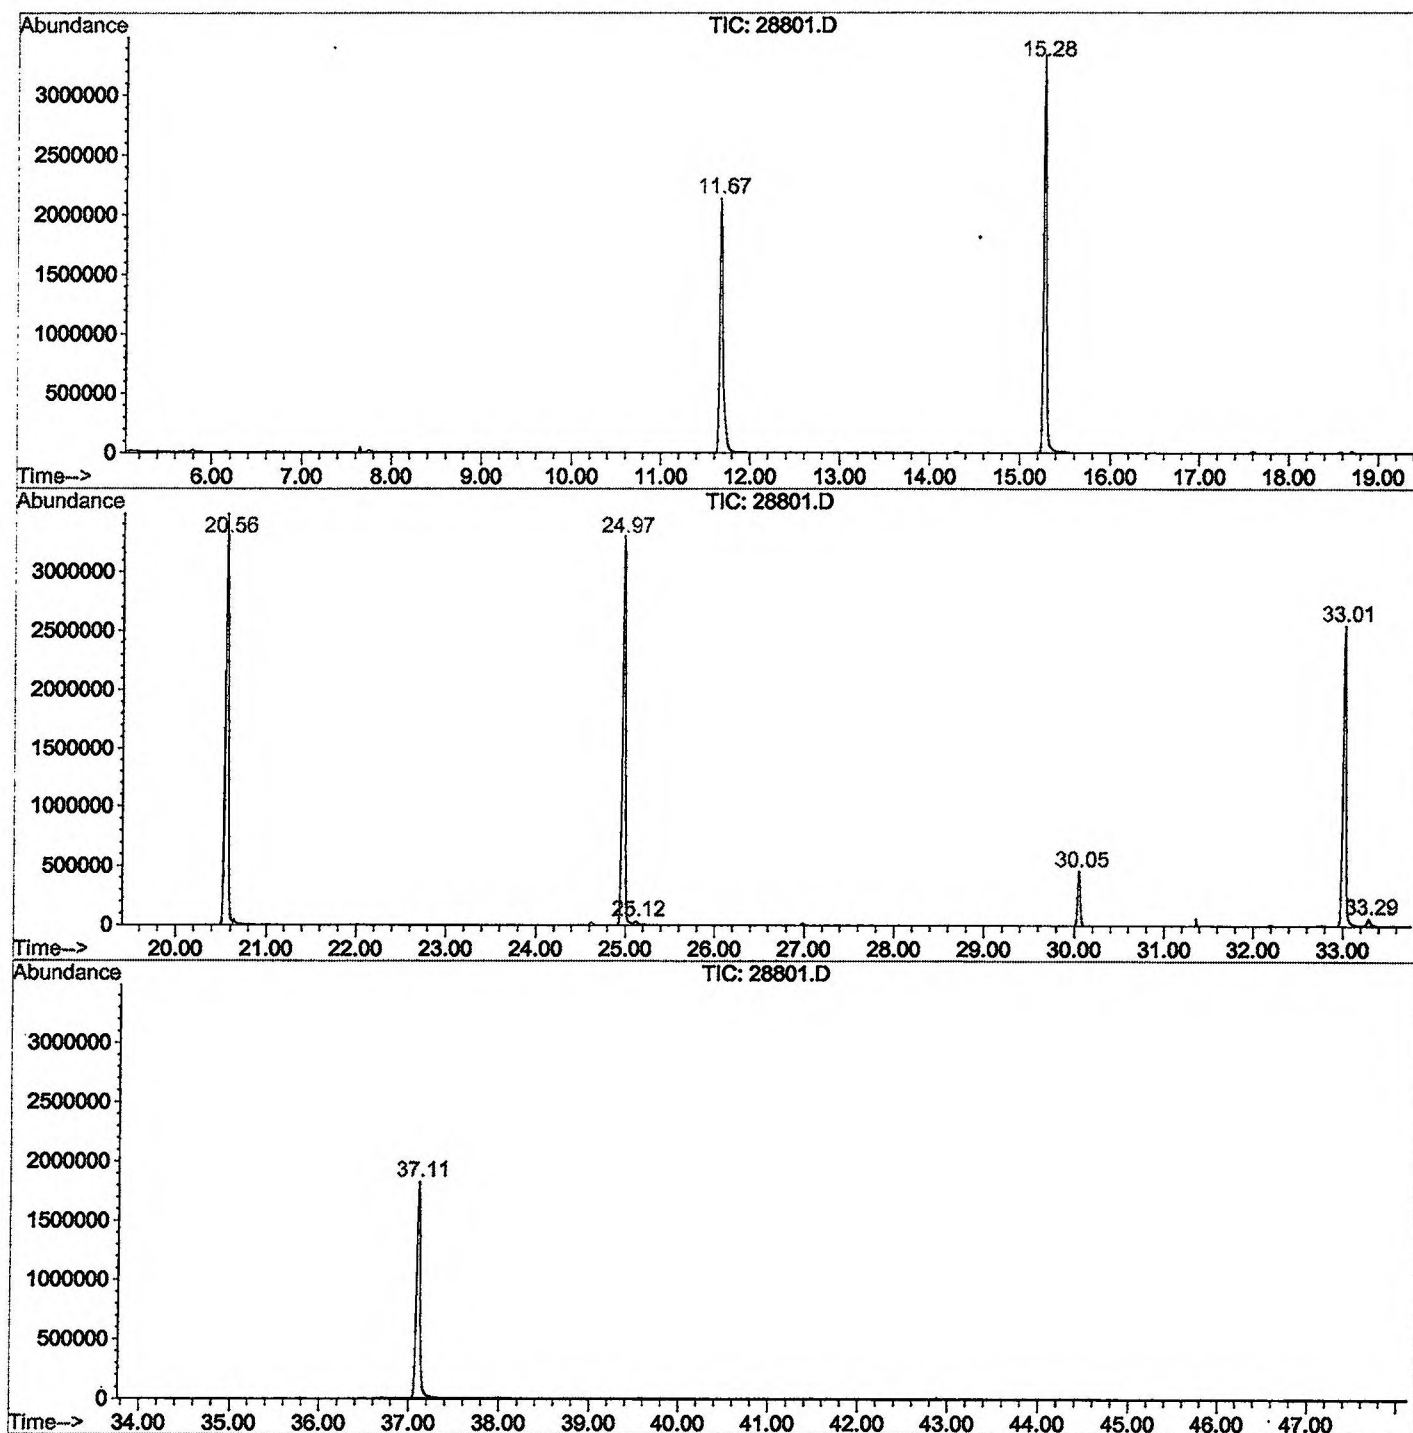

28801.D GCMS1126.M

Wed Dec 12 11:33:24 2001

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 7 Dec 2001 2:01 am
 Data File: C:\HPCHEM\1\DATA\DEC0601\28801.D
 Name: 11/27 gc/ms scan
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc

28801.D GCMS1126.M	Wed Dec 12	11:33:29	2001					