

Comments for Sample AD28855 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 12-16-2001 Time: 09:54:07

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds, except for the presence of bis(2-Ethylhexyl)phthalate at an estimated level of 0.35 ug/L. It is also present in the Laboratory BLank at 0.30 ug/L. Recoveries for 1 of the 43 compounds in the LCS Standard was above its acceptance range. This sample was received with a pH of less than 2.

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 12/16/2001 Time: 09:54:11

Sample: AD28855
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 12/12/01 11:28 Ended: 12/12/01 11:28 Analyst: MG
Result source: manual entry
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		104		5.0

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0601\28855.D

Vial: 34

Acq On : 7 Dec 2001 7:53 am

Operator: 209 GALOS

Sample : 11/27 gc/ms scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 11 12:08 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Nov 28 15:06:24 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.68	152	1128408	20.00	ug/l	-0.02
15) Naphthalene-d8	15.27	136	4302572	20.00	ug/l	-0.03
26) Acenaphthene-d10	20.55	164	2103647	20.00	ug/l	-0.02
42) Phenanthrene-d10	24.98	188	3025749	20.00	ug/l	-0.01
53) Chrysene-d12	33.01	240	1856324	20.00	ug/l	-0.02
59) Perylene-d12	37.10	264	1151610	20.00	ug/l	-0.02

System Monitoring Compounds

52) 2,4-DDD	30.05	235	187332	5.20	ug/mL	-0.02
Spiked Amount	5.000		Recovery	=	104.00%	

Target Compounds

					Qvalue
2) Pyridine	0.00	79	0	N.D.	
3) N-nitroso-dimethyl amine	5.22	74	375	N.D.	
4) Phenol	10.78	94	129	N.D.	
5) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
6) 2-Chlorophenol	0.00	128	0	N.D.	
7) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
8) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
9) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
10) 2-Methylphenol	12.35	108	102	N.D.	
11) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
12) 3&4-Methylphenol	0.00	108	0	N.D.	
13) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
14) Hexachloroethane	0.00	117	0	N.D.	
16) Nitrobenzene	12.93	77	108	N.D.	
17) Isophorone	13.56	82	669	N.D.	
18) 2-Nitrophenol	0.00	139	0	N.D.	
19) 2,4-Dimethylphenol	0.00	107	0	N.D.	
20) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
21) 2,4-Dichlorophenol	0.00	162	0	N.D.	
22) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
23) Naphthalene	15.33	128	1617	N.D.	
24) Hexachlorobutadiene	0.00	225	0	N.D.	
25) 4-Chloro-3-methylphenol	0.00	107	0	N.D.	
27) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
28) 2,4,6-Trichlorophenol	0.00	196	0	N.D.	

(#)=qualifier out of range (m)=manual integration

28855.D GCMS1126.M Tue Dec 11 15:37:38 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0601\28855.D

Vial: 34

Acq On : 7 Dec 2001 7:53 am

Operator: 209 GALOS

Sample : 11/27 gc/ms scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 11 12:08 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Nov 28 15:06:24 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
29) 2,4,5-Trichlorophenol	0.00	196	0	N.D.	
30) 2-Chloronaphthalene	0.00	162	0	N.D.	
31) Dimethylphthalate	0.00	163	0	N.D.	
32) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
33) Acenaphthylene	0.00	152	0	N.D.	
34) Acenaphthene	0.00	153	0	N.D.	
35) 2,4-Dinitrophenol	0.00	184	0	N.D.	
36) 4-Nitrophenol	21.21	65	188	N.D.	
37) 2,4-Dinitrotoluene	21.09	165	205	N.D.	
38) Diethylphthalate	22.07	149	2457	N.D.	
39) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
40) Fluorene	0.00	166	0	N.D.	
41) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
43) 4,6-Dinitro-2-methylphenol	0.00	198	0	N.D.	
44) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
45) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
46) Hexachlorobenzene	0.00	284	0	N.D.	
47) Pentachlorophenol	0.00	266	0	N.D.	
48) Phenanthrene	24.99	178	1204	N.D.	
49) Anthracene	24.99	178	1204	N.D.	
50) Di-n-butylphthalate	26.99	149	22025	N.D.	
51) Fluoranthene	0.00	202	0	N.D.	
54) Pyrene	0.00	202	0	N.D.	
55) Butylbenzylphthalate	31.50	149	341	N.D.	
56) Benzo(a)anthracene	33.01	228	4287	N.D.	
57) Bis(2-ethylhexyl)phthalate	33.29	149	39630	0.35 ug/l	99
58) Chrysene	33.01	228	4287	N.D.	
60) Di-n-Octylphthalate	35.08	149	513	N.D.	
61) Benzo(b)fluoranthene	0.00	252	0	N.D.	
62) Benzo(k)fluoranthene	0.00	252	0	N.D.	
63) Benzo(a)pyrene	37.10	252	5058	N.D.	
64) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
65) Dibenz(a,h)anthracene	0.00	278	0	N.D.	
66) Benzo(g,h,i)perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration

28855.D GCMS1126.M

Tue Dec 11 15:37:43 2001

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC0601\28855.D
Acq On : 7 Dec 2001 7:53 am
Sample : 11/27 gc/ms scan
Misc :
MS Integration Params: RTEINT.P
Quant Time: Dec 11 12:08 2001

Vial: 34
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Nov 28 15:06:24 2001
Response via : Initial Calibration

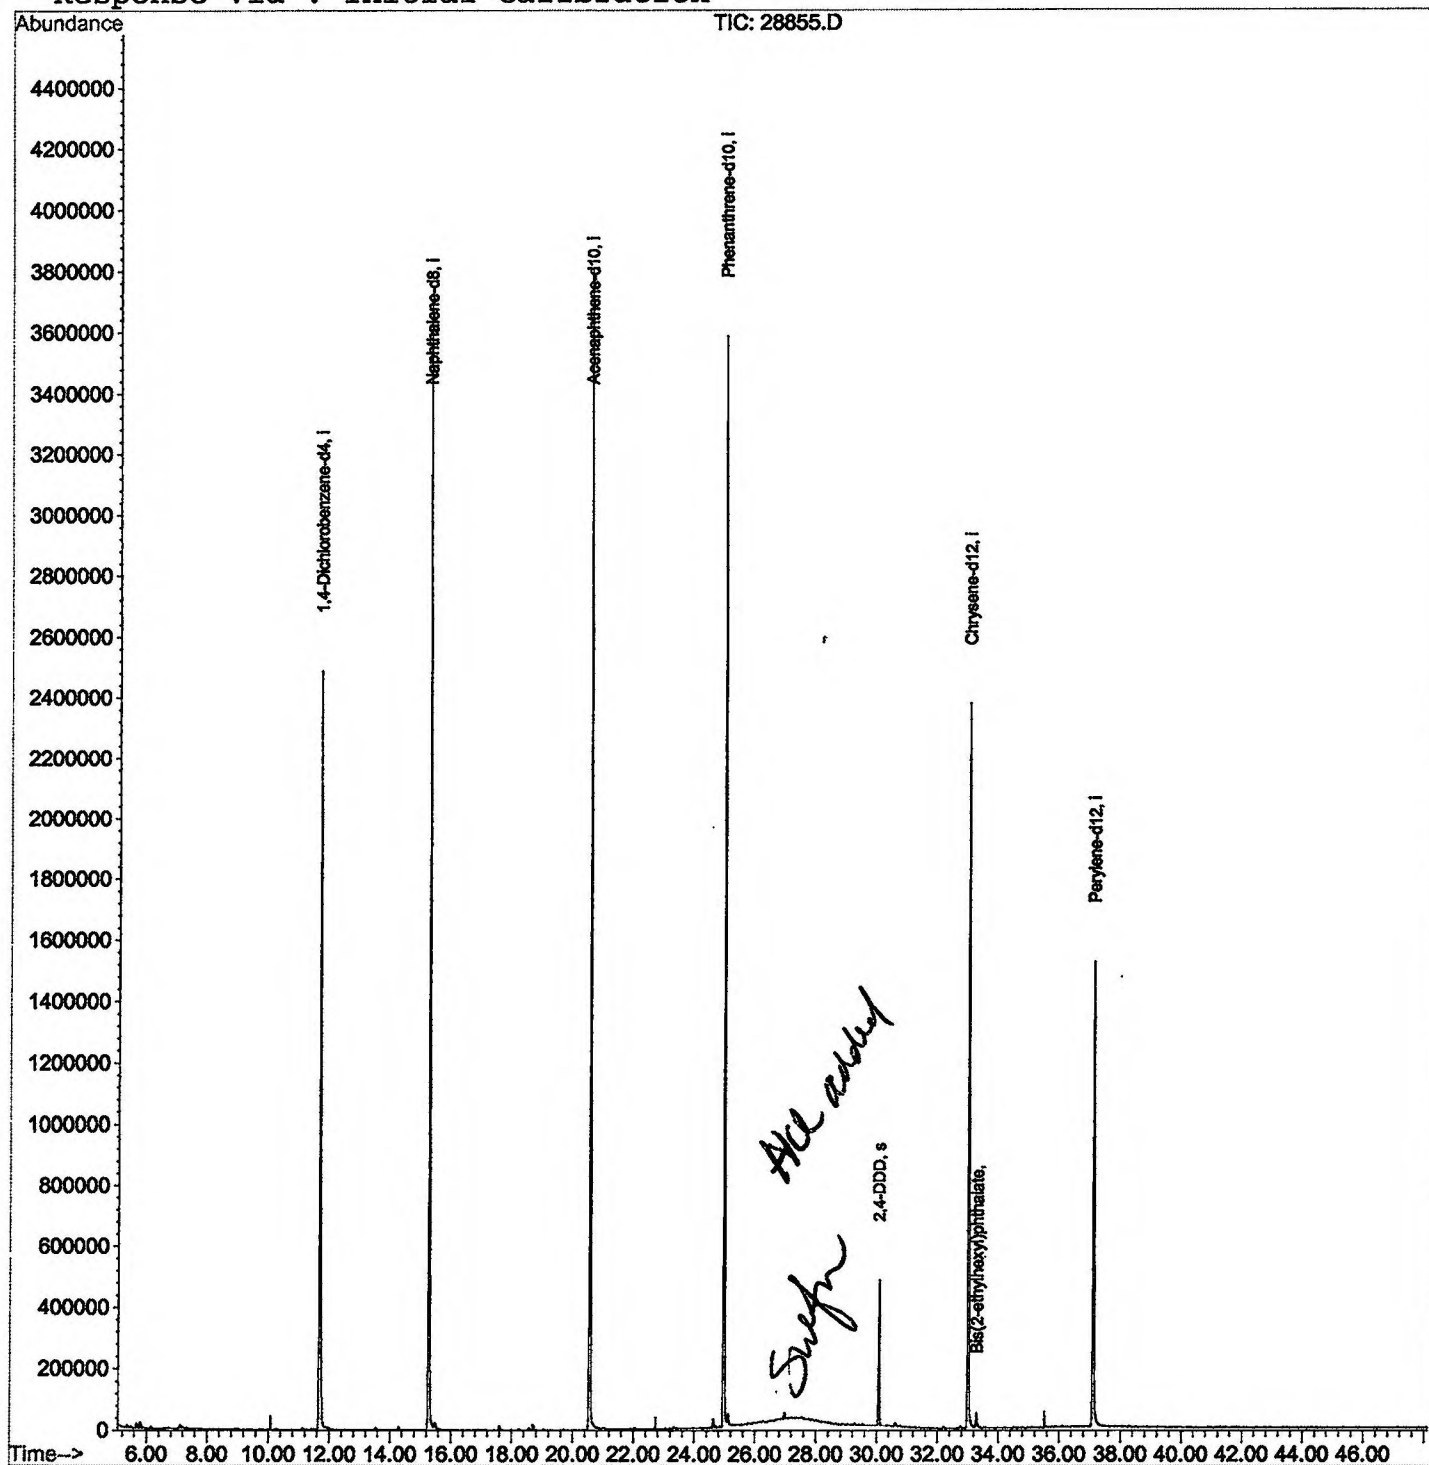

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC0601\28855.D
 Acq On : 7 Dec 2001 7:53 am
 Sample : 11/27 gc/ms scan
 Misc :
 MS Integration Params: LSCINT.P

Vial: 34
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	11.675	716	722	741	rBV	2485561	6104420	71.14%	14.448%
2	15.274	1108	1114	1132	rBV	3697859	8050465	93.82%	19.054%
3	20.553	1682	1689	1705	rBV	3810550	8581063	100.00%	20.310%
4	24.978	2164	2171	2182	rBV2	3576966	7978685	92.98%	18.884%
5	25.115	2183	2186	2193	rVB	35050	90816	1.06%	0.215%
6	30.054	2718	2724	2733	rVB	469477	1005372	11.72%	2.380%
7	33.010	3038	3046	3063	rBV2	2373679	5806747	67.67%	13.744%
8	33.295	3071	3077	3087	rBV	46339	129161	1.51%	0.306%
9	37.105	3483	3492	3508	rBV2	1515220	4503455	52.48%	10.659%

Sum of corrected areas: 42250184

28855.D GCMS1126.M Wed Dec 12 11:35:35 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC0601\28855.D
Operator : 209 GALOS
Acquired : 7 Dec 2001 7:53 am using AcqMethod GCMS1126
Instrument : GC/MS 209
Sample Name: 11/27 gc/ms scan
Misc Info :
Vial Number: 34
Quant File :GCMS1126.RES (RTE Integrator)

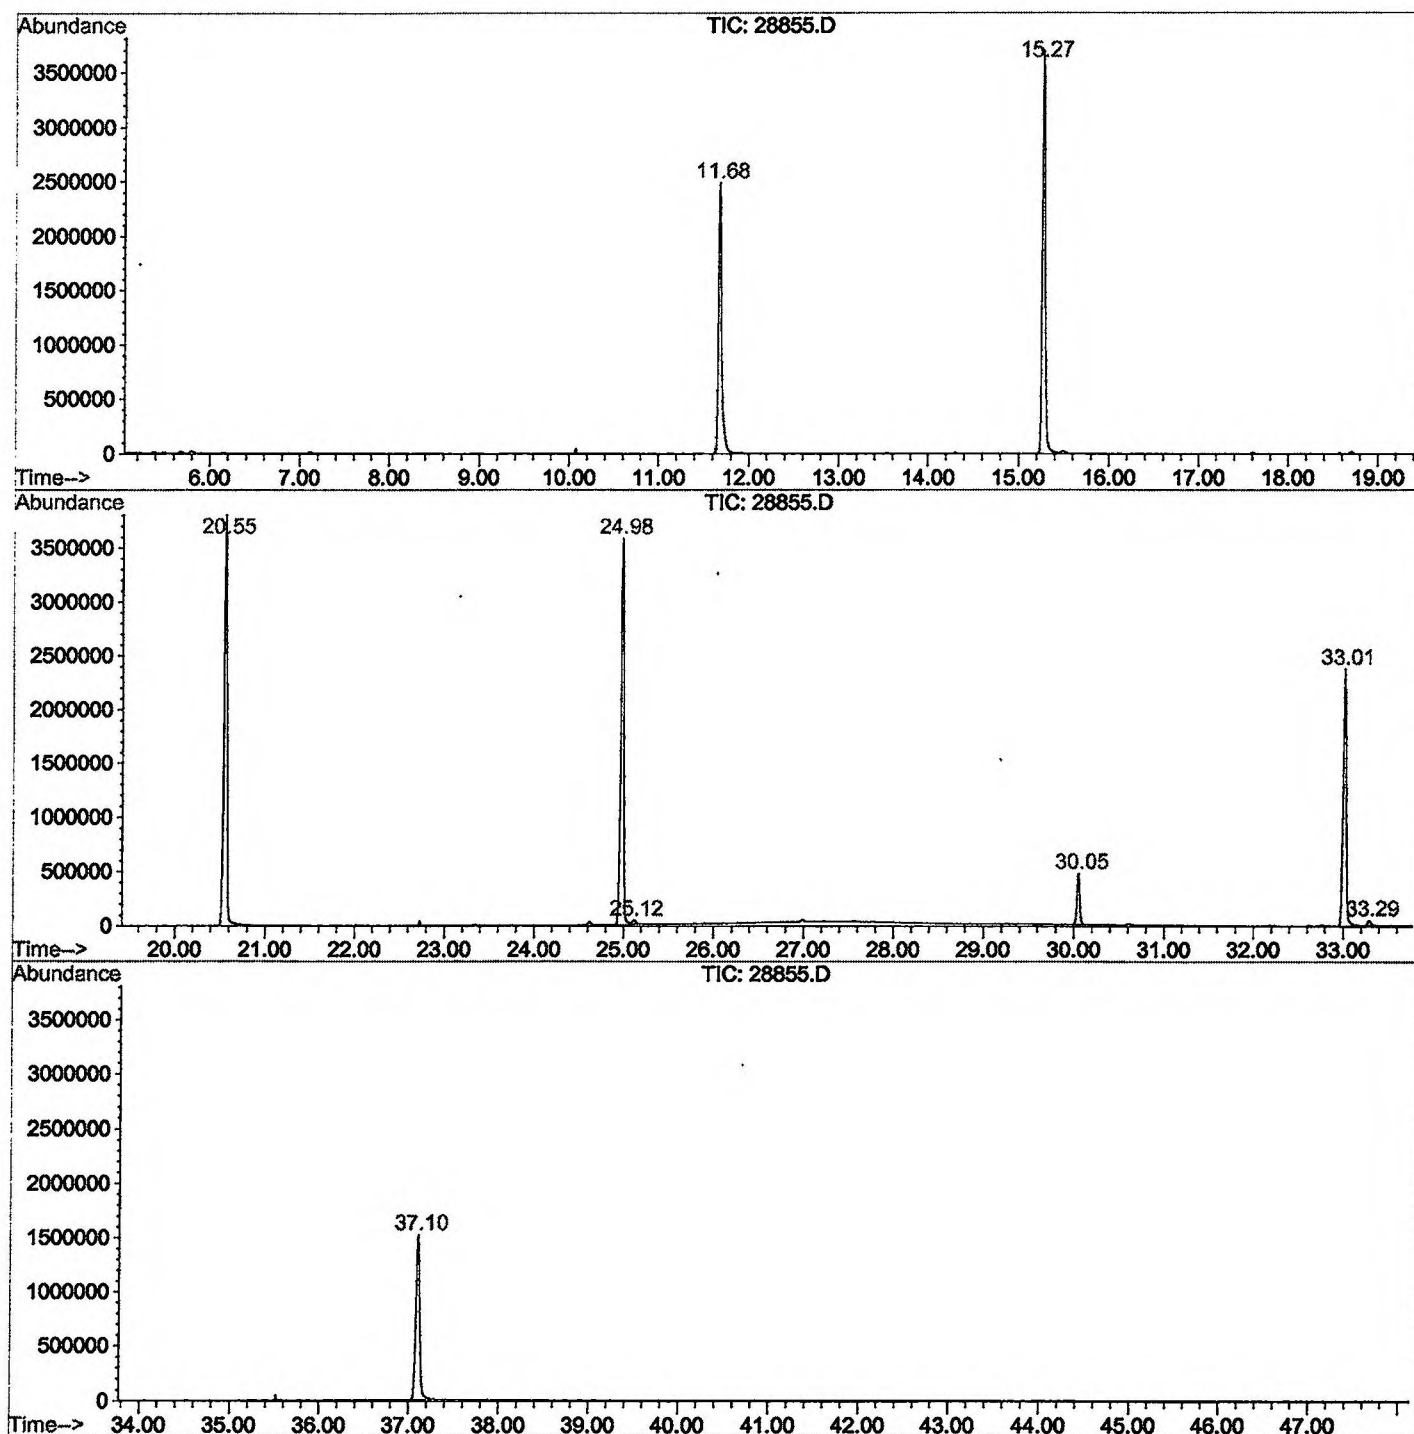

28855.D GCMS1126.M

Wed Dec 12 11:35:40 2001

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 7 Dec 2001 7:53 am
 Data File: C:\HPCHEM\1\DATA\DEC0601\28855.D
 Name: 11/27 gc/ms scan
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc

28855.D GCMS1126.M			Wed Dec 12 11:35:45 2001					