

Method 508 test

Date Extracted 1/28/01

Page

GCMS

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
	<u>CO</u>	<u>500ul</u>		<u>1ul</u>			<u>2ul</u>					
	<u>air peak</u>				<u>1ul</u>							
	<u>air ch</u>											
	<u>RT 100</u>											
	<u>SPK 1232</u>											
<u>28318</u>	<u>spike peak</u>											
<u>28318</u>	<u>spike dup peak</u>											
<u>28320</u>	<u>spike 101</u>											
<u>28320</u>	<u>spike dup peak</u>											
<u>28323</u>	<u>spike oil</u>											
<u>28323</u>	<u>spike dup ch</u>											
<u>28319</u>	<u>sample</u>											
<u>28320</u>												
<u>28321</u>												
<u>28322</u>												
<u>28323</u>												
<u>28324</u>												
<u>28342</u>												
<u>28348</u>												
<u>28349</u>												
<u>28350</u>												
Remarks Reviewed by, <u>CB 5/11/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type - <u>sp. peak</u> Solv. lot# NaCl lot# Na2SO4 lot#												
STANDARD	INT STD LOG#											
CALIBRATION												
REF/SPIKE												
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE												
LPC												
ENDRIN/DDT												

Analyst AD/MN
revision 4/12/01

Verified by

Reviewed by
Date 1/15/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\DEC2801.S

Comment: 208

Operator: GALOS

Data Path: C:\HPCHEM\1\DATA\dec2801\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	NP112701	
2	Sample	2	LB	NP112701	gcms unknown 11/28
3	Sample	3	28850	NP112701	gcms unknown 11/28
4	Sample	4	28319	NP112701	gcms unknown 11/28
5	Sample	5	28847	NP112701	gcms unknown 11/28
6	Sample	6	28848	NP112701	gcms unknown 11/28
7	Sample	7	28849	NP112701	gcms unknown 11/28
8	Sample	8	28323	NP112701	gcms unknown 11/28
9	Sample	9	28320	NP112701	gcms unknown 11/28
10	Sample	10	28324	NP112701	gcms unknown 11/28
11	Sample	11	28321	NP112701	gcms unknown 11/28
12	Sample	12	28322	NP112701	gcms unknown 11/28

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC2801\DFTPP.D

Acq On : 28 Dec 2001 7:54 am

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP112701.M (RTE Integrator)


Title : 208 625/TCLP calibration table

Vial: 1

Operator: GALOS

Inst : GC/MS Ins

Multiplr: 1.00

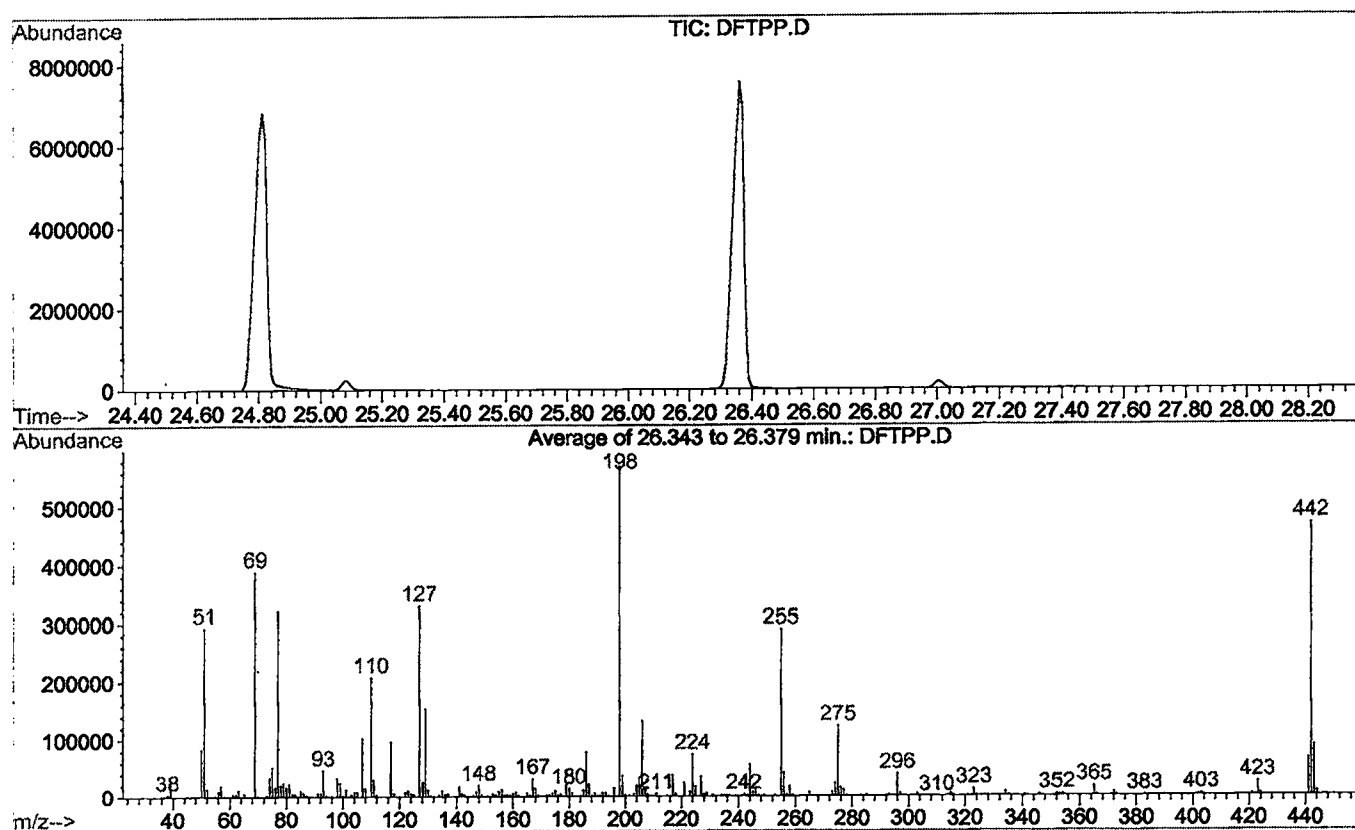

Spectrum Information: Average of 26.343 to 26.379 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	51.4	293184	PASS
68	69	0.00	2	0.1	439	PASS
69	198	0.00	100	68.3	389544	PASS
70	69	0.00	2	0.5	1813	PASS
127	198	40	60	58.0	330957	PASS
197	198	0.00	1	0.1	353	PASS
198	198	100	100	100.0	570688	PASS
199	198	5	9	6.6	37775	PASS
275	198	10	30	21.7	123739	PASS
365	198	1	99	3.2	18255	PASS
441	443	1	99	74.6	66526	PASS
442	198	40	110	82.4	469978	PASS
443	442	17	23	19.0	89221	PASS

DFTPP.D NP112701.M

Mon Dec 31 09:46:10 2001