

Comments for Sample AD28969 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 12-15-2001 Time: 09:15:18

A GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds, except for the presence of bis(2-Ethylhexyl)phthalate at an estimated level of 0.41 ug/L. It is also present in the Laboratory Blank at 0.41 ug/L. Recoveries for 5 of the 43 compounds in the LCS Standard were above their acceptance ranges.

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 12/15/2001 Time: 09:15:20

Sample: AD28969
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 12/15/01 09:13 Ended: 12/15/01 09:13 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Scan 24 BBL	PARCET (1144)			8.0

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0701\28969.D

Vial: 14

Acq On : 8 Dec 2001 3:37 am

Operator: 209 GALOS

Sample : 11/29 gc/ms scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 12 14:51 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Nov 28 15:06:24 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.67	152	845969	20.00	ug/l	-0.02
10) Naphthalene-d8	15.27	136	3240298	20.00	ug/l	-0.03
17) Acenaphthene-d10	20.55	164	1642541	20.00	ug/l	-0.02
29) Phenanthrene-d10	24.98	188	2338941	20.00	ug/l	-0.01
38) Chrysene-d12	33.01	240	1468338	20.00	ug/l	-0.02
44) Perylene-d12	37.10	264	845848	20.00	ug/l	-0.01

System Monitoring Compounds

37) 2,4-DDD	30.05	235	161579	5.80	ug/mL	-0.02
Spiked Amount	5.000		Recovery	=	116.00%	

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) N-nitroso-dimethyl amine	5.13	74	110	N.D.		
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.		
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.		
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	13.57	82	183	N.D.		
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	15.34	128	844	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-Chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	21.02	165	264	N.D.		
25) Diethylphthalate	22.08	149	1078	N.D.		
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		

(#)=qualifier out of range (m)=manual integration

28969.D GCMS1126.M

Thu Dec 13 15:37:27 2001

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC0701\28969.D

Vial: 14

Acq On : 8 Dec 2001 3:37 am

Operator: 209 GALOS

Sample : 11/29 gc/ms scan

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 12 14:51 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Nov 28 15:06:24 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	
32) Hexachlorobenzene	0.00	284	0	N.D.	
33) Phenanthrene	24.98	178	1012	N.D.	
34) Anthracene	24.98	178	1012	N.D.	
35) Di-n-butylphthalate	26.99	149	33958	N.D.	
36) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	31.50	149	1837	N.D.	
41) Benzo(a)anthracene	33.01	228	3703	N.D.	
42) Bis(2-ethylhexyl)phthalate	33.29	149	36805	0.41 ug/l	99
43) Chrysene	33.01	228	3703	N.D.	
45) Di-n-Octylphthalate	35.04	149	566	N.D.	
46) Benzo(b)fluoranthene	0.00	252	0	N.D.	
47) Benzo(k)fluoranthene	0.00	252	0	N.D.	
48) Benzo(a)pyrene	37.10	252	3947	N.D.	
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.	
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration

28969.D GCMS1126.M

Thu Dec 13 15:37:31 2001

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC0701\28969.D
Acq On : 8 Dec 2001 3:37 am
Sample : 11/29 gc/ms scan
Misc :
MS Integration Params: RTEINT.P
Quant Time: Dec 12 14:51 2001

Vial: 14
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Thu Dec 13 14:40:46 2001
Response via : Initial Calibration

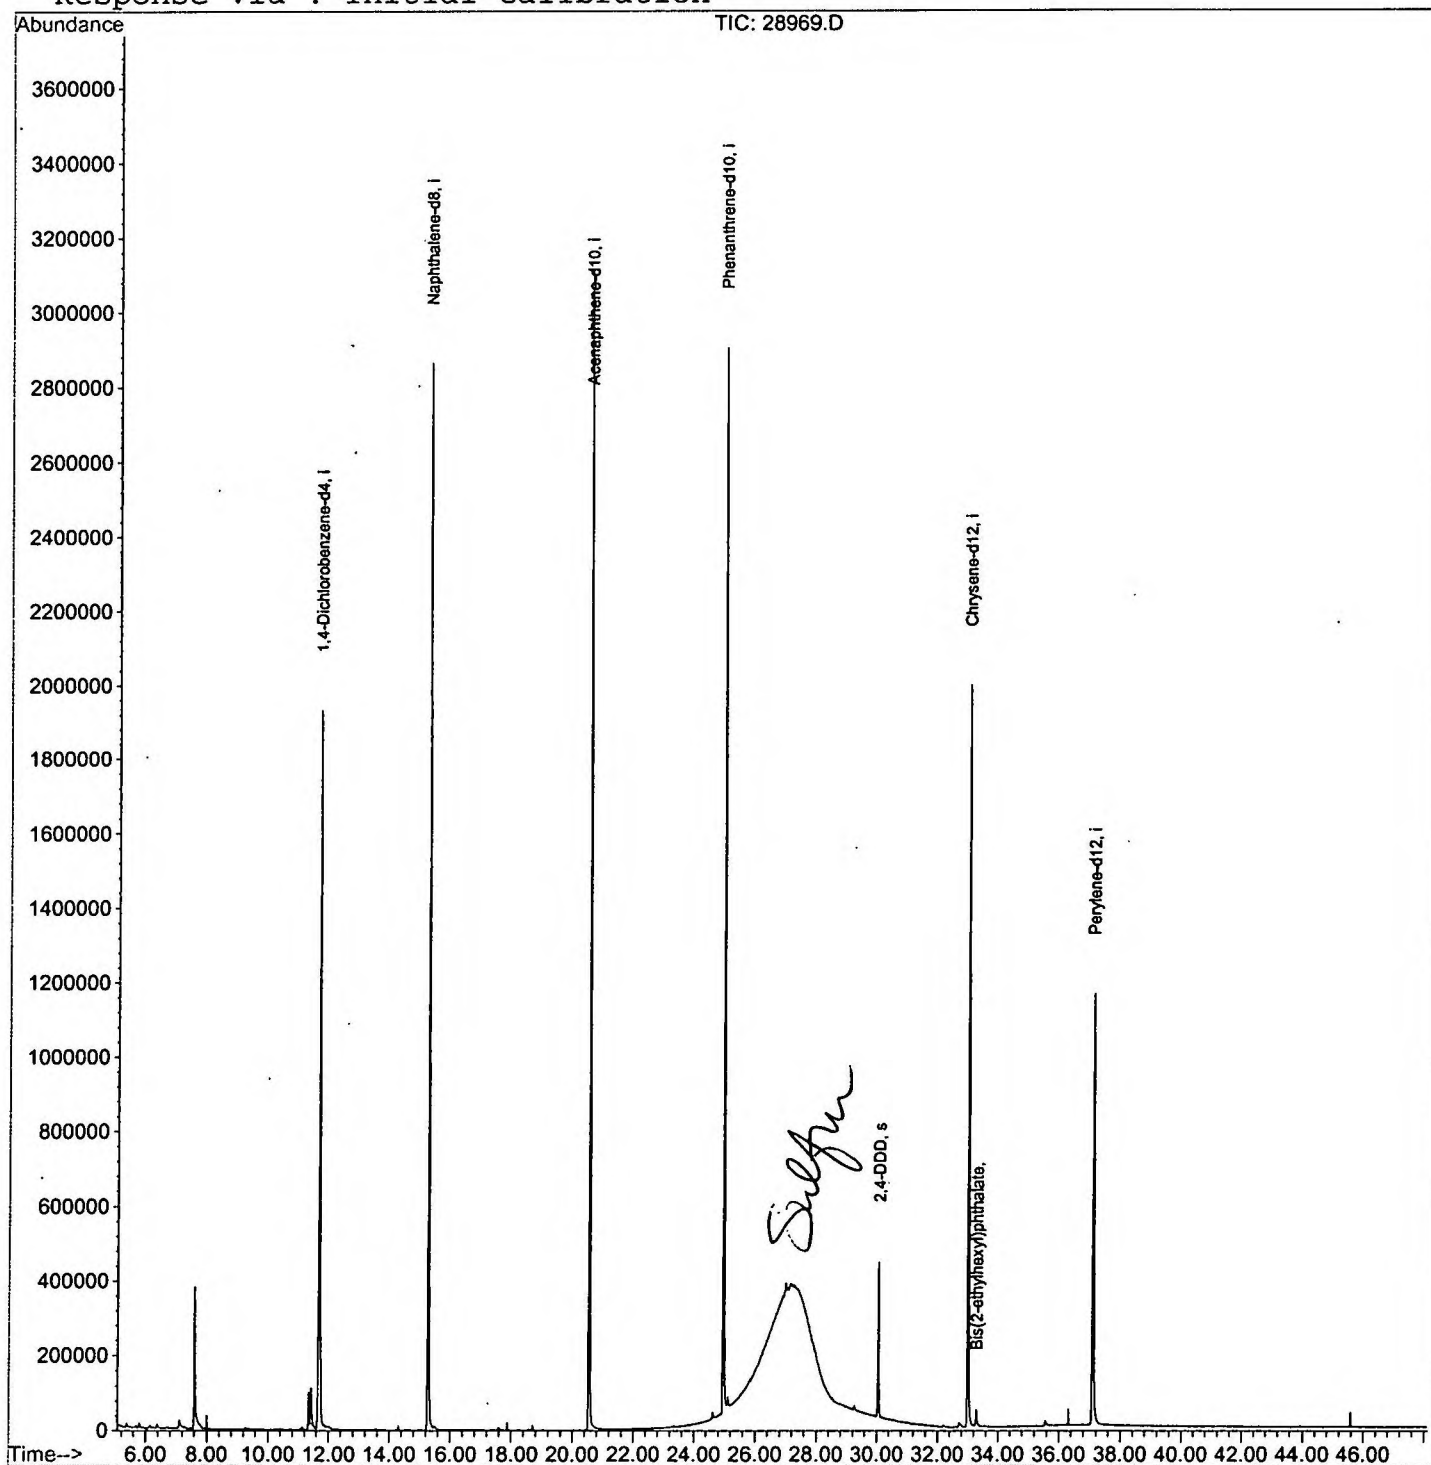

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC0701\28969.D

Acq On : 8 Dec 2001 3:37 am

Sample : 11/29 gc/ms scan

Misc :

MS Integration Params: LSCINT.P

Vial: 14

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.599	274	278	301	rBV	379334	968201	14.34%	2.809%
2	11.344	681	686	691	rBV	100743	231631	3.43%	0.672%
3	11.427	691	695	704	rVB	105220	269973	4.00%	0.783%
4	11.675	715	722	740	rBV	1928973	4916950	72.81%	14.267%
5	15.273	1109	1114	1132	rBV	2862528	6082906	90.07%	17.650%
6	20.552	1683	1689	1705	rBV	3115173	6753426	100.00%	19.595%
7	24.977	2164	2171	2182	rBV2	2861848	6233448	92.30%	18.087%
8	25.115	2183	2186	2194	rVB	26473	78280	1.16%	0.227%
9	30.054	2719	2724	2732	rVB	416607	891375	13.20%	2.586%
10	33.010	3039	3046	3068	rBV2	1991247	4620780	68.42%	13.407%
11	33.285	3072	3076	3086	rVB	44205	121897	1.80%	0.354%
12	37.104	3484	3492	3513	rBV2	1155049	3295670	48.80%	9.562%


Sum of corrected areas: 34464537

28969.D GCMS1126.M

Thu Dec 13 10:28:21 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC0701\28969.D
 Operator : 209 GALOS
 Acquired : 8 Dec 2001 3:37 am using AcqMethod GCMS1126
 Instrument : GC/MS 209
 Sample Name: 11/29 gc/ms scan
 Misc Info :
 Vial Number: 14
 Quant File :GCMS1126.RES (RTE Integrator)

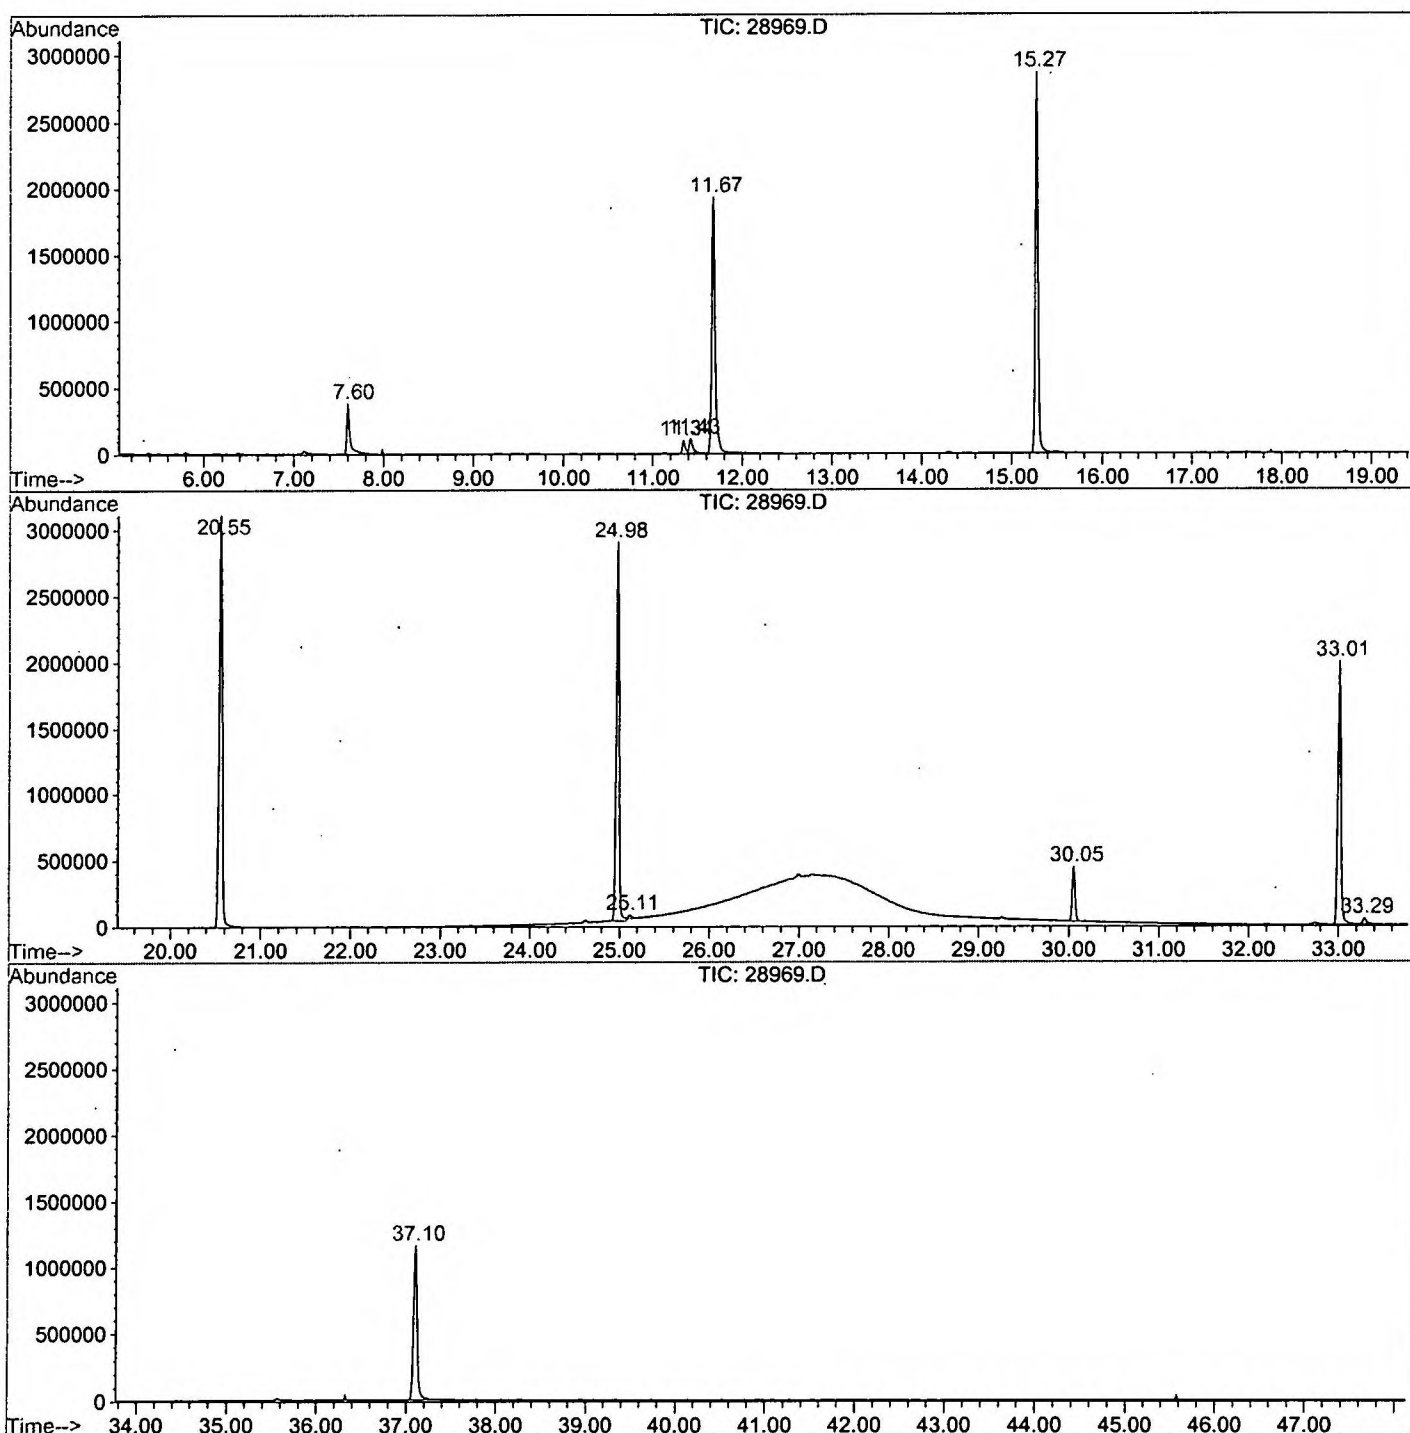

28969.D GCMS1126.M

Thu Dec 13 10:28:27 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC0701\28969.D.
 Acq On : 8 Dec 2001 3:37 am
 Sample : 11/29 gc/ms scan
 Misc :
 MS Integration Params: LSCINT.P


Vial: 14
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 Silane, tetramethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.60	3.94 ug/l	968201	1,4-Dichlorobenzene-d4	11.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Silane, tetramethyl-	88	C4H12Si	000075-76-3	25
2		N-Ethylformamide	73	C3H7NO	000627-45-2	9
3		Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	9
4		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

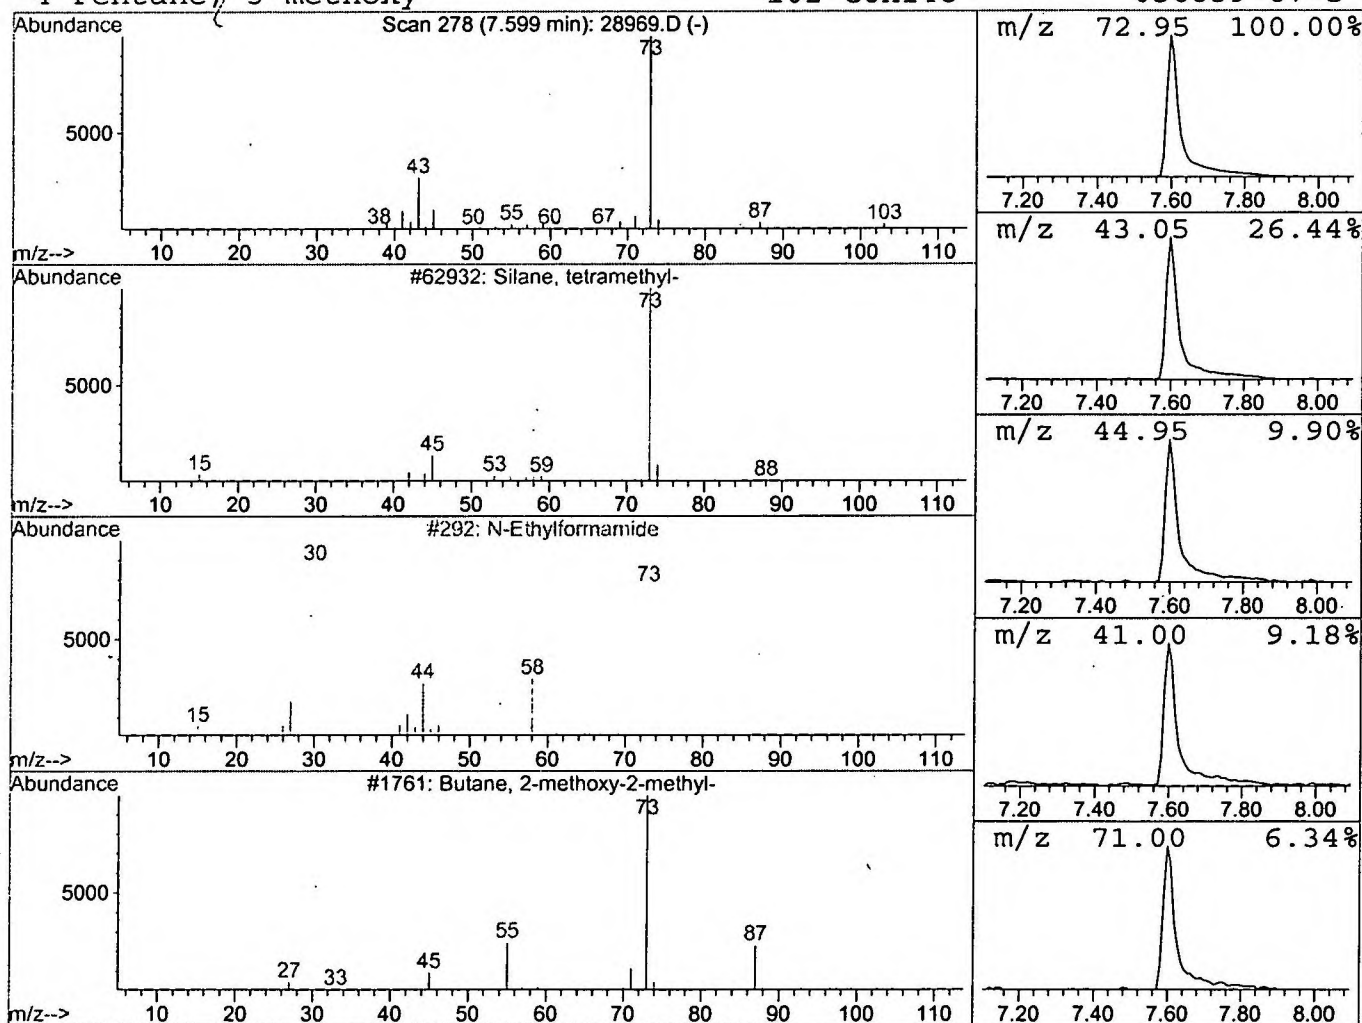

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC0701\28969.D
Acq On : 8 Dec 2001 3:37 am
Sample : 11/29 gc/ms scan
Misc :
MS Integration Params: LSCINT.P










Vial: 14
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 2 2-Propanol, 1-(2-methoxy-1-met Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.34	0.94 ug/l	231631	1,4-Dichlorobenzene-d4	11.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Propanol, 1-(2-methoxy-1-methylet	148	C7H16O3	020324-32-7	90
2			2-Butanol, 3,3'-oxybis-	162	C8H18O3	054305-61-2	64
3			2-Propanol, 1,1'-oxybis-	134	C6H14O3	000110-98-5	56
4			1-Propanol, 2-(2-hydroxypropoxy) -	134	C6H14O3	000106-62-7	53

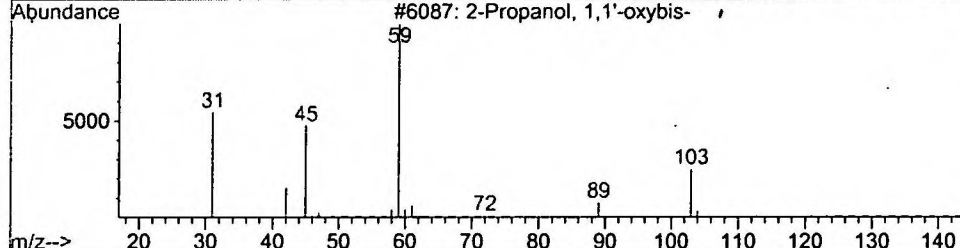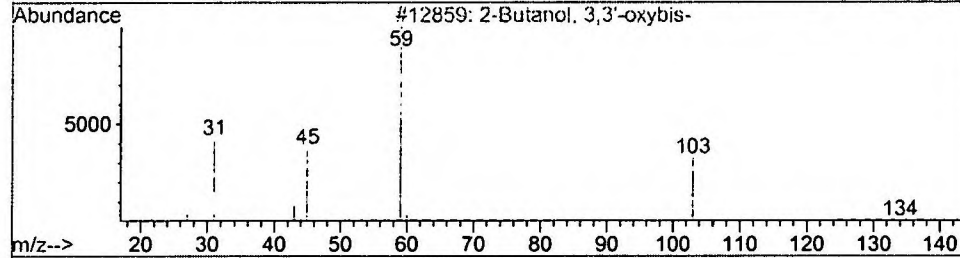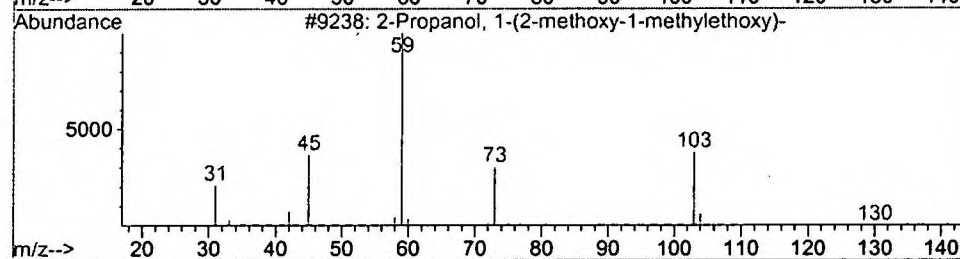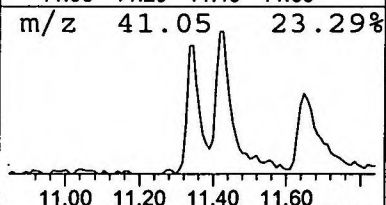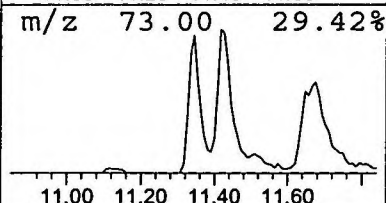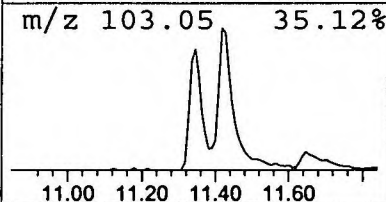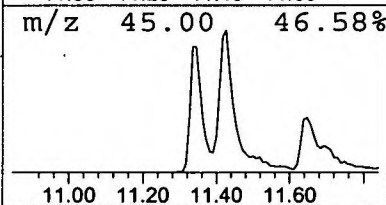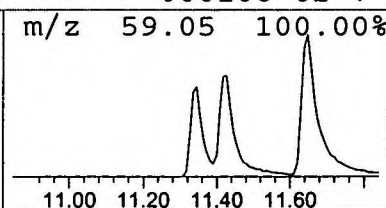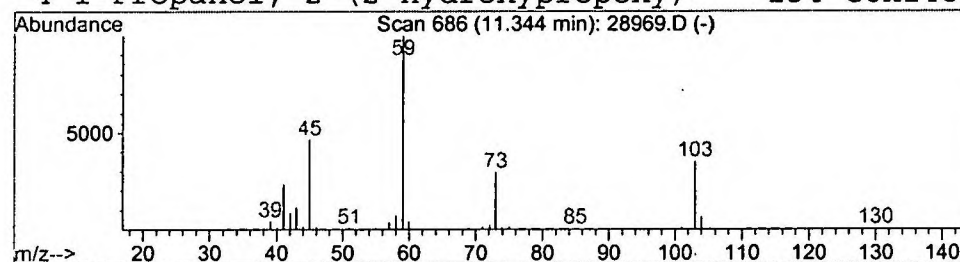

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC0701\28969.D
Acq On : 8 Dec 2001 3:37 am
Sample : 11/29 gc/ms scan
Misc :
MS Integration Params: LSCINT.P









Vial: 14
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 3 2-Propanol, 1-(2-methoxy-1-met Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.43	1.10 ug/l	269973	1,4-Dichlorobenzene-d4	11.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Propanol, 1-(2-methoxy-1-methylet	148	C7H16O3	020324-32-7	83		
2	2-Butanol, 3,3'-oxybis-	162	C8H18O3	054305-61-2	64		
3	2-Propanol, 1-(2-methoxypropoxy)-	148	C7H16O3	013429-07-7	50		
4	1-Propanol, 2-(2-hydroxypropoxy)-	134	C6H14O3	000106-62-7	45		

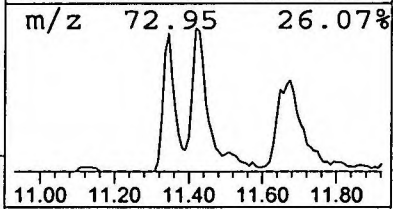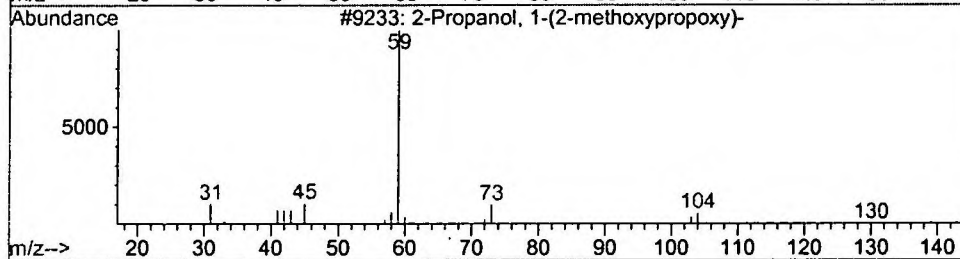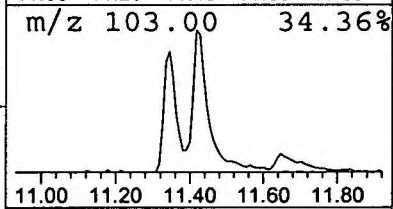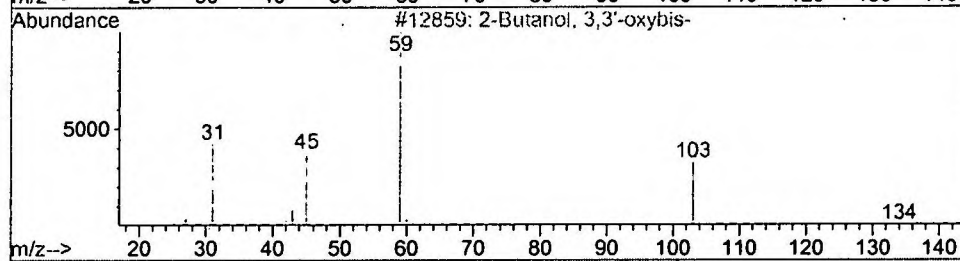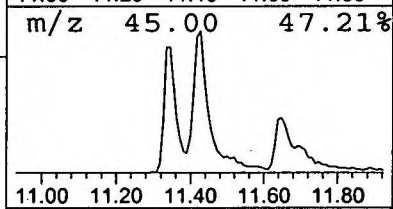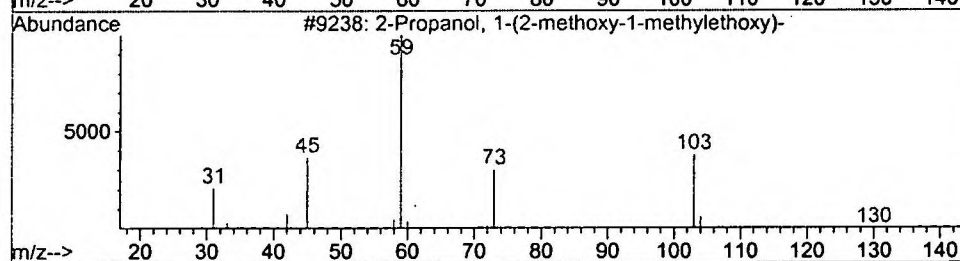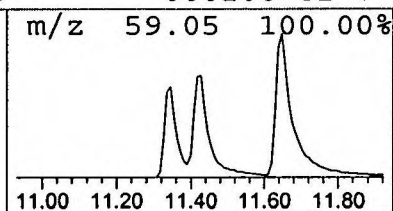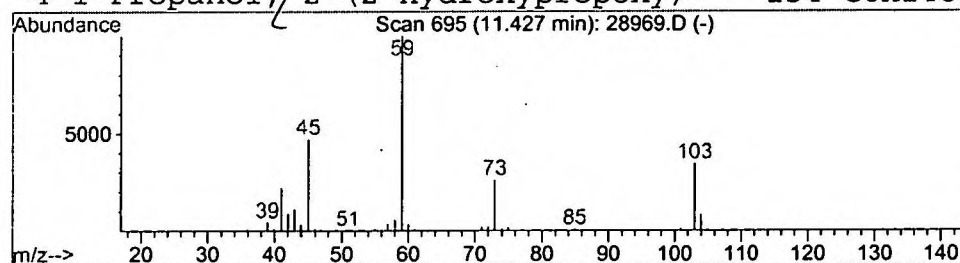

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 8 Dec 2001 3:37 am
Data File: C:\HPCHEM\1\DATA\DEC0701\28969.D
Name: 11/29 gc/ms scan
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Silane, tetramethyl-	7.60	3.9	ug/l	968201	ISTD01	11.67	4916950	20.0
2-Propanol , 1-(2-met	11.34	0.9	ug/l	231631	ISTD01	11.67	4916950	20.0
2-Propanol , 1-(2-met	11.43	1.1	ug/l	269973	ISTD01	11.67	4916950	20.0

28969.D GCMS1126.M Thu Dec 13 10:28:46 2001