

Method 508 mod

Date Extracted 12/3/01

Page 1

ref

B6CMS-16020

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count	Notes
LB		500 mL		1 mL	0.5 mL		1 mL		7		
Ref											
29189											
29189											
29136											
29135											
28596	- See batch										✓
28599	ref extract										
29231											
29234											
29232											
29233											
29230											
29287											
Remarks 29189 was very acidic. 3 mL 6M NaOH added to bring pH to 7. 29187 was not extracted by accident. drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type - <u>sep fun</u> Solv. lot# <u>V39466</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V39400</u> STANDARD INT STD LOG# CALIBRATION REF/SPIKE <u>91759</u> MDL/MDRF Q. CHECK INT. STD. SURROGATE <u>GCMS 112001</u> LPC ENDRIN/DDT Reviewed by <u>DN</u> Date <u>12/18/11</u>											

Analyst LF/EH
revision 4/12/01

Verified by _____

Reviewed by DN
Date 12/18/11

Sequence Name: C:\HPCHEM\1\SEQUENCE\DCE1001.S

Comment: INST 209; 30Mx0.25umX0.50

Operator: 209 GALOS

Data Path: C:\HPCHEM\1\data\dec1001\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

(X) Full Method

(X) Inject Anyway

() Reprocessing Only

() Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP2	GCMS1126	
2 Sample	2	CAL40	GCMS1126	
3 Sample	3	LB	GCMS1126	gc/ms scan 11/30
4 Sample	4	REF	GCMS1126	gc/ms scan 11/30
5 Sample	1	DFTPP1	GCMS1126	
6 Sample	5	29188	GCMS1126	gc/ms scan 11/30
7 Sample	6	29187	GCMS1126	gc/ms scan 11/30
8 Sample	7	29023	GCMS1126	gc/ms scan 11/30
9 Sample	8	29141	GCMS1126	gc/ms scan 11/30
10 Sample	9	29022	GCMS1126	gc/ms scan 11/30
11 Sample	10	29134	GCMS1126	gc/ms scan 11/30
12 Sample	11	29139	GCMS1126	gc/ms scan 11/30
13 Sample	12	29190	GCMS1126	gc/ms scan 11/30
14 Sample	13	LBB	GCMS1126	gc/ms scan 12/3
15 Sample	14	REFB	GCMS1126	gc/ms scan 12/3
16 Sample	15	29233	GCMS1126	gc/ms scan 12/3
17 Sample	16	29232	GCMS1126	gc/ms scan 12/3
18 Sample	17	29287	GCMS1126	gc/ms scan 12/3
19 Sample	18	29230	GCMS1126	gc/ms scan 12/3
20 Sample	19	29136	GCMS1126	gc/ms scan 12/3
21 Sample	20	29189	GCMS1126	gc/ms scan 12/3
22 Sample	21	29596	GCMS1126	gc/ms scan 12/3
23 Sample	22	29135	GCMS1126	gc/ms scan 12/3
24 Sample	23	29239	GCMS1126	gc/ms scan 12/3
25 Sample	1	DFTPP3	GCMS1126	
26 Sample	2	CAL40A	GCMS1126	
27 Sample	24	29231	GCMS1126	gc/ms scan 12/3
28 Sample	25	LBC	GCMS1126	gc/ms scan 11/30a
29 Sample	26	REFA	GCMS1126	gc/ms scan 11/30a
30 Sample	27	29088	GCMS1126	gc/ms scan 11/30a
31 Sample	28	29027	GCMS1126	gc/ms scan 11/30a
32 Sample	29	29025	GCMS1126	gc/ms scan 11/30a
33 Sample	30	29026	GCMS1126	gc/ms scan 11/30a
34 Sample	31	29024	GCMS1126	gc/ms scan 11/30a
35 Sample	32	29028	GCMS1126	gc/ms scan 11/30a
36 Sample	33	29137	GCMS1126	gc/ms scan 11/30a
37 Sample	34	29029	GCMS1126	gc/ms scan 11/30a
38 Sample	35	29086	GCMS1126	gc/ms scan 11/30a
39 Sample	36	29089	GCMS1126	gc/ms scan 11/30a
40 Sample	37	29140	GCMS1126	gc/ms scan 11/30a
41 Sample	38	29138	GCMS1126	gc/ms scan 11/30a
42 Sample	3	LBD	GCMS1126	gc/ms scan 12/4


Last Modified: Wed Dec 12 10:37:46 2001

Page: 1

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC1001\DFTPP1.D
 Acq On : 10 Dec 2001 1:39 pm
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : M:\INSTRU~1\209\METHODS\NP091101.M (RTE Integrator)
 Title : 209 625/TCLP calibration table 7/16/01

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

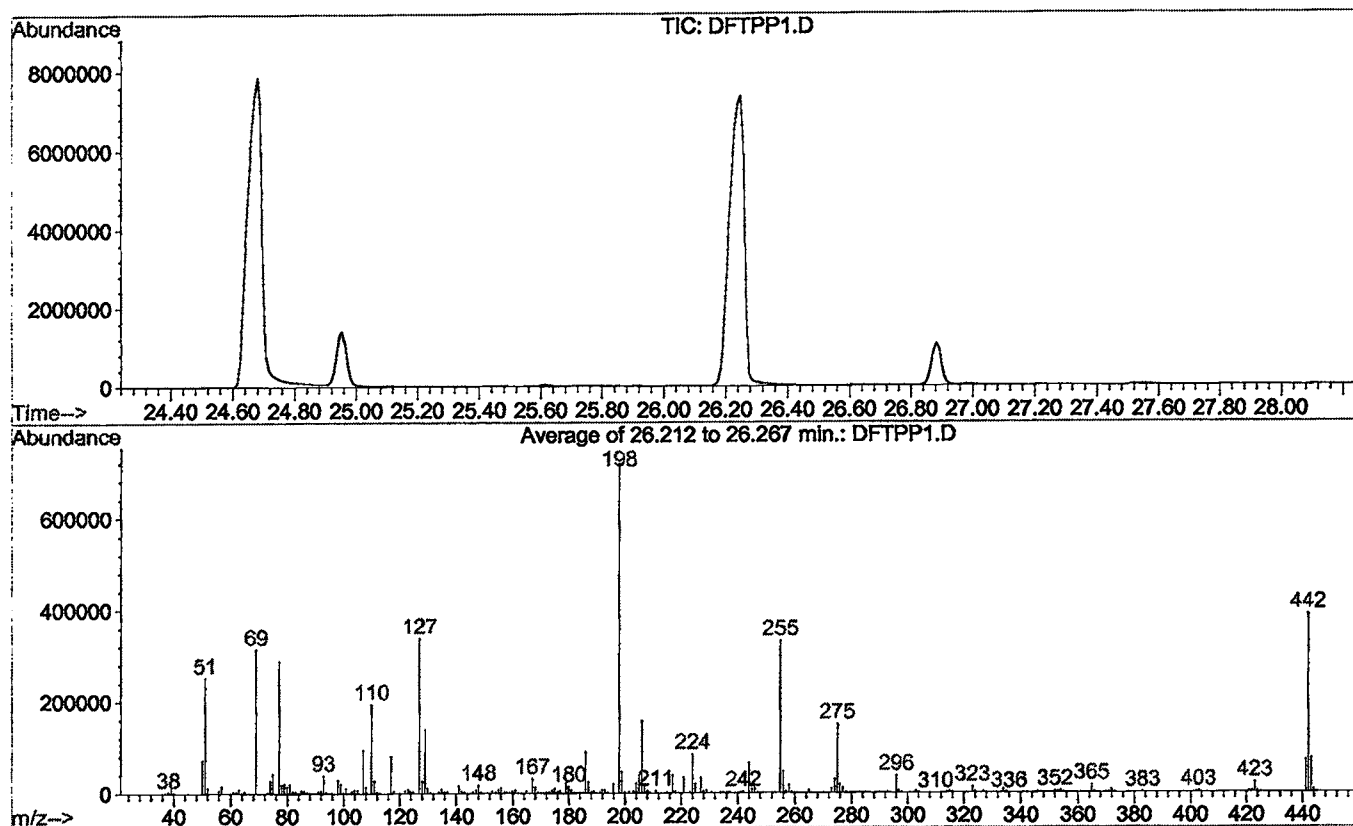

Spectrum Information: Average of 26.212 to 26.267 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	35.2	252874	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.8	314791	PASS
70	69	0.00	2	0.0	54	PASS
127	198	40	60	47.1	338177	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	718153	PASS
199	198	5	9	6.7	48293	PASS
275	198	10	30	20.8	149621	PASS
365	198	1	100	2.4	17584	PASS
441	443	0.01	100	94.5	70941	PASS
442	198	40	110	54.1	388443	PASS
443	442	17	23	19.3	75074	PASS