

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 12/28/2001 Time: 14:53:21

Sample: AD29235
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 12/28/01 14:52 Ended: 12/28/01 14:52 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		127		5.0

Comments for Sample AD29235 - Analysis \$GCMS

Westchester Dept. of Labs & Research

Analyst: Vinci, David L

Date: 12-28-2001 Time: 14:53:33

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1001\29235.D

Vial: 8

Acq On : 12 Dec 2001 6:34 am

Operator: 209 GALOS

Sample : gc/ms scan 12/4

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 19 12:46 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Nov 28 15:06:24 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	11.67	152	875590	20.00	ug/l	-0.03
10) Naphthalene-d8	15.28	136	3340047	20.00	ug/l	-0.03
17) Acenaphthene-d10	20.55	164	1712414	20.00	ug/l	-0.03
29) Phenanthrene-d10	24.97	188	2346540	20.00	ug/l	-0.02
38) Chrysene-d12	33.00	240	1485832	20.00	ug/l	-0.03
44) Perylene-d12	37.10	264	1051283	20.00	ug/l	-0.02

System Monitoring Compounds

37) 2,4-DDD	30.05	235	177162	6.34	ug/mL	-0.02
Spiked Amount	5.000		Recovery	=	126.80%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	5.30	74	210	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.33	128	1655	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	21.02	165	216	N.D.	
25) Diethylphthalate	22.09	149	660	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#)= qualifier out of range (m) = manual integration

29235.D GCMS1126.M Wed Dec 19 16:35:03 2001

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC1001\29235.D

Vial: 8

Acq On : 12 Dec 2001 6:34 am

Operator: 209 GALOS

Sample : gc/ms scan 12/4

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: RTEINT.P

Quant Time: Dec 19 12:46 2001

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Nov 28 15:06:24 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.04	178	237	N.D.		
34) Anthracene	25.04	178	237	N.D.		
35) Di-n-butylphthalate	26.98	149	38831	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.01	228	3186	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.29	149	18341	N.D.		
43) Chrysene	33.01	228	3186	N.D.		
45) Di-n-Octylphthalate	35.02	149	793	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.10	252	4301	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

29235.D GCMS1126.M Wed Dec 19 16:35:07 2001

Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC1001\29235.D

Acq On : 12 Dec 2001 6:34 am

Sample : gc/ms scan 12/4

Misc :

MS Integration Params: RTEINT.P

Quant Time: Dec 19 12:46 2001

Vial: 8

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00


Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 14 12:19:30 2001

Response via : Initial Calibration

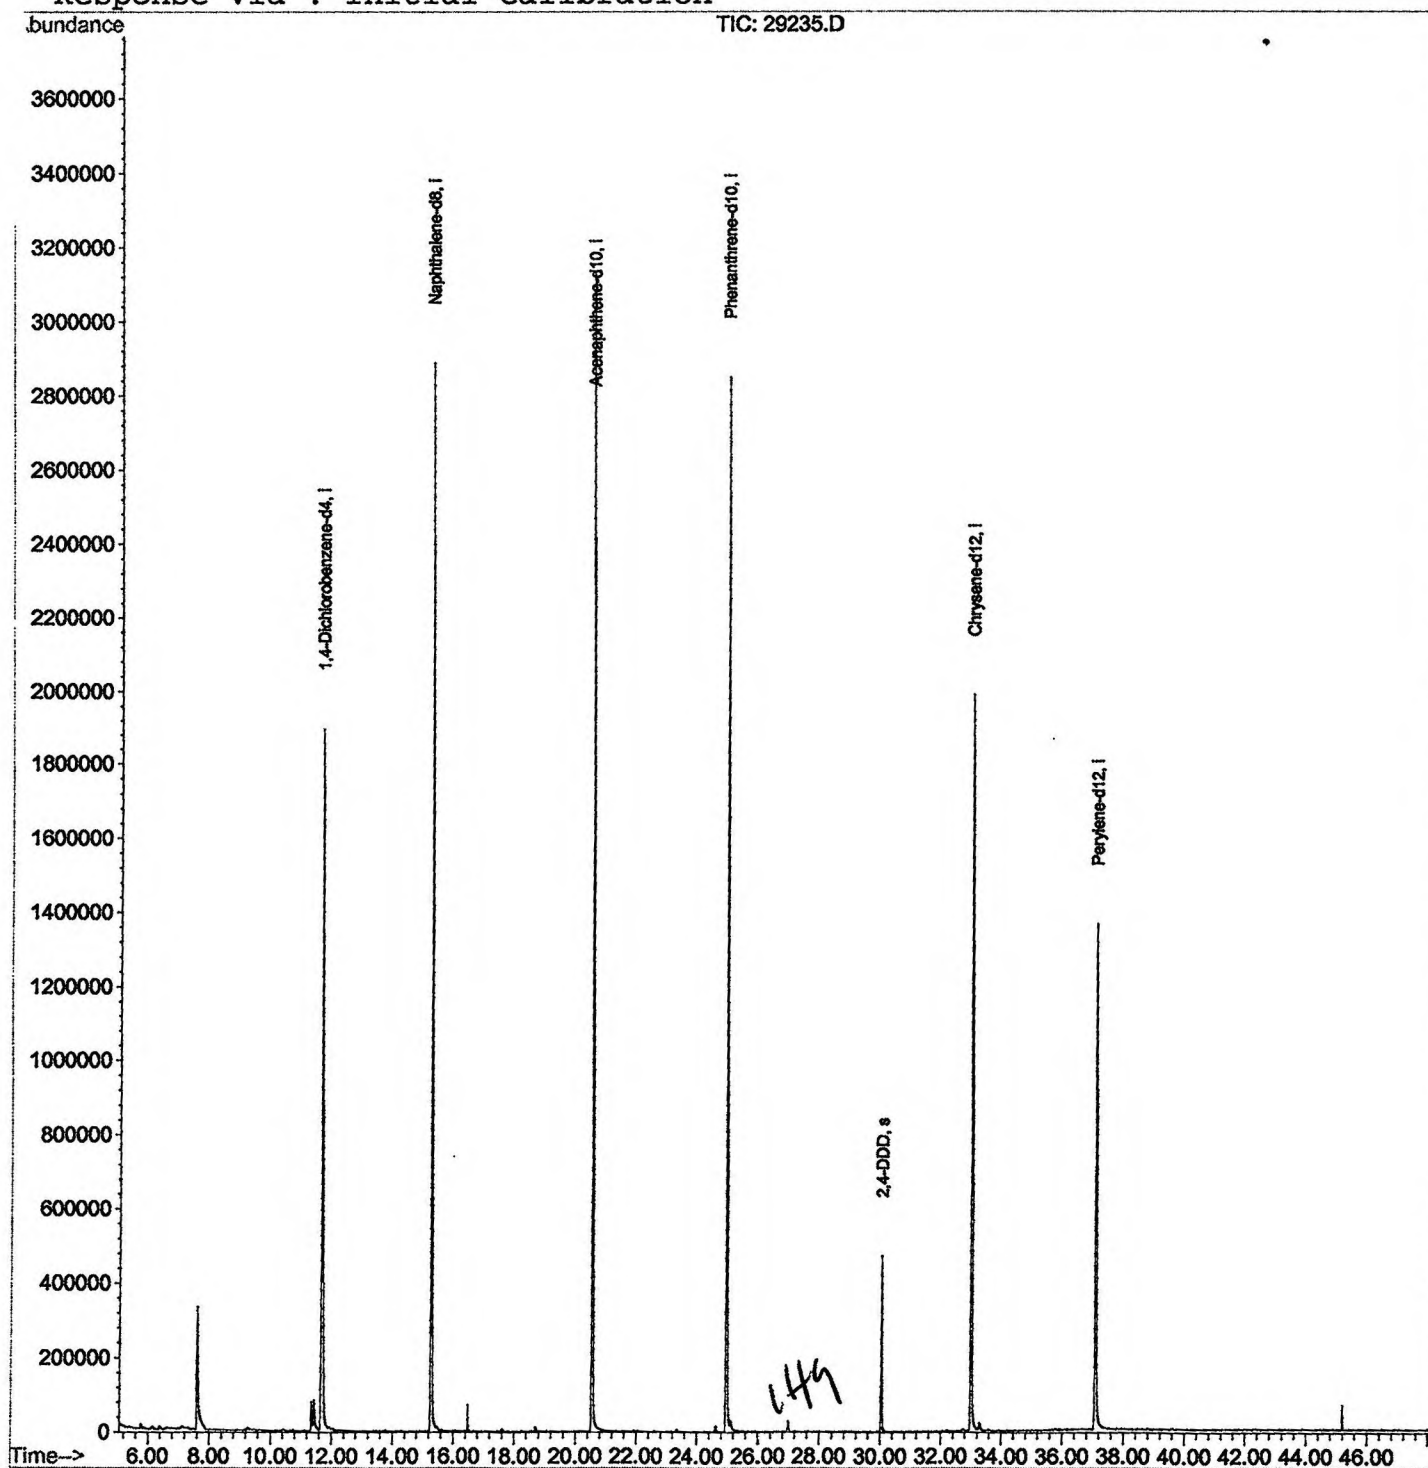

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC1001\29235.D
 Acq On : 12 Dec 2001 6:34 am
 Sample : gc/ms scan 12/4
 Disc :
 S Integration Params: LSCINT.P

Vial: 8
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


Peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.603	275	279	309	rBV	329226	1030334	14.72%	2.882%
2	11.348	683	687	692	rBV	78314	183997	2.63%	0.515%
3	11.431	692	696	715	rVB	81854	269635	3.85%	0.754%
4	11.670	715	722	745	rBV	1894119	5114626	73.06%	14.306%
5	15.277	1109	1115	1133	rBV	2886304	6331790	90.45%	17.710%
6	20.547	1683	1689	1711	rBV	3136165	7000548	100.00%	19.581%
7	24.972	2164	2171	2183	rBV2	2849001	6256330	89.37%	17.499%
8	25.119	2184	2187	2198	rVB2	24542	79646	1.14%	0.223%
9	30.049	2718	2724	2731	rBV	472046	954783	13.64%	2.671%
10	33.005	3039	3046	3064	rBV2	1988880	4658009	66.54%	13.029%
11	37.099	3484	3492	3509	rBV	1362569	3872131	55.31%	10.831%

Sum of corrected areas: 35751829

29235.D GCMS1126.M Wed Dec 19 12:52:37 2001

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC1001\29235.D
 Operator : 209 GALOS
 Acquired : 12 Dec 2001 6:34 am using AcqMethod GCMS1126
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 12/4
 Misc Info :
 Vial Number: 8
 Quant File :GCMS1126.RES (RTE Integrator)

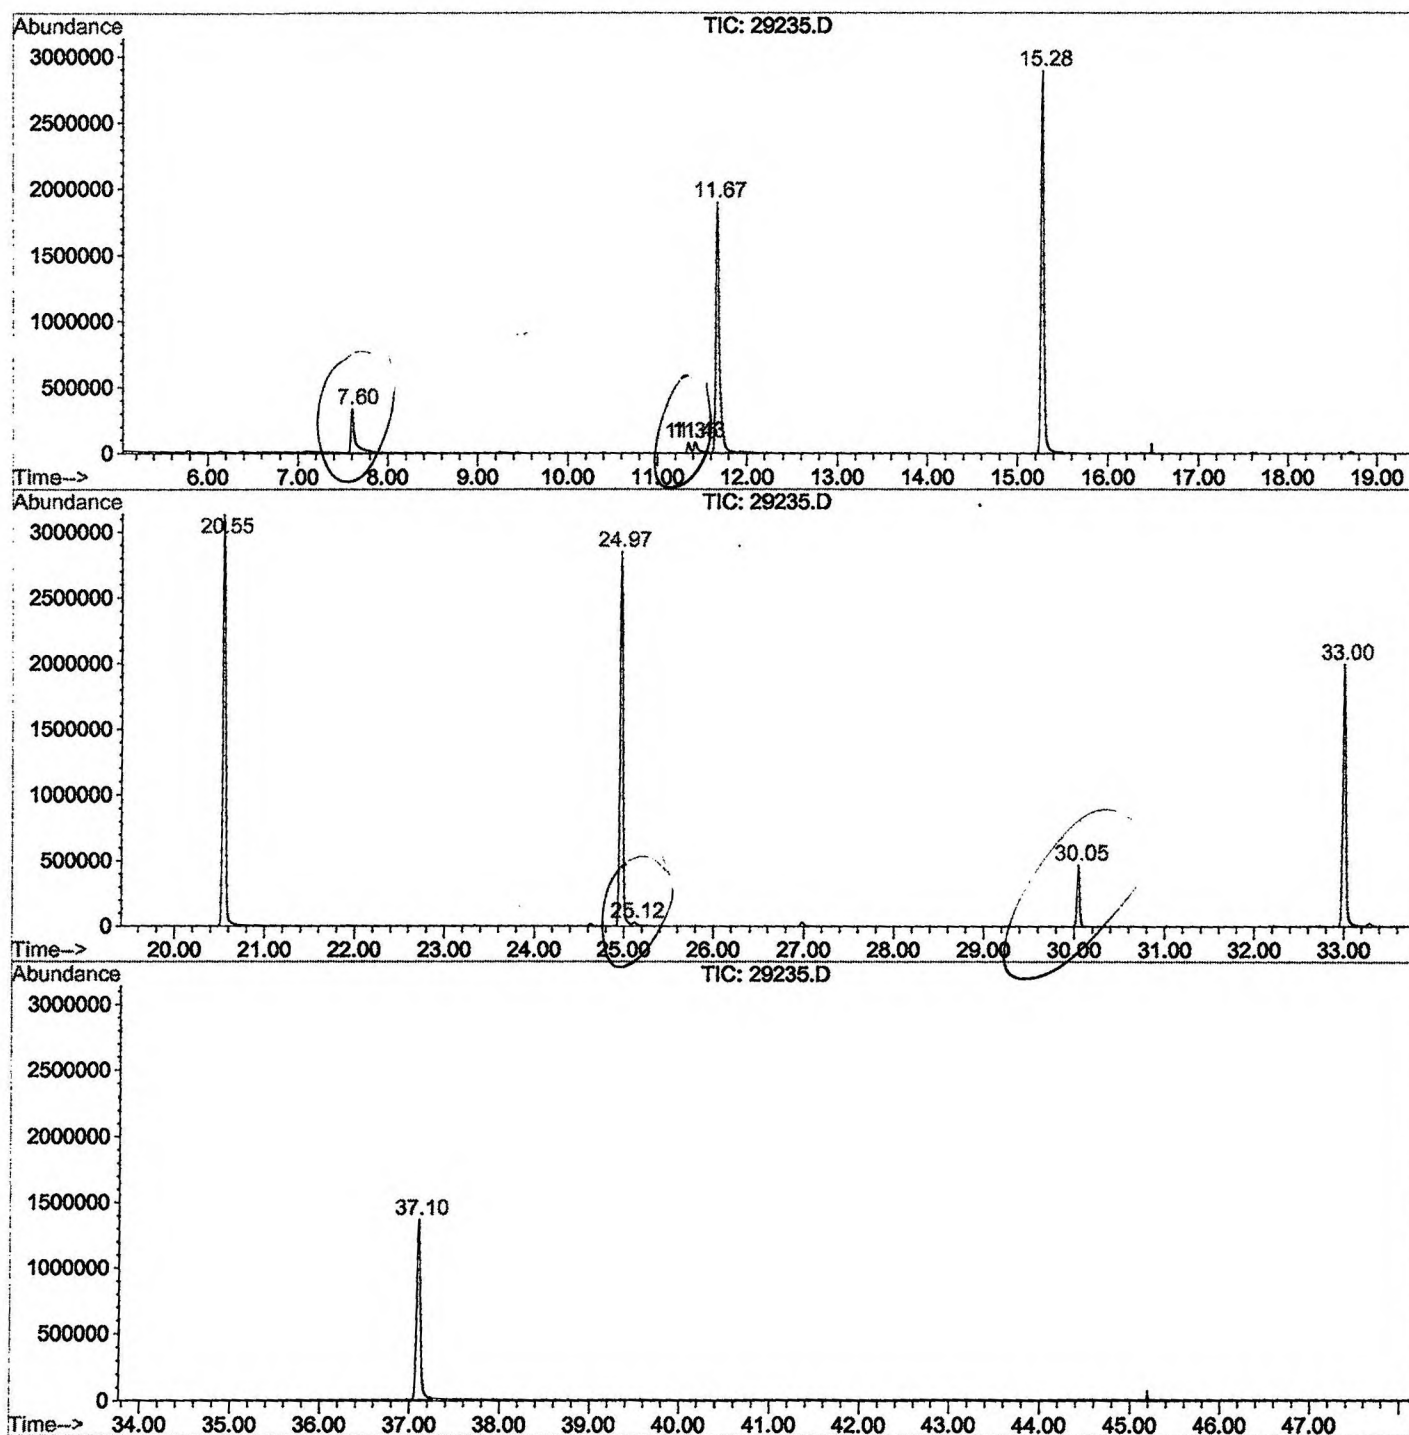

29235.D GCMS1126.M

Wed Dec 19 12:52:44 2001

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC1001\29235.D
 Acq On : 12 Dec 2001 6:34 am
 Sample : gc/ms scan 12/4
 Misc :
 MS Integration Params: LSCINT.P


Vial: 8
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 N-Ethylformamide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.60	4.03 ug/l	1030330	1,4-Dichlorobenzene-d4	11.67

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	N-Ethylformamide	73	C3H7NO	000627-45-2	9
2	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
3	1,3-Dioxolane, 2-(3-bromo-5,5,5-tri	352	C10H16BrCl3O2	000000-00-0	9
4	1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	7

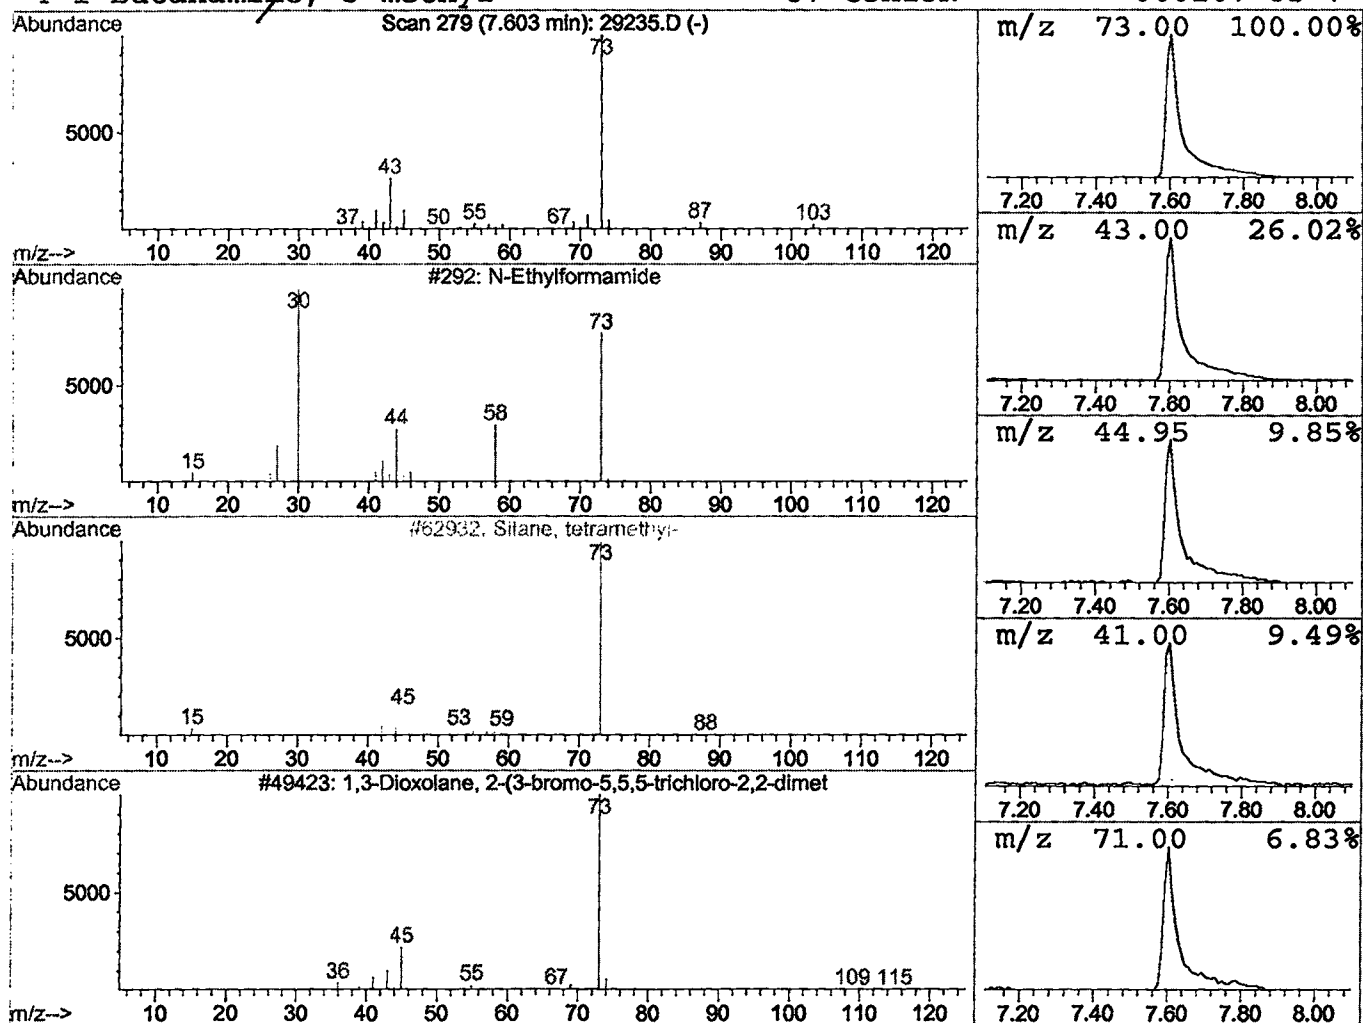

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC1001\29235.D
 Acq On : 12 Dec 2001 6:34 am
 Sample : gc/ms scan 12/4
 Misc :
 MS Integration Params: LSCINT.P


Vial: 8
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 2 2-Propanol, 1-(2-methoxy-1-met Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.35	0.72 ug/l	183997	1,4-Dichlorobenzene-d4	11.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Propanol, 1-(2-methoxy-1-methylet	148	C7H16O3	020324-32-7	72
2			2-Butanol, 3,3'-oxybis-	162	C8H18O3	054305-61-2	64
3			2-Propanol, 1,1'-oxybis-	134	C6H14O3	000110-98-5	56
4			2-Propanol, 1-(2-methoxypropoxy) -	148	C7H16O3	013429-07-7	47

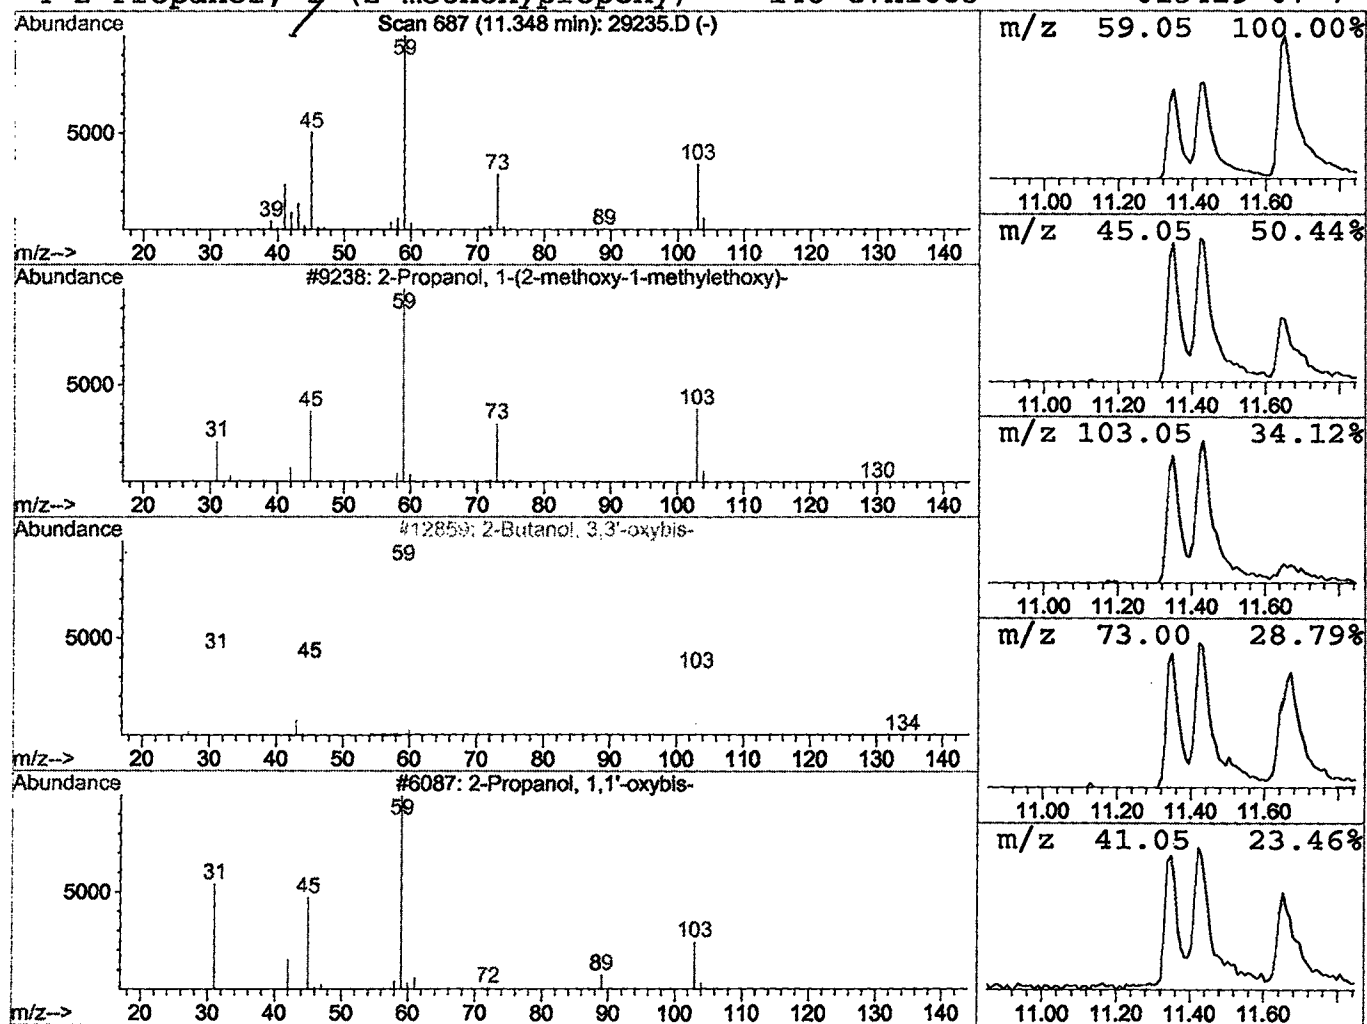

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC1001\29235.D
 Acq On : 12 Dec 2001 6:34 am
 Sample : gc/ms scan 12/4
 Misc :
 MS Integration Params: LSCINT.P


Vial: 8
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 3 2-Propanol, 1-(2-methoxy-1-met Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.43	1.05 ug/l	269635	1,4-Dichlorobenzene-d4	11.67

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Propanol,	1-(2-methoxy-1-methylet	148	C7H16O3	020324-32-7	90
2	2-Propanol,	1,1'-oxybis-	134	C6H14O3	000110-98-5	56
3	2-Butanol,	3,3'-oxybis-	162	C8H18O3	054305-61-2	50
4	1-Propanol,	2-(2-hydroxypropoxy) -	134	C6H14O3	000106-62-7	42

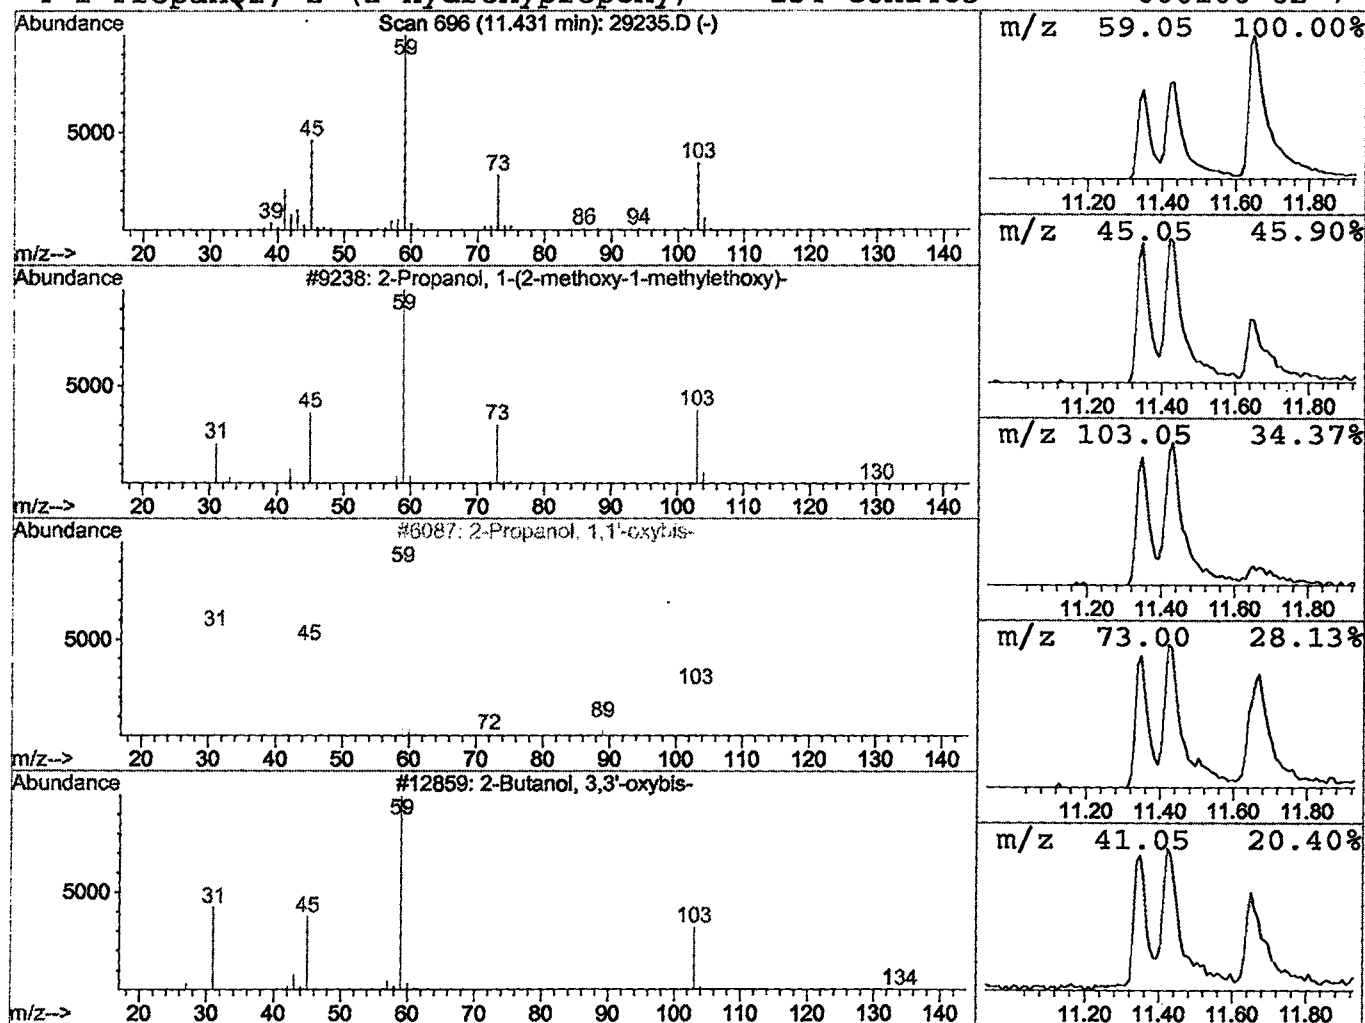

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 12 Dec 2001 6:34 am
Data File: C:\HPCHEM\1\DATA\DEC1001\29235.D
Name: gc/ms scan 12/4
Disc:
Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
N-Ethylformamide	7.60	4.0	ug/l	1030330	ISTD01	11.67	5114630	20.0
2-Propanol, 1-(2-met	11.35	0.7	ug/l	183997	ISTD01	11.67	5114630	20.0
2-Propanol, 1-(2-met	11.43	1.1	ug/l	269635	ISTD01	11.67	5114630	20.0

29235.D GCMS1126.M Wed Dec 19 12:53:14 2001