

Method 508 mod

Date Extracted 12/6/01

Page _____

ref

6CMS-16131

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
LB ✓		500 mL		1 mL			1 mL	4B	7	
Ref ✓					0.5 mL			9B		
29187 ✓	acidic	Neutralized					12/10/01	14A		
29966 ✓								1B		
29524 ✓								5A		
29463 ✓								10A		
29464 ✓								9A		
29518 ✓								10B		
29517 ✓								9B		
29521 ✓								5B		
29520 ✓								1A		
Reviewed by, <i>[Signature]</i>										
Remarks 29187 was very acidic → pH ≈ 1. About 2 mL of 6M NaOH were added to bring the pH to 7.										
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type - <u>spun</u> Solv. lot# <u>V43E07</u> NaCl lot# Na2SO4 lot#										
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE	91759									
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE	6CMS #62									
LPC	1P260 (F)									
ENDRIN/DDT										

Analyst LF/EH
revision 4/12/01

Verified by _____

Reviewed by *[Signature]*
Date 1/4/02

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC1201\DFTPP.D

Acq On : 12 Dec 2001 10:47 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

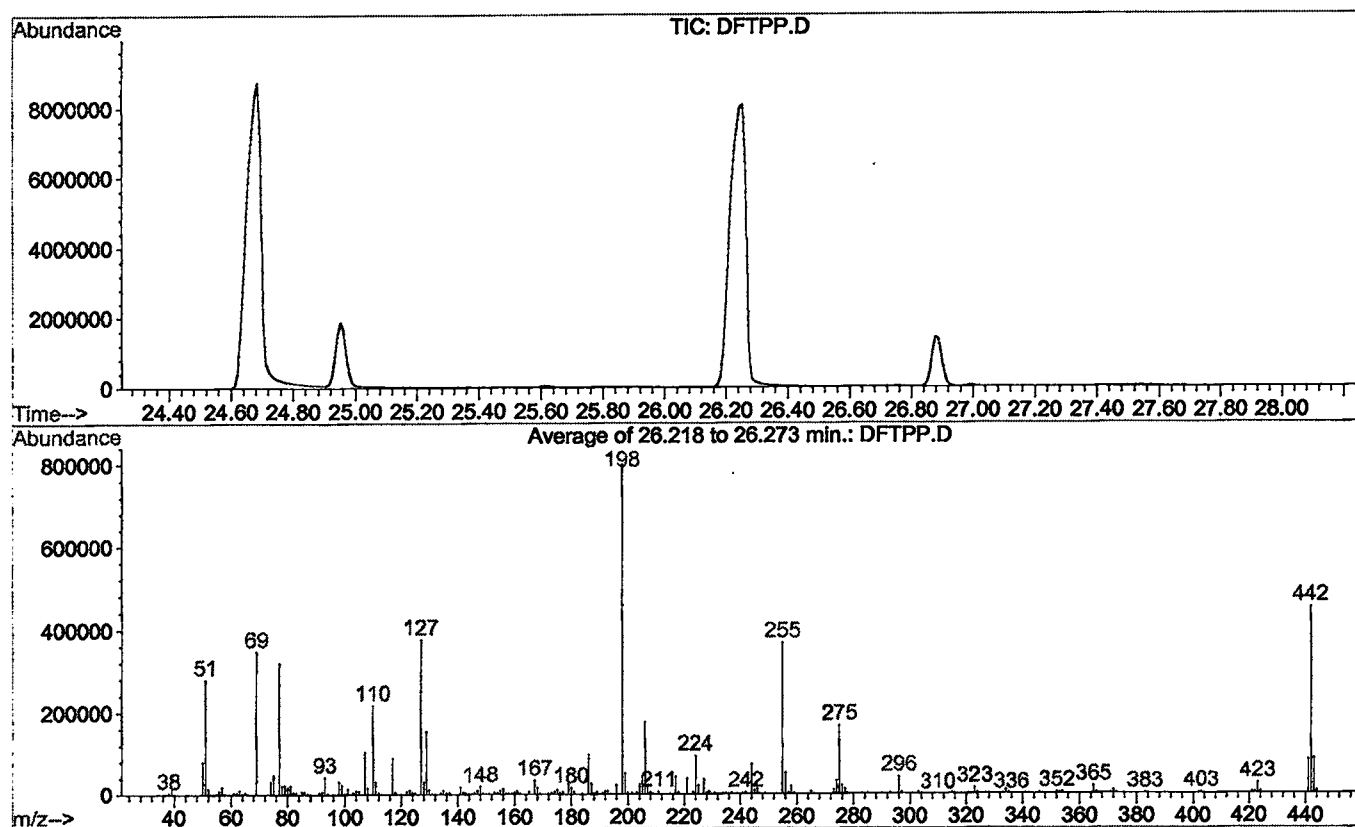

Spectrum Information: Average of 26.218 to 26.273 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	35.1	280730	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.5	348389	PASS
70	69	0.00	2	0.0	77	PASS
127	198	40	60	47.2	377585	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	800229	PASS
199	198	5	9	6.6	52431	PASS
275	198	10	30	21.0	167777	PASS
365	198	1	100	2.4	19596	PASS
441	443	0.01	100	94.6	82423	PASS
442	198	40	110	56.3	450514	PASS
443	442	17	23	19.3	87131	PASS

DFTPP.D GCMS1126.M

Thu Dec 20 10:46:32 2001