

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 01/08/2002 Time: 12:07:43

Sample: AD29522
 Analysis: \$B1GCMS Blank for GCMS Scan
 Units: ug
 Started: 1/8/02 12:03 Ended: 1/8/02 12:03 Analyst: MG
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	MDL
1	n-Nitrosodimethylamine		< MDL	2.0
2	bis(2-Chloroethyl)ether		< MDL	2.0
3	1,3-Dichlorobenzene		< MDL	2.0
4	1,4-Dichlorobenzene		< MDL	2.0
5	1,2-Dichlorobenzene		< MDL	2.0
6	2,2'-oxybis(1-Chloropropane)		< MDL	2.0
7	n-Nitrosodi-n-propylamine		< MDL	2.0
8	Hexachloroethane		< MDL	2.0
9	Nitrobenzene		< MDL	2.0
10	Isophorone		< MDL	2.0
11	bis(2-Chloroethoxy)methane		< MDL	2.0
12	1,2,4-Trichlorobenzene		< MDL	2.0
13	Naphthalene		< MDL	2.0
14	Hexachlorobutadiene		< MDL	2.0
15	Hexachlorocyclopentadiene		< MDL	2.0
16	2-Chloronaphthalene		< MDL	2.0
17	Dimethylphthalate		< MDL	2.0
18	2,6-Dinitrotoluene		< MDL	2.0
19	Acenaphthylene		< MDL	2.0
20	Acenaphthene		< MDL	2.0
21	2,4-Dinitrotoluene		< MDL	2.0
22	Diethylphthalate		< MDL	2.0
23	4-Chlorophenylphenylether		< MDL	2.0
24	Fluorene		< MDL	2.0
25	Azobenzene/1,2-Diphenylhydraz		< MDL	2.0
26	n-Nitrosodiphenylamine		< MDL	2.0
27	4-Bromophenylphenylether		< MDL	2.0
28	Hexachlorobenzene		< MDL	2.0
29	Phenanthrene		< MDL	2.0
30	Anthracene		< MDL	2.0
31	Di-n-butylphthalate		< MDL	2.0
32	Fluoranthene		< MDL	2.0
33	Pyrene		< MDL	2.0
34	Butylbenzylphthalate		< MDL	2.0
35	Benzo(a)anthracene		< MDL	2.0
36	bis(2-Ethylhexyl)phthalate		< MDL	2.0
37	Chrysene		< MDL	2.0
38	Di-n-octylphthalate		< MDL	2.0
39	Benzo(b)fluoranthene		< MDL	2.0
40	Benzo(k)fluoranthene		< MDL	2.0
41	Benzo(a)pyrene		< MDL	2.0
42	Indeno(1,2,3-cd)pyrene		< MDL	2.0
43	Dibenz(a,h)anthracene		< MDL	2.0
44	Benzo(g,h,i)perylene		< MDL	2.0

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC3101\LBF.D

Vial: 59

Acq On : 2 Jan 2002 11:08 pm

Operator: 209 GALOS

Sample : gcms scan 12/7

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 2 23:57 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	11.67	152	2099094	20.00	ug/l	-0.03
10) Naphthalene-d8	15.28	136	8131202	20.00	ug/l	-0.03
17) Acenaphthene-d10	20.57	164	3965083	20.00	ug/l	0.00
29) Phenanthrene-d10	24.99	188	6090086	20.00	ug/l	0.00
38) Chrysene-d12	33.03	240	3783053	20.00	ug/l	0.00
44) Perylene-d12	37.13	264	2166512	20.00	ug/l	0.00

System Monitoring Compounds

37) 2,4-DDD	30.07	235	164815	2.46	ug/mL	0.00
Spiked Amount	5.000		Recovery	=	49.20%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	5.29	74	287	N.D.
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	12.59	117	178	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	15.33	128	1413	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	20.57	153	282	N.D.
24) 2,4-Dinitrotoluene	21.32	165	937	N.D.
25) Diethylphthalate	22.16	149	327	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#)= qualifier out of range (m)= manual integration

LBF.D GCMS1126.M Wed Jan 16 11:38:38 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\DEC3101\LBF.D

Vial: 59

Acq On : 2 Jan 2002 11:08 pm

Operator: 209 GALOS

Sample : gcms scan 12/7

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Jan 2 23:57 2002

Quant Results File: GCMS1126.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

DataAcq Meth : GCMS1126

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	24.98	178	2507	N.D.		
34) Anthracene	24.98	178	2507	N.D.		
35) Di-n-butylphthalate	27.04	149	21639	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.03	228	9880	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.31	149	10750	N.D.		
43) Chrysene	33.03	228	9880	N.D.		
45) Di-n-Octylphthalate	35.04	149	196	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.13	252	9181	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

LBF.D GCMS1126.M

Wed Jan 16 11:38:42 2002

Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\DEC3101\LBF.D

Acq On : 2 Jan 2002 11:08 pm

Sample : gcms scan 12/7

Misc :

MS Integration Params: GOOFY.P

Quant Time: Jan 2 23:57 2002

Vial: 59

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00


Quant Results File: GCMS1126.RES

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Dec 28 15:11:00 2001

Response via : Initial Calibration

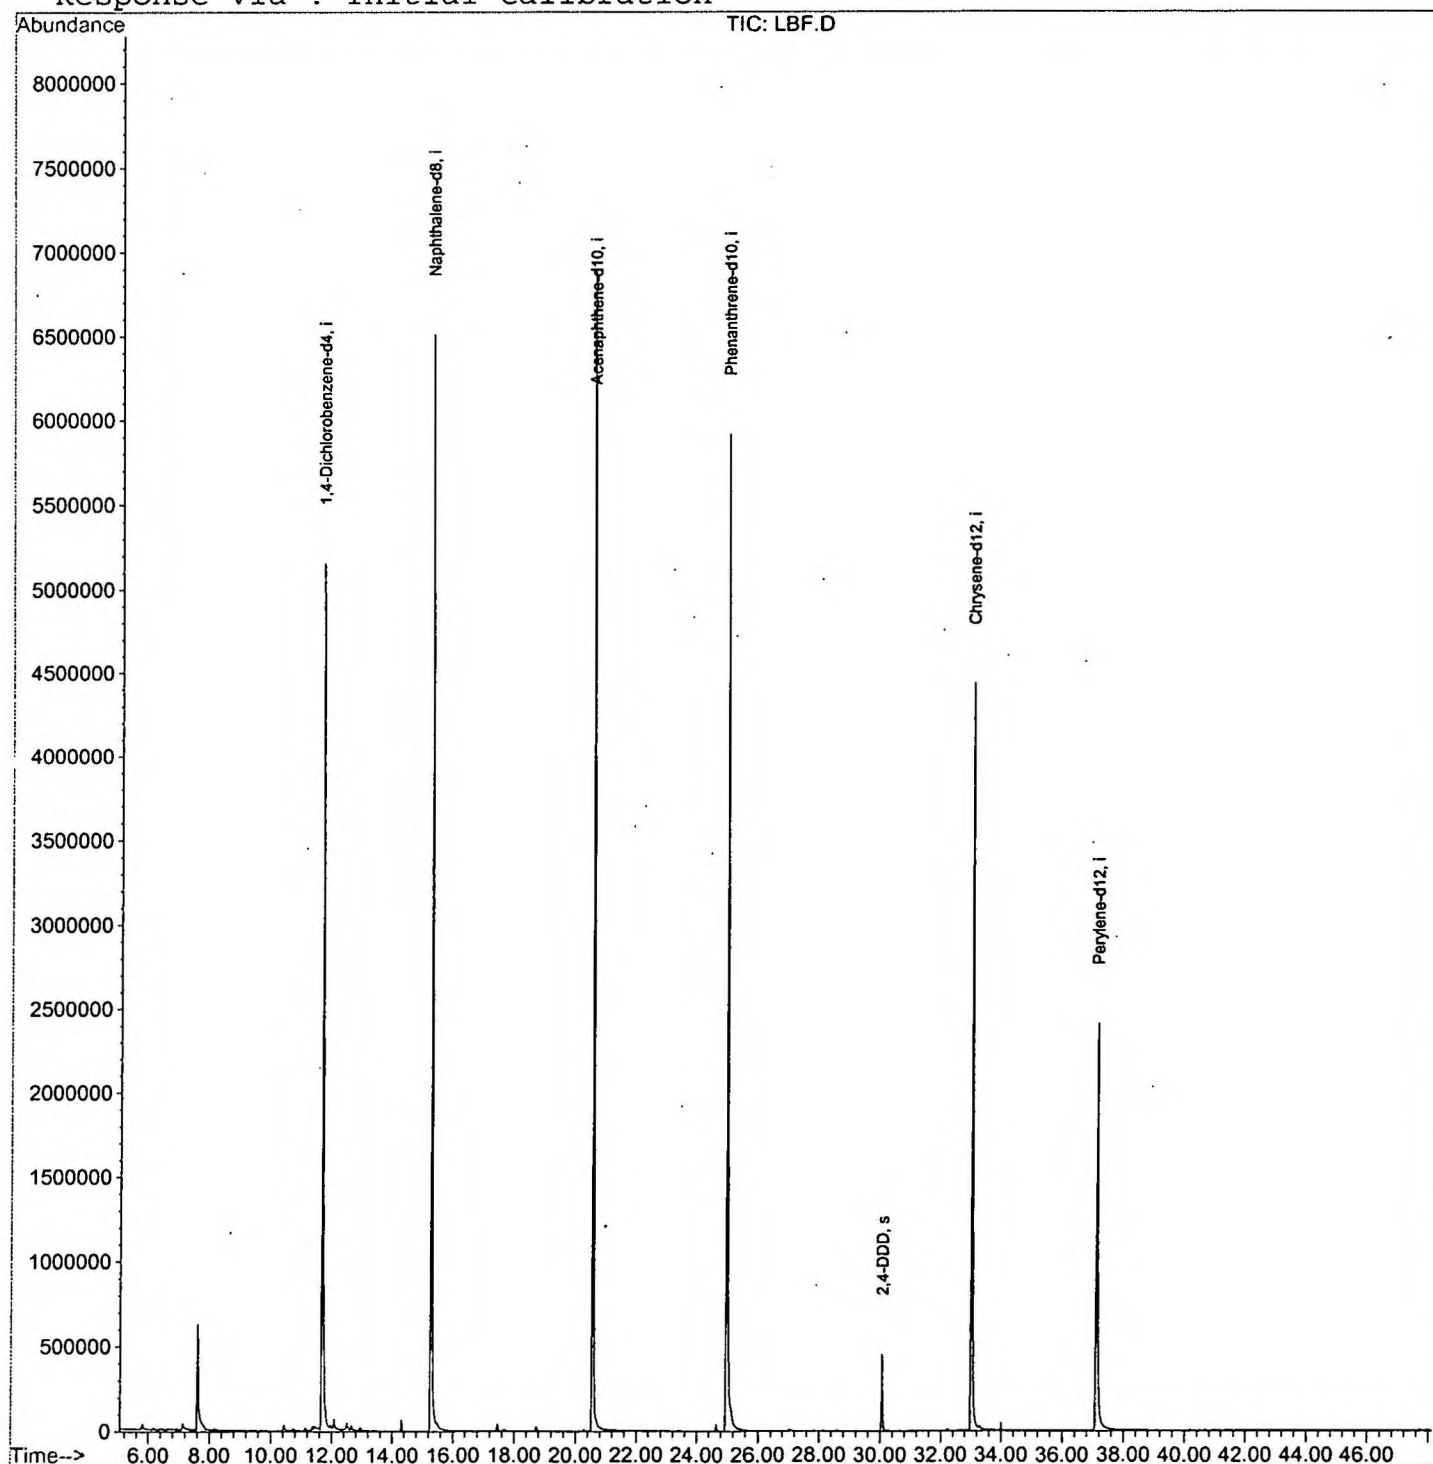

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\DEC3101\LBF.D

Acq On : 2 Jan 2002 11:08 pm

Sample : gcms scan 12/7

Misc :

MS Integration Params: LSCINT.P

Vial: 59

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	7.614	275	280	312	rBV	621804	2009585	11.61%	2.300%
2	11.672	717	722	751	rBV	5145547	13445849	77.67%	15.392%
3	15.280	1109	1115	1134	rBV	6509581	16290871	94.10%	18.649%
4	20.568	1683	1691	1717	rBV2	6898783	17312618	100.00%	19.818%
5	24.993	2165	2173	2219	rBV2	5917470	17079091	98.65%	19.551%
6	30.069	2720	2726	2739	rBV	449280	1049936	6.06%	1.202%
7	33.034	3041	3049	3074	rBV2	4434539	12145952	70.16%	13.904%
8	37.129	3486	3495	3528	rBV	2405914	8023520	46.34%	9.185%


Sum of corrected areas: 87357422

LBF.D GCMS1126.M

Wed Jan 16 15:07:35 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\DEC3101\LBF.D
 Operator : 209 GALOS
 Acquired : 2 Jan 2002 11:08 pm using AcqMethod GCMS1126
 Instrument : GC/MS 209
 Sample Name: gcms scan 12/7
 Misc Info :
 Vial Number: 59
 Quant File :GCMS1126.RES (RTE Integrator)

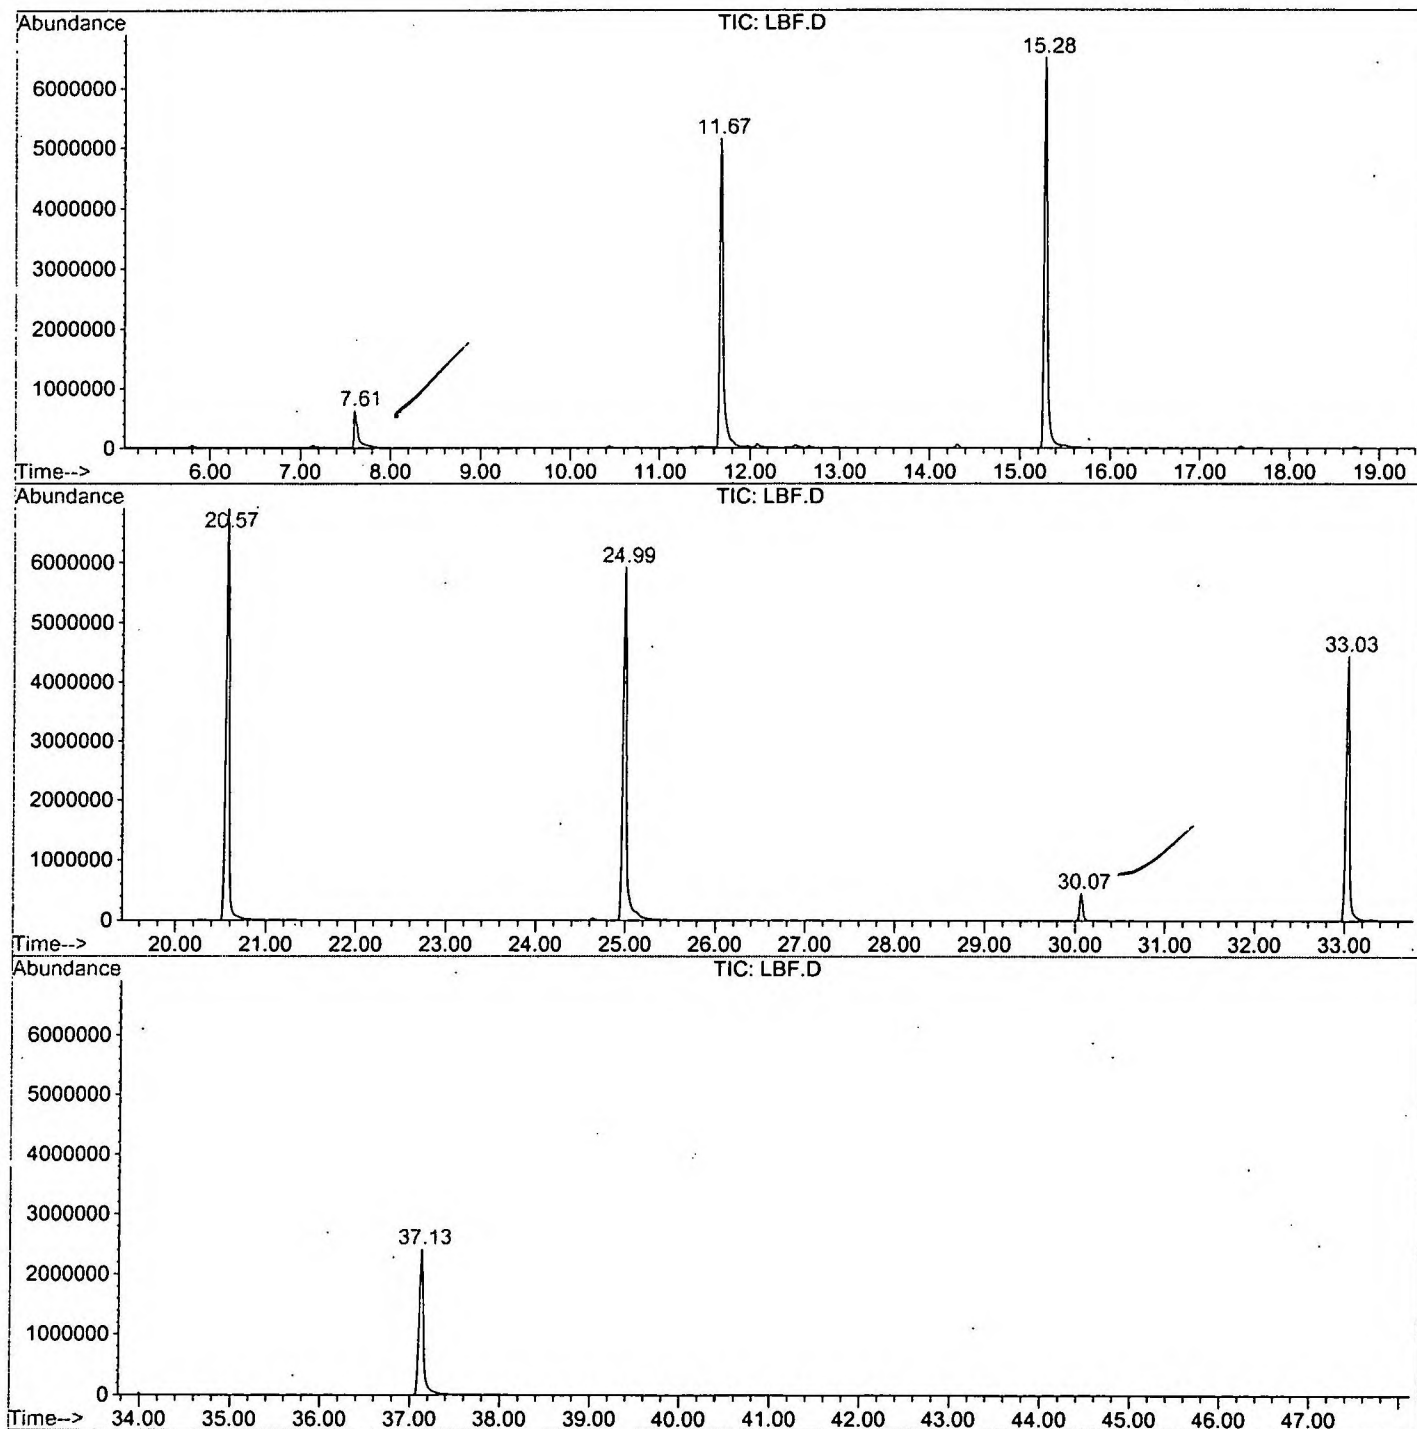

LBF.D GCMS1126.M

Wed Jan 16 15:07:41 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\DEC3101\LBF.D
 Acq On : 2 Jan 2002 11:08 pm
 Sample : gcms scan 12/7
 Misc :
 MS Integration Params: LSCINT.P


Vial: 59
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 Pentane, 3-methoxy- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.61	2.99 ug/l	2009590	1,4-Dichlorobenzene-d4	11.67

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	25
2			N-Ethylformamide	73	C3H7NO	000627-45-2	9
3			1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	9
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

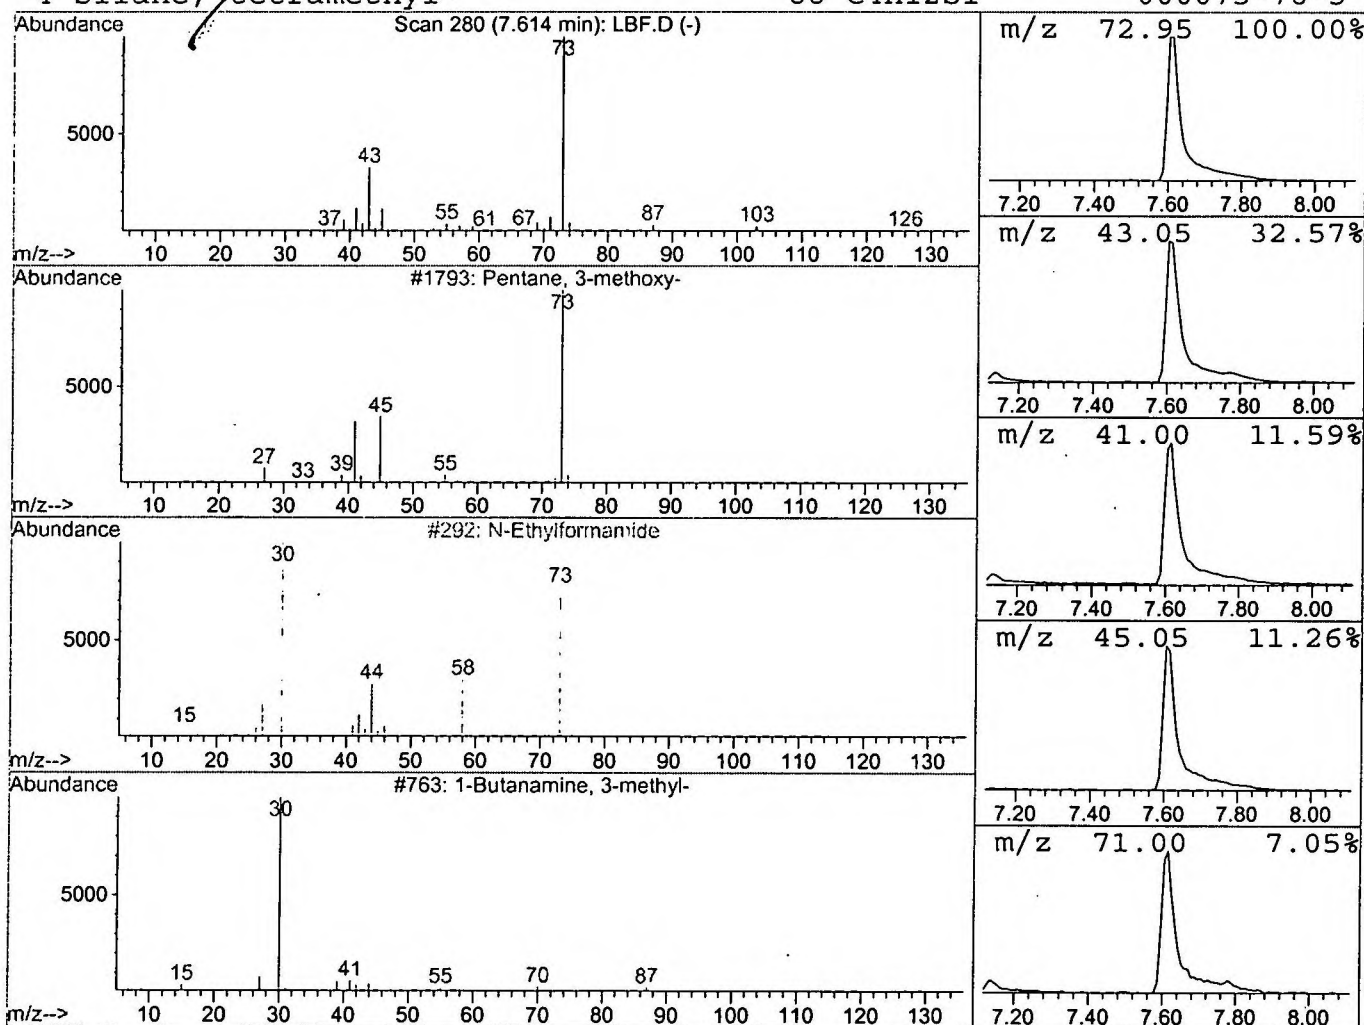

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 2 Jan 2002 11:08 pm
 Data File: C:\HPCHEM\1\DATA\DEC3101\LBF.D
 Name: gcms scan 12/7
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Pentane, 3-methoxy-	7.61	3.0	ug/l	2009590	ISTD01	11.67	13445800	20.0
LBF.D GCMS1126.M	Wed Jan 16 15:07:50 2002							