

Method 508 mod

Date Extracted 12/11/01

Page 54

ref

GCMS - 16494

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB ✓	Ref ✓	500mL		1mL	0.5mL		1mL	10B	7			
29962 ✓								10A				
30011 ✓								6B				
30012 ✓								5A				
30013 ✓								4B				
30014 ✓								6A				
30015 ✓								3A				
30016 ✓								2B				
29963 ✓								1A				
29964 ✓								3B				
29972 ✓								5B				
								2A				
Remarks												
Reviewed by <u>JB 5/15/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -												
Extraction type - <u>sep fun</u> Solv. lot# <u>V39466</u> NaCl lot# <u>V11599</u> Na2SO4 lot# <u>V39400</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REP/SPIKE	<u>91759</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	<u>GCMS 12110</u>											
LPC												
ENDRIN/DDT												

Analyst LF
Revision 4/12/01

Verified by _____

Reviewed by DM
Date 1/28/02

DFTPP

Data File : C:\HPCHEM\1\DATA\DEC1801\DFTPP.D

Acq On : 18 Dec 2001 4:03 pm

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS1126.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

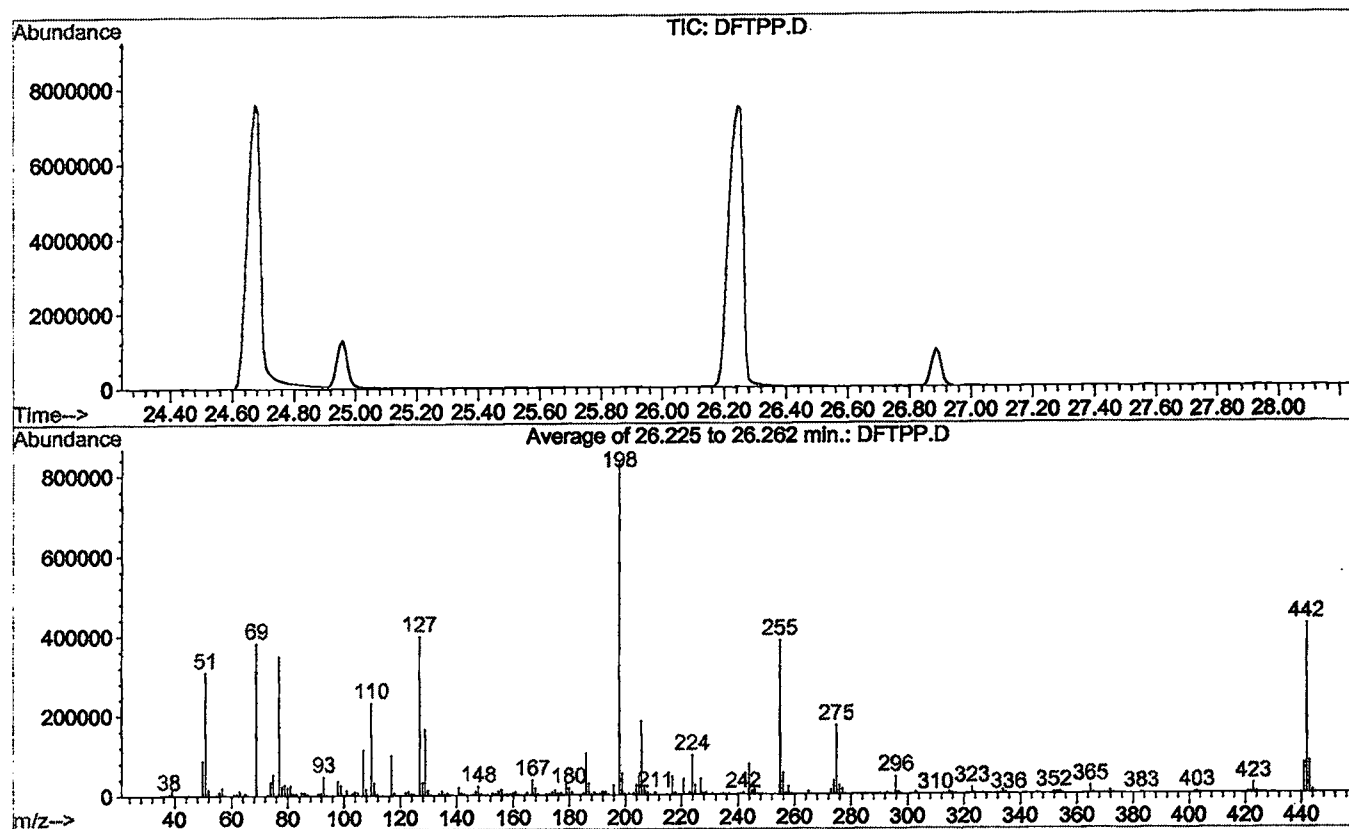

Spectrum Information: Average of 26.225 to 26.262 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	37.5	309760	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.4	383501	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	48.3	399117	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	826496	PASS
199	198	5	9	6.6	54878	PASS
275	198	10	30	20.9	173069	PASS
365	198	1	100	2.5	20557	PASS
441	443	0.01	100	93.9	76933	PASS
442	198	40	110	51.4	425165	PASS
443	442	17	23	19.3	81957	PASS

DFTPP.D GCMS1126.M

Tue Jan 15 09:49:24 2002