


File : C:\MSDCHEM\1\DATA\031202\DFTB0312.D  
 Operator : McLean  
 Acquired : 12 Mar 2002 8:13 pm using AcqMethod 508SCAN  
 Instrument : Instrumen  
 Sample Name: DFTPP  
 Misc Info :  
 Vial Number: 1

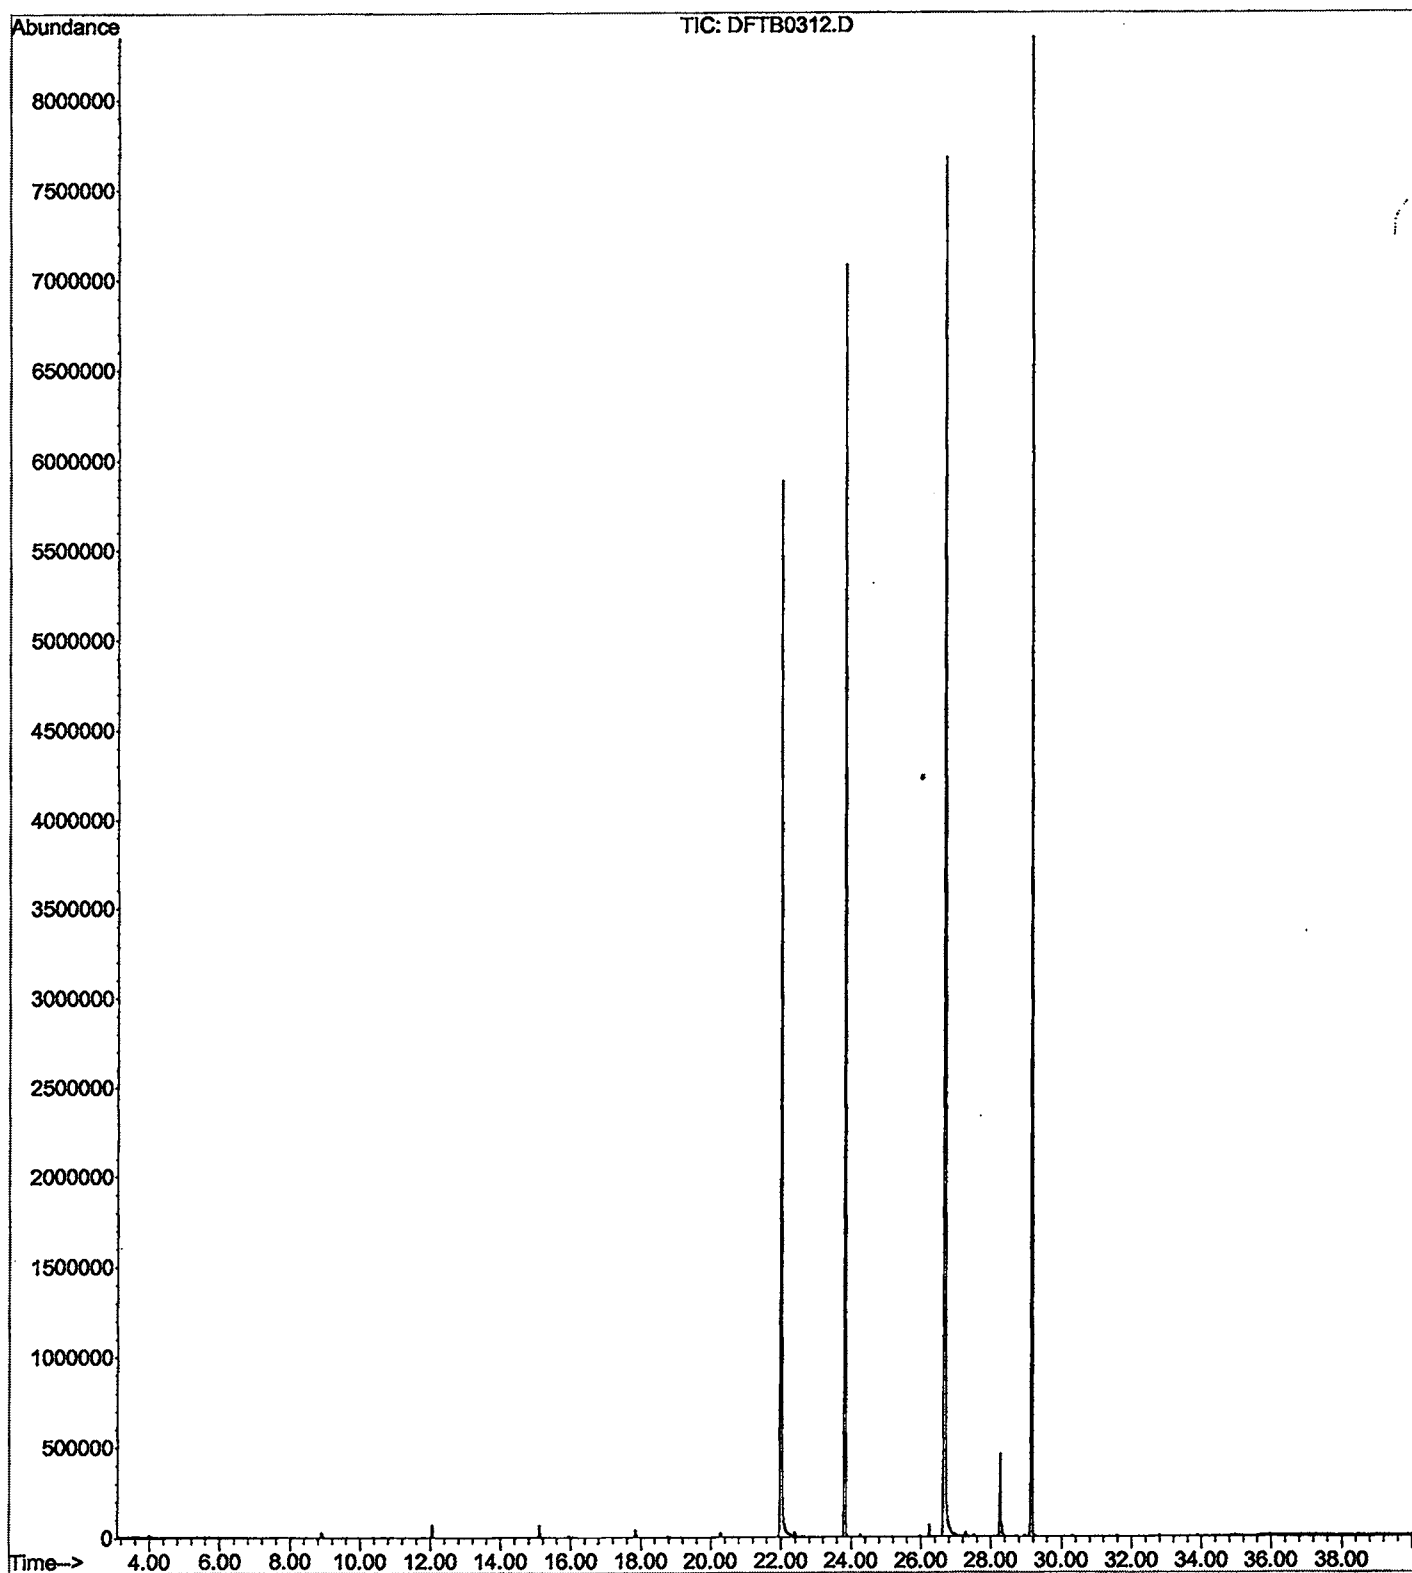

DFTPP

Data File : C:\MSDCHEM\1\DATA\031202\DFTB0312.D

Acq On : 12 Mar 2002 8:13 pm

Sample : DFTPP

Misc :

MS Integration Params: BENZO.P

Vial: 1

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Spectrum Information: Scan 2288

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 51.7         | 426176     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 5391       | PASS                |
| 69             | 198             | 0.00            | 100             | 43.7         | 360640     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 1637       | PASS                |
| 127            | 198             | 10              | 80              | 48.0         | 395712     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 50              | 100             | 100.0        | 824896     | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 53272      | PASS                |
| 275            | 198             | 10              | 60              | 22.2         | 183104     | PASS                |
| 365            | 198             | 1               | 100             | 2.6          | 21528      | PASS                |
| 441            | 443             | 0.01            | 100             | 80.2         | 101360     | PASS                |
| 442            | 198             | 50              | 100             | 83.1         | 685568     | PASS                |
| 443            | 442             | 15              | 24              | 18.4         | 126400     | PASS                |

DFTB0312.D 5080302.M

Thu Mar 14 12:46:35 2002