



User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 03/29/2002 Time: 10:41:55

Sample: AE03618
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 3/29/02 10:41 Ended: 3/29/02 10:41 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surf 2,4-DDD	USPEC	131		5.0

Comments for Sample AE03618 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 03-29-2002 Time: 10:42:04

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recoveries for 5 of the 43 compounds in the LCS Standard were outside of their acceptance limits. New limits will be calculated.

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\031202\3618.D

Acq On : 13 Mar 2002 1:07 am

Sample : FB 2/19/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Mar 15 14:01:40 2002

Vial: 55

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080302.RES

Quant Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Thu Mar 14 13:02:27 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.54	150	1497739	20.00	ug/L	0.00
10) Naphthalene-d8	13.03	136	4082669	20.00	ug/L	0.00
17) Acenaphthene-d10	18.13	164	2290116	20.00	ug/L	0.00
29) Phenanthrene-d10	22.50	188	3537738	20.00	ug/L	0.00
38) Chrysene-d12	30.31	240	3447771	20.00	ug/L	0.00
44) Perylene-d12	34.19	264	2245067	20.00	ug/L	0.00

System Monitoring Compounds

37) 2,4-ddd surr	27.43	235	275583	6.53	ug/L	0.00
Spiked Amount	5.000		Recovery	= 130.60%		

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	3.24	74	7446	0.22 ug/L	100
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D. d	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
32) Hexachlorobenzene	0.00	284	0	N.D.	
33) Phenanthrene	0.00	178	0	N.D.	
34) Anthracene	0.00	178	0	N.D.	
35) Di-n-butylphthalate	0.00	149	0	N.D. d	
36) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	0.00	149	0	N.D.	
41) Benzo (a) anthracene	0.00	228	0	N.D. d	
42) Bis (2-ethylhexyl) phthala	0.00	149	0	N.D. d	
43) Chrysene	0.00	228	0	N.D. d	
45) Di-n-Octylphthalate	0.00	149	0	N.D.	
46) Benzo (b) fluoranthene	0.00	252	0	N.D.	

(#)=qualifier out of range (m)=manual integration

3618.D 5080302.M Fri Mar 15 14:03:02 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\031202\3618.D

Vial: 55

Acq On : 13 Mar 2002 1:07 am

Operator: McLean

Sample : FB 2/19/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Mar 15 14:01:40 2002

Quant Results File: 5080302.RES

Quant Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Thu Mar 14 13:02:27 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0	N.D.		
48) Benzo (a) pyrene	0.00	252	0	N.D.	d	
49) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
50) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
51) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

3618.D 5080302.M

Fri Mar 15 14:03:02 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\031202\3618.D

Vial: 55

Acq On : 13 Mar 2002 1:07 am

Operator: McLean

Sample : FB 2/19/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Mar 15 14:02 2002


Quant Results File: 5080302.RES

Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Thu Mar 14 13:02:27 2002

Response via : Initial Calibration

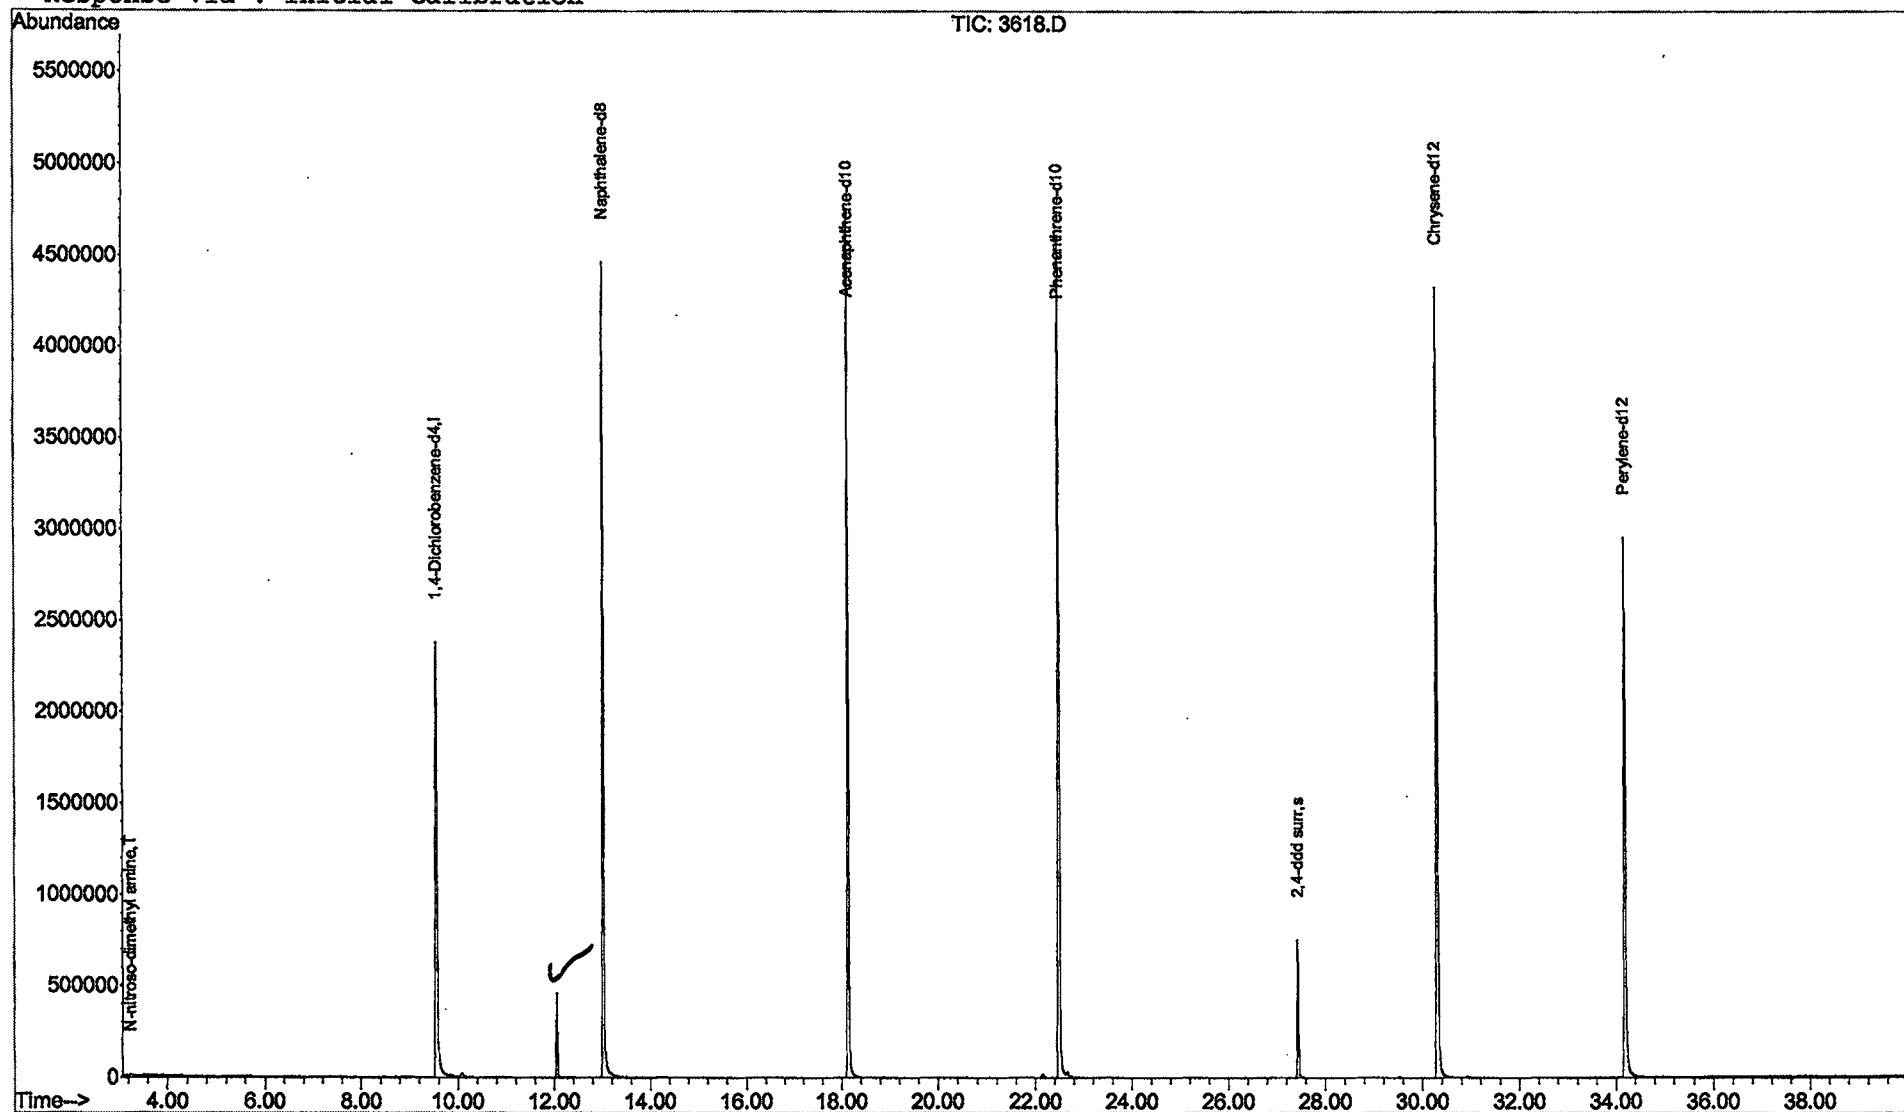

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\031202\3618.D
 Acq On : 13 Mar 2002 1:07 am
 Sample : FB 2/19/02
 Misc :
 MS Integration Params: LSCINT.P

Vial: 55
 Operator: McLean
 Inst : Instrumen
 Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)
 Title : Quantitation For Method 508gcscan
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.543	708	713	739	rBV	2380078	6247114	61.74%	11.578%
2	12.056	984	990	995	rBV2	459037	778214	7.69%	1.442%
3	13.026	1091	1097	1112	rBV	4464474	8736151	86.34%	16.192%
4	18.133	1654	1660	1678	rBV	4745476	9490036	93.79%	17.589%
5	22.496	2135	2141	2155	rBV2	4602129	9772255	96.58%	18.112%
6	27.430	2681	2685	2697	rBV	752817	1433216	14.16%	2.656%
7	30.314	2996	3003	3027	rBV2	4325030	10118141	100.00%	18.753%
8	34.187	3423	3430	3444	rBV2	2956889	7379978	72.94%	13.678%

Sum of corrected areas: 53955105

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\031202\3618.D
 Operator : McLean
 Acquired : 13 Mar 2002 1:07 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: FB 2/19/02
 Misc Info :
 Vial Number: 55
 Quant File :5080302.RES (RTE Integrator)

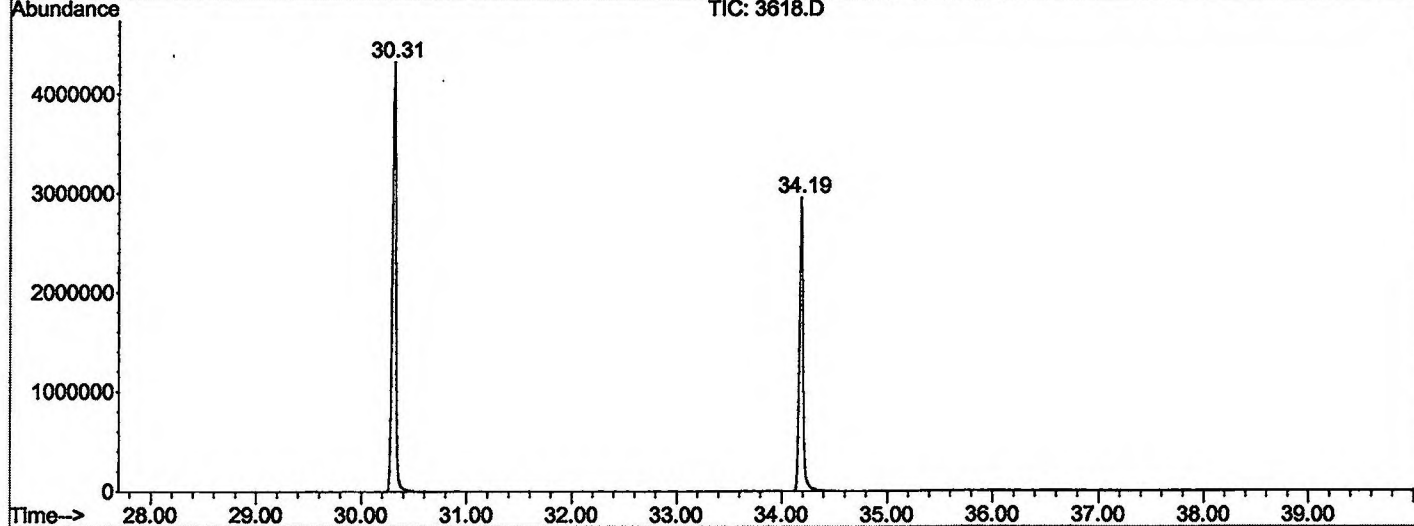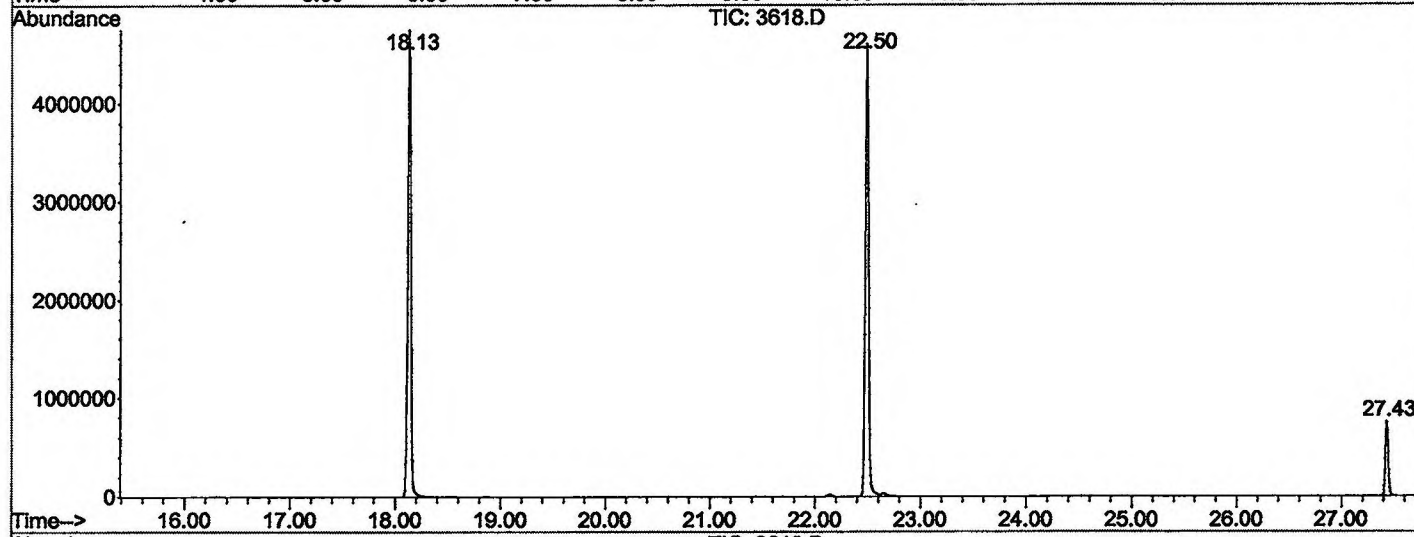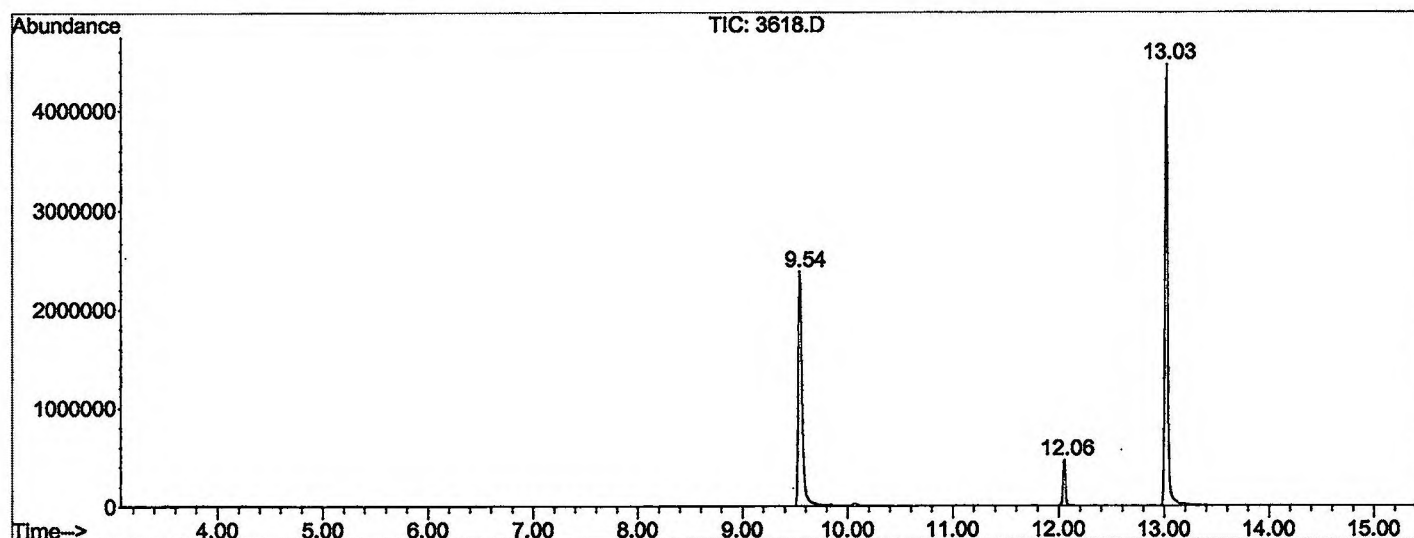

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\031202\3618.D
 Acq On : 13 Mar 2002 1:07 am
 Sample : FB 2/19/02
 Misc :
 MS Integration Params: LSCINT.P










Vial: 55
 Operator: McLean
 Inst : Instrumen
 Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)
 Title : Quantitation For Method 508gcscan
 Library : C:\DATABASE\WILEY7N.L

 Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.06	1.78 ug/L	778214	Naphthalene-d8	13.03

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	68
2			N-(Trifluoroacetyl)-O,O',O''-tris...	495	C20H36F3NO4Si3	054135-51-2	43
3			Benzoic acid, 2-[(trimethylsilyl)...	282	C13H22O3Si2	003789-85-3	38
4			Butanamide, 2,2,3,3,4,4,4-hepta...	493	C18H26F7NO3Si2	055471-01-7	38

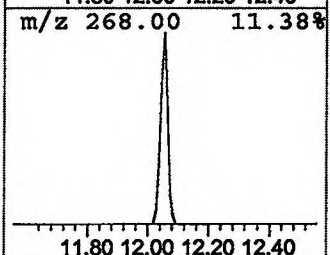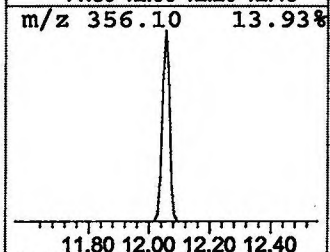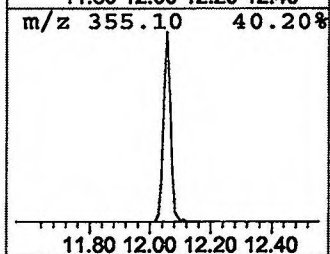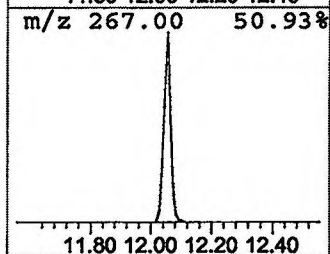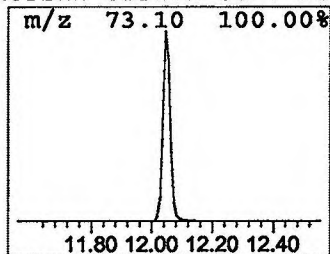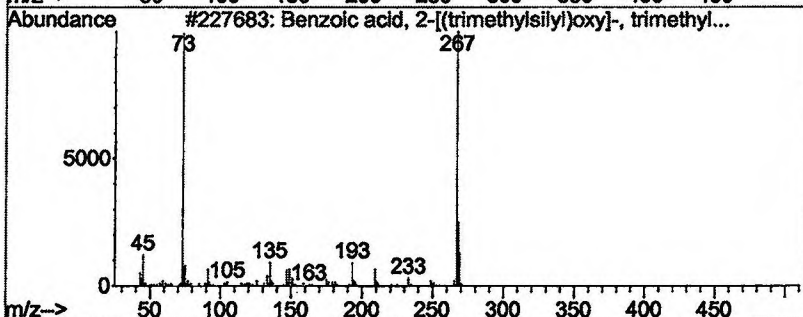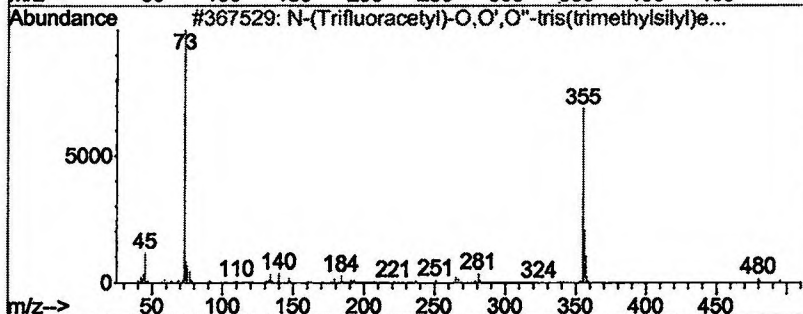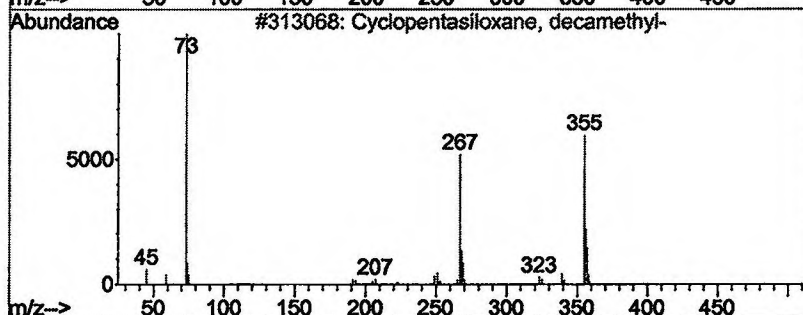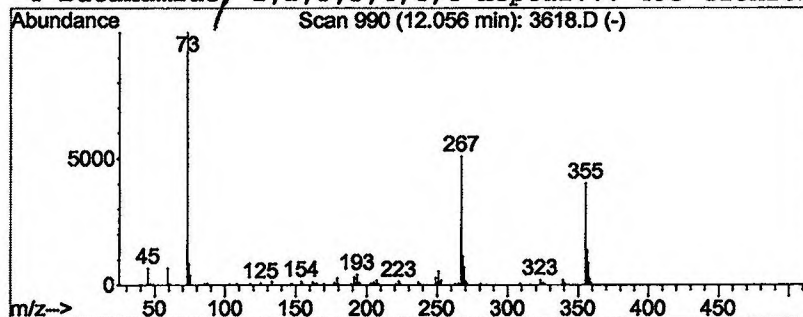

Tentatively Identified Compound (LSC) summary

Operator ID: McLean Date Acquired: 13 Mar 2002 1:07 am
 Data File: C:\MSDCHEM\1\DATA\031202\3618.D
 Name: FB 2/19/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasiloxan...	12.06	1.8 ug/L		778214	2	13.03	8736150	20.0