

Injection Log

Directory: c:\hpcchem\1\data\feb2102

ne	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
	1	dftpp.d	1.			21 Feb 02 12:29
	2	cal40.d	1.			21 Feb 02 14:06
	29	surr.d	1.			21 Feb 02 15:05
	3	lb.d	1.	gc/ms scan 1/22		21 Feb 02 16:03
	4	ref.d	1.	gc/ms scan 1/22		21 Feb 02 17:02
	5	1329.d	1.	gc/ms scan 1/22		21 Feb 02 18:01
	6	472.d	1.	gc/ms scan 1/22		21 Feb 02 19:01
	7	1435.d	1.	gc/ms scan 1/22		21 Feb 02 20:00
	8	1436.d	1.	gc/ms scan 1/22		21 Feb 02 21:00
	9	1437.d	1.	gc/ms scan 1/22		21 Feb 02 21:59
	10	1438.d	1.	gc/ms scan 1/22		21 Feb 02 22:58
	11	1439.d	1.	gc/ms scan 1/22		21 Feb 02 23:57
	12	1440.d	1.	gc/ms scan 1/22		22 Feb 02 00:56
	13	1441.d	1.	gc/ms scan 1/22		22 Feb 02 01:55
	14	1442.d	1.	gc/ms scan 1/22		22 Feb 02 02:54
	15	1462.d	1.	gc/ms scan 1/22		22 Feb 02 03:53
	1	dftpp2.d	1.	gc/ms scan 1/22		22 Feb 02 04:52
	2	cal40a.d	1.	gc/ms scan 1/22		22 Feb 02 05:51
	16	lba.d	1.	gc/ms scan 1/22		22 Feb 02 06:50
	17	refa.d	1.	gc/ms scan 1/22		22 Feb 02 07:49
	18	1463.d	1.	gc/ms scan 1/22		22 Feb 02 08:48
	19	1464.d	1.	gc/ms scan 1/22		22 Feb 02 09:47
	20	1465.d	1.	gc/ms scan 1/22		22 Feb 02 10:47
	21	1498.d	1.	gc/ms scan 1/22		22 Feb 02 11:46
	22	1499.d	1.	gc/ms scan 1/22		22 Feb 02 12:45
	23	1500.d	1.	gc/ms scan 1/22		22 Feb 02 13:44
	24	1501.d	1.	gc/ms scan 1/22		22 Feb 02 14:43
	25	1502.d	1.	gc/ms scan 1/22		22 Feb 02 15:43
	26	1503.d	1.	gc/ms scan 1/22		22 Feb 02 16:46
	27	1504.d	1.	gc/ms scan 1/22		22 Feb 02 17:45
	28	1505.d	1.	gc/ms scan 1/22		22 Feb 02 18:45
	30	lbb.d	1.	gc/ms scan 2/21		22 Feb 02 19:44
	31	refb.d	1.	gc/ms scan 2/21		22 Feb 02 20:43
	32	refb2.d	1.	gc/ms scan 2/21		22 Feb 02 21:42
	33	31549.d	1.	gc/ms scan 2/21		22 Feb 02 22:41
	34	31587.d	1.	gc/ms scan 2/21		22 Feb 02 23:40
	35	31499.d	1.	gc/ms scan 2/21		23 Feb 02 00:39
	36	31498.d	1.	gc/ms scan 2/21		23 Feb 02 01:38
	37	31551.d	1.	gc/ms scan 2/21		23 Feb 02 02:37
	38	31591.d	1.	gc/ms scan 2/21		23 Feb 02 03:36
	39	31589.d	1.	gc/ms scan 2/21		23 Feb 02 04:35
	40	31590.d	1.	gc/ms scan 2/21		23 Feb 02 05:34
	41	31588.d	1.	gc/ms scan 2/21		23 Feb 02 06:33
	42	31592.d	1.	gc/ms scan 2/21		23 Feb 02 07:32
	43	31630.d	1.	gc/ms scan 2/21 fb		23 Feb 02 08:31
	1	dftpp3.d	1.			23 Feb 02 09:29
	2	cal40b.d	1.			23 Feb 02 10:28
	44	lbc.d	1.	gc/ms scan 1/14		23 Feb 02 11:27
	45	refc.d	1.	gc/ms scan 1/14		23 Feb 02 12:27
	46	refc2.d	1.	gc/ms scan 1/14		23 Feb 02 13:26
	47	3385.d	1.	gc/ms scan 1/14		23 Feb 02 14:25
	48	3386.d	1.	gc/ms scan 1/14		23 Feb 02 15:24
	49	3387.d	1.	gc/ms scan 1/14		23 Feb 02 16:23
	50	3388.d	1.	gc/ms scan 1/14		23 Feb 02 17:22
	51	3389.d	1.	gc/ms scan 1/14		23 Feb 02 18:21
	52	3390.d	1.	gc/ms scan 1/14		23 Feb 02 19:20
	53	3391.d	1.	gc/ms scan 1/14		23 Feb 02 20:19

Original
Sequence log
accidentally
overwritten

using this
3/14/2 Don

Injection Log

Directory: c:\hpchem\1\data\feb2102

ie	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
	54	3434.d	1.	gc/ms scan 1/14		23 Feb 02 21:18
	55	3435.d	1.	gc/ms scan 1/14		23 Feb 02 22:17
	56	3436.d	1.	gc/ms scan 1/14		23 Feb 02 23:16
	57	lbd.d	1.	gc/ms scan 2/21		24 Feb 02 00:14
	58	refd.d	1.	gc/ms scan 2/21		24 Feb 02 01:13
	59	refd2.d	1.	gc/ms scan 2/21		24 Feb 02 02:12
	60	938.d	1.	gc/ms scan 2/21		24 Feb 02 03:10
	61	939.d	1.	gc/ms scan 2/21		24 Feb 02 04:09
	62	940.d	1.	gc/ms scan 2/21		24 Feb 02 05:08
	63	941.d	1.	gc/ms scan 2/21		24 Feb 02 06:06
	64	942.d	1.	gc/ms scan 2/21		24 Feb 02 07:05
	65	1143.d	1.	gc/ms scan 2/21		24 Feb 02 08:04
	66	1153.d	1.	gc/ms scan 2/21		24 Feb 02 09:02
	67	1155.d	1.	gc/ms scan 2/21		24 Feb 02 10:01
	68	1154.d	1.	gc/ms scan 2/21		24 Feb 02 11:00
	69	1137.d	1.	gc/ms scan 2/21		24 Feb 02 11:59
	1	dfpp4.d	1.			24 Feb 02 12:58
	2	cal40c.d	1.			24 Feb 02 13:56
	70	lbe.d	1.	gc/ms scan 2/22		24 Feb 02 14:55
	71	refe.d	1.	gc/ms scan 2/22		24 Feb 02 15:54
	72	refe2.d	1.	gc/ms scan 2/22		24 Feb 02 16:53
	73	3833.d	1.	gc/ms scan 2/22		24 Feb 02 17:52
	74	3834.d	1.	gc/ms scan 2/22		24 Feb 02 18:51
	75	3835.d	1.	gc/ms scan 2/22 fb		24 Feb 02 19:50
	76	3914.d	1.	gc/ms scan 2/22		24 Feb 02 20:48
	77	3915.d	1.	gc/ms scan 2/22		24 Feb 02 21:47
	78	3916.d	1.	gc/ms scan 2/22 fb		24 Feb 02 22:46
	79	4024.d	1.	gc/ms scan 2/22		24 Feb 02 23:45
	80	4025.d	1.	gc/ms scan 2/22		25 Feb 02 00:43
	81	4026.d	1.	gc/ms scan 2/22		25 Feb 02 01:42
	82	4027.d	1.	gc/ms scan 2/22		25 Feb 02 02:41

DFTPP

Data File : C:\HPCHEM\1\DATA\FEB2102\DFTPP4.D

Acq On : 24 Feb 2002 12:58 pm

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

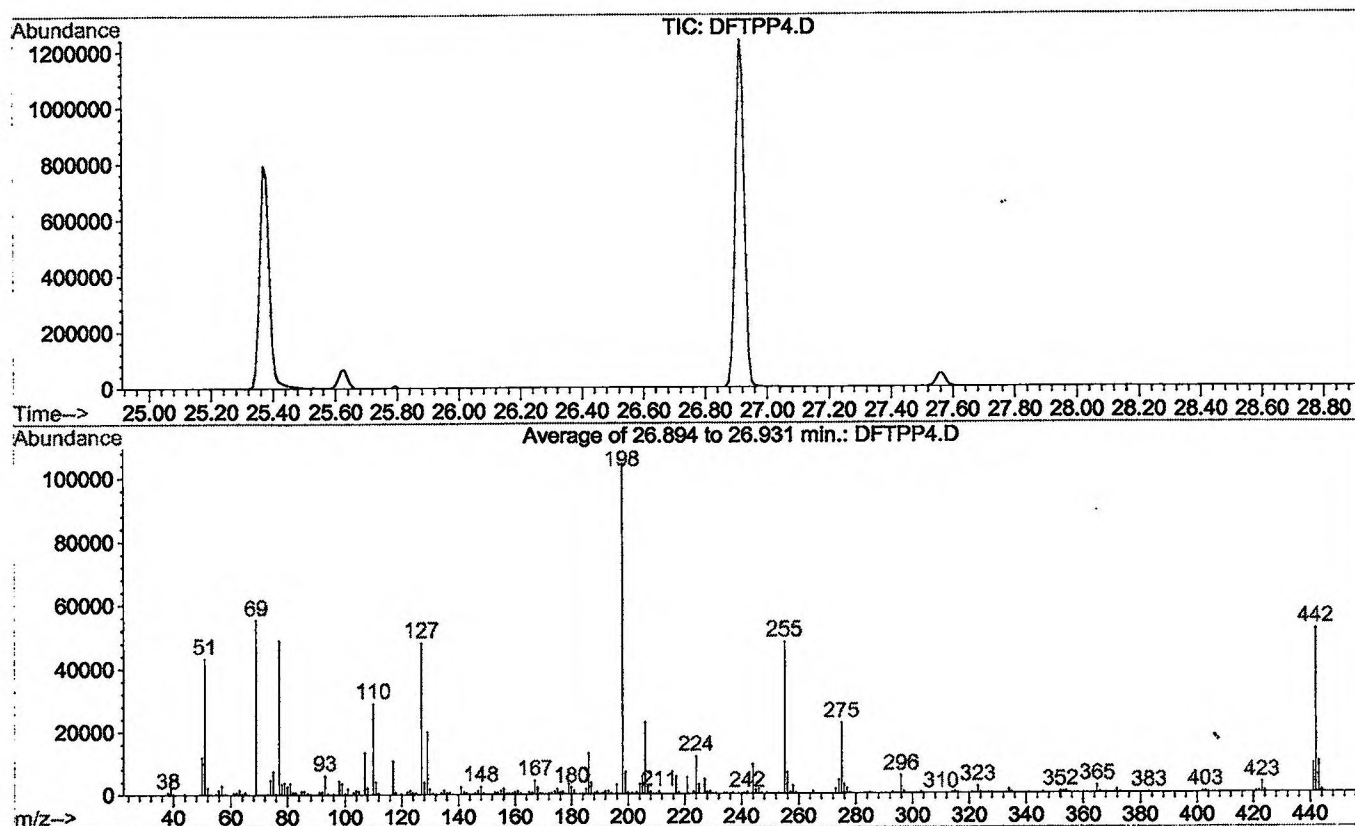

Spectrum Information: Average of 26.894 to 26.931 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	41.6	43429	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	53.2	55421	PASS
70	69	0.00	2	0.1	34	PASS
127	198	40	60	46.3	48266	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	104272	PASS
199	198	5	9	6.8	7126	PASS
275	198	10	30	21.7	22610	PASS
365	198	1	100	2.4	2452	PASS
441	443	0.01	100	93.4	9365	PASS
442	198	40	110	49.9	51982	PASS
443	442	17	23	19.3	10032	PASS

DFTPP4.D GCMS0208.M

Wed Mar 13 10:59:43 2002