

Jser: Fakhouri, Morgan
 Vestchester Dept. of Labs & Research
 Date: 03/13/2002 Time: 11:32:01

Sample: AE03454
 Analysis: \$B1GCMS Blank for GCMS Scan
 Units: ug
 Started: 3/13/02 11:31 Ended: 3/13/02 11:31 Analyst: MF
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	n-Nitrosodimethylamine		< MDL		2.0
2	bis(2-Chloroethyl)ether		< MDL		2.0
3	1,3-Dichlorobenzene		< MDL		2.0
4	1,4-Dichlorobenzene		< MDL		2.0
5	1,2-Dichlorobenzene		< MDL		2.0
6	2,2'-oxybis(1-Chloropropane)		< MDL		2.0
7	n-Nitrosodi-n-propylamine		< MDL		2.0
8	Hexachloroethane		< MDL		2.0
9	Nitrobenzene		< MDL		2.0
10	Isophorone		< MDL		2.0
11	bis(2-Chloroethoxy)methane		< MDL		2.0
12	1,2,4-Trichlorobenzene		< MDL		2.0
13	Naphthalene		< MDL		2.0
14	Hexachlorobutadiene		< MDL		2.0
15	2-Chloronaphthalene		< MDL		2.0
16	Dimethylphthalate		< MDL		2.0
17	2,6-Dinitrotoluene		< MDL		2.0
18	Acenaphthylene		< MDL		2.0
19	Acenaphthene		< MDL		2.0
20	2,4-Dinitrotoluene		< MDL		2.0
21	Diethylphthalate		< MDL		2.0
22	4-Chlorophenylphenylether		< MDL		2.0
23	Fluorene		< MDL		2.0
24	Azobenzene/1,2-Diphenylhydraz		< MDL		2.0
25	n-Nitrosodiphenylamine		< MDL		2.0
26	4-Bromophenylphenylether		< MDL		2.0
27	Hexachlorobenzene		< MDL		2.0
28	Phenanthrene		< MDL		2.0
29	Anthracene		< MDL		2.0
30	Di-n-butylphthalate		< MDL		2.0
31	Fluoranthene		< MDL		2.0
32	Pyrene		< MDL		2.0
33	Butylbenzylphthalate		< MDL		2.0
34	Benzo(a)anthracene		< MDL		2.0
35	bis(2-Ethylhexyl)phthalate		< MDL		2.0
36	Chrysene		< MDL		2.0
37	Di-n-octylphthalate		< MDL		2.0
38	Benzo(b)fluoranthene		< MDL		2.0
39	Benzo(k)fluoranthene		< MDL		2.0
40	Benzo(a)pyrene		< MDL		2.0
41	Indeno(1,2,3-cd)pyrene		< MDL		2.0
42	Dibenz(a,h)anthracene		< MDL		2.0
43	Benzo(g,h,i)perylene		< MDL		2.0

Data File : C:\MSDCHEM\1\DATA\022802\0226LB.D

Vial: 6

Acq On : 28 Feb 2002 3:05 pm

Operator: McLean

Sample : GC MS SCAN 2/27

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Mar 13 06:39:56 2002

Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.58	150	1109289	20.00	ug/L	0.00
10) Naphthalene-d8	13.05	136	2907742	20.00	ug/L	0.00
17) Acenaphthene-d10	18.16	164	1636799	20.00	ug/L	0.00
29) Phenanthrene-d10	22.52	188	2498938	20.00	ug/L	0.00
38) Chrysene-d12	30.34	240	2345323	20.00	ug/L	-0.02
44) Perylene-d12	34.21	264	1459711	20.00	ug/L	0.00

System Monitoring Compounds

37) 2,4-ddd surr	27.46	235	213713	5.39	ug/L	0.00
Spiked Amount	5.000		Recovery	=	107.80%	

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.		
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.		
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.		
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	0.00	128	0	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	18.16	165	211255	9.28	ug/L #	25
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
25) Diethylphthalate	0.00	149	0	N.D.		
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
28) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.		
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	0.00	149	0	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo (a) anthracene	0.00	228	0	N.D. d		
42) Bis (2-ethylhexyl) phthala	30.94	149	25143	0.24	ug/L	93
43) Chrysene	0.00	228	0	N.D. d		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo (b) fluoranthene	0.00	252	0	N.D.		

(#)=qualifier out of range (m)=manual integration

0226LB.D 5080202.M Wed Mar 13 06:40:54 2002

Data File : C:\MSDCHEM\1\DATA\022802\0226LB.D

Vial:- 6

Acq On : 28 Feb 2002 3:05 pm

Operator: McLean

Sample : GC MS SCAN 2/27

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Mar 13 06:39:56 2002

Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0	N.D.		
48) Benzo (a) pyrene	0.00	252	0	N.D.	d	
49) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
50) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
51) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

0226LB.D 5080202.M Wed Mar 13 06:40:54 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\022802\0226LB.D

Acq On : 28 Feb 2002 3:05 pm

Sample : GC MS SCAN 2/27

Misc :

MS Integration Params: BENZO.P

Quant Time: Mar 13 6:40 2002

Vial: 6

Operator: McLean

Inst : Instrumen

Multiplr: 1.00


Quant Results File: 5080202.RES

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

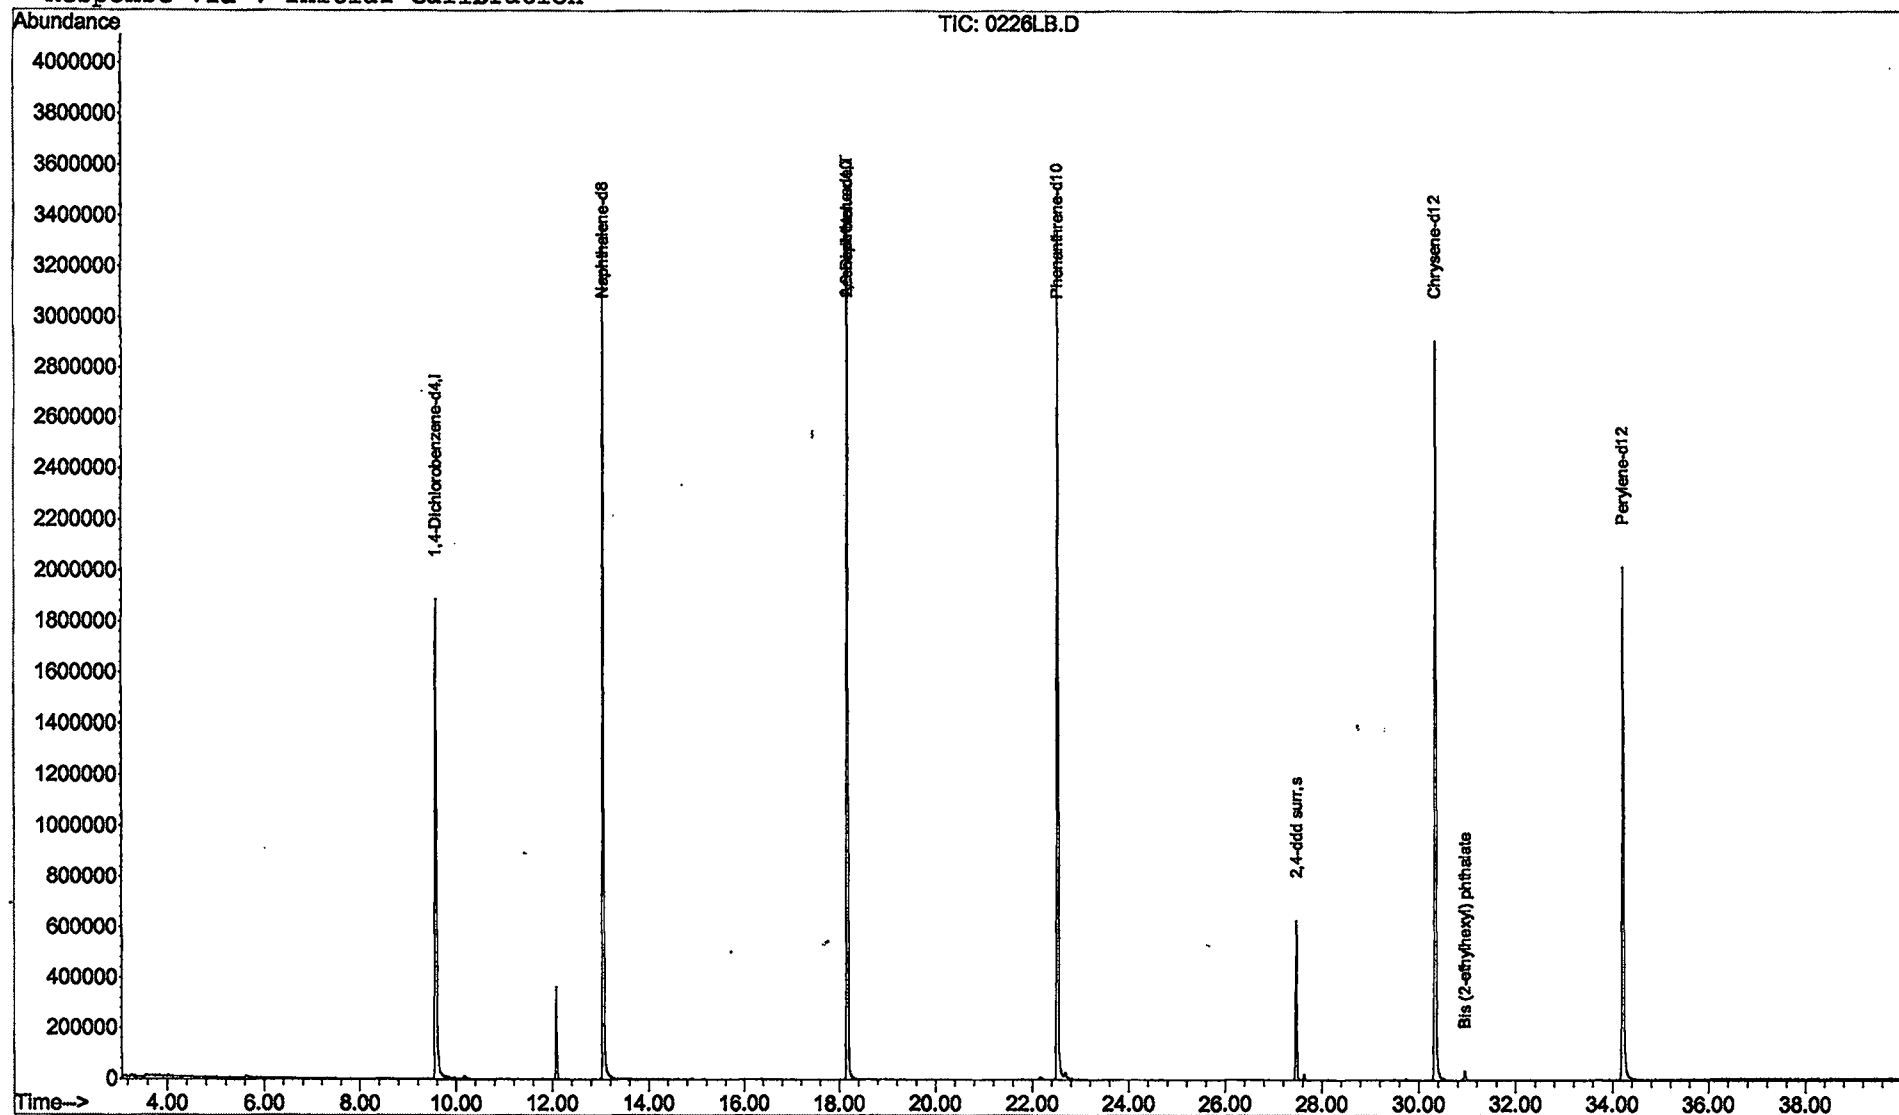

0226LB.D 5080202.M

Wed Mar 13 06:40:55 2002

Data File : C:\MSDCHEM\1\DATA\022802\0226LB.D

Vial: 6

Acq On : 28 Feb 2002 3:05 pm

Operator: McLean

Sample : GC MS SCAN 2/27

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.579	712	717	738	rBV	1886830	4646191	67.72%	12.226%
2	12.083	988	993	1000	rBV	363930	565427	8.24%	1.488%
3	13.053	1095	1100	1116	rBV	3368242	6301390	91.84%	16.582%
4	18.160	1658	1663	1684	rBV	3424077	6775303	98.75%	17.829%
5	22.523	2138	2144	2156	rBV2	3345896	6860967	100.00%	18.054%
6	22.677	2158	2161	2171	rVB3	25489	79069	1.15%	0.208%
7	27.457	2684	2688	2696	rBB	630714	1127807	16.44%	2.968%
8	30.332	2998	3005	3020	rBV	2912054	6763255	98.58%	17.797%
9	30.940	3069	3072	3077	rVB2	37573	72069	1.05%	0.190%
10	34.214	3425	3433	3450	rBV2	2018675	4810393	70.11%	12.658%

Sum of corrected areas: 38001871

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\022802\0226LB.D
 Operator : McLean
 Acquired : 28 Feb 2002 3:05 pm using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: GC MS SCAN 2/27
 Misc Info :
 Vial Number: 6
 Quant File : 5080202.RES (RTE Integrator)

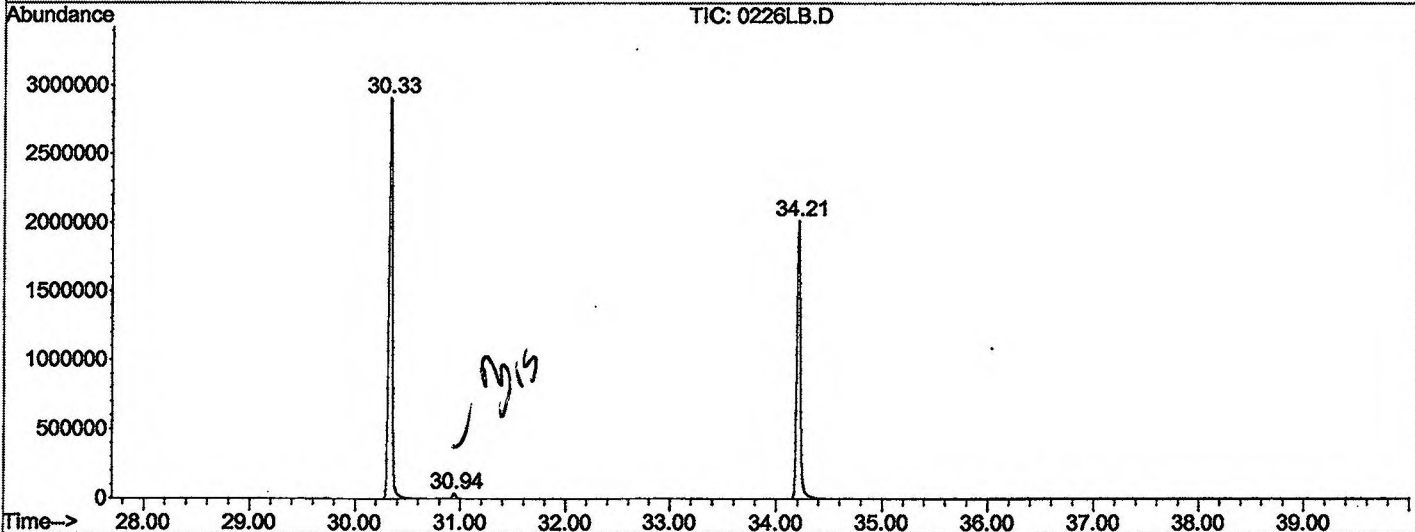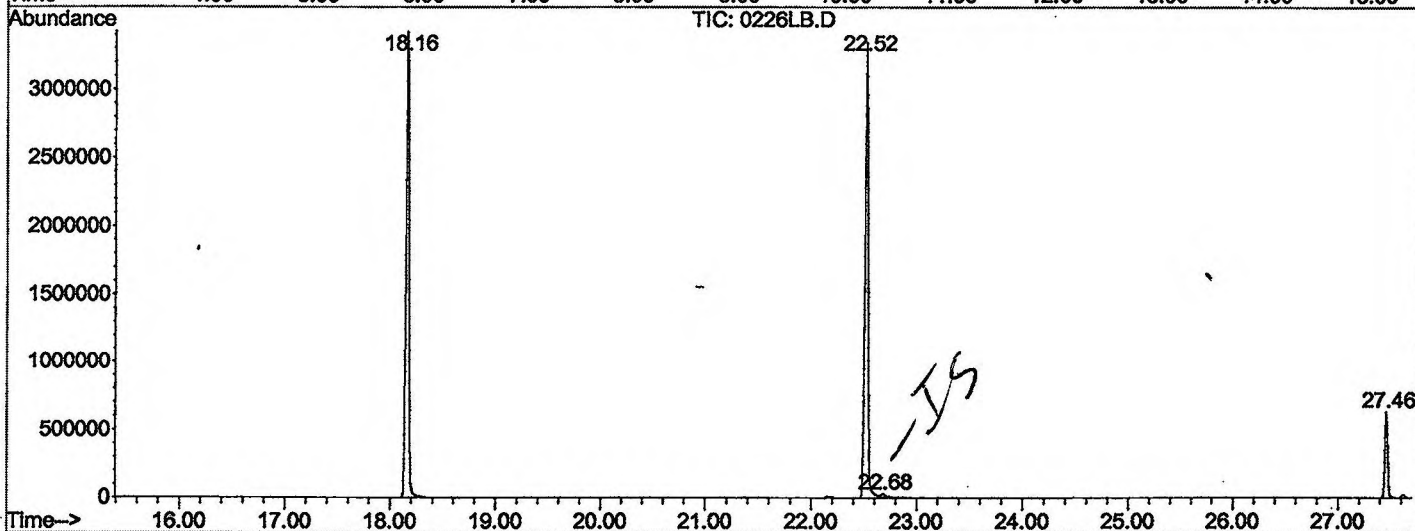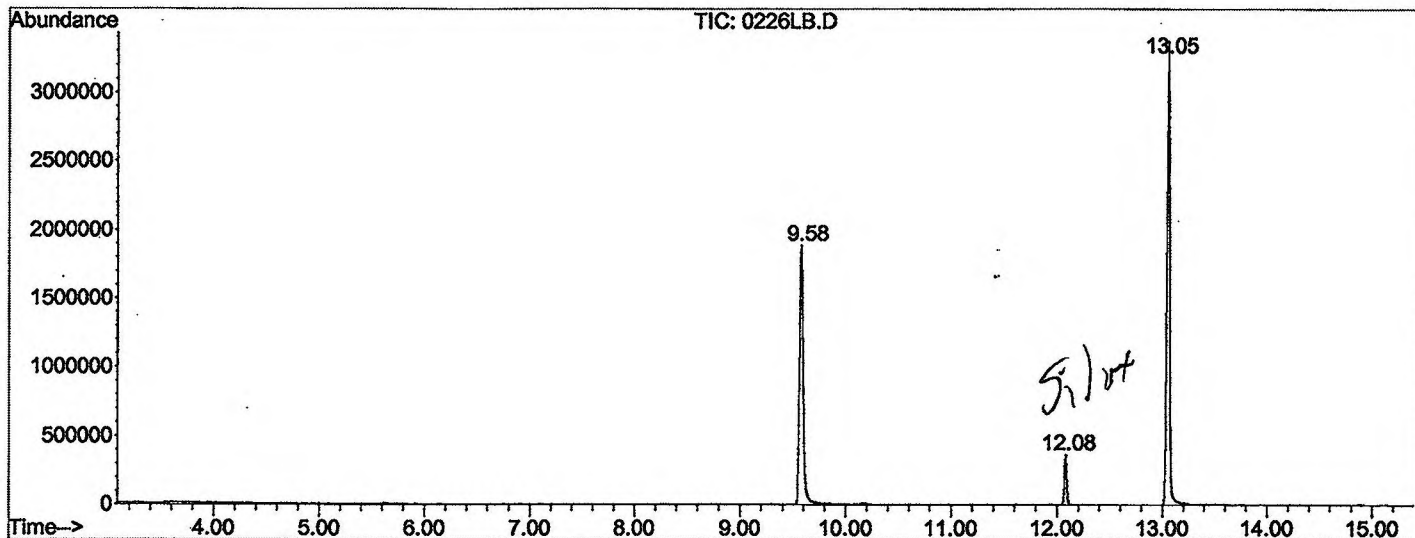

Data File : C:\MSDCHEM\1\DATA\022802\0226LB.D
Acq On : 28 Feb 2002 3:05 pm
Sample : GC MS SCAN 2/27
Misc :
MS Integration Params: LSCINT.P










Vial: 6
Operator: McLean
Inst : Instrumen
Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Library : C:\DATABASE\WILEY7N.L

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.08	1.79 ug/L	565427	Naphthalene-d8	13.05

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	91
2		Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	58
3		Benzoic acid, 2-[(trimethylsilyl)-	282	C13H22O3Si2	003789-85-3	47
4		Phenethylamine, N-methyl-.beta.,...	399	C18H37NO3Si3	010538-85-9	38

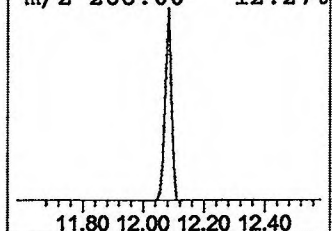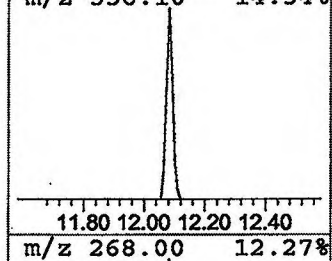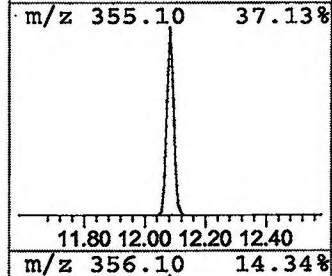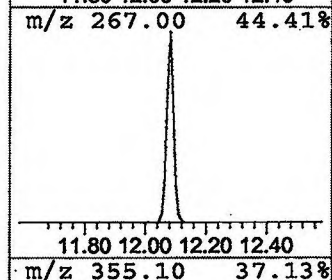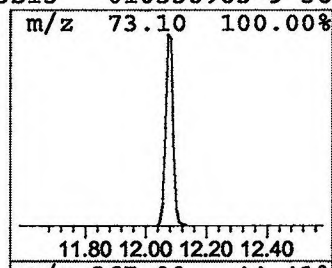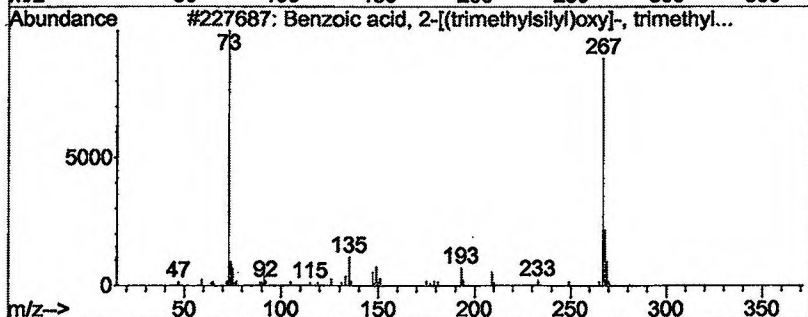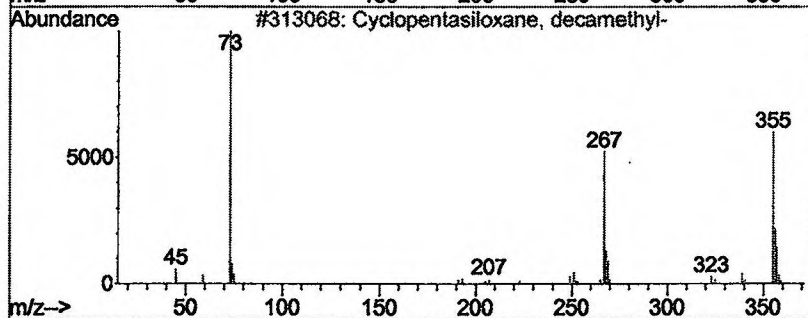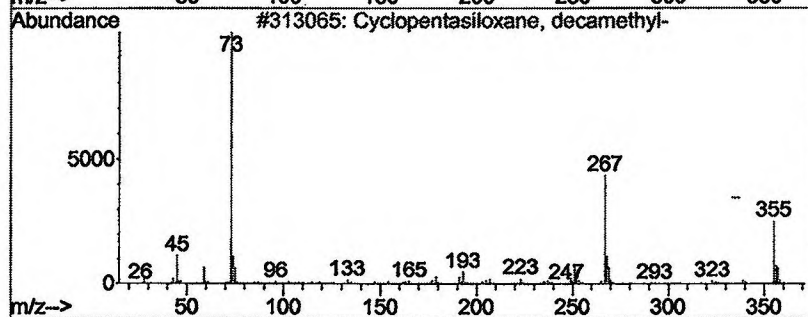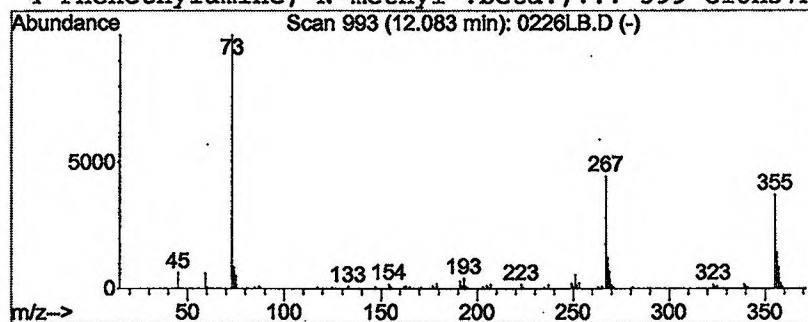

Operator ID: McLean Date Acquired: 28 Feb 2002 3:05 pm
 Data File: C:\MSDCHEM\1\DATA\022802\0226LB.D
 Name: GC MS SCAN 2/27
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
Cyclopentasiloxan...	12.08	1.8	ug/L	565427	2	13.05	6301390	20.0