

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 03/14/2002 Time: 16:55:51

Sample: AE03454
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 3/14/02 16:55 Ended: 3/14/02 16:55 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		97		5.0

Comments for Sample AE03454 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 03-14-2002 Time: 16:56:51

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recoveries for 2 of the 43 compounds in the LCS Standard were outside their acceptance ranges.

Data File : C:\MSDCHEM\1\DATA\022802\03454FB.D

Vial: 29

Acq On : 1 Mar 2002 11:32 am

Operator: McLean

Sample : MS CSAN FB Q

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Mar 13 06:52:18 2002

Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.58	150	1184911	20.00	ug/L	0.00
10) Naphthalene-d8	13.05	136	3148201	20.00	ug/L	0.00
17) Acenaphthene-d10	18.16	164	1750722	20.00	ug/L	0.00
29) Phenanthrene-d10	22.52	188	2629225	20.00	ug/L	0.00
38) Chrysene-d12	30.33	240	2331481	20.00	ug/L	-0.03
44) Perylene-d12	34.21	264	1588060	20.00	ug/L	0.00

System Monitoring Compounds

37) 2,4-ddd surr	27.46	235	201700	4.83	ug/L	0.00
Spiked Amount	5.000		Recovery	=	96.60%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2 ' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D. d	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
32) Hexachlorobenzene	0.00	284	0	N.D.	
33) Phenanthrene	0.00	178	0	N.D.	
34) Anthracene	0.00	178	0	N.D.	
35) Di-n-butylphthalate	24.67	149	2534	0.01 ug/L	79
36) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	0.00	149	0	N.D.	
41) Benzo (a) anthracene	0.00	228	0	N.D. d	
42) Bis (2-ethylhexyl) phthala	30.94	149	54926	0.52 ug/L	98
43) Chrysene	0.00	228	0	N.D. d	
45) Di-n-Octylphthalate	0.00	149	0	N.D.	
46) Benzo (b) fluoranthene	0.00	252	0	N.D.	

(#)= qualifier out of range (m) = manual integration

03454FB.D 5080202.M Wed Mar 13 06:53:18 2002

Page 1

Data File : C:\MSDCHEM\1\DATA\022802\03454FB.D

Vial: 29

Acq On : 1 Mar 2002 11:32 am

Operator: McLean

Sample : MS CSAN FB Q

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Mar 13 06:52:18 2002

Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0	N.D.		
48) Benzo (a) pyrene	0.00	252	0	N.D. d		
49) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
50) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
51) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

03454FB.D 5080202.M Wed Mar 13 06:53:18 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\022802\03454FB.D

Acq On : 1 Mar 2002 11:32 am

Sample : MS CSAN FB Q

Misc :

MS Integration Params: BENZO.P

Quant Time: Mar 13 6:53 2002

Vial: 29

Operator: McLean

Inst : Instrumen

Multiplr: 1.00


Quant Results File: 5080202.RES

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

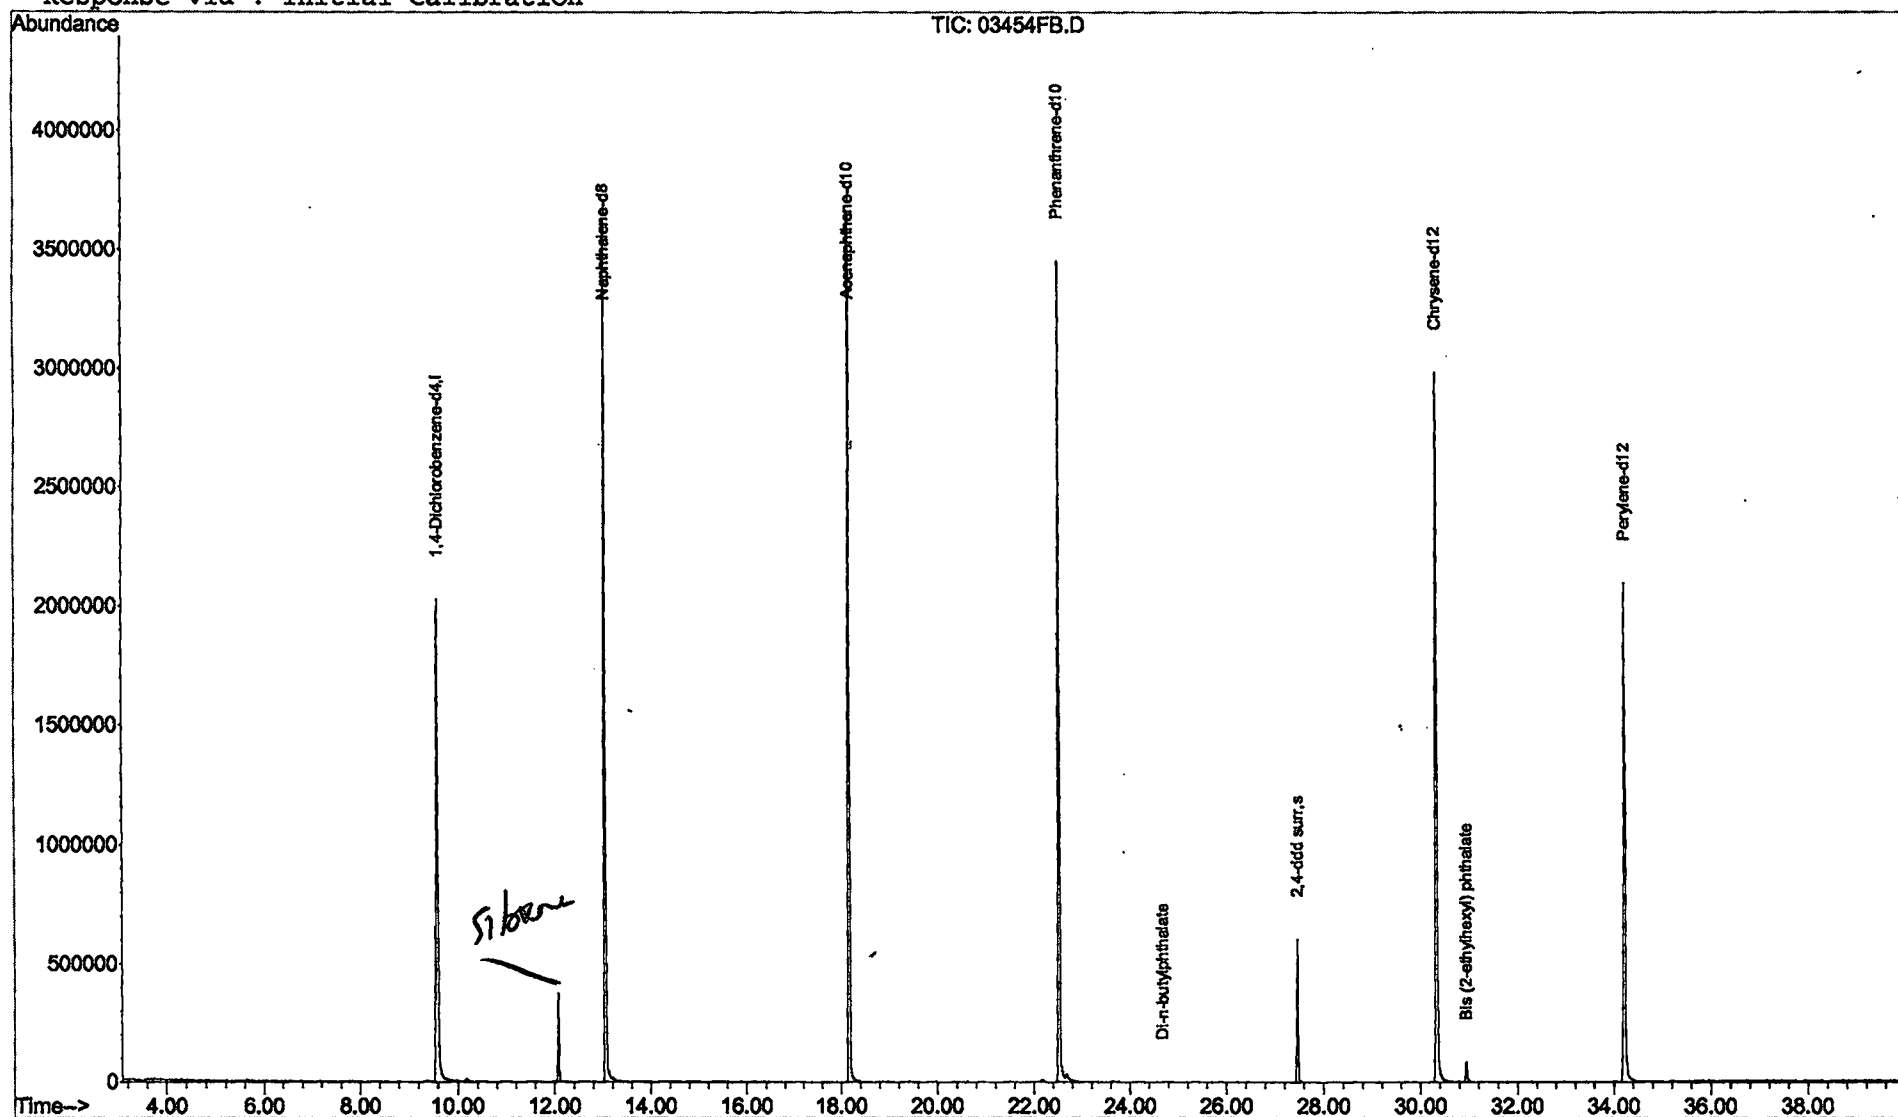

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\022802\03454FB.D

Vial: 29

Acq On : 1 Mar 2002 11:32 am

Operator: McLean

Sample : MS CSAN FB Q

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.579	712	717	738	rBV	2026121	5026022	69.01%	12.474%
2	12.083	988	993	997	rBV	376229	614803	8.44%	1.526%
3	13.053	1095	1100	1113	rBV	3620135	6781881	93.11%	16.832%
4	18.160	1657	1663	1677	rBV	3659006	7283455	100.00%	18.077%
5	22.523	2138	2144	2158	rBV2	3452932	7242802	99.44%	17.976%
6	22.677	2158	2161	2170	rVB	26140	74081	1.02%	0.184%
7	27.457	2684	2688	2700	rVB	603474	1054093	14.47%	2.616%
8	30.332	2998	3005	3025	rBV2	2983223	6827822	93.74%	16.947%
9	30.940	3067	3072	3080	rBV	82988	183083	2.51%	0.454%
10	34.214	3425	3433	3456	rBV2	2095166	5202377	71.43%	12.912%

Sum of corrected areas: 40290419

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\022802\03454FB.D
 Operator : McLean
 Acquired : 1 Mar 2002 11:32 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: MS CSAN FB Q
 Misc Info :
 Vial Number: 29
 Quant File :5080202.RES (RTE Integrator)

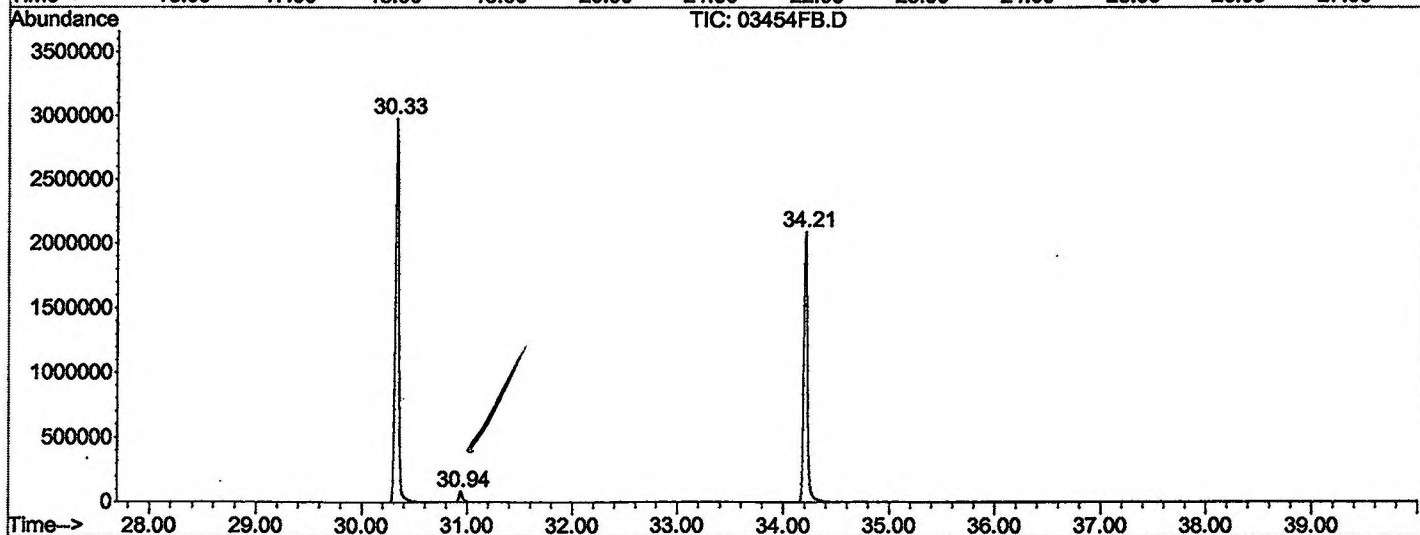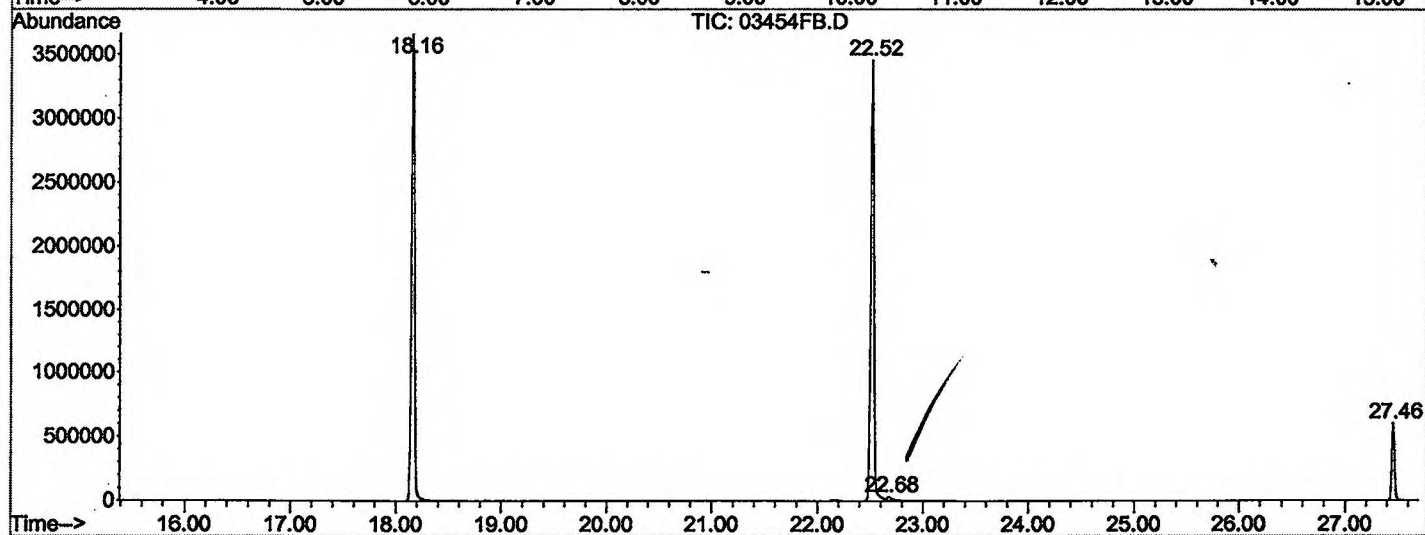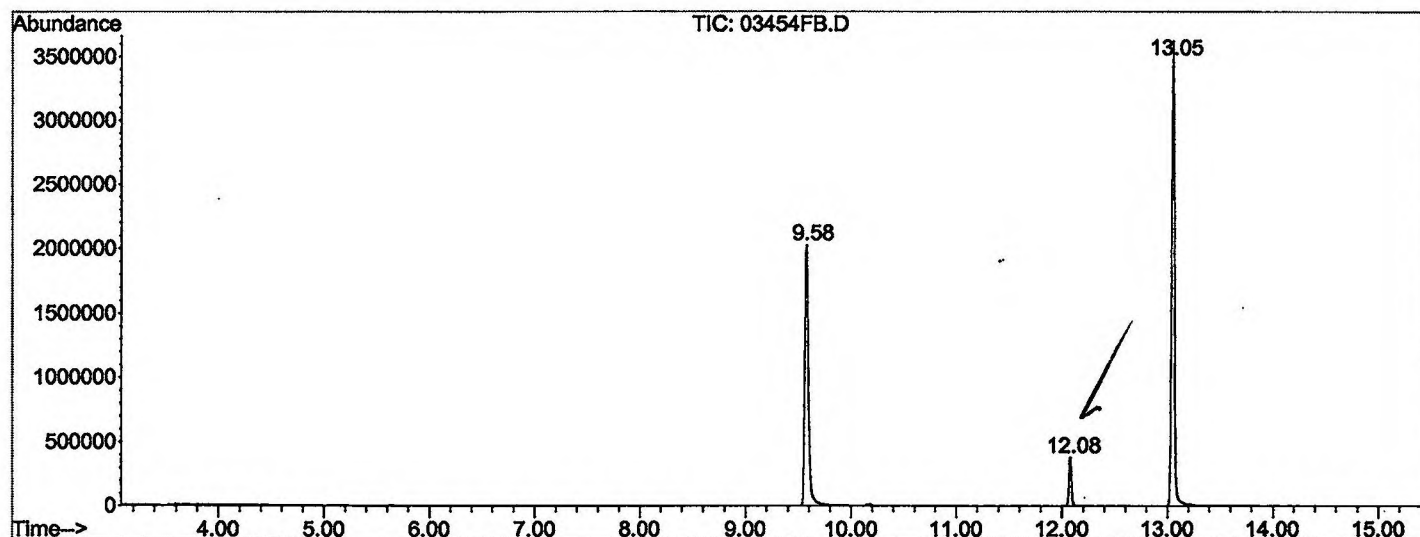

Data File : C:\MSDCHEM\1\DATA\022802\03454FB.D

Acq On : 1 Mar 2002 11:32 am

Sample : MS CSAN FB Q

Misc :

MS Integration Params: LSCINT.P

Vial: 29

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)










Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.08	1.81 ug/L	614803	Naphthalene-d8	13.05

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	74
2			N-(Trifluoroacetyl)-N,O,O',O''-t...	553	C22H42F3NO4Si4	000000-00-0	47
3			Benzeneethanamine, N-[(pentafluo...	563	C24H34F5NO3Si3	055429-13-5	43
4			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	43

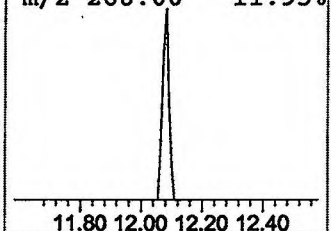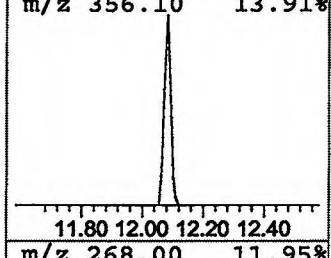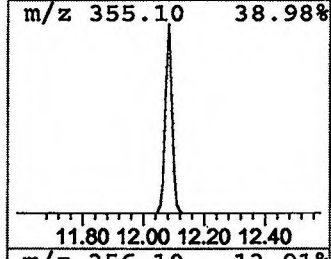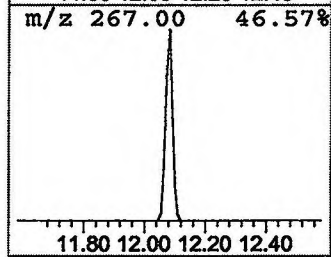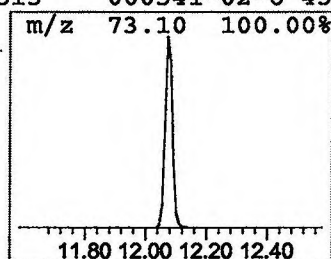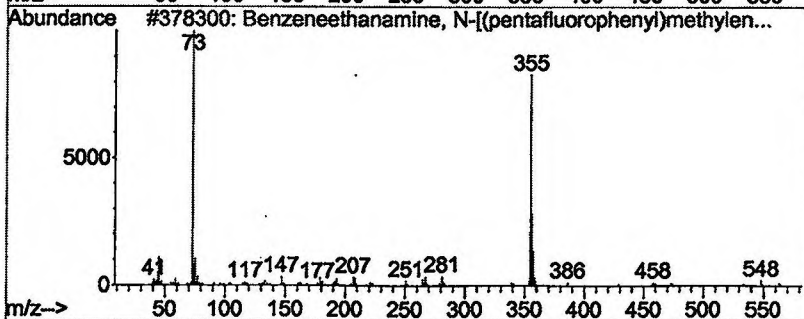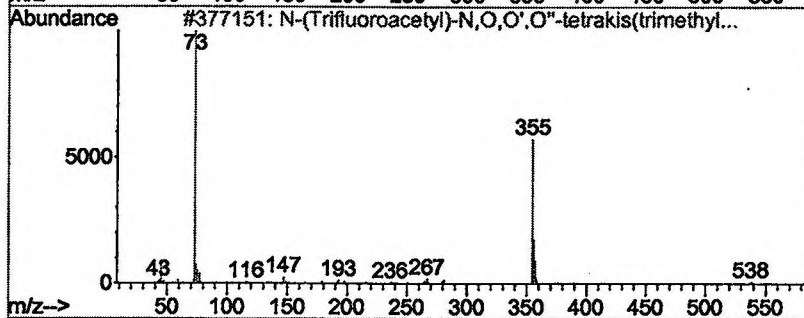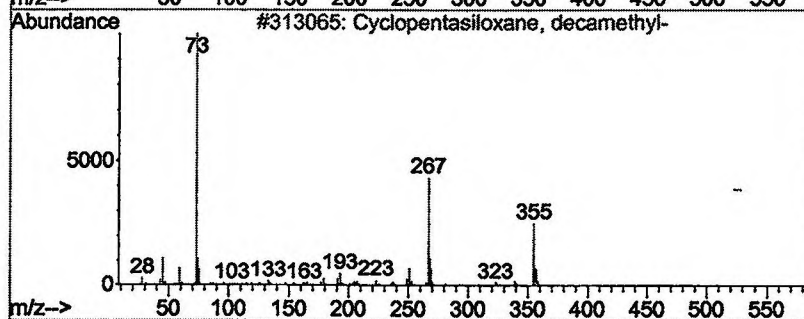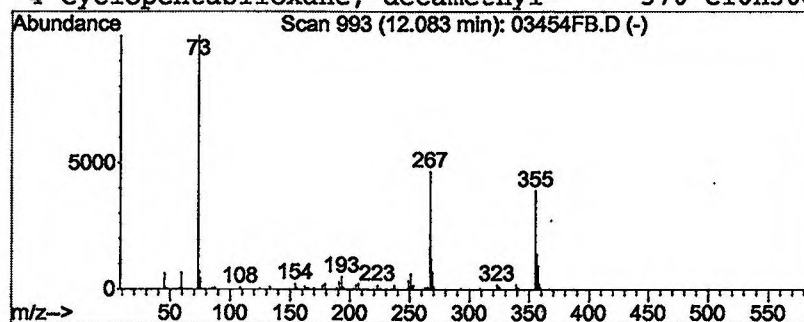

Operator ID: McLean Date Acquired: 1 Mar 2002 11:32 am
 Data File: C:\MSDCHEM\1\DATA\022802\03454FB.D
 Name: MS CSAN FB Q
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	#	--Internal Standard---		
						RT	Resp	Conc
Cyclopentasiloxan...	12.08	1.8 ug/L		614803	2	13.05	6781880	20.0