

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 03/14/2002 Time: 17:01:37

Sample: AE03438
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 3/14/02 17:00 Ended: 3/14/02 17:00 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		96		5.0

Comments for Sample AE03438 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 03-14-2002 Time: 17:01:56

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recoveries for 2 of the 43 compounds in the LCS Standard were outside their acceptance ranges.

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\022802\03438.D

Acq On : 1 Mar 2002 8:15 am

Sample :

Misc :

MS Integration Params: BENZO.P

Quant Time: Mar 13 06:47:06 2002

Vial: 25

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.58	150	1107186	20.00	ug/L	0.00
10) Naphthalene-d8	13.05	136	2944504	20.00	ug/L	0.00
17) Acenaphthene-d10	18.16	164	1650064	20.00	ug/L	0.00
29) Phenanthrene-d10	22.52	188	2532112	20.00	ug/L	0.00
38) Chrysene-d12	30.33	240	2319076	20.00	ug/L	-0.03
44) Perylene-d12	34.21	264	1455345	20.00	ug/L	-0.02

System Monitoring Compounds

37) 2,4-ddd surr	27.46	235	192460	4.79	ug/L	0.00
Spiked Amount	5.000		Recovery	=	95.80%	

Target Compounds

					Qvalue	
2) N-nitroso-dimethyl amine	3.30	74	17623	0.53	ug/L	100
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.		
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.		
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	0.00	128	0	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	18.16	165	209193	9.11	ug/L #	25
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
25) Diethylphthalate	0.00	149	0	N.D.		
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.		
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	24.67	149	4949	0.03	ug/L	79
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo (a) anthracene	0.00	228	0	N.D.		
42) Bis (2-ethylhexyl) phthala	30.94	149	68361	0.65	ug/L	94
43) Chrysene	0.00	228	0	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo (b) fluoranthene	0.00	252	0	N.D.		

(#)= qualifier out of range (m) = manual integration

03438.D 5080202.M Wed Mar 13 06:47:53 2002

Page 1

Data File : C:\MSDCHEM\1\DATA\022802\03438.D

Acq On : 1 Mar 2002 8:15 am

Sample :

Misc :

MS Integration Params: BENZO.P

Quant Time: Mar 13 06:47:06 2002

Vial: 25

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0	N.D.		
48) Benzo (a) pyrene	0.00	252	0	N.D.	d	
49) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
50) Dibenzo (a,h) anthracene	0.00	278	0	N.D.		
51) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

03438.D 5080202.M Wed Mar 13 06:47:53 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\022802\03438.D

Acq On : 1 Mar 2002 8:15 am

Sample :

Misc :

MS Integration Params: BENZO.P

Quant Time: Mar 13 6:47 2002

Vial: 25

Operator: McLean

Inst : Instrumen

Multiplr: 1.00


Quant Results File: 5080202.RES

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

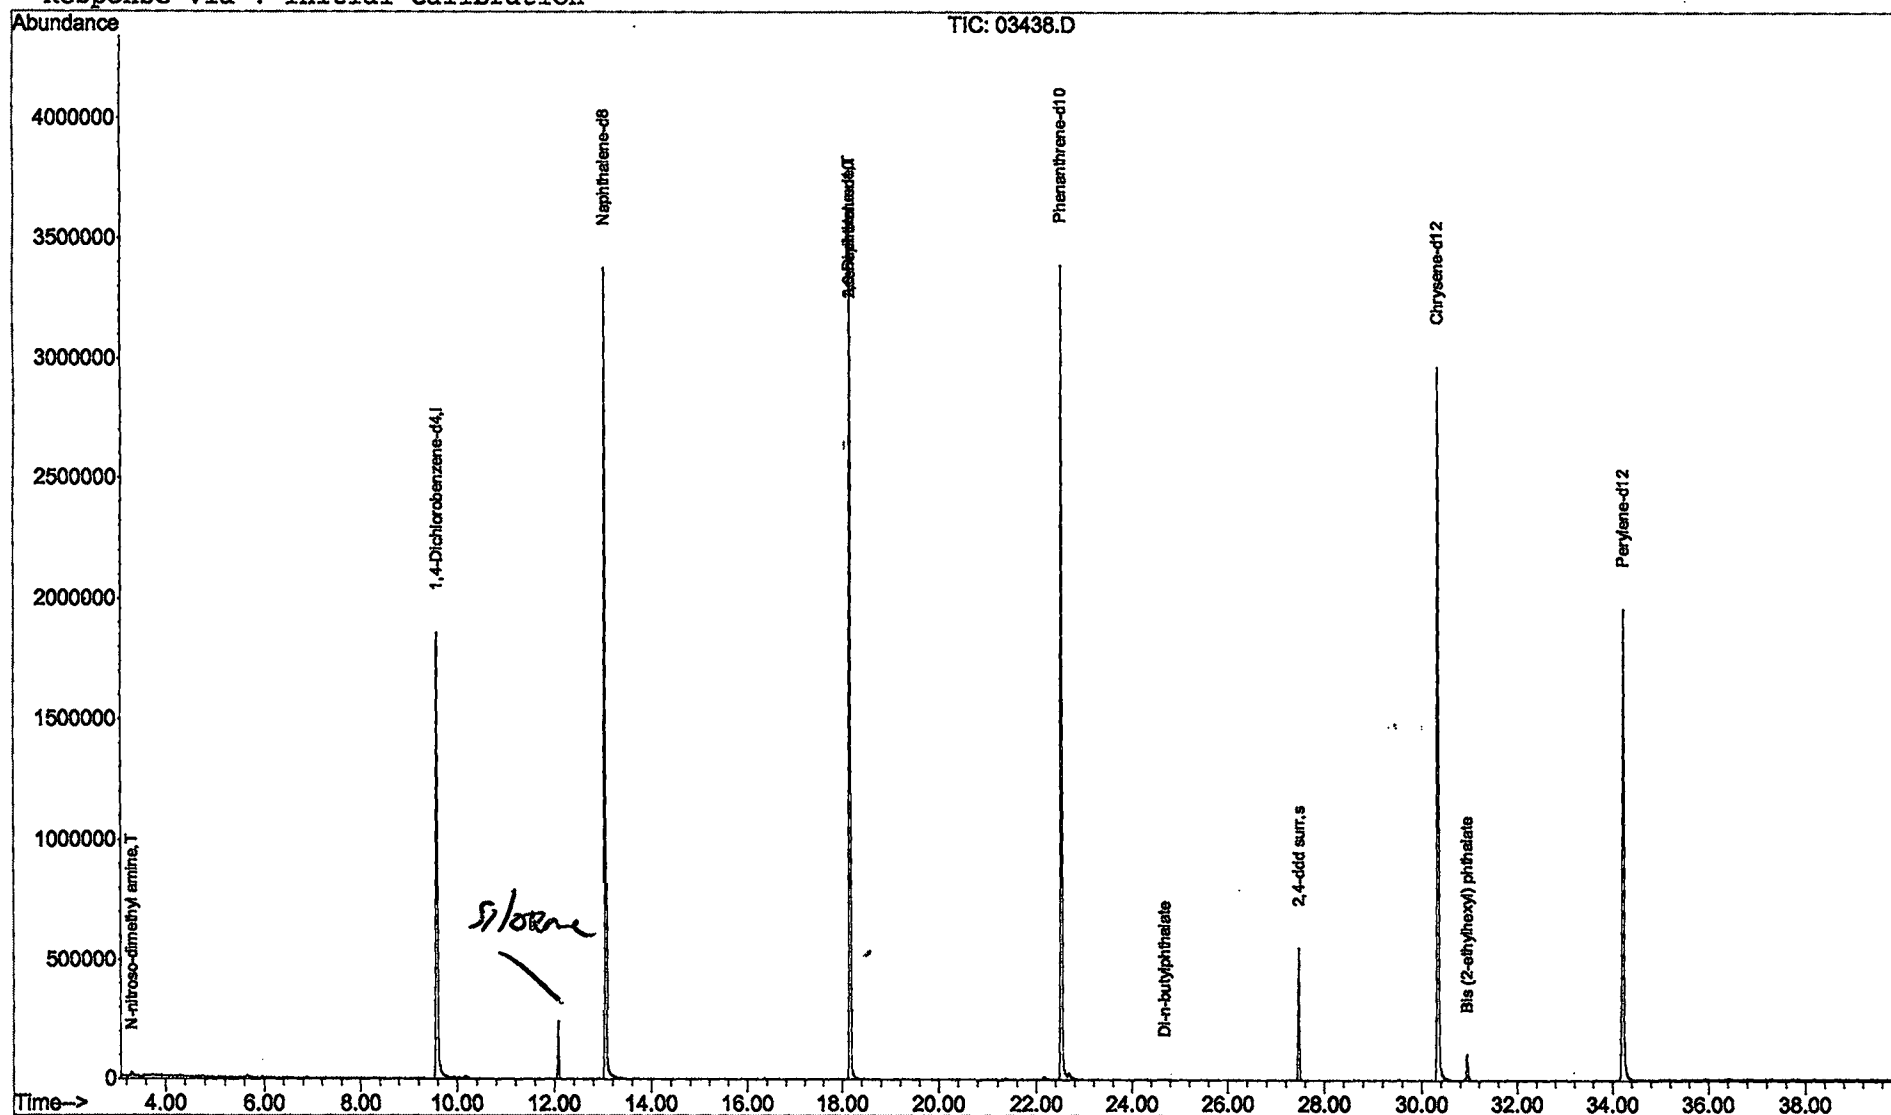


03438.D 5080202.M



Wed Mar 13 06:47:54 2002

Page 3

File : C:\MSDCHEM\1\DATA\022802\03438.D
 Operator : McLean
 Acquired : 1 Mar 2002 8:15 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name:
 Misc Info :
 Vial Number: 25

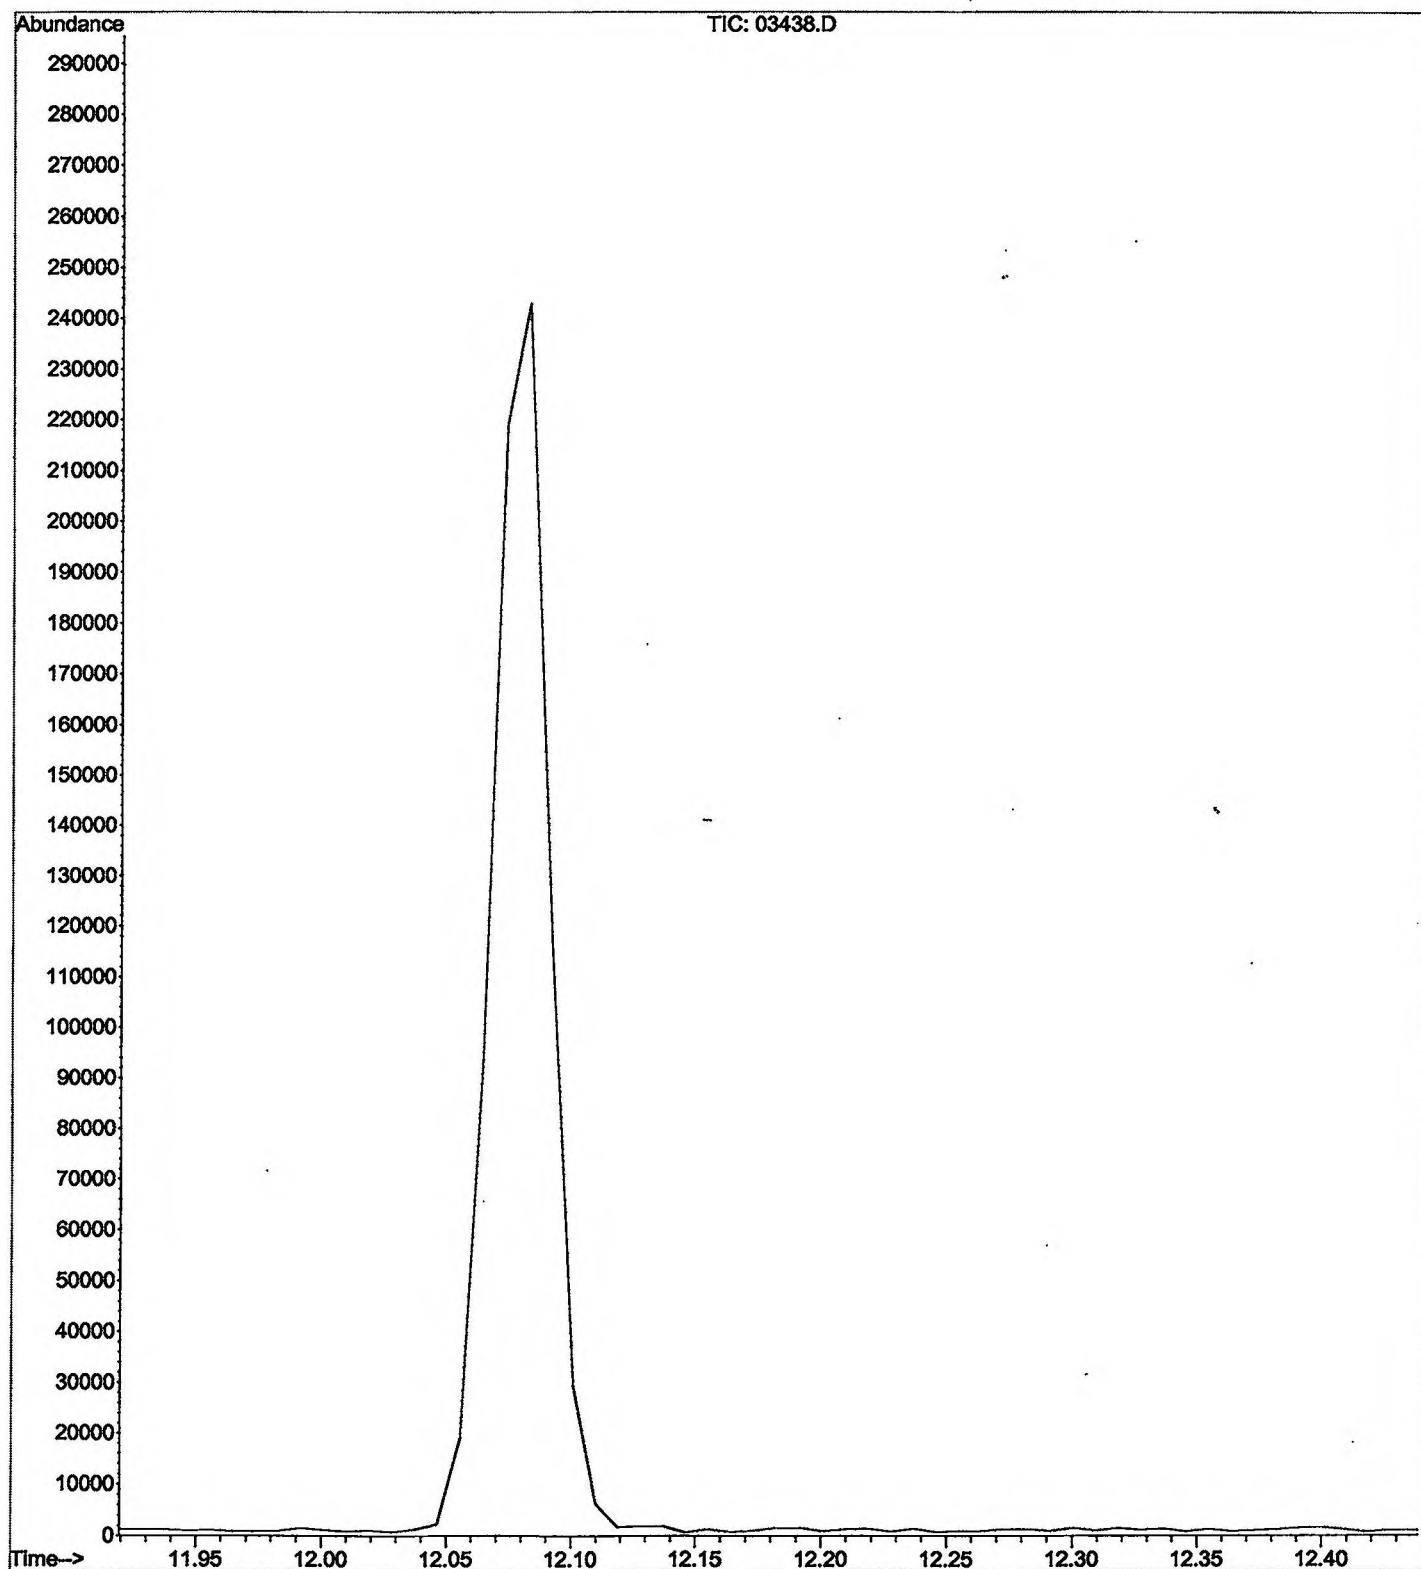

Library Searched : C:\Database\wiley7n.1
 Quality : 78
 ID : Cyclopentasiloxane, decamethyl-

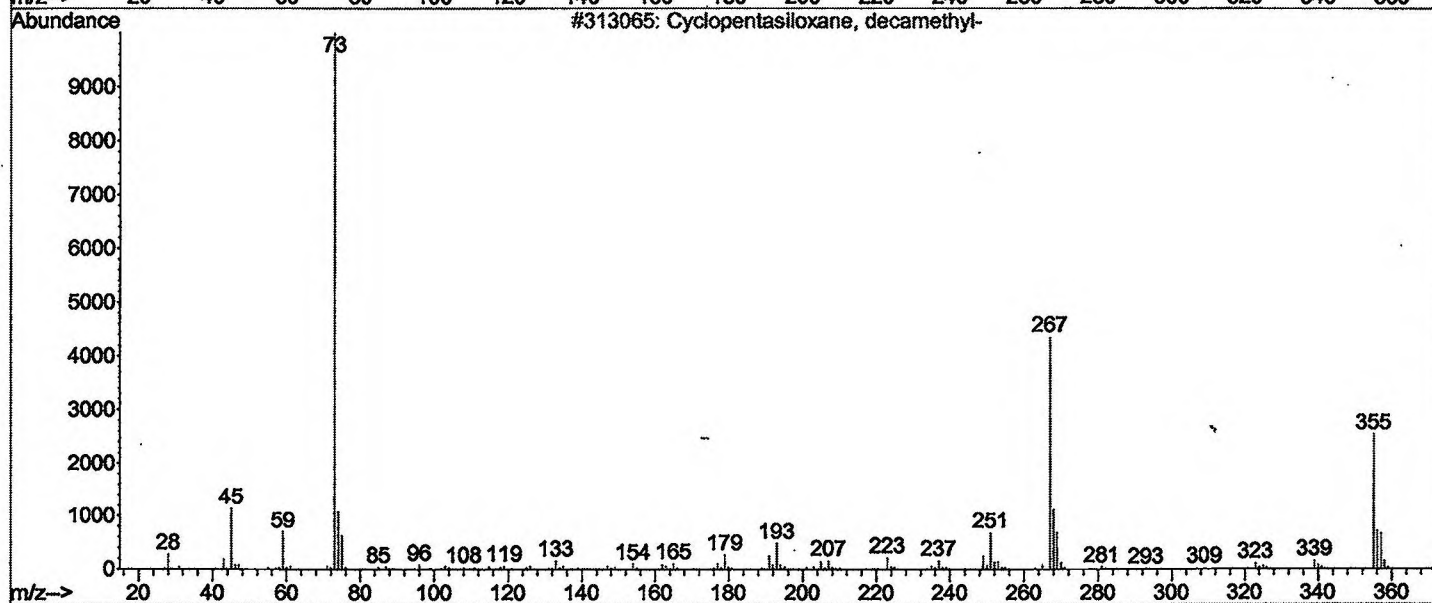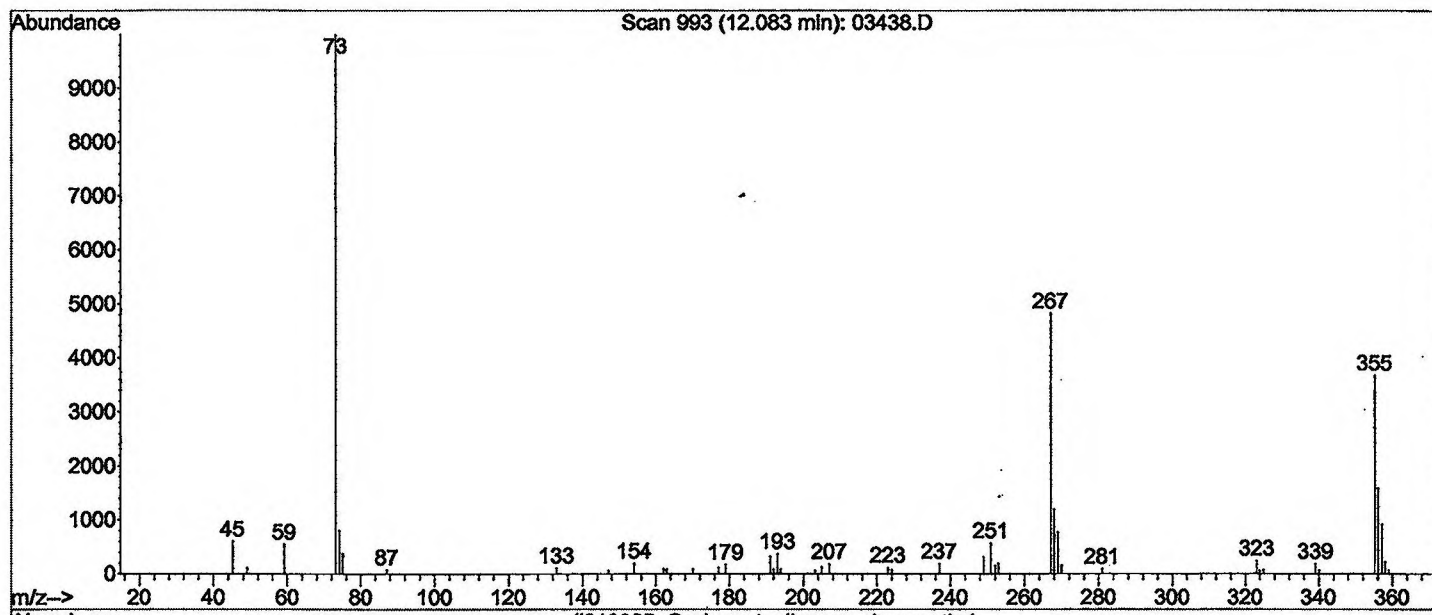

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\022802\03438.D

Vial: 25

Acq On : 1 Mar 2002 8:15 am

Operator: McLean

Sample :

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.579	712	717	732	rBV	1857400	4649302	66.77%	12.208%
2	12.083	988	993	997	rBV	241656	393853	5.66%	1.034%
3	13.053	1095	1100	1113	rBV	3378552	6400121	91.92%	16.806%
4	18.160	1657	1663	1681	rBV	3617729	6884748	98.88%	18.078%
5	22.523	2138	2144	2158	rBV2	3391295	6963027	100.00%	18.284%
6	27.457	2683	2688	2696	rBV	551735	1009815	14.50%	2.652%
7	30.332	2998	3005	3025	rBV2	2970343	6726707	96.61%	17.663%
8	30.940	3067	3072	3082	rVB	107214	236451	3.40%	0.621%
9	34.205	3425	3432	3455	rBV2	1962182	4819374	69.21%	12.655%

Sum of corrected areas: 38083398

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\022802\03438.D
 Operator : McLean
 Acquired : 1 Mar 2002 8:15 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name:
 Misc Info :
 Vial Number: 25
 Quant File :5080202.RES (RTE Integrator)

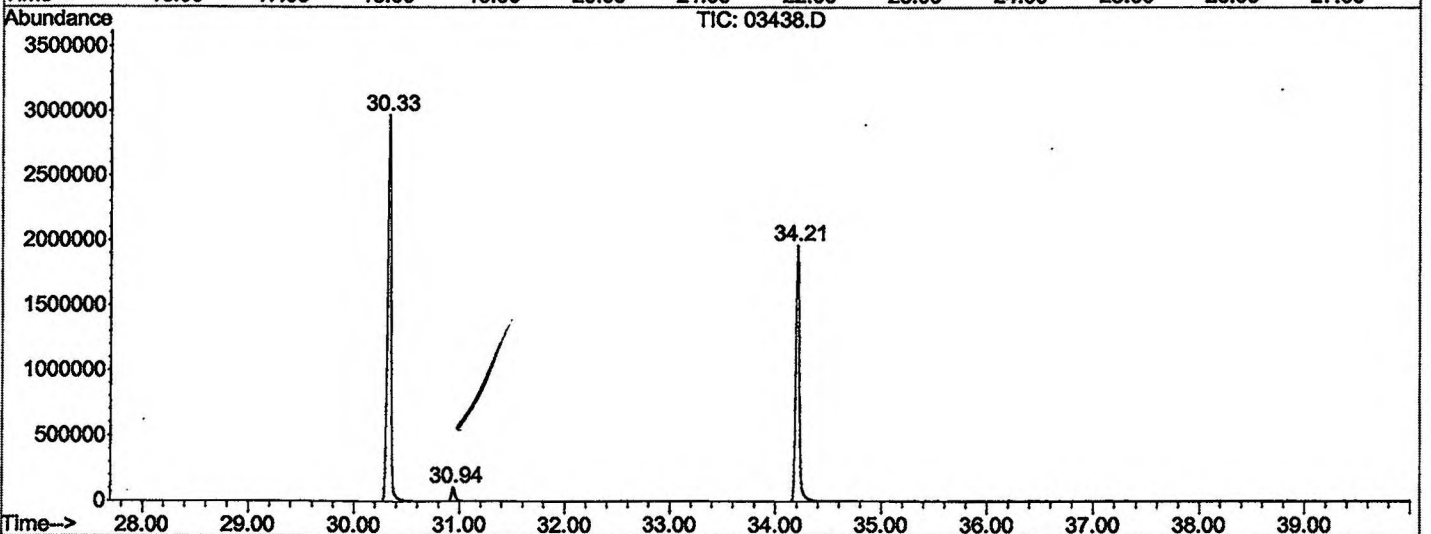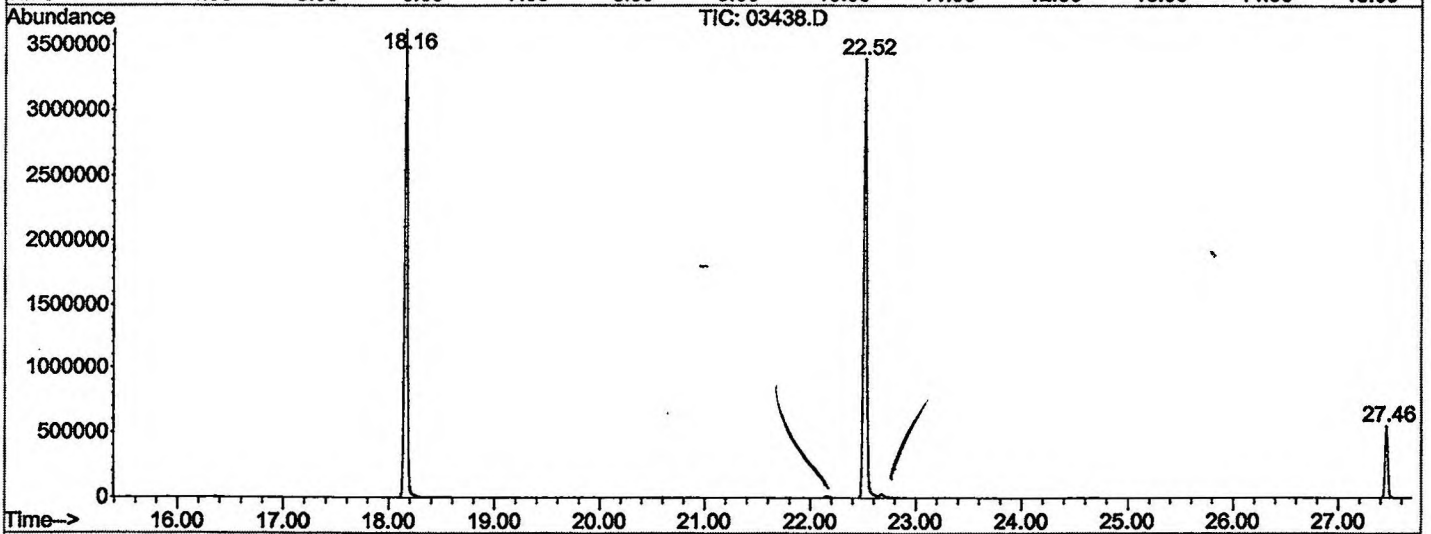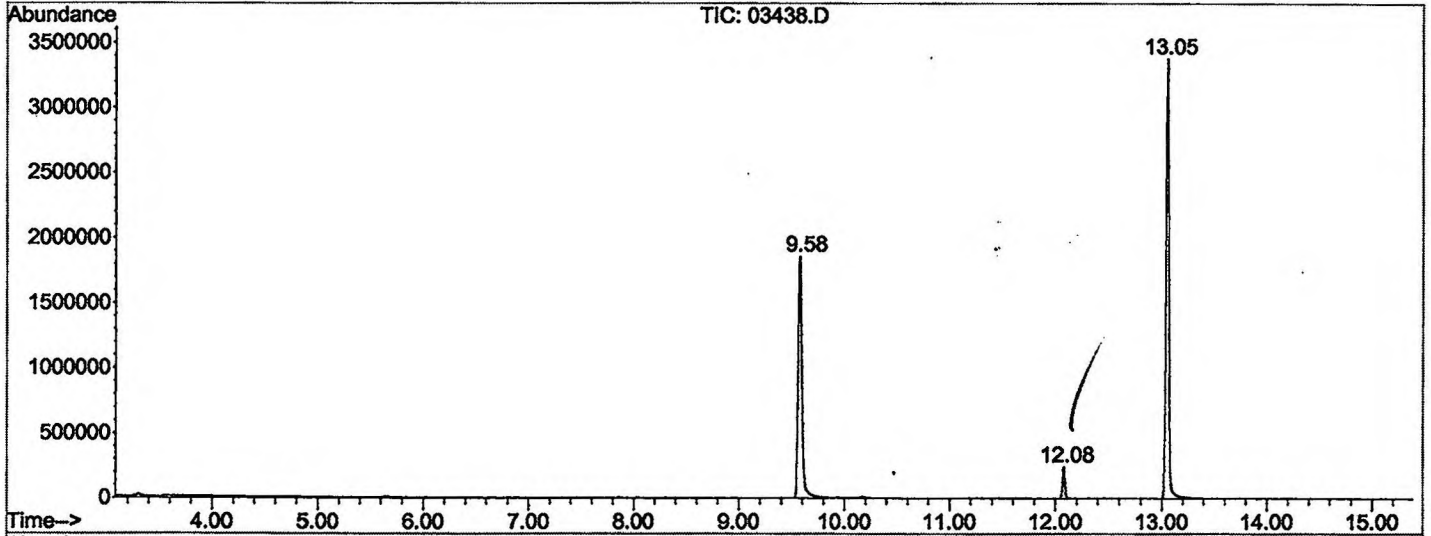

Data File : C:\MSDCHEM\1\DATA\022802\03438.D

Acq On : 1 Mar 2002 8:15 am

Sample :

Misc :

MS Integration Params: LSCINT.P

Vial: 25

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)










Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.08	1.23 ug/L	393853	Naphthalene-d8	13.05

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	78
2		Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	49
3		Phenethylamine, N-methyl-.beta.,...	399	C18H37NO3Si3	010538-85-9	43
4		Benzeneacetic acid, .alpha.,4-bi...	384	C17H32O4Si3	037148-64-4	38

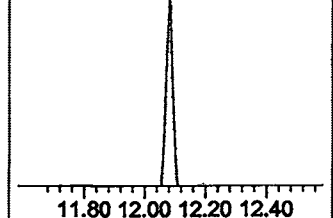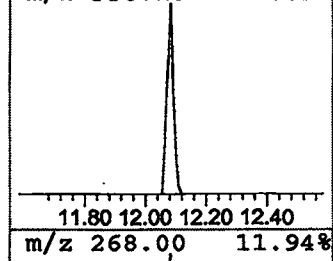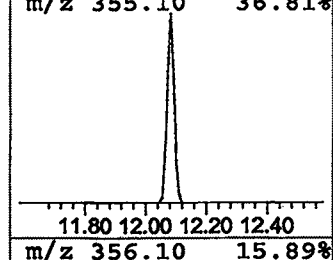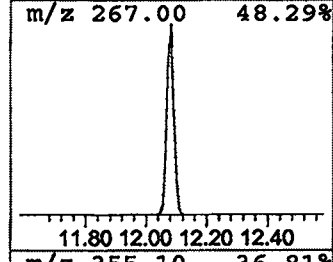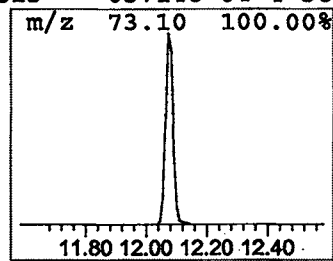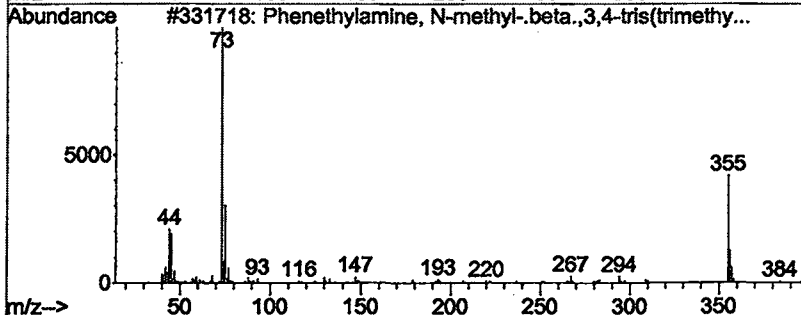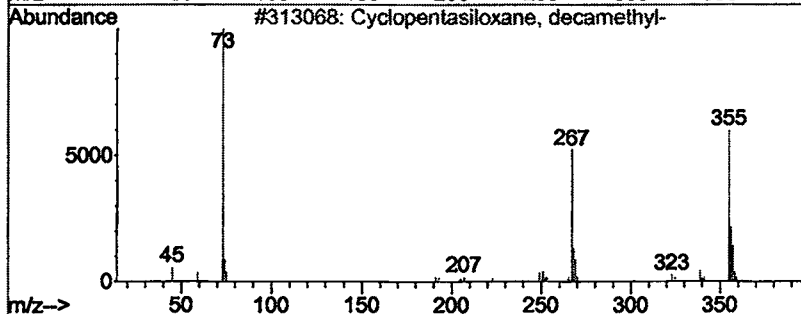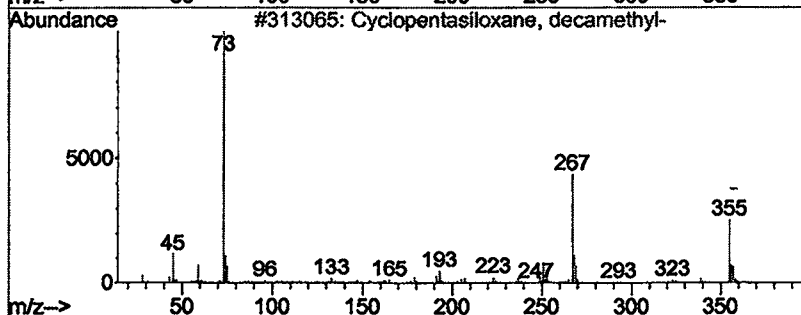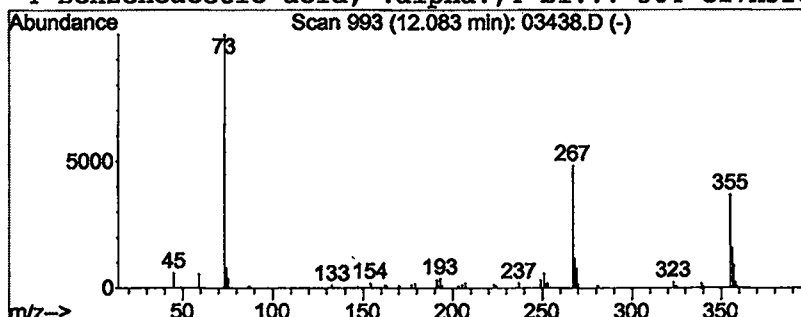

Operator ID: McLean Date Acquired: 1 Mar 2002 8:15 am
 Data File: C:\MSDCHEM\1\DATA\022802\03438.D
 Name:
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.D

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasiloxan...	12.08	1.2 ug/L		393853	2	13.05	6400120	20.0