

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 03/14/2002 Time: 17:03:06

Sample: AE03439
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 3/14/02 17:02 Ended: 3/14/02 17:02 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		110		5.0

Comments for Sample AE03439 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 03-14-2002 Time: 17:03:10

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recoveries for 2 of the 43 compounds in the LCS Standard were outside their acceptance ranges.

Data File : C:\MSDCHEM\1\DATA\022802\03439.D

Acq On : 1 Mar 2002 9:04 am

Sample :

Misc :

MS Integration Params: BENZO.P

Quant Time: Mar 13 06:49:11 2002

Vial: 26

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.58	150	894189	20.00	ug/L	0.00
10) Naphthalene-d8	13.05	136	2391567	20.00	ug/L	0.00
17) Acenaphthene-d10	18.16	164	1342686	20.00	ug/L	0.00
29) Phenanthrene-d10	22.51	188	2027436	20.00	ug/L	-0.02
38) Chrysene-d12	30.33	240	1869338	20.00	ug/L	-0.03
44) Perylene-d12	34.21	264	1177894	20.00	ug/L	-0.02

System Monitoring Compounds

37) 2,4-ddd surr	27.46	235	176605	5.49	ug/L	0.00
Spiked Amount	5.000		Recovery	=	109.80%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) N-nitroso-dimethyl amine	3.29	74	12011	0.44	ug/L	100
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.		
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.		
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	0.00	128	0	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	18.16	165	172234	9.22	ug/L #	25
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
25) Diethylphthalate	0.00	149	0	N.D.		
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.		
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	24.67	149	3091	0.02	ug/L	79
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo (a) anthracene	0.00	228	0	N.D. d		
42) Bis (2-ethylhexyl) phthala	30.94	149	142578	1.68	ug/L	99
43) Chrysene	30.33	228	4491	0.04	ug/L	44
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo (b) fluoranthene	0.00	252	0	N.D.		

(#) = qualifier out of range (m) = manual integration

03439.D 5080202.M Wed Mar 13 06:50:01 2002

Data File : C:\MSDCHEM\1\DATA\022802\03439.D

Acq On : 1 Mar 2002 9:04 am

Sample :

Misc :

MS Integration Params: BENZO.P

Quant Time: Mar 13 06:49:11 2002

Vial: 26

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080202.RES

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0		N.D.	
48) Benzo (a) pyrene	0.00	252	0		N.D. d	
49) Indeno (1,2,3-cd) pyrene	0.00	276	0		N.D.	
50) Dibenz (a,h) anthracene	0.00	278	0		N.D.	
51) Benzo (g,h,i) perylene	0.00	276	0		N.D.	

(#) = qualifier out of range (m) = manual integration

03439.D 5080202.M Wed Mar 13 06:50:01 2002

Data File : C:\MSDCHEM\1\DATA\022802\03439.D

Acq On : 1 Mar 2002 9:04 am

Sample :

Misc :

MS Integration Params: BENZO.P

Quant Time: Mar 13 6:49 2002

Vial: 26

Operator: McLean

Inst : Instrumen

Multiplr: 1.00


Quant Results File: 5080202.RES

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Feb 25 19:17:14 2002

Response via : Initial Calibration

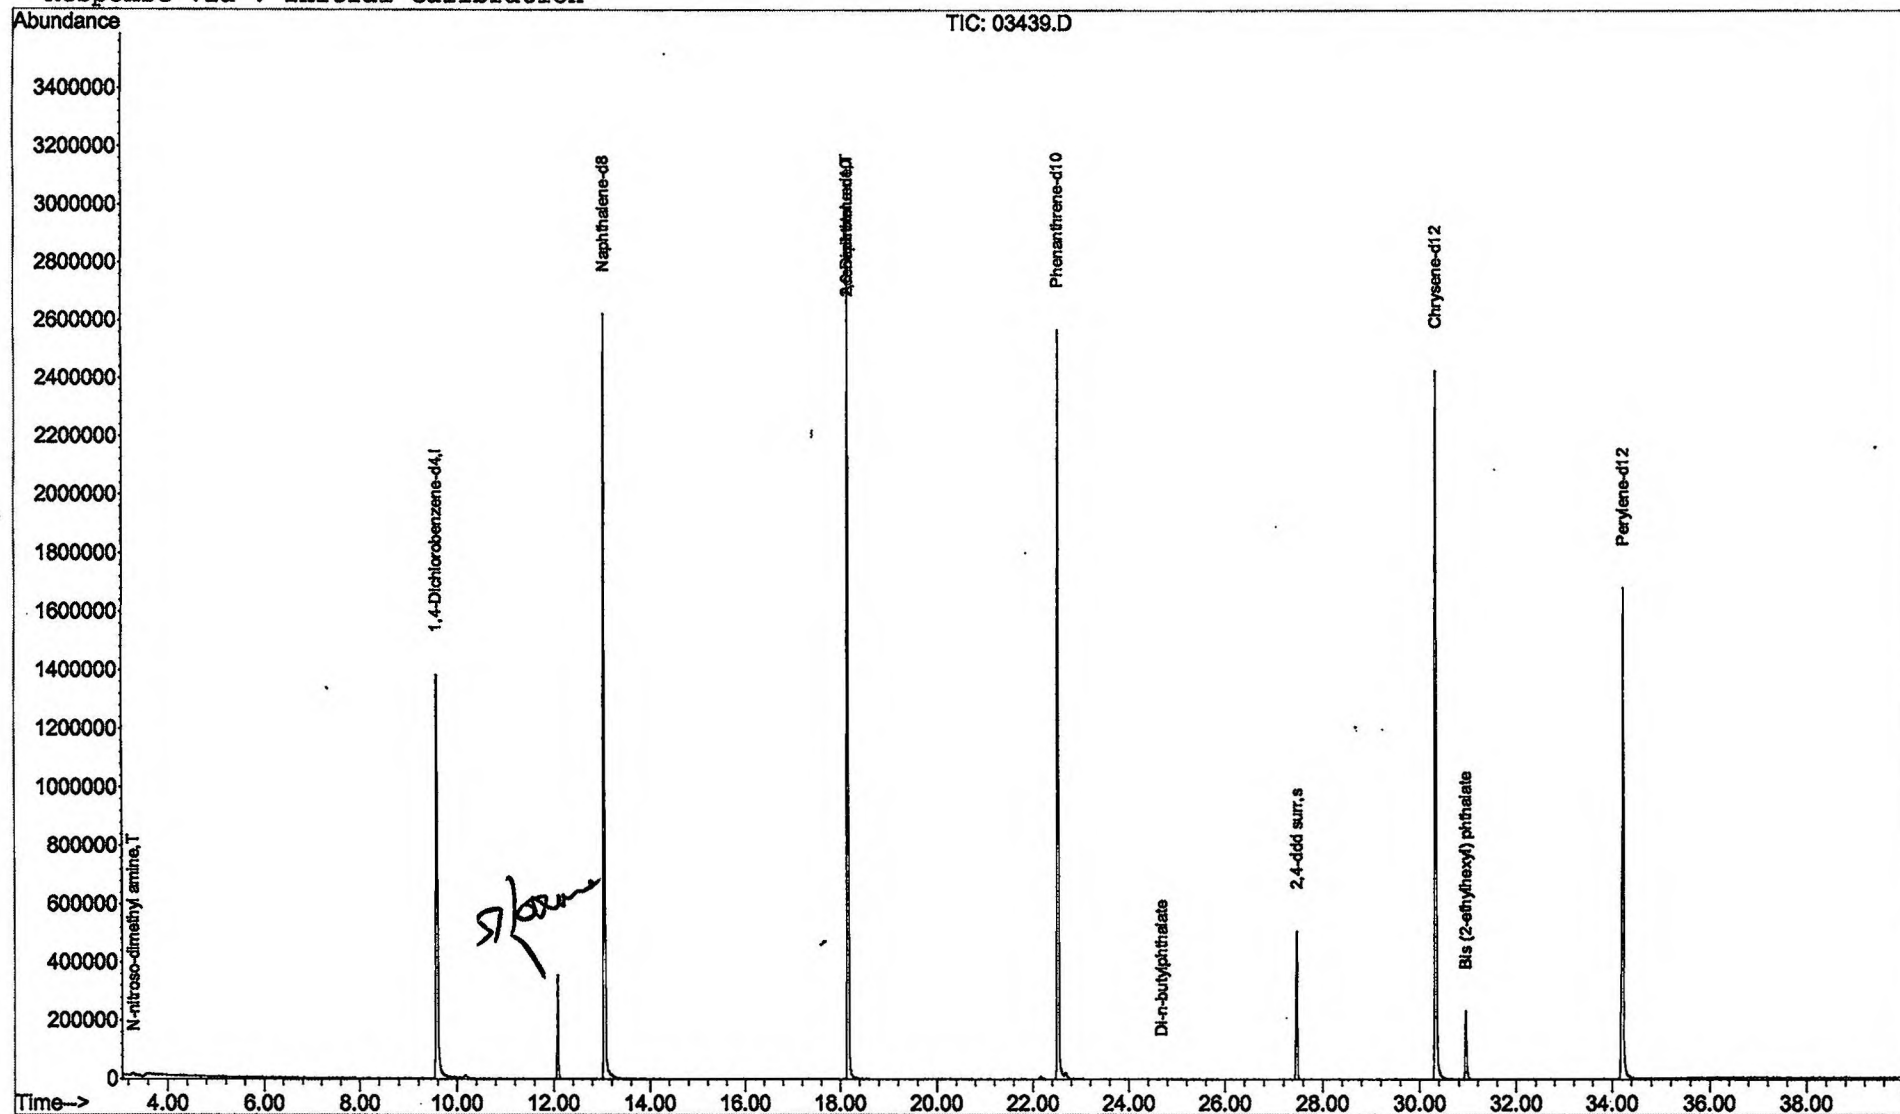

Data File : C:\MSDCHEM\1\DATA\022802\03439.D Vial: 26
Acq On : 1 Mar 2002 9:04 am Operator: McLean
Sample : Inst : Instrumen
Misc : Multiplr: 1.00
MS Integration Params: LSCINT.P

Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.570	712	716	736	rBV	1384878	3742057	67.01%	11.945%
2	12.083	988	993	1000	rBV	355754	604011	10.82%	1.928%
3	13.053	1094	1100	1114	rBV	2624280	5142655	92.09%	16.416%
4	18.160	1657	1663	1678	rBV	2985198	5563258	99.62%	17.758%
5	22.514	2138	2143	2157	rBV2	2571617	5584519	100.00%	17.826%
6	22.668	2157	2160	2174	rVB2	19672	73148	1.31%	0.233%
7	27.457	2684	2688	2697	rBB	507999	919381	16.46%	2.935%
8	30.332	2998	3005	3025	rBV	2430378	5394733	96.60%	17.220%
9	30.940	3067	3072	3085	rBV	234741	506506	9.07%	1.617%
10	34.205	3425	3432	3444	rBV	1683478	3797197	68.00%	12.121%

Sum of corrected areas: 31327465

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\022802\03439.D
 Operator : McLean
 Acquired : 1 Mar 2002 9:04 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name:
 Misc Info :
 Vial Number: 26
 Quant File :5080202.RES (RTE Integrator)

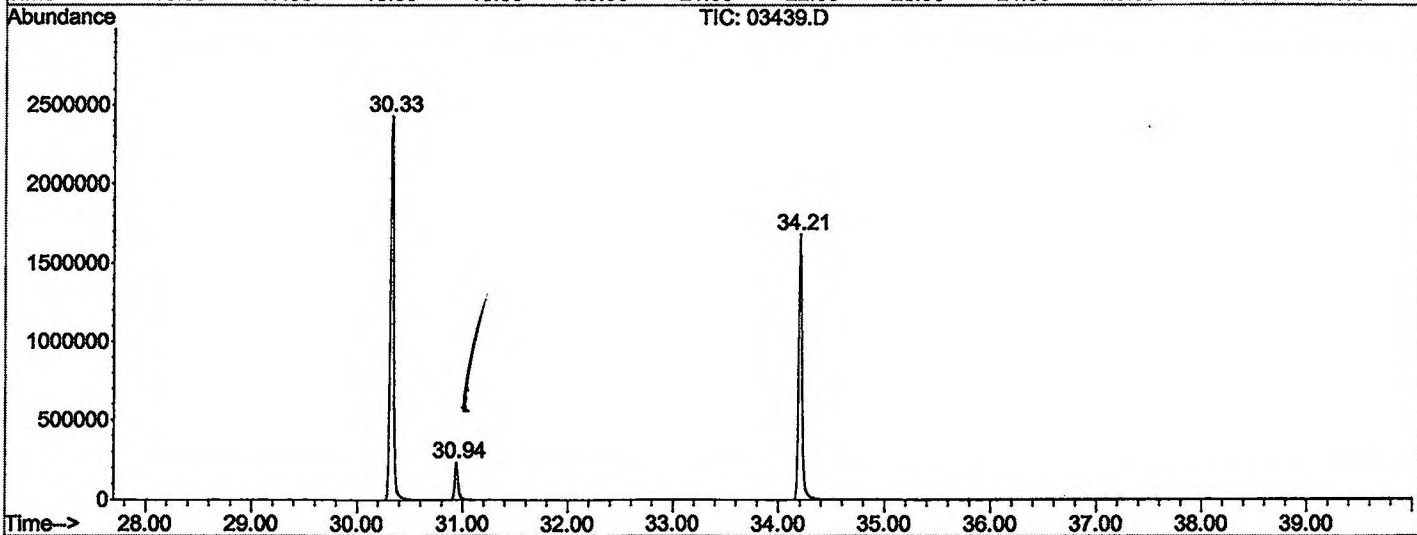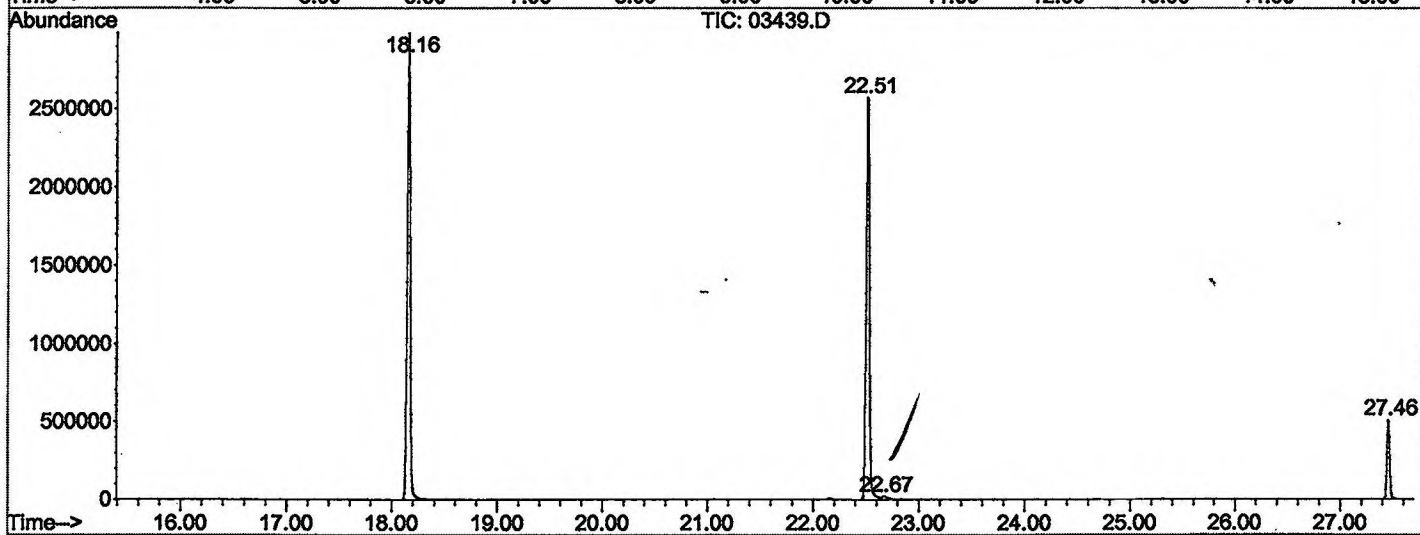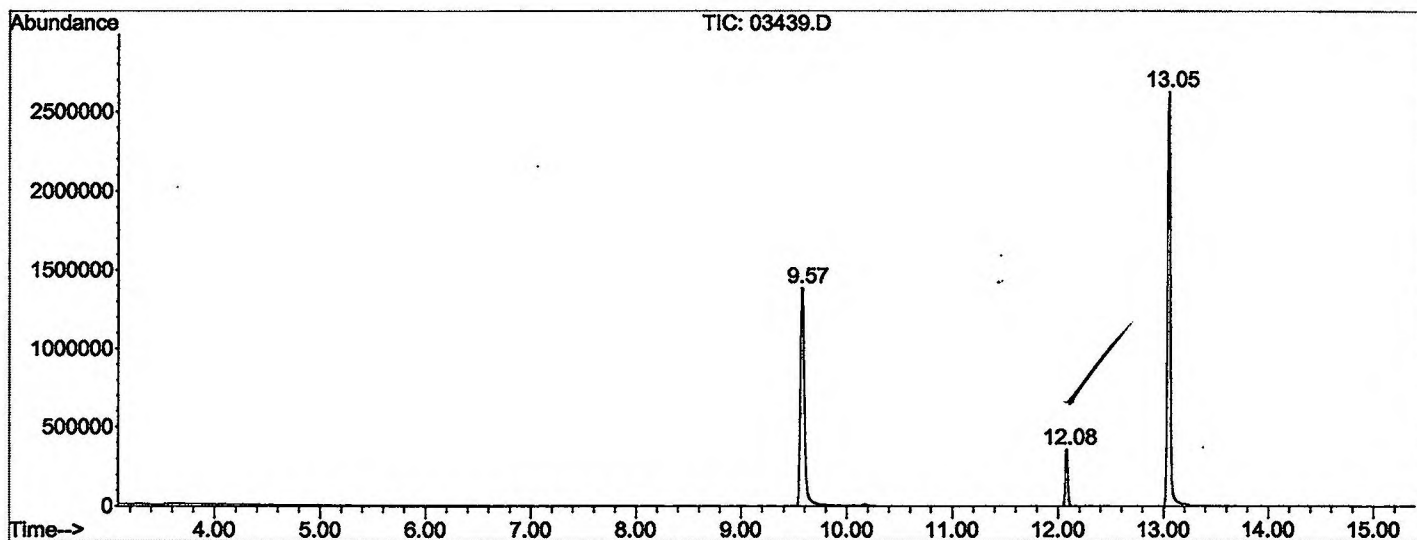

Data File : C:\MSDCHEM\1\DATA\022802\03439.D

Acq On : 1 Mar 2002 9:04 am

Sample :

Misc :

MS Integration Params: LSCINT.P

Vial: 26

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)










Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.08	2.35 ug/L	604011	Naphthalene-d8	13.05

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	64
2			Phenethylamine, N-methyl-.beta.,...	399	C18H37NO3Si3	010538-85-9	47
3			3,4-DIHYDROXYMANDELIC ACID-TETRATMS	472	C20H40O5Si4	000000-00-0	38
4			N-(Trifluoroacetyl)-N,O,O',O''-t...	553	C22H42F3NO4Si4	000000-00-0	38

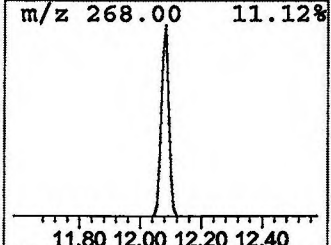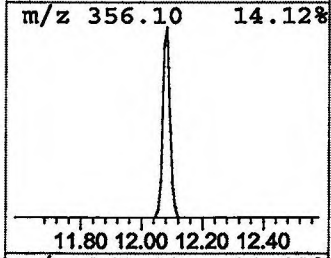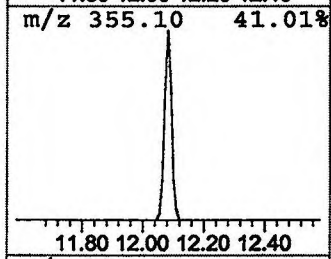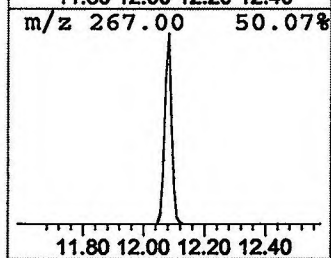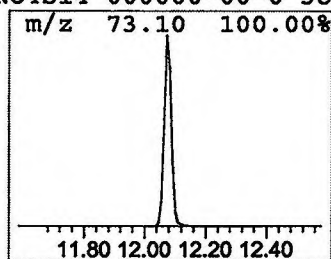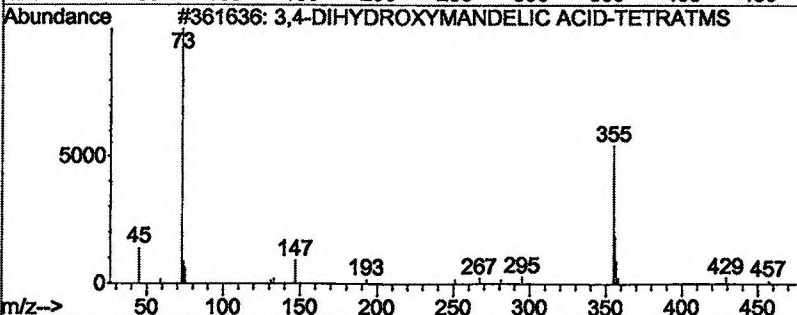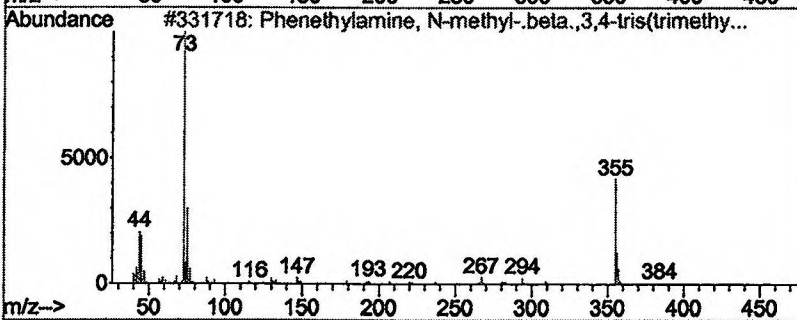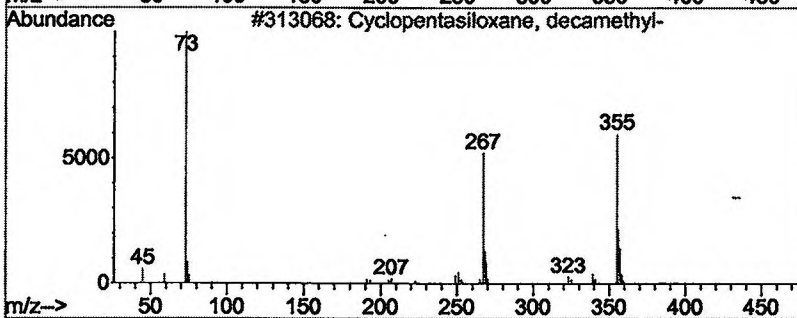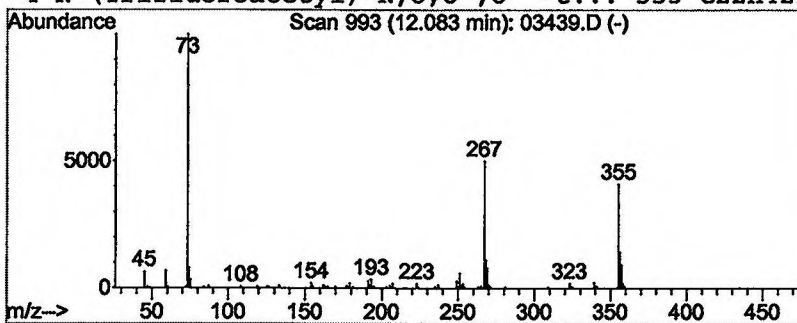

Operator ID: McLean Date Acquired: 1 Mar 2002 9:04 am
 Data File: C:\MSDCHEM\1\DATA\022802\03439.D
 Name:
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080202.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Cyclopentasiloxan...	12.08	2.3	ug/L	604011	2	13.05	5142660	20.0