

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 03/29/2002 Time: 10:03:28

Sample: AE04034
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 3/29/02 10:03 Ended: 3/29/02 10:03 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		113		5.0

Comments for Sample AE04034 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 03-29-2002 Time: 10:03:50

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recoveries for 3 of the 43 compounds in the LCS Standard were outside of their acceptance limits. New limits will be calculated.

Data File : C:\HPCHEM\1\DATA\MAR2202\4034.D

Vial: 40

Acq On : 24 Mar 2002 8:34 am

Operator:

Sample : gc/ms scan 2/25

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 26 10:24 2002

Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Mar 08 08:54:27 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0308

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.26	152	449570	20.00	ug/l	-0.09
10) Naphthalene-d8	15.90	136	1810401	20.00	ug/l	-0.10
17) Acenaphthene-d10	21.21	164	1010047	20.00	ug/l	-0.10
29) Phenanthrene-d10	25.66	188	1532049	20.00	ug/l	-0.11
38) Chrysene-d12	33.72	240	1021540	20.00	ug/l	-0.13
44) Perylene-d12	37.97	264	605510	20.00	ug/l	-0.15

System Monitoring Compounds

37) 2,4-DDD	30.73	235	92667	5.65 8.32 ug/mL	0.24
Spiked Amount	5.000		Recovery	= 166.40% 113%	Qvalue

Target Compounds

2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	15.96	128	376	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	21.50	165	337	N.D.
25) Diethylphthalate	22.69	149	386	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#)=qualifier out of range (m)=manual integration

4034.D GCMS0308.M Tue Mar 26 10:25:04 2002

Page 1

Data File : C:\HPCHEM\1\DATA\MAR2202\4034.D

Vial: 40

Acq On : 24 Mar 2002 8:34 am

Operator:

Sample : gc/ms scan 2/25

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 26 10:24 2002

Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Mar 08 08:54:27 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0308

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.66	178	474	N.D.		
34) Anthracene	25.66	178	474	N.D.		
35) Di-n-butylphthalate	27.62	149	4986	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.73	228	2413	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.93	149	66299	1.62	ug/l	97
43) Chrysene	33.73	228	2413	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.98	252	2345	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

4034.D GCMS0308.M Tue Mar 26 10:25:07 2002


Page 2

Data File : C:\HPCHEM\1\DATA\MAR2202\4034.D
 Acq On : 24 Mar 2002 8:34 am
 Sample : gc/ms scan 2/25
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Mar 26 10:24 2002

Vial: 40
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0308.RES

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Mar 08 08:54:27 2002
 Response via : Initial Calibration

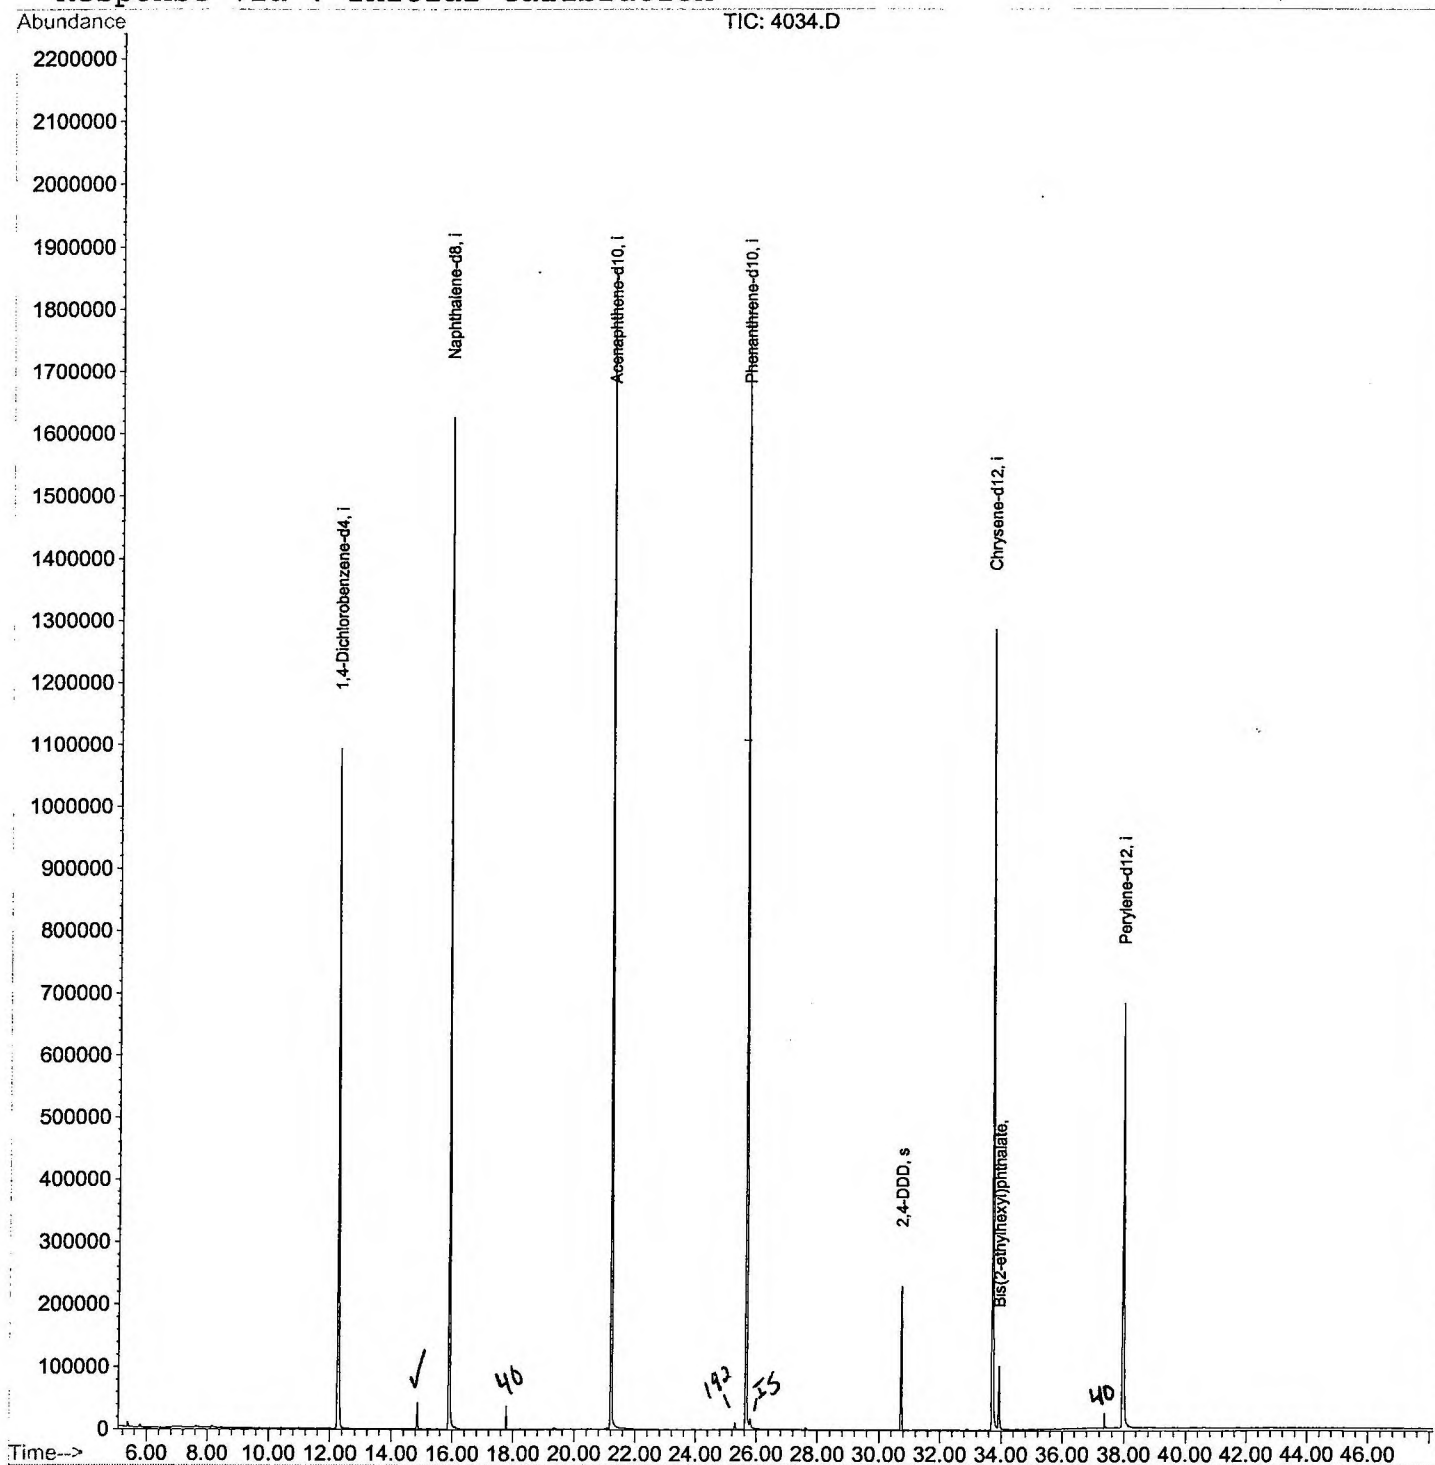

Data File : C:\HPCHEM\1\DATA\MAR2202\4034.D

Vial: 40

Acq On : 24 Mar 2002 8:34 am

Operator:

Sample : gc/ms scan 2/25

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	12.263	780	786	803	rVB	1092704	2457270	63.23%	12.667%
2	14.861	1061	1069	1074	rBV	42825	81235	2.09%	0.419%
3	15.899	1176	1182	1200	rBV	1625844	3404121	87.59%	17.547%
4	21.214	1754	1761	1772	rBV	1866560	3886476	100.00%	20.034%
5	25.657	2238	2245	2255	rBV2	1812024	3824583	98.41%	19.715%
6	30.734	2792	2798	2804	rVB	230885	461493	11.87%	2.379%
7	33.718	3116	3123	3141	rBV2	1287264	2973222	76.50%	15.326%
8	33.929	3141	3146	3158	rVB	101603	219172	5.64%	1.130%
9	37.968	3578	3586	3610	rBV2	681765	2091951	53.83%	10.784%


Sum of corrected areas: 19399523

4034.D GCMS0308.M

Tue Mar 26 10:46:34 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAR2202\4034.D
Operator :
Acquired : 24 Mar 2002 8:34 am using AcqMethod GCMS0308
Instrument : GC/MS 209
Sample Name: gc/ms scan 2/25
Misc Info :
Vial Number: 40
Quant File :GCMS0308.RES (RTE Integrator)

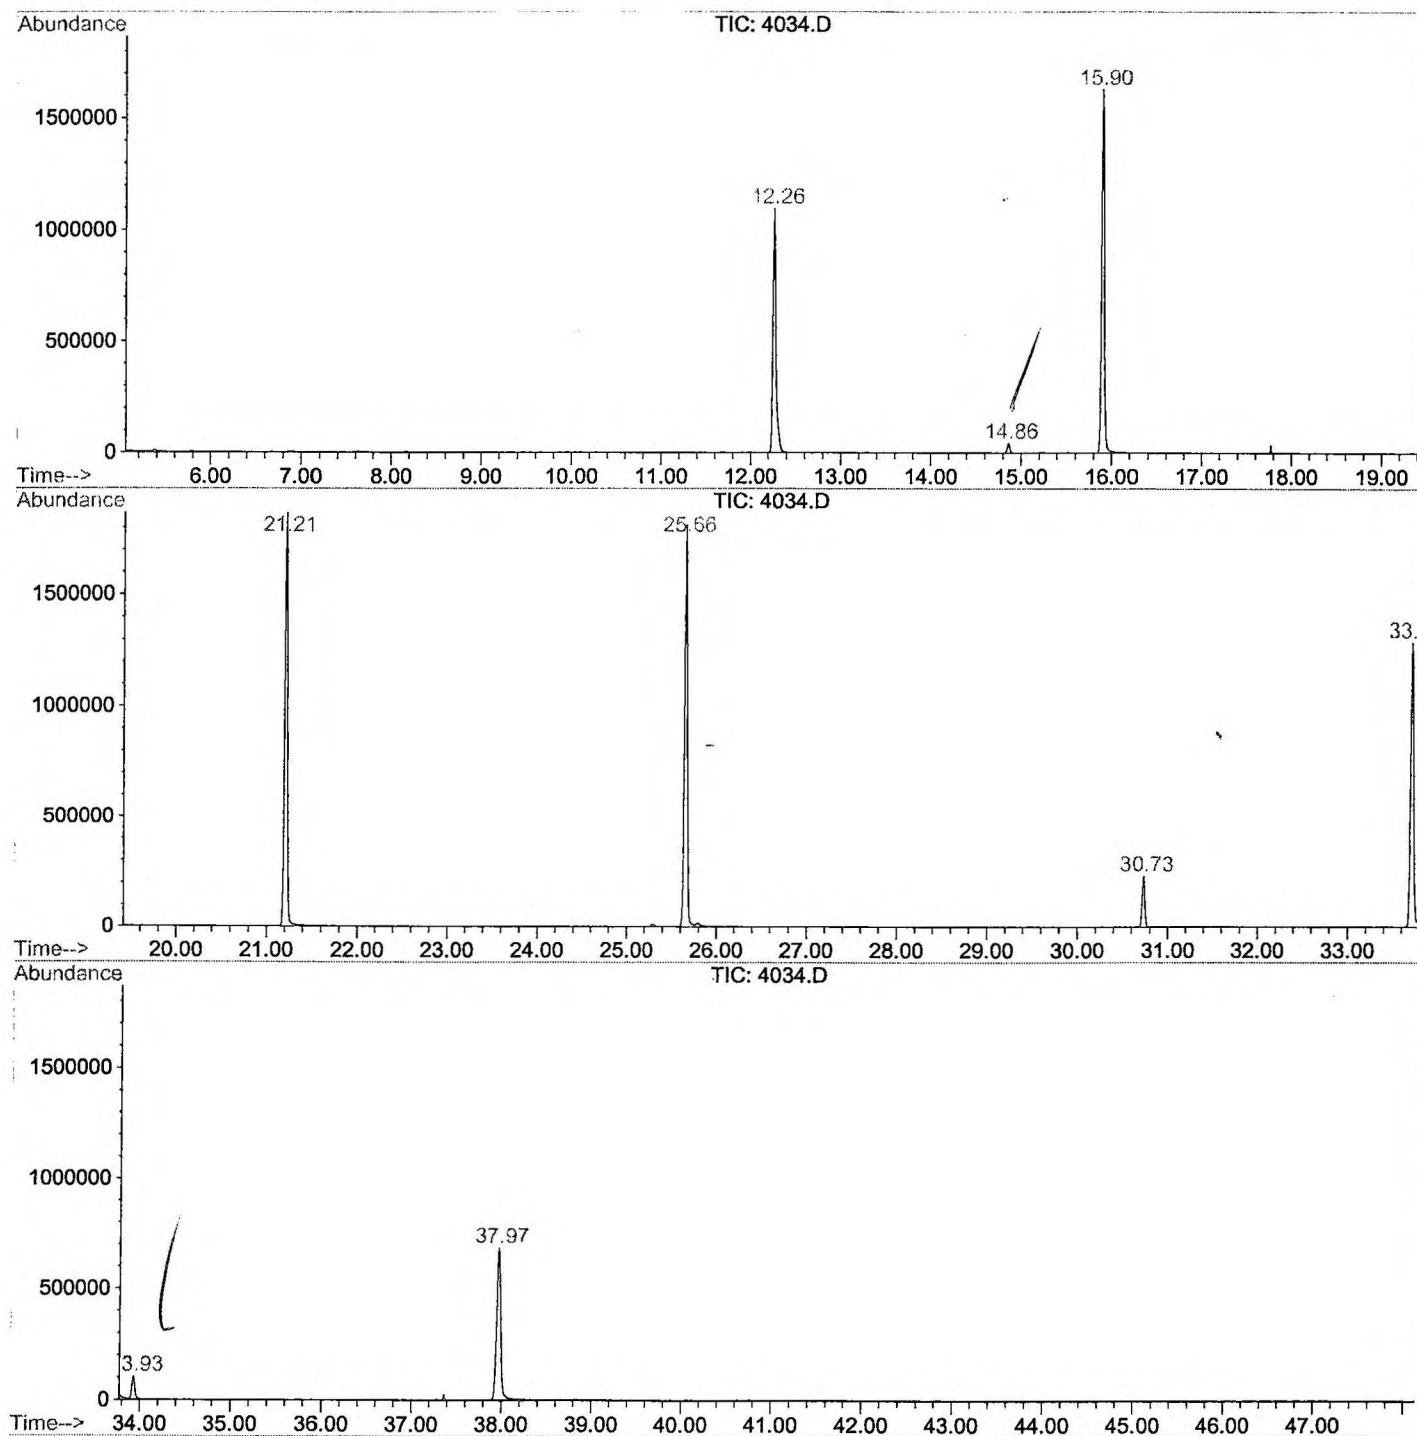

4034.D GCMS0308.M

Tue Mar 26 10:46:40 2002





Data File : C:\HPCHEM\1\DATA\MAR2202\4034.D
Acq On : 24 Mar 2002 8:34 am
Sample : gc/ms scan 2/25
Misc :
MS Integration Params: LSCINT.P

Vial: 40
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 Cyclopentasiloxane, decamethyl Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
14.86	0.48 ug/l	81235	Naphthalene-d8	15.90	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	64
2	Phenethylamine, N-methyl-.beta.,3,4	399	C18H37NO3Si3	010538-85-9	38
3	Benzeneethanamine, N-[(pentafluorop	563	C24H34F5NO3Si3	055429-13-5	38
4	Benzoic acid, 2,4-bis[(trimethylsil	370	C16H30O4Si3	010586-16-0	38

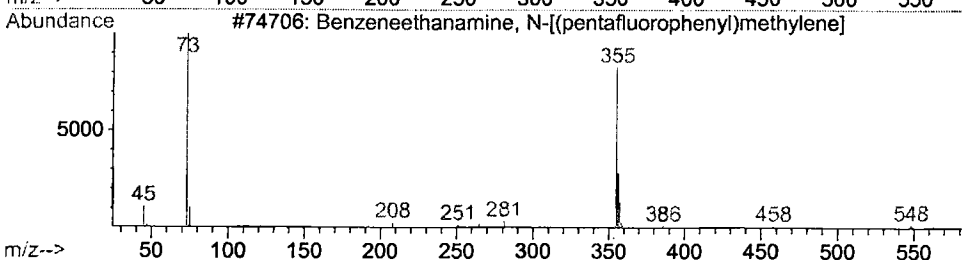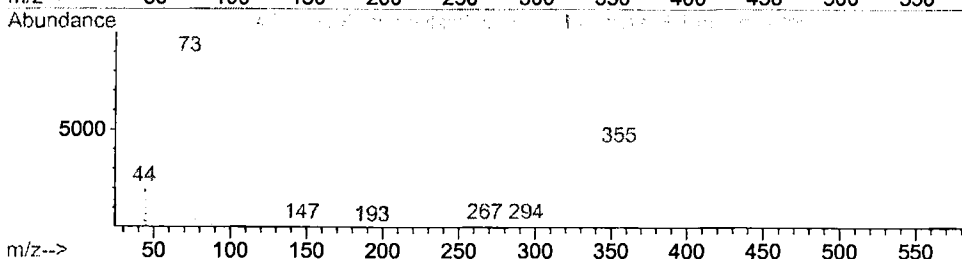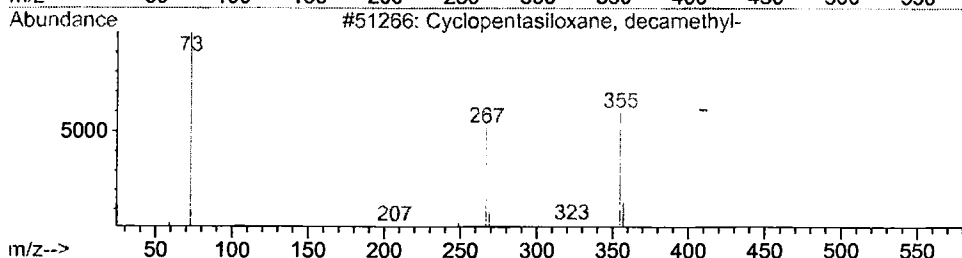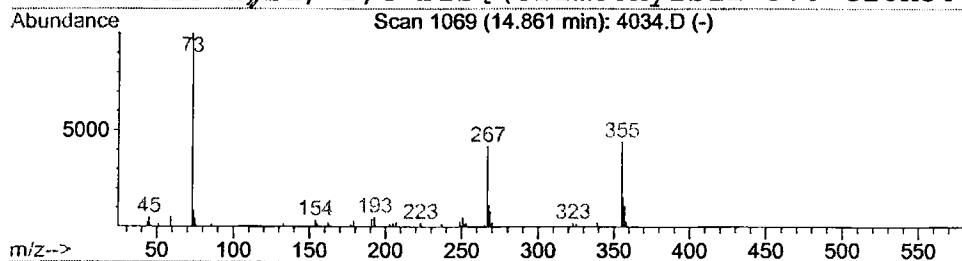

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 24 Mar 2002 8:34 am
 Data File: C:\HPCHEM\1\DATA\MAR2202\4034.D
 Name: gc/ms scan 2/25
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Cyclopentasiloxane,	14.86	0.5	ug/l	81235	ISTD02	15.90	3404120	20.0
4034.D GCMS0308.M	Tue Mar 26 10:46:48 2002							