

NYC-WTC_000039028

DFTPP

Data File : C:\MSDCHEM\1\DATA\031702\DFTPP.D

Acq On : 17 Mar 2002 9:51 pm

Sample :

Misc :

MS Integration Params: BENZO.P

Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)


Title : Quantitation For Method 508gcscan

Vial: 1

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

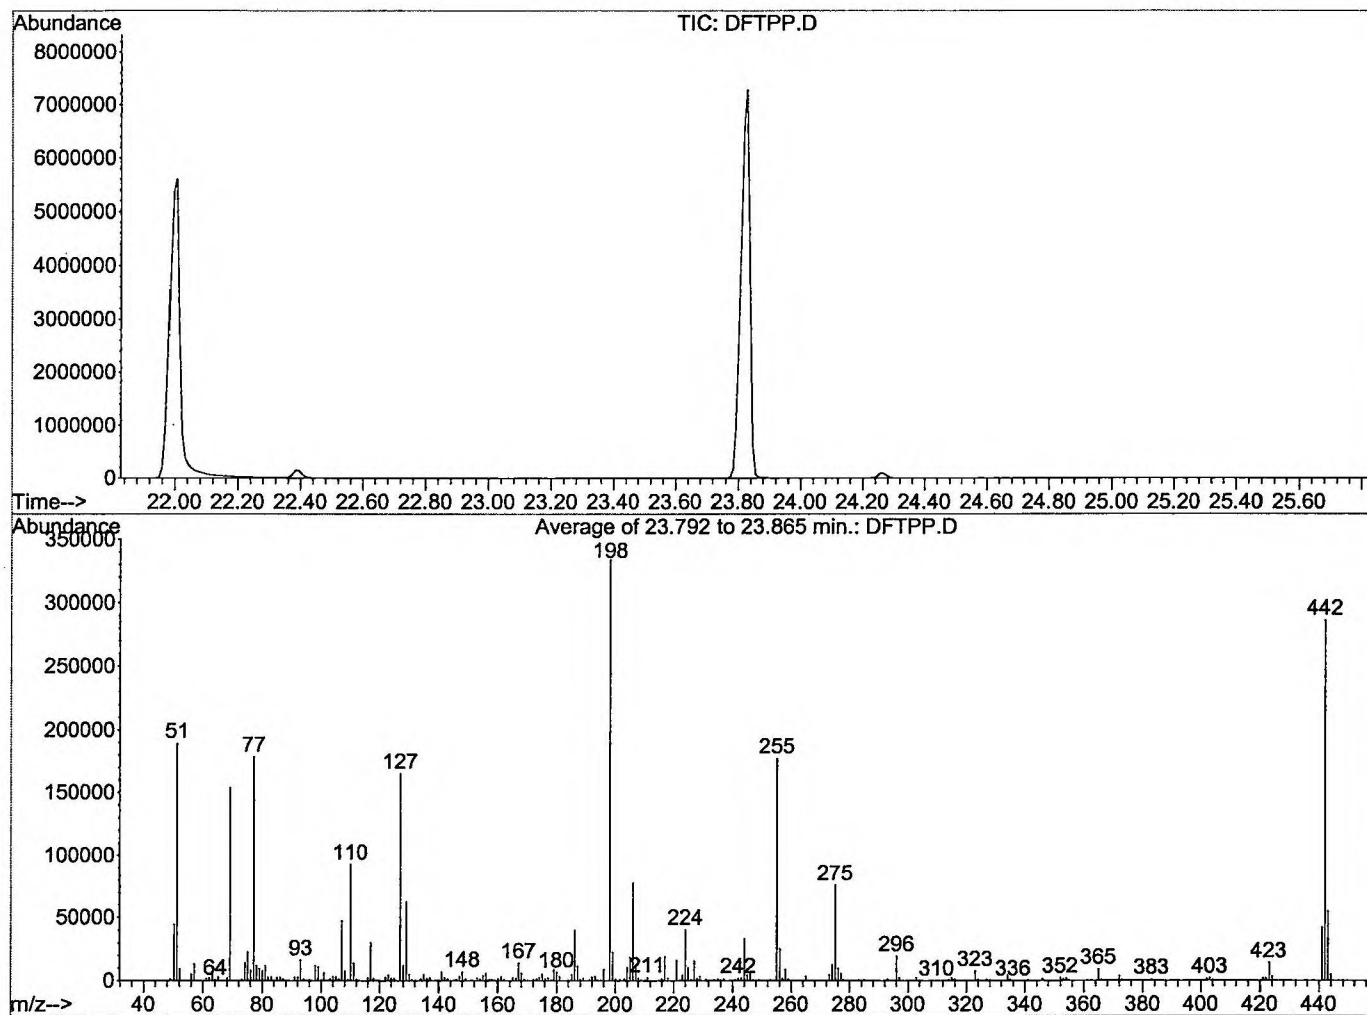

Spectrum Information: Average of 23.792 to 23.865 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.8	189698	PASS
68	69	0.00	2	1.4	2198	PASS
69	198	0.00	100	46.1	153941	PASS
70	69	0.00	2	0.4	623	PASS
127	198	10	80	49.5	165288	PASS
197	198	0.00	2	0.0	139	PASS
198	198	50	100	100.0	333813	PASS
199	198	5	9	6.7	22516	PASS
275	198	10	60	22.8	76101	PASS
365	198	1	100	2.7	9109	PASS
441	443	0.01	100	77.1	42331	PASS
442	198	50	100	85.7	286216	PASS
443	442	15	24	19.2	54918	PASS