

Method 508 MODDate Extracted 3-15-02Page 9 0

REE

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500 μ l		1ml			1ml		7			
REF1	SPILLED -				1ml							
REF2					1ml							
6267												
6268												
6269												
6270												
6271												
6301												
6302												
Remarks												
Reviewed by, <u>LB 6/6/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type - <u>SEP. FUNNEL</u> Solv. lot# <u>M17262</u> NaCl lot# <u>V39618</u> Na2SO4 lot# <u>V46623</u>												
STANDARD	INT STD LOG#											
CALIBRATION												
REF SPIKE	<u>2193</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.												
SURROGATE	<u>GCMS 2160A</u>											
LPC												
ENDRIN/DDT												

Analyst BN
revision 4/12/01


Verified by _____

Reviewed by DW
Date 3/22/02

DFTPP

Data File : C:\MSDCHEM\1\DATA\031602\DFTPP.D
 Acq On : 16 Mar 2002 6:15 pm
 Sample : 3/15
 Misc :
 MS Integration Params: BENZO.P
 Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)
 Title : Quantitation For Method 508gcscan

Vial: 1
 Operator: McLean
 Inst : Instrumen
 Multiplr: 1.00

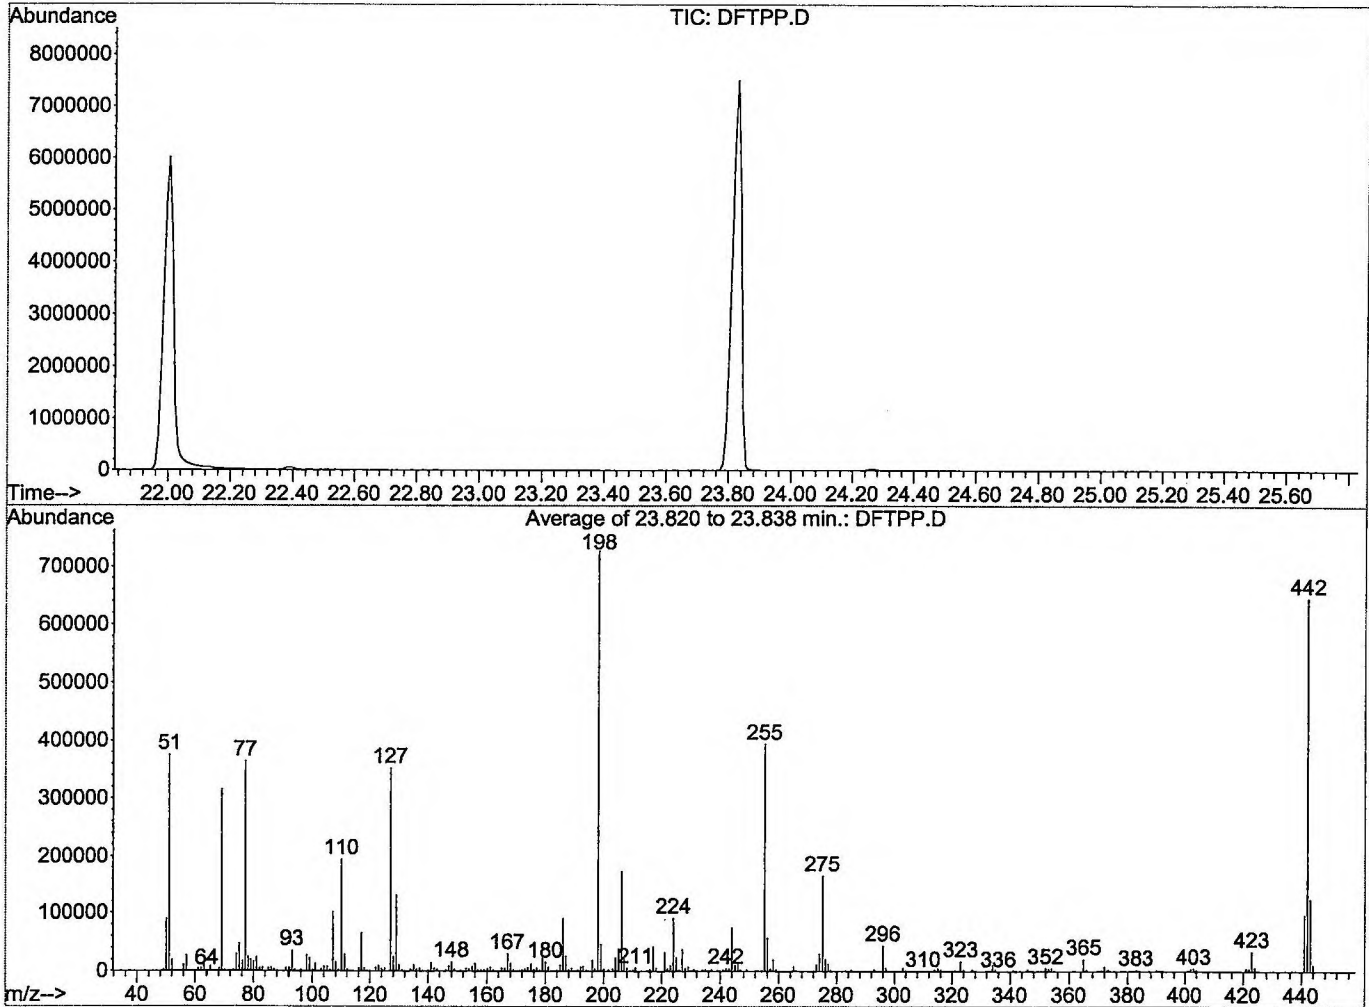

Spectrum Information: Average of 23.820 to 23.838 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.6	375253	PASS
68	69	0.00	2	1.4	4572	PASS
69	198	0.00	100	43.4	315434	PASS
70	69	0.00	2	0.5	1553	PASS
127	198	10	80	48.5	352234	PASS
197	198	0.00	2	0.6	4473	PASS
198	198	50	100	100.0	726954	PASS
199	198	5	9	6.4	46474	PASS
275	198	10	60	22.8	165994	PASS
365	198	1	100	2.9	20944	PASS
441	443	0.01	100	78.7	97208	PASS
442	198	50	100	88.9	646293	PASS
443	442	15	24	19.1	123576	PASS