

Method 508 modDate Extracted 3-19-02Page 15

Ref

#GCMS-18060

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500ul		1ml		2A	1ml		7			
Ref 1					1ml	8A						
Ref 2					↓	1A						
6436	FB					1B						
6449						4B						
6450						2A						
6451						4A						
6452						2B						
6453						1B						
6454						1A						
6455						8B						
6456	FB					4A						
6457						2B						
6458												
Remarks												
Reviewed by <u>CB 6/6/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type <u>sep Fun</u>		Solv. lot# <u>X01E19</u>		NaCl lot# <u>V39618</u>		Na2SO4 lot# <u>V46623</u>						
STANDARD	INT STD LOG#											
CALIBRATION	<u>1104100V</u>											
REF SPIKE	<u>2193</u>											
MDL/MDRF												
Q CHECK												
INT STD	<u>040802</u>											
SURROGATE	<u>GCMS 2160 A</u>											
LPC												
ENDRN/DDT												

Analyst EH
Revision 4/12/01Verified by ingReviewed by DN
Date 4/14/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\APR1702.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\apr1702\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch


☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0412	
2	Sample	2	CAL20	GCMS0412	
3	Sample	3	LB	GCMS0412	gc/ms scan 3/19
4	Sample	4	REF1	GCMS0412	gc/ms scan 3/19
5	Sample	5	REF2	GCMS0412	gc/ms scan 3/19
6	Sample	6	6430	GCMS0412	gc/ms scan 3/19 fb
7	Sample	7	6449	GCMS0412	gc/ms scan 3/19
8	Sample	8	6450	GCMS0412	gc/ms scan 3/19
9	Sample	9	6451	GCMS0412	gc/ms scan 3/19
10	Sample	10	6452	GCMS0412	gc/ms scan 3/19
11	Sample	11	6453	GCMS0412	gc/ms scan 3/19
12	Sample	12	6454	GCMS0412	gc/ms scan 3/19
13	Sample	13	6455	GCMS0412	gc/ms scan 3/19
14	Sample	14	6456	GCMS0412	gc/ms scan 3/19 fb
15	Sample	15	6457	GCMS0412	gc/ms scan 3/19
16	Sample	16	LBA	GCMS0412	gc/ms scan 4/8
17	Sample	17	REFA1	GCMS0412	gc/ms scan 4/8
18	Sample	18	REFA2	GCMS0412	gc/ms scan 4/8
19	Sample	19	5749	GCMS0412	gc/ms scan 4/8
20	Sample	20	8209	GCMS0412	gc/ms scan 4/8
21	Sample	21	8210	GCMS0412	gc/ms scan 4/8
22	Sample	22	8211	GCMS0412	gc/ms scan 4/8
23	Sample	23	8212	GCMS0412	gc/ms scan 4/8
24	Sample	24	8213	GCMS0412	gc/ms scan 4/8
25	Sample	25	8214	GCMS0412	gc/ms scan 4/8
26	Sample	26	8215	GCMS0412	gc/ms scan 4/8
27	Sample	27	8216	GCMS0412	gc/ms scan 4/8 fb
28	Sample	3	SURR	GCMS0412	

DFTPP

Data File : C:\HPCHEM\1\DATA\APR1702\DFTPP.D
 Acq On : 17 Apr 2002 8:12 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

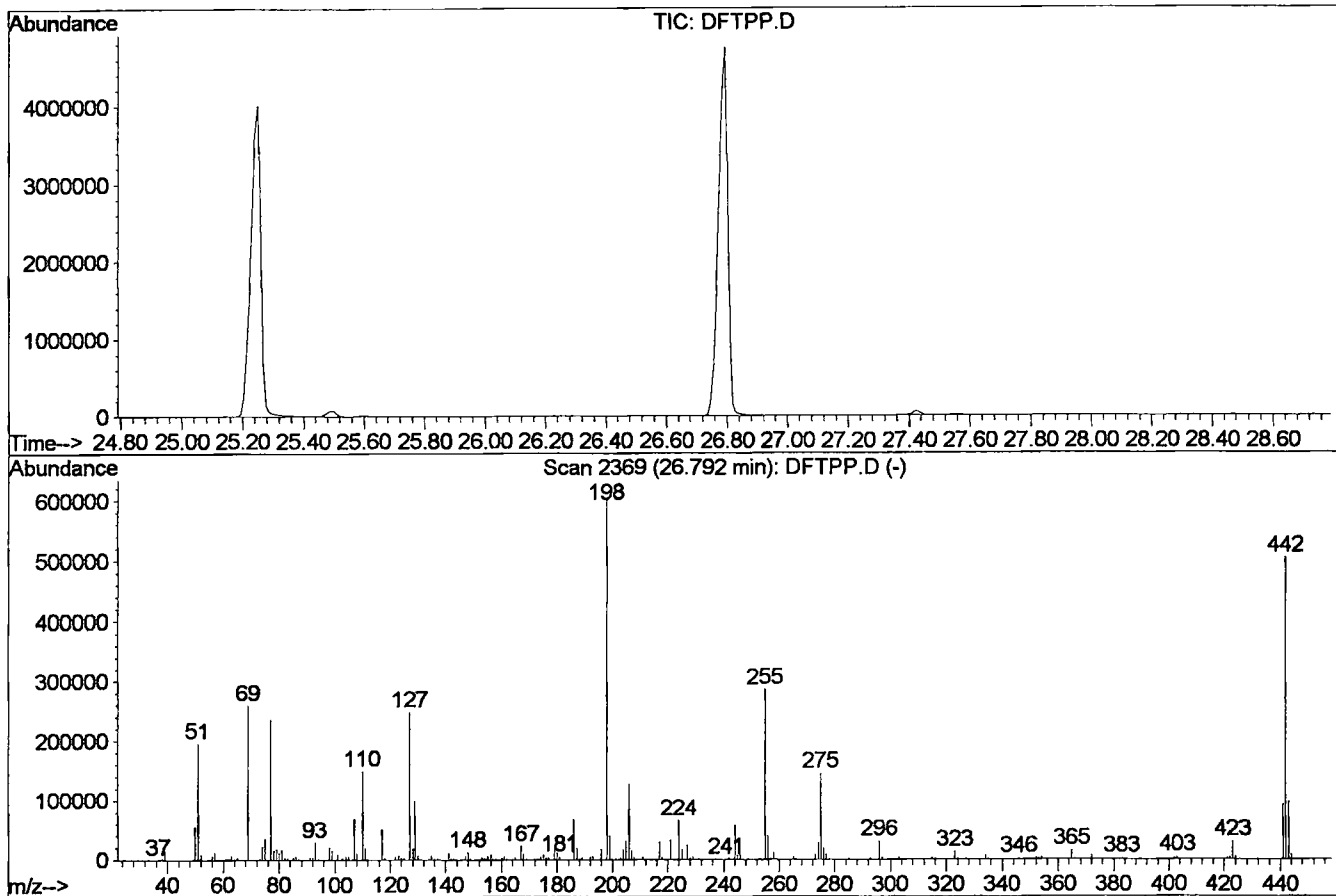

Spectrum Information: Scan 2369

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60 ✓	32.5	196153	PASS
68	69	0.00	2 ✓	0.0	0	PASS
69	198	0.00	100 ✓	43.0	260034	PASS
70	69	0.00	2 ✓	0.0	0	PASS
127	198	40	60 ✓	41.2	249246	PASS
197	198	0.00	1 ✓	0.0	0	PASS
198	198	100	100 ✓	100.0	604285	PASS
199	198	5	9 ✓	6.7	40208	PASS
275	198	10	30 ✓	24.0	145125	PASS
365	198	1	100 ✓	2.5	15138	PASS
441	443	0.01	100 ✓	95.2	92455	PASS
442	198	40 51	110 ✓	83.5	504424	PASS
443	442	17	23 ✓	19.3	97106	PASS