


File : C:\MSDCHEM\1\DATA\041502\DFTA0415.D
 Operator : Bohlk
 Acquired : 15 Apr 2002 9:58 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: DFTPP
 Misc Info :
 Vial Number: 1

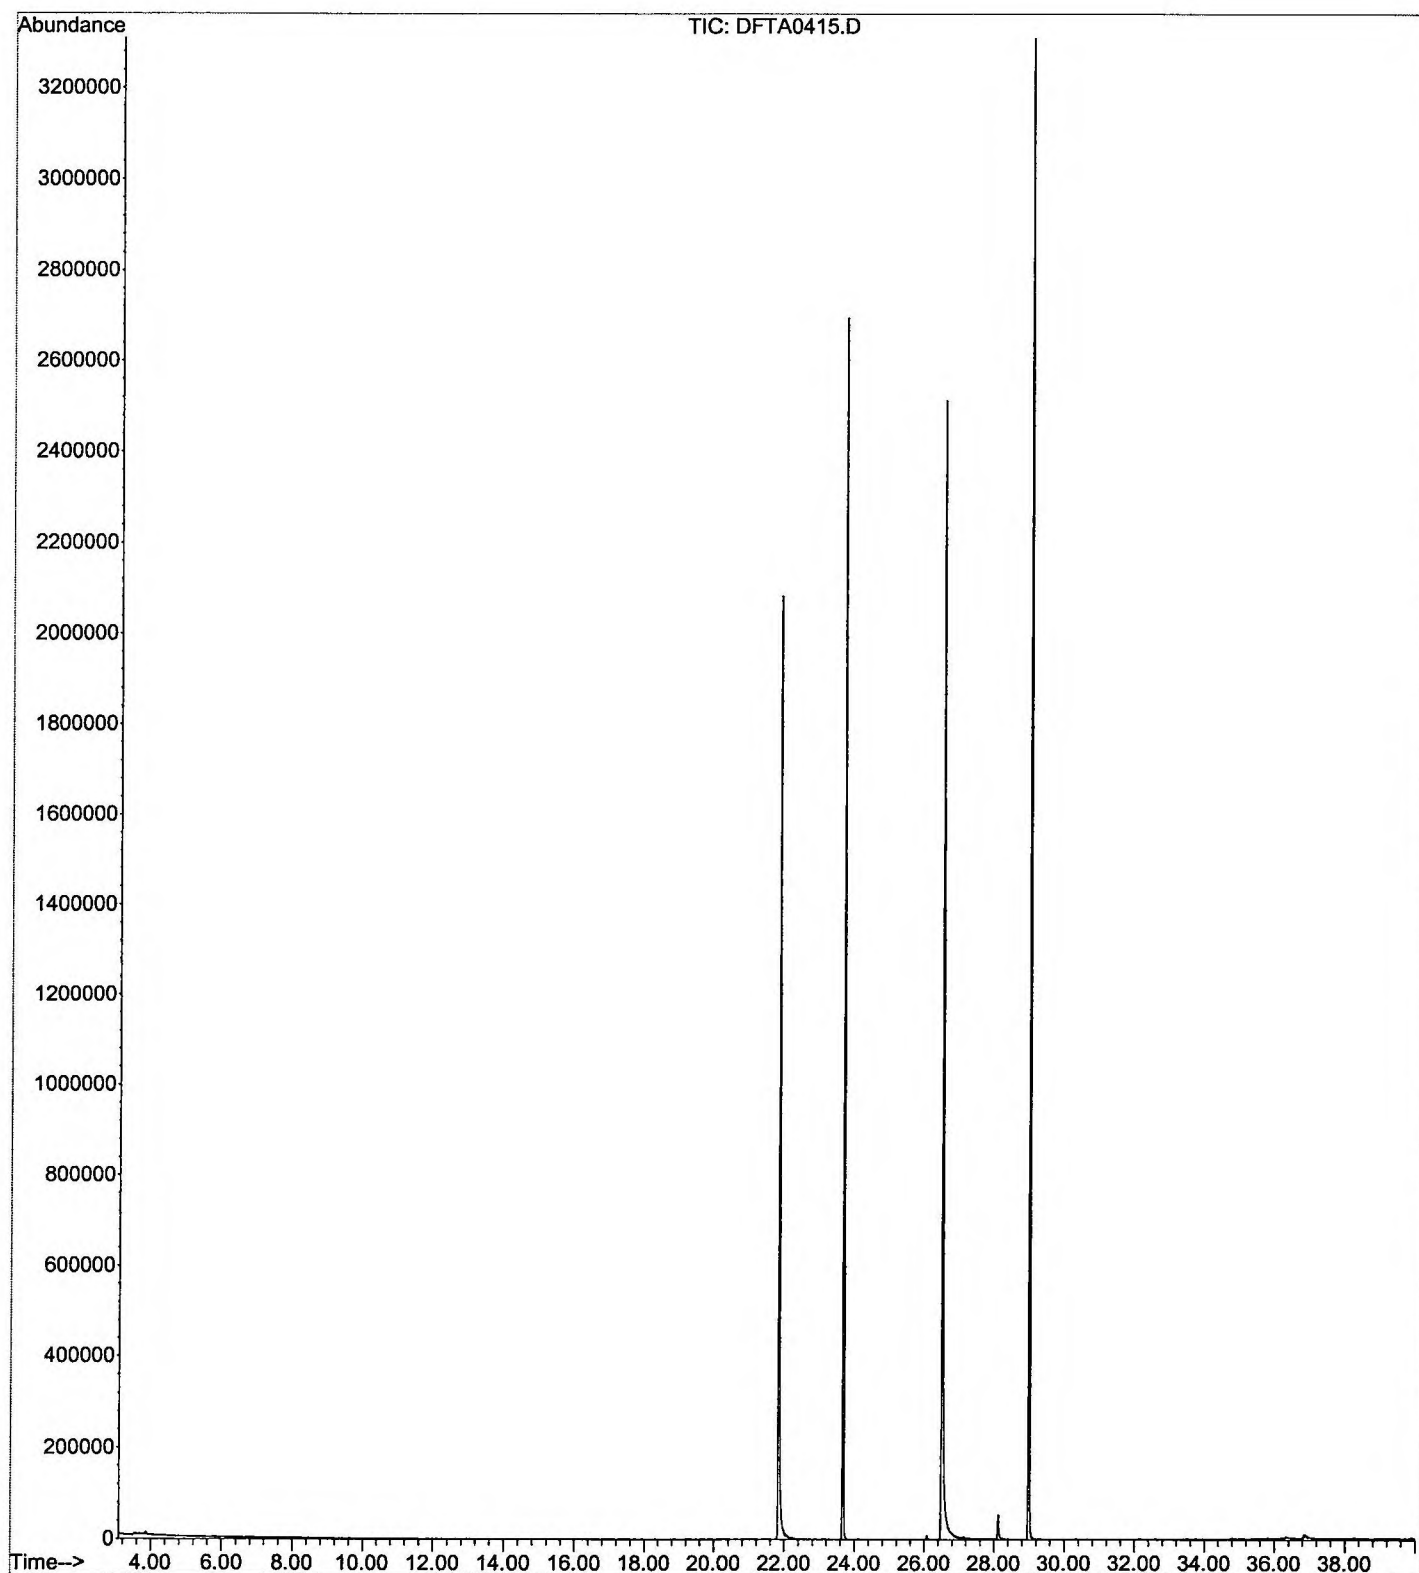

DFTPP

✓ Data File : C:\MSDCHEM\1\DATA\041502\DFTA0415.D
Acq On : 15 Apr 2002 9:58 am
Sample : DFTPP
Misc :
MS Integration Params: BENZO.P

Vial: 1
Operator: Bohlk
Inst : Instrumen
Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
Title : Quantitation For Method 508gcscan

Spectrum Information: Scan 3506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	45.2	150720	PASS
68	69	0.00	2	1.1	1810	PASS
69	198	0.00	100	47.3	157952	PASS
70	69	0.00	2	0.5	812	PASS
127	198	40	60	50.8	169472	PASS
197	198	0.00	1	0.4	1407	PASS
198	198	100	100	100.0	333632	PASS
199	198	5	9	6.6	21960	PASS
275	198	10	30	20.0	66840	PASS
365	198	1	100	2.0	6652	PASS
441	443	0.01	100	79.4	27248	PASS
442	198	40	110	50.2	167552	PASS
443	442	17	23	20.5	34304	PASS

DFTA0415.D 5080402BBC.M

Mon Apr 15 10:38:50 2002