



User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 04/18/2002 Time: 12:26:20

Sample: AE06587
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 4/18/2002 12:25 Ended: 4/18/2002 12:25 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	MDL
1	Other unknown compounds		.	
2	Surr_2,4-DDD		114	5.0

Comments for Sample AE06587 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-18-2002 Time: 12:26:30

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\041502\6587.D

Acq On : 15 Apr 2002 6:16 pm

Sample : SAMPLE 6587 3/20/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 17 17:39:22 2002

Vial: 11

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.41	152	404966	40.00	ug/L	0.00
10) Naphthalene-d8	12.88	136	1838905	40.00	ug/L	0.00
17) Acenaphthene-d10	17.99	164	1001284	40.00	ug/L	0.00
30) Phenanthrene-d10	22.33	188	1438263	40.00	ug/L	0.00
39) Chrysene-d12	30.14	240	1147267	40.00	ug/L	-0.01
45) Perylene-d12	34.01	264	695869	40.00	ug/L	0.00

System Monitoring Compounds

28) TCMX (SURR)	0.00	244	0	0.00	ug/L	
Spiked Amount	10.000		Recovery	=	0.00%	
38) 2,4-DDD (SURR)	27.28	235	122072	11.40	ug/L	0.01
Spiked Amount	10.000		Recovery	=	114.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	d
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
32) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	0.00	178	0	N.D.	
35) Anthracene	0.00	178	0	N.D.	
36) Di-n-butylphthalate	0.00	149	0	N.D.	
37) Fluoranthene	0.00	202	0	N.D.	
40) Pyrene	0.00	202	0	N.D.	
41) Butylbenzylphthalate	0.00	149	0	N.D.	
42) Benzo (a) anthracene	0.00	228	0	N.D.	d
43) Bis (2-ethylhexyl) phthala	30.78	149	8058	0.28	ug/L 83
44) Chrysene	0.00	228	0	N.D.	d

(#)= qualifier out of range (m) = manual integration

6587.D 5080402BBC.M Wed Apr 17 17:41:06 2002

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\041502\6587.D

Acq On : 15 Apr 2002 6:16 pm

Sample : SAMPLE 6587 3/20/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 17 17:39:22 2002

Vial: 11

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo (b) fluoranthene	0.00	252	0	N.D.		
48) Benzo (k) fluoranthene	0.00	252	0	N.D.		
49) Benzo (a) pyrene	0.00	252	0	N.D.		
50) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
51) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
52) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

6587.D 5080402BBC.M Wed Apr 17 17:41:07 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\041502\6587.D

Acq On : 15 Apr 2002 6:16 pm

Sample : SAMPLE 6587 3/20/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 17 17:40 2002

Vial: 11

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00


Quant Results File: 5080402BBC.RES

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

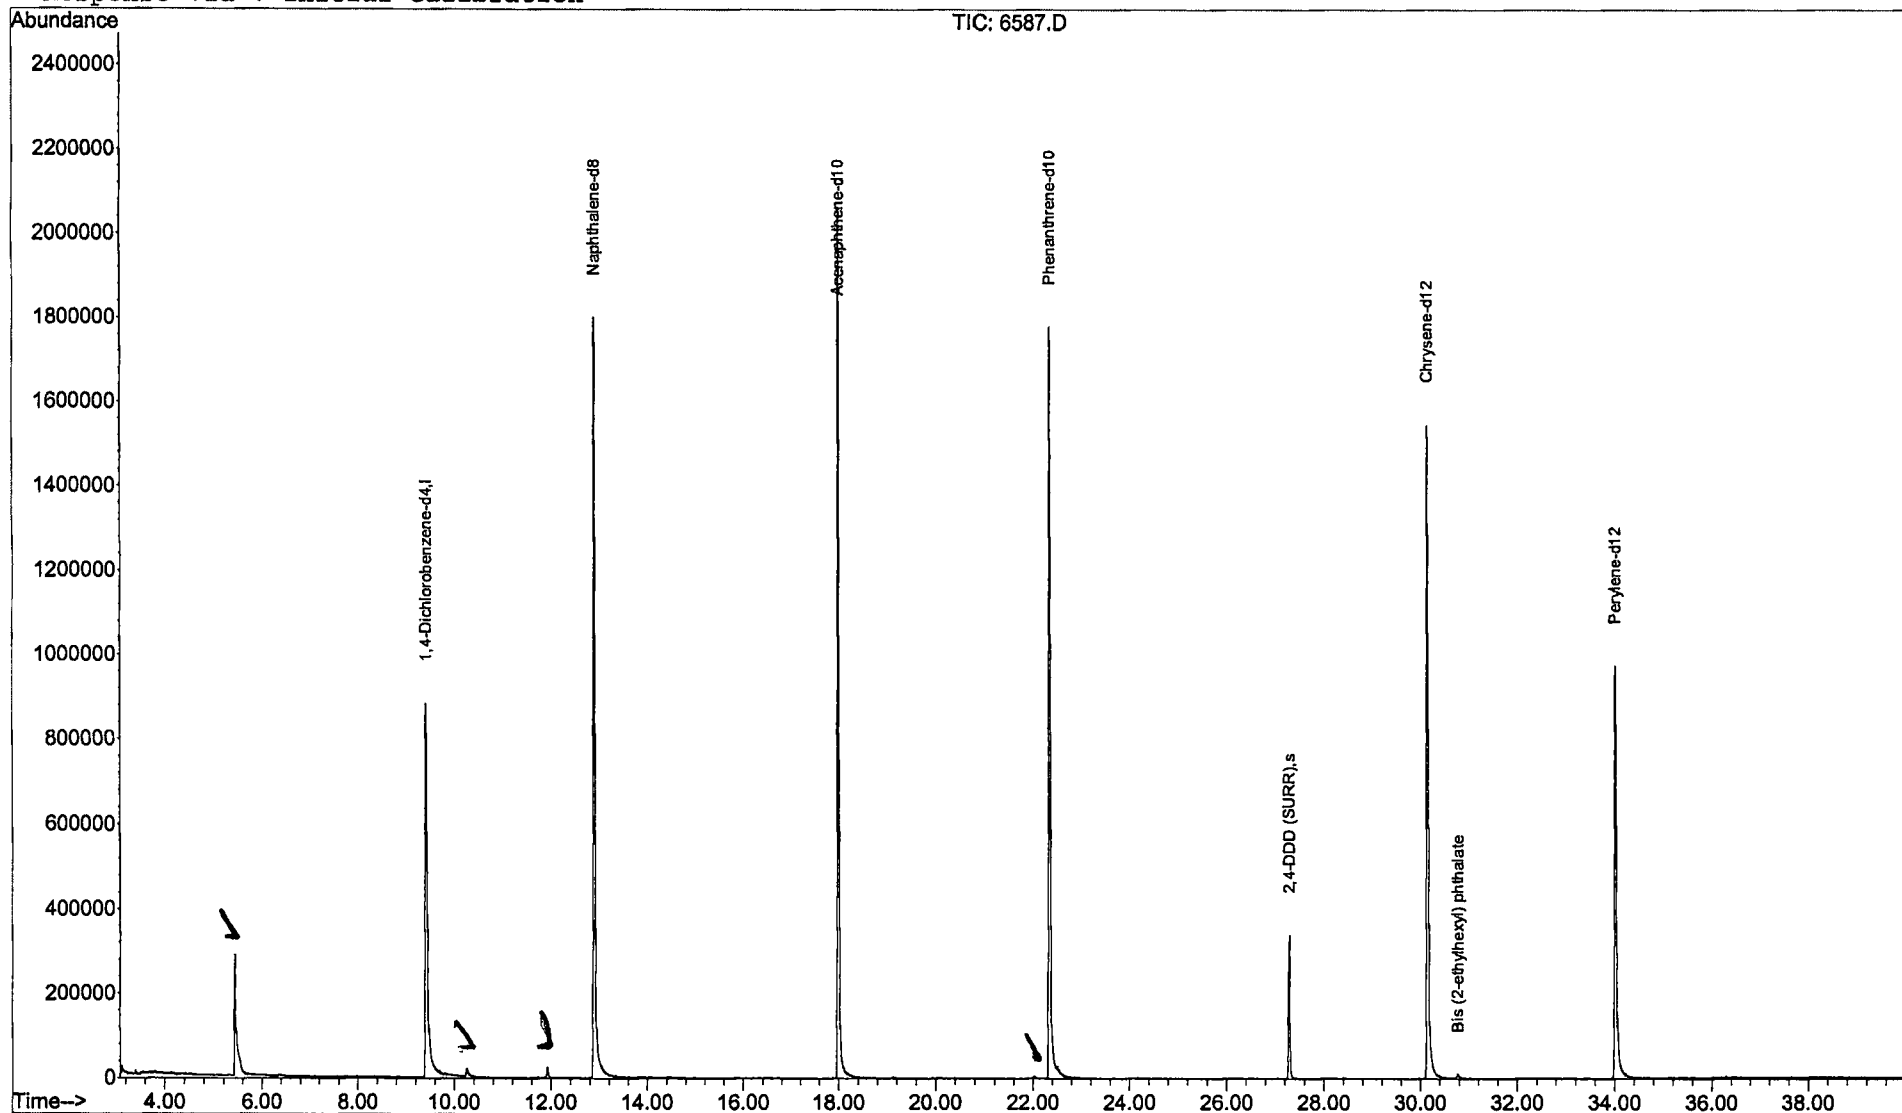

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\041502\6587.D Vial: 11
Acq On : 15 Apr 2002 6:16 pm Operator: Bohlk
Sample : SAMPLE 6587 3/20/02 Inst : Instrumen
Misc : Multiplr: 1.00
MS Integration Params: LSCINT.P

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.429	396	400	426	rBV	284950	832895	19.50%	3.670%
2	9.407	1071	1077	1099	rBV	880664	2596508	60.79%	11.440%
3	10.259	1215	1222	1229	rBV3	18490	51260	1.20%	0.226%
4	11.928	1499	1506	1513	rBV	24317	43451	1.02%	0.191%
5	12.880	1661	1668	1695	rBV	1800490	3999789	93.65%	17.622%
6	17.985	2529	2537	2554	rBV	2058052	4271145	100.00%	18.818%
7	22.339	3269	3278	3303	rBV2	1778763	4140291	96.94%	18.241%
8	27.281	4112	4119	4131	rBV	337449	664827	15.57%	2.929%
9	30.142	4596	4606	4628	rBV2	1544727	3583350	83.90%	15.788%
10	34.014	5256	5265	5282	rBV2	974011	2513789	58.86%	11.075%

Sum of corrected areas: 22697305

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\041502\6587.D
 Operator : Bohlk
 Acquired : 15 Apr 2002 6:16 pm using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: SAMPLE 6587 3/20/02
 Misc Info :
 Vial Number: 11
 Quant File :5080402BBC.RES (RTE Integrator)

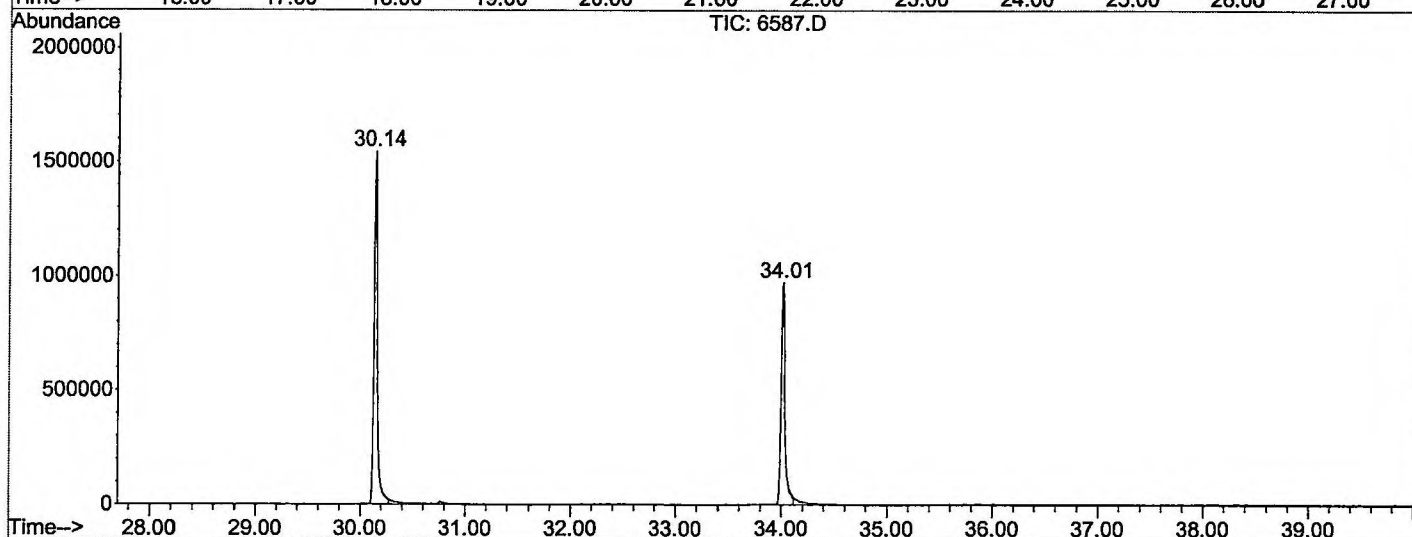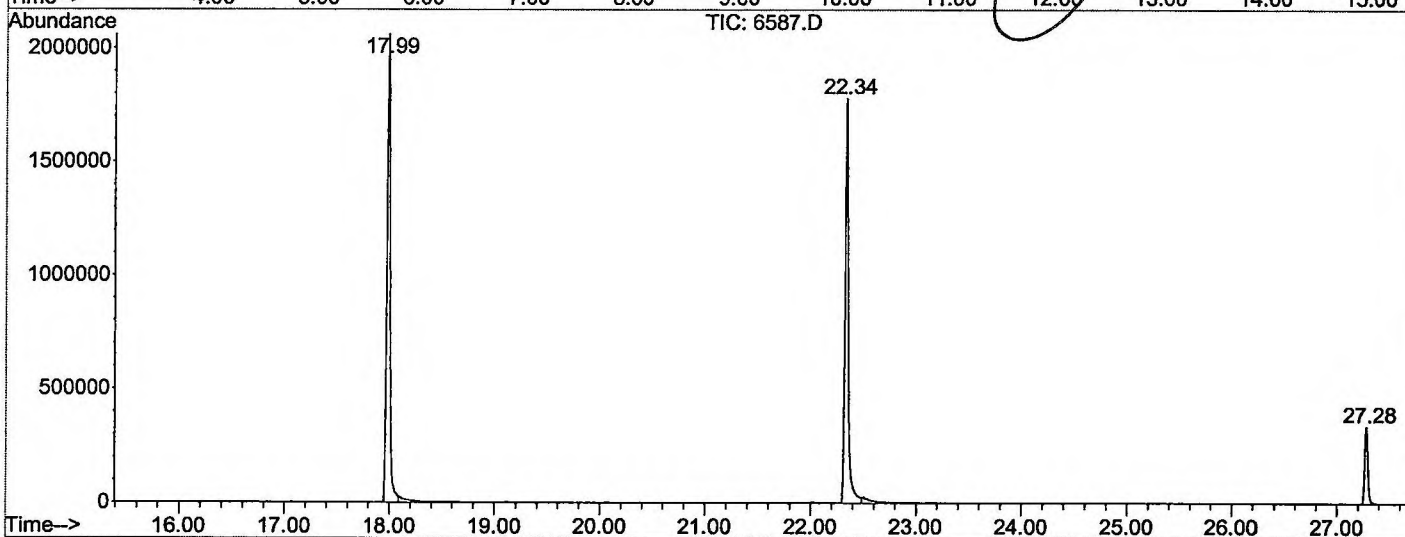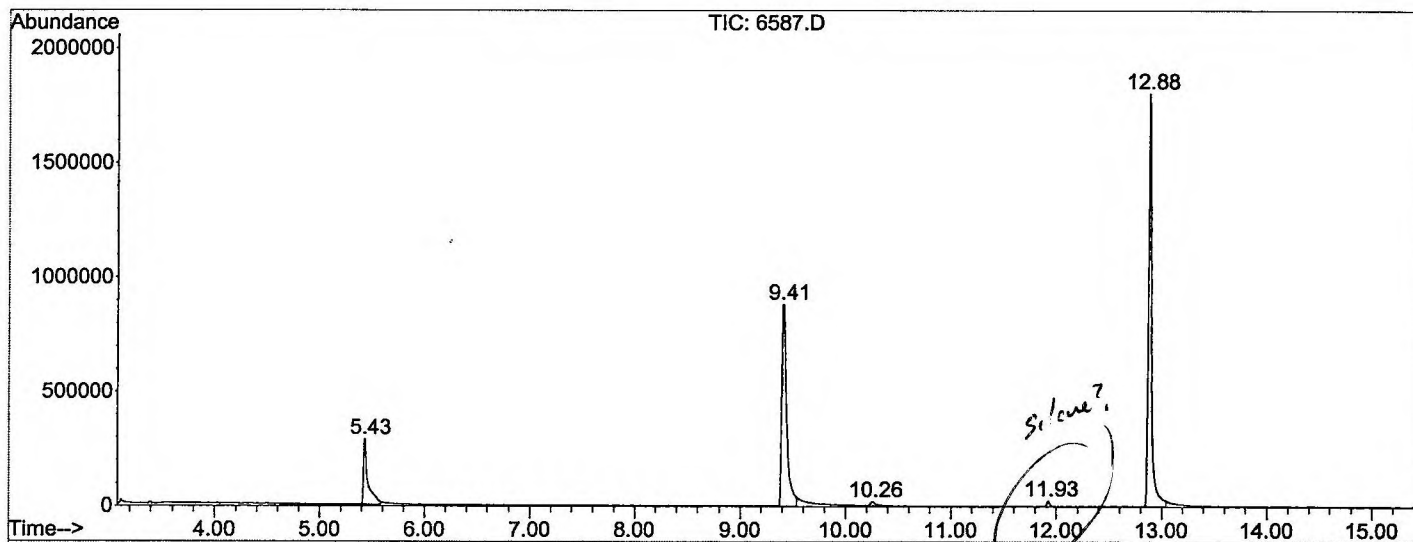

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\041502\6587.D

Acq On : 15 Apr 2002 6:16 pm

Sample : SAMPLE 6587 3/20/02

Misc :

MS Integration Params: LSCINT.P

Vial: 11

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)










Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 Butane, 2-methoxy-2-methyl-... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.43	12.83 ug/L	832895	1,4-Dichlorobenzene-d4	9.41

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl- \$\$ E...	102	C6H14O	000994-05-8	36
2			3-(CYCLOHEX-3'-EN-YL)PROPANOL \$\$...	174	C8H14O4	015745-87-6	33
3			Acetic acid, 3-[1,3]dioxolan-2-y...	174	C8H14O4	000000-00-0	33
4			N-Ethylformamide \$\$ N-Formylethy...	73	C3H7NO	000627-45-2	9

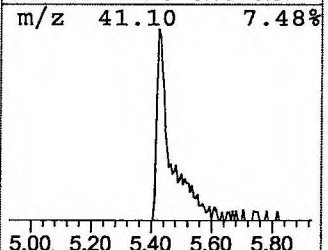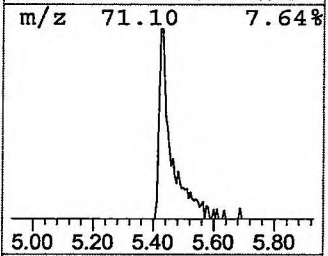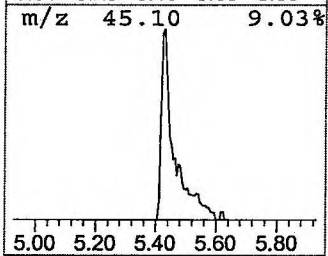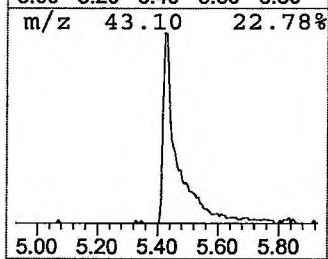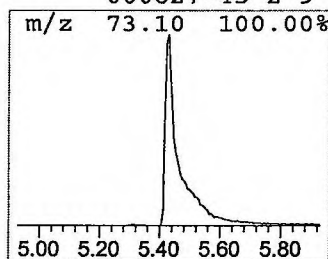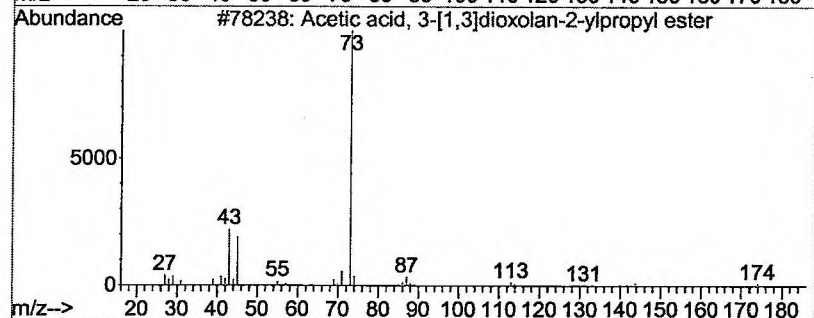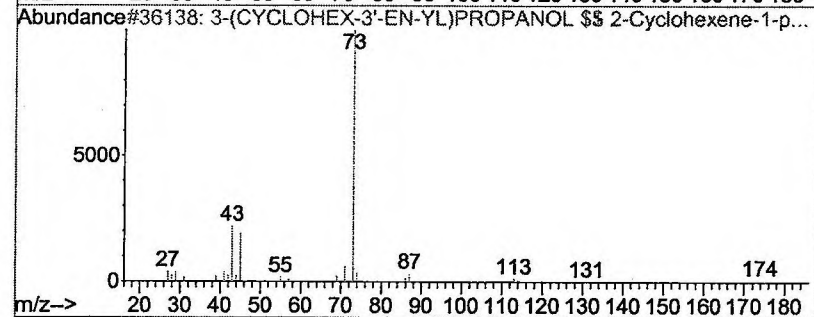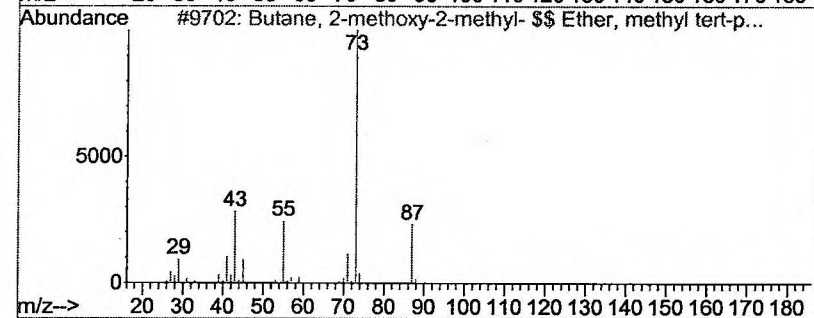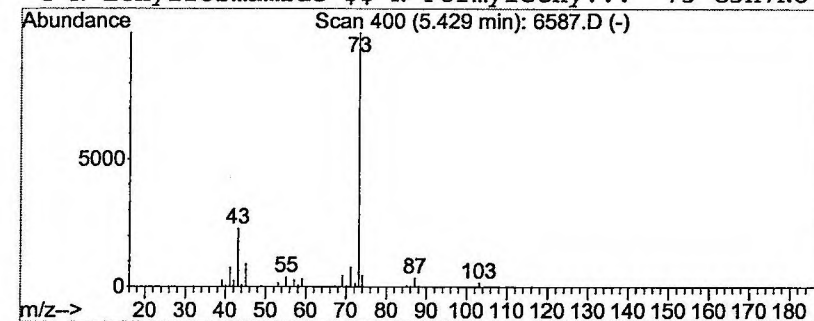

Tentatively Identified Compound (LSC) summary

Operator ID: Bohlk Date Acquired: 15 Apr 2002 6:16 pm
 Data File: C:\MSDCHEM\1\DATA\041502\6587.D
 Name: SAMPLE 6587 3/20/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	5.43	12.8	ug/L	832895	1	9.41	2596510	40.0