

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 04/19/2002 Time: 10:31:27

Sample: AE06797
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 4/19/02 10:31 Ended: 4/19/02 10:31 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		86		5.0

Comments for Sample AE06797 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-19-2002 Time: 10:31:57

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Data File : C:\MSDCHEM\1\DATA\041602\6797.D

Vial: 15

Acq On : 16 Apr 2002 8:10 pm

Operator: Bohlk

Sample : SAMPLE 6797 3/21/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 18 17:58:58 2002

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.41	152	392284	40.00	ug/L	0.00
10) Naphthalene-d8	12.88	136	1818954	40.00	ug/L	0.00
17) Acenaphthene-d10	17.99	164	1014175	40.00	ug/L	0.00
30) Phenanthrene-d10	22.33	188	1447802	40.00	ug/L	0.00
39) Chrysene-d12	30.14	240	1168111	40.00	ug/L	-0.02
45) Perylene-d12	34.01	264	717810	40.00	ug/L	0.00

System Monitoring Compounds

28) TCMX (SURR)	0.00	244	0	0.00	ug/L	
Spiked Amount	10.000		Recovery	=	0.00%	
38) 2,4-DDD (SURR)	27.27	235	92126	8.55	ug/L	0.00
Spiked Amount	10.000		Recovery	=	85.50%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	d
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2 ' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
32) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	0.00	178	0	N.D.	
35) Anthracene	0.00	178	0	N.D.	
36) Di-n-butylphthalate	0.00	149	0	N.D.	
37) Fluoranthene	0.00	202	0	N.D.	
40) Pyrene	0.00	202	0	N.D.	
41) Butylbenzylphthalate	0.00	149	0	N.D.	
42) Benzo (a) anthracene	0.00	228	0	N.D.	
43) Bis (2-ethylhexyl) phthala	0.00	149	0	N.D.	d
44) Chrysene	0.00	228	0	N.D.	

(#)=qualifier out of range (m)=manual integration

6797.D 5080402BBC.M

Thu Apr 18 18:00:03 2002

Page 1

Data File : C:\MSDCHEM\1\DATA\041602\6797.D

Vial: 15

Acq On : 16 Apr 2002 8:10 pm

Operator: Bohlk

Sample : SAMPLE 6797 3/21/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 18 17:58:58 2002

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo (b) fluoranthene	0.00	252	0	N.D.		
48) Benzo (k) fluoranthene	0.00	252	0	N.D.		
49) Benzo (a) pyrene	0.00	252	0	N.D.		
50) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
51) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
52) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

6797.D 5080402BBC.M Thu Apr 18 18:00:03 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\041602\6797.D

Acq On : 16 Apr 2002 8:10 pm

Sample : SAMPLE 6797 3/21/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 18 17:59 2002

Vial: 15

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00


Quant Results File: 5080402BBC.RES

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

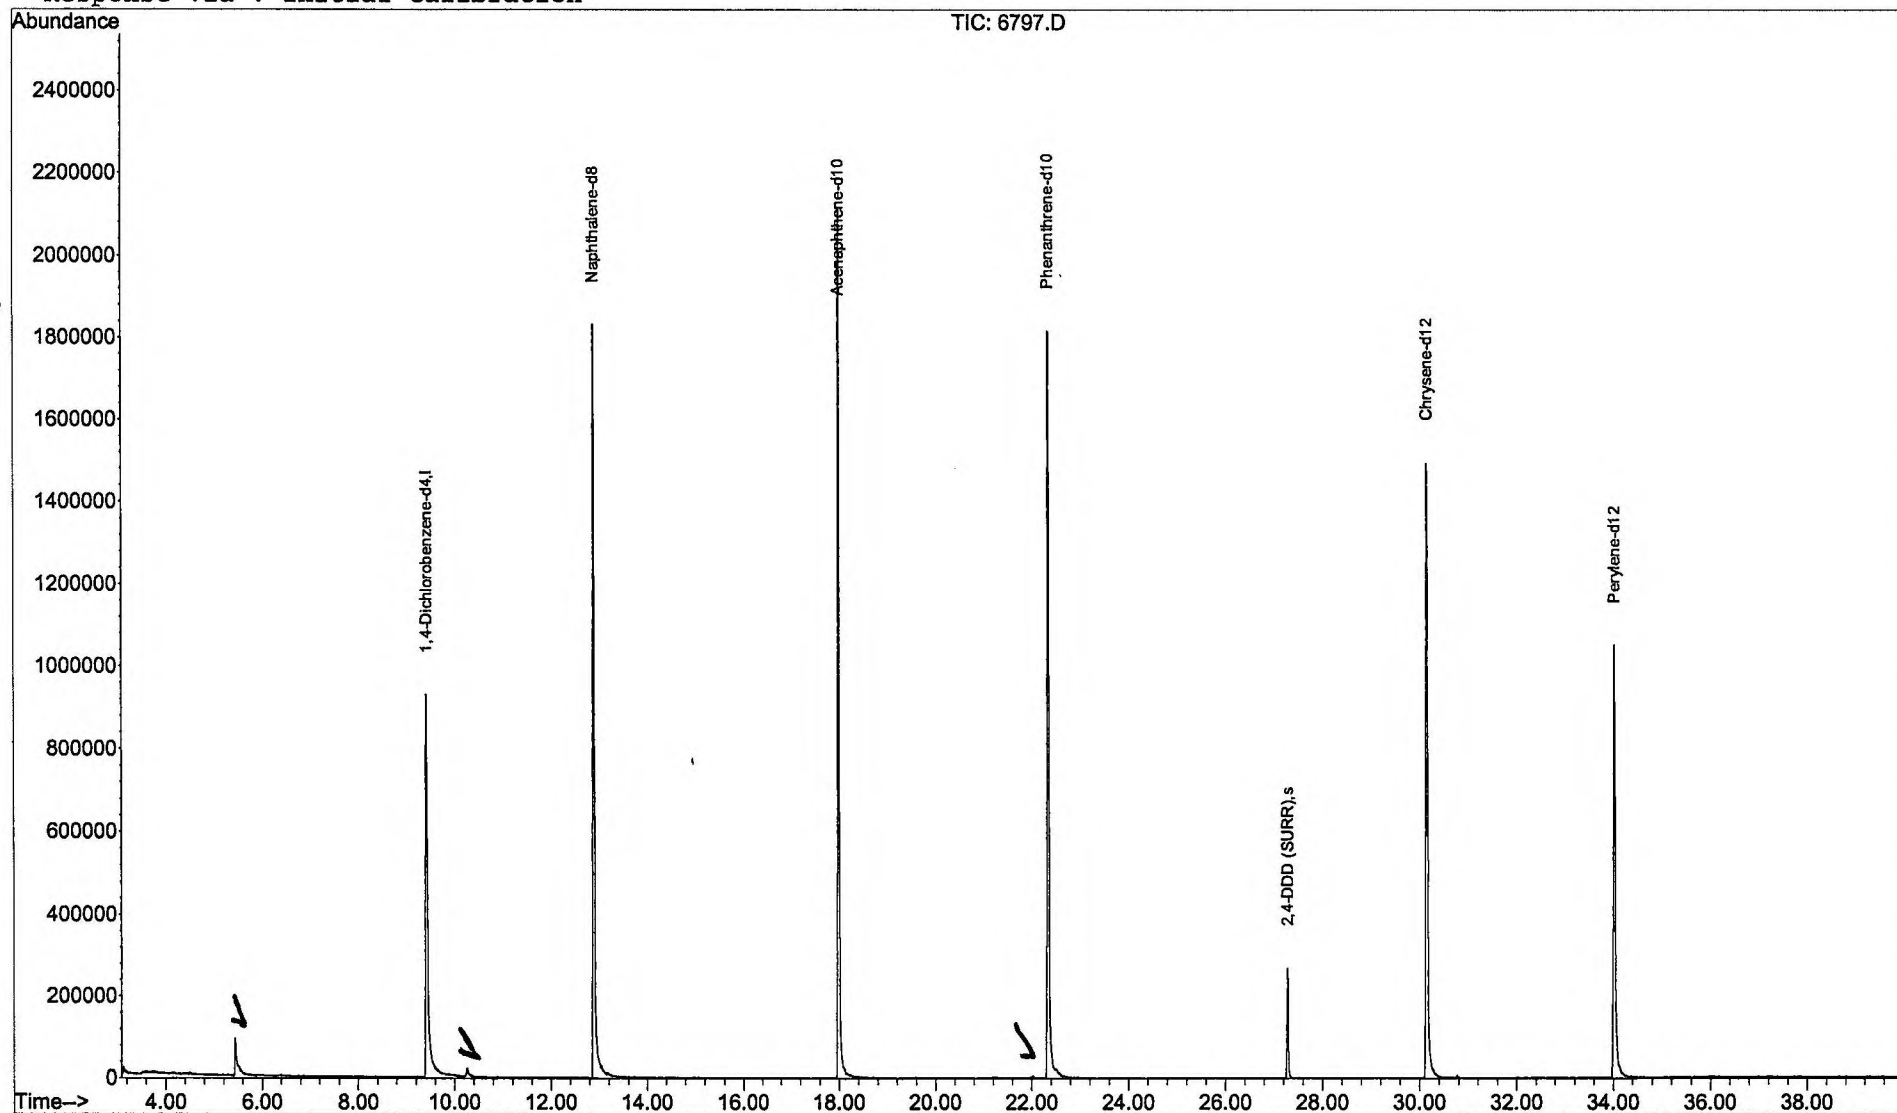

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\041602\6797.D

Vial: 15

Acq On : 16 Apr 2002 8:10 pm

Operator: Bohlk

Sample : SAMPLE 6797 3/21/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.435	397	401	417	rBV	90927	262303	5.98%	1.190%
2	9.407	1071	1077	1099	rBV	927771	2591766	59.08%	11.761%
3	10.259	1215	1222	1231	rBV3	17828	46906	1.07%	0.213%
4	12.880	1661	1668	1684	rBV	1829867	3839736	87.53%	17.424%
5	17.986	2528	2537	2562	rBV	2112792	4386895	100.00%	19.907%
6	22.334	3269	3277	3301	rBV2	1815909	4172217	95.11%	18.933%
7	27.275	4112	4118	4130	rBV3	267027	495095	11.29%	2.247%
8	30.136	4595	4605	4625	rBV2	1493555	3644336	83.07%	16.537%
9	34.014	5255	5265	5281	rBV	1050014	2597613	59.21%	11.788%

Sum of corrected areas: 22036867

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\041602\6797.D
 Operator : Bohlk
 Acquired : 16 Apr 2002 8:10 pm using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: SAMPLE 6797 3/21/02
 Misc Info :
 Vial Number: 15
 Quant File :5080402BBC.RES (RTE Integrator)

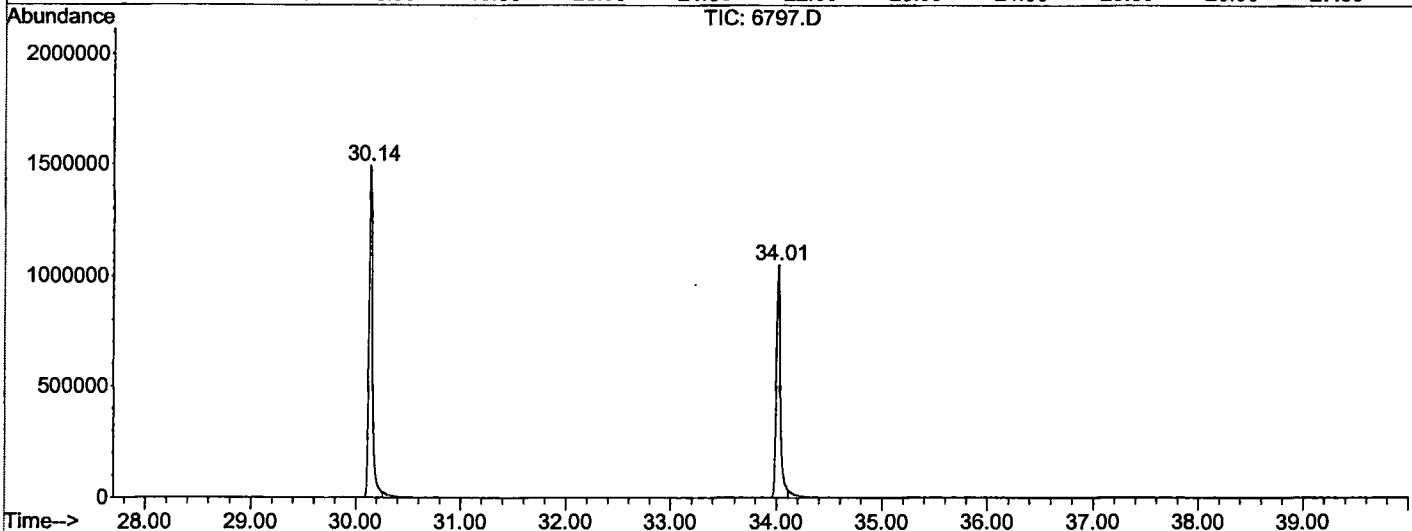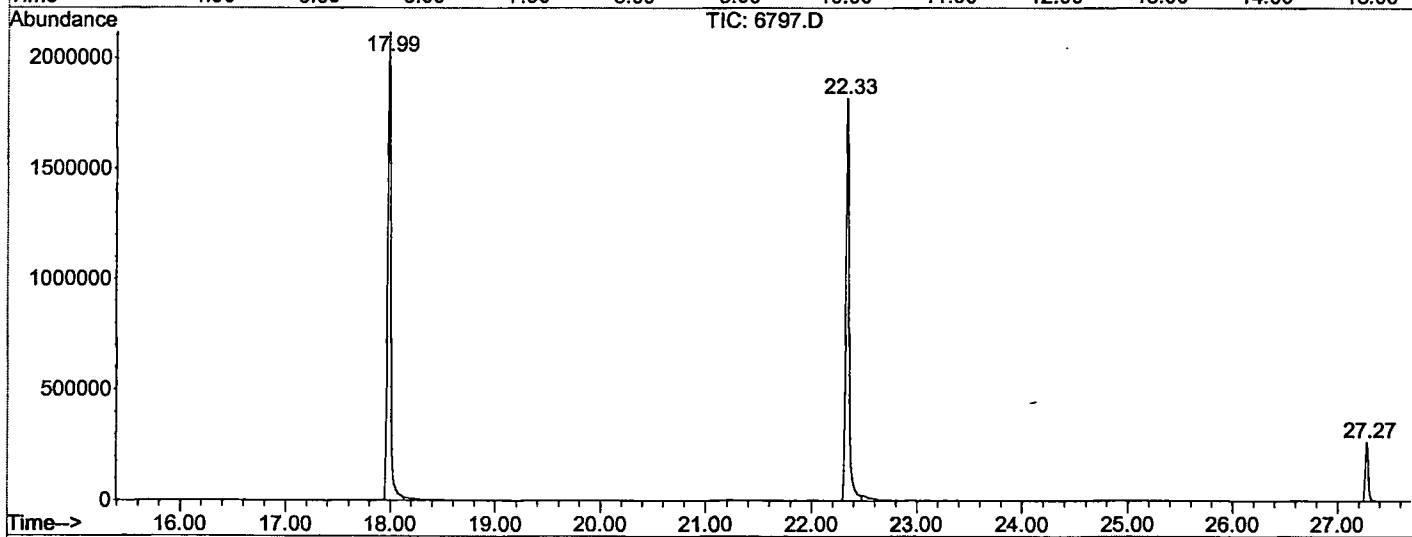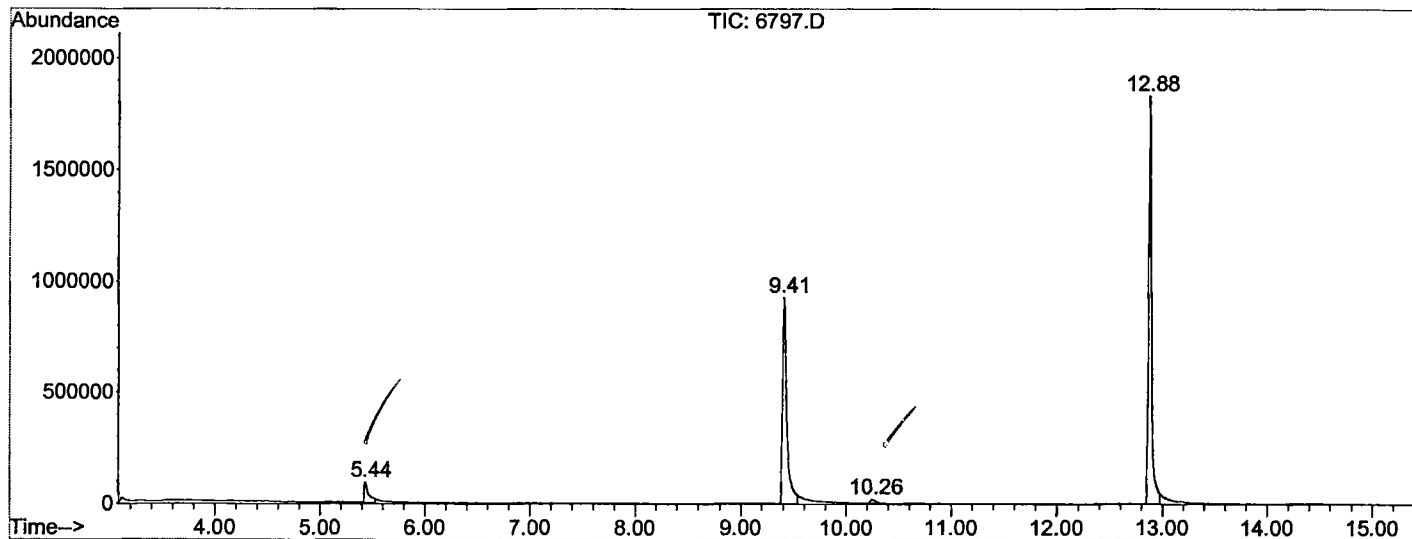

Data File : C:\MSDCHEM\1\DATA\041602\6797.D

Acq On : 16 Apr 2002 8:10 pm

Sample : SAMPLE 6797 3/21/02

Misc :

MS Integration Params: LSCINT.P

Vial: 15

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)










Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 3-(CYCLOHEX-3'-EN-YL)PROPAN... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.44	4.05 ug/L	262303	1,4-Dichlorobenzene-d4	9.41

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-(CYCLOHEX-3'-EN-YL)PROPANOL \$\$...	174	C8H14O4	015745-87-6	38
2			Acetic acid, 3-[1,3]dioxolan-2-y...	174	C8H14O4	000000-00-0	38
3			Butane, 2-methoxy-2-methyl- \$\$ E...	102	C6H14O	000994-05-8	36
4			N-Ethylformamide \$\$ N-Formylethy...	73	C3H7NO	000627-45-2	9

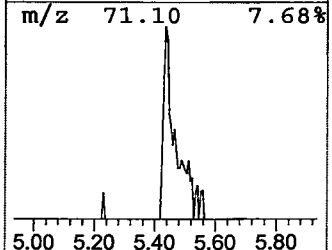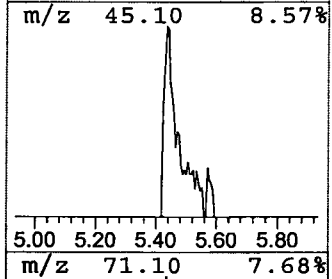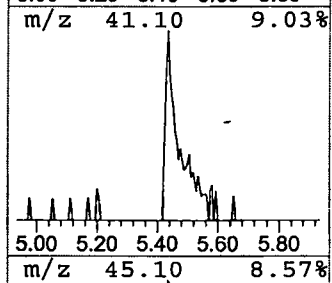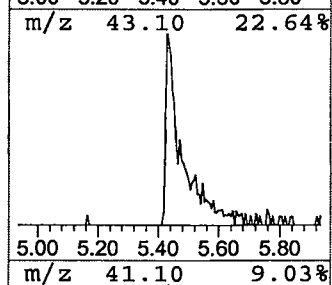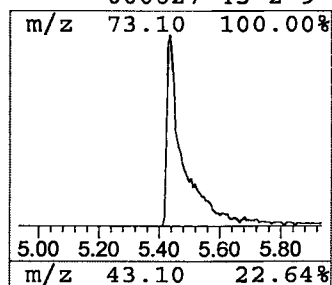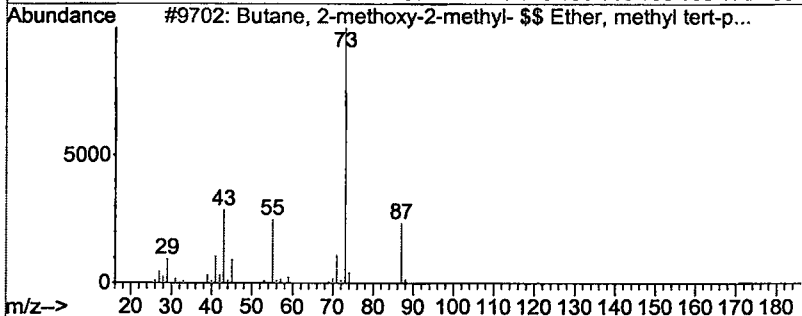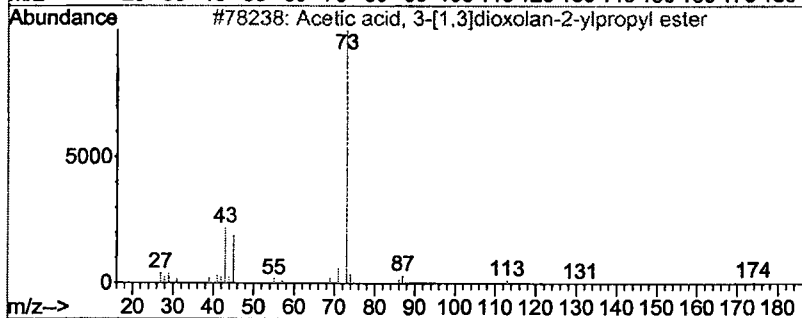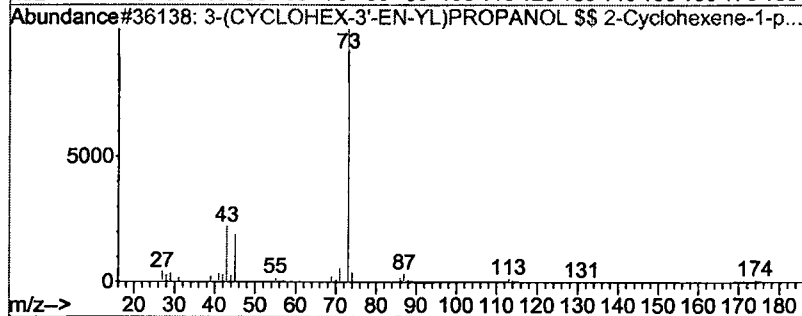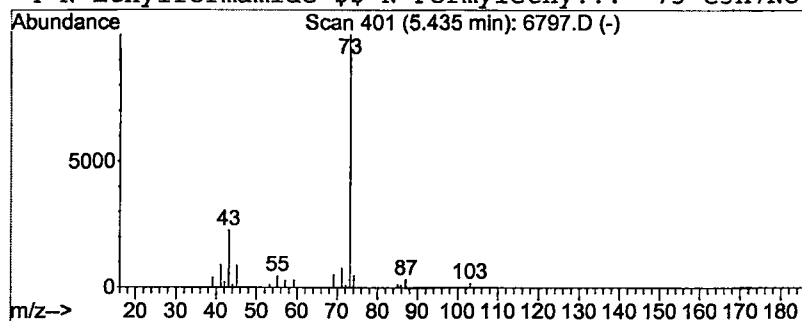

Tentatively Identified Compound (LSC) summary

Operator ID: Bohlk Date Acquired: 16 Apr 2002 8:10 pm
 Data File: C:\MSDCHEM\1\DATA\041602\6797.D
 Name: SAMPLE 6797 3/21/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
3-(CYCLOHEX-3'-EN...	5.44	4.0	ug/L	262303	1	9.41	2591770	40.0