

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 04/19/2002 Time: 10:02:27

Sample: AE06796
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 4/19/02 10:01 Ended: 4/19/02 10:01 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		95		5.0

Comments for Sample AE06796 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-19-2002 Time: 10:02:52

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Data File : C:\MSDCHEM\1\DATA\041602\6796.D

Vial: 14

Acq On : 16 Apr 2002 7:21 pm

Operator: Bohlk

Sample : SAMPLE 6796 3/21/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 18 17:54:44 2002

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.41	152	464820	40.00	ug/L	0.00
10) Naphthalene-d8	12.88	136	2076302	40.00	ug/L	0.00
17) Acenaphthene-d10	17.99	164	1185184	40.00	ug/L	0.00
30) Phenanthrene-d10	22.34	188	1683228	40.00	ug/L	0.00
39) Chrysene-d12	30.14	240	1333187	40.00	ug/L	-0.01
45) Perylene-d12	34.01	264	832990	40.00	ug/L	0.00

System Monitoring Compounds

28) TCMX (SURR)	0.00	244	0	0.00	ug/L	
Spiked Amount	10.000		Recovery	=	0.00%	
38) 2,4-DDD (SURR)	27.28	235	118912	9.49	ug/L	0.01
Spiked Amount	10.000		Recovery	=	94.90%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	d
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2 ' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
32) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	0.00	178	0	N.D.	
35) Anthracene	0.00	178	0	N.D.	
36) Di-n-butylphthalate	0.00	149	0	N.D.	
37) Fluoranthene	0.00	202	0	N.D.	
40) Pyrene	0.00	202	0	N.D.	
41) Butylbenzylphthalate	0.00	149	0	N.D.	
42) Benzo (a) anthracene	0.00	228	0	N.D.	d
43) Bis (2-ethylhexyl) phthala	30.77	149	4175	0.13	ug/L 85
44) Chrysene	0.00	228	0	N.D.	d

(#)= qualifier out of range (m)= manual integration

6796.D 5080402BBC.M Thu Apr 18 17:56:07 2002

Page 1

Data File : C:\MSDCHEM\1\DATA\041602\6796.D

Vial: 14

Acq On : 16 Apr 2002 7:21 pm

Operator: Bohlk

Sample : SAMPLE 6796 3/21/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 18 17:54:44 2002

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo (b) fluoranthene	0.00	252	0	N.D.		
48) Benzo (k) fluoranthene	0.00	252	0	N.D.		
49) Benzo (a) pyrene	0.00	252	0	N.D.	d	
50) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
51) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
52) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

6796.D 5080402BBC.M Thu Apr 18 17:56:07 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\041602\6796.D

Acq On : 16 Apr 2002 7:21 pm

Sample : SAMPLE 6796 3/21/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 18 17:55 2002

Vial: 14

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00


Quant Results File: 5080402BBC.RES

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

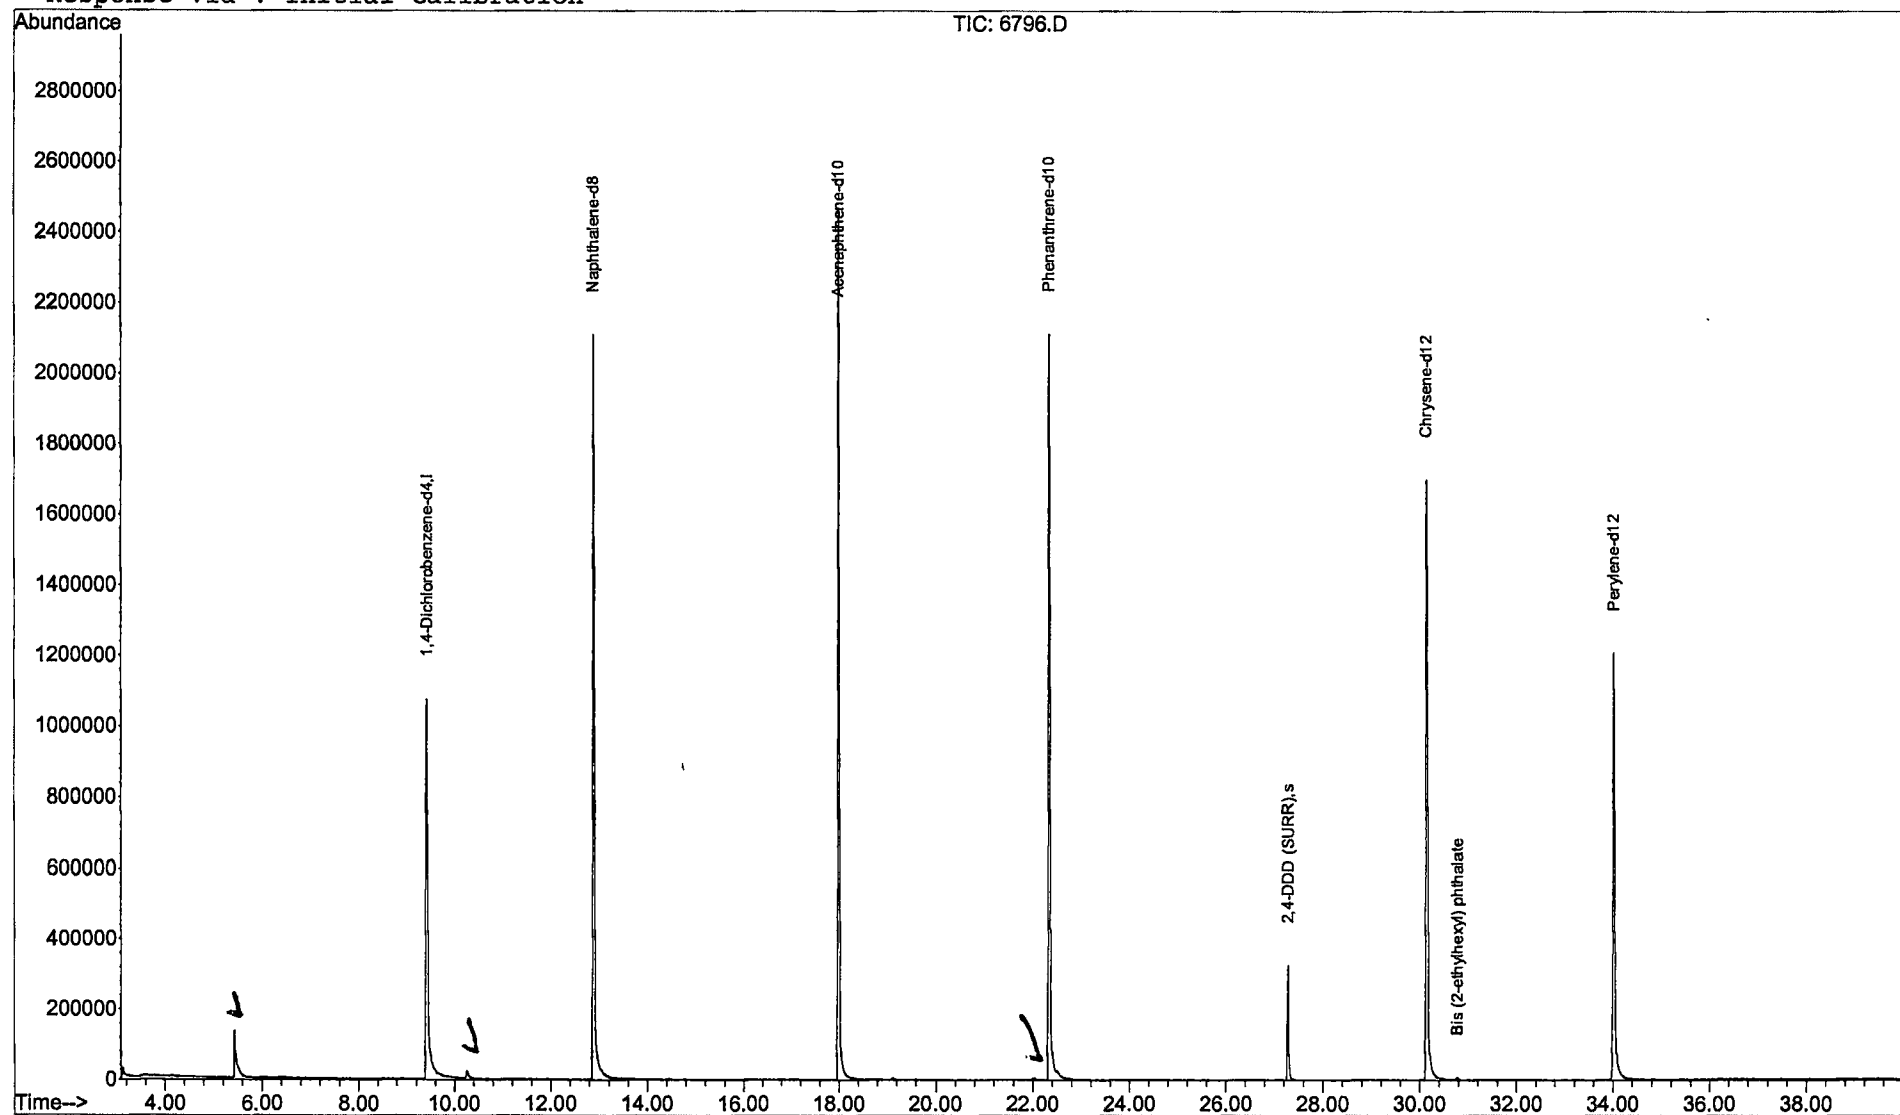

Data File : C:\MSDCHEM\1\DATA\041602\6796.D

Vial: 14

Acq On : 16 Apr 2002 7:21 pm

Operator: Bohlk

Sample : SAMPLE 6796 3/21/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.435	397	401	426	rBV	132244	399390	7.91%	1.545%
2	9.413	1071	1078	1102	rBV	1073745	3016410	59.73%	11.665%
3	10.253	1215	1221	1230	rBV3	21040	59728	1.18%	0.231%
4	12.880	1661	1668	1694	rBV	2110706	4543796	89.98%	17.572%
5	17.985	2529	2537	2560	rBV	2464640	5049725	100.00%	19.529%
6	22.339	3269	3278	3298	rBV2	2112730	4814573	95.34%	18.619%
7	27.281	4112	4119	4130	rBV	324522	629552	12.47%	2.435%
8	30.142	4597	4606	4632	rBV2	1698838	4238978	83.94%	16.393%
9	34.014	5255	5265	5297	rBV2	1205816	3105790	61.50%	12.011%

Sum of corrected areas: 25857942

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\041602\6796.D
 Operator : Bohlk
 Acquired : 16 Apr 2002 7:21 pm using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: SAMPLE 6796 3/21/02
 Misc Info :
 Vial Number: 14
 Quant File :5080402BBC.RES (RTE Integrator)

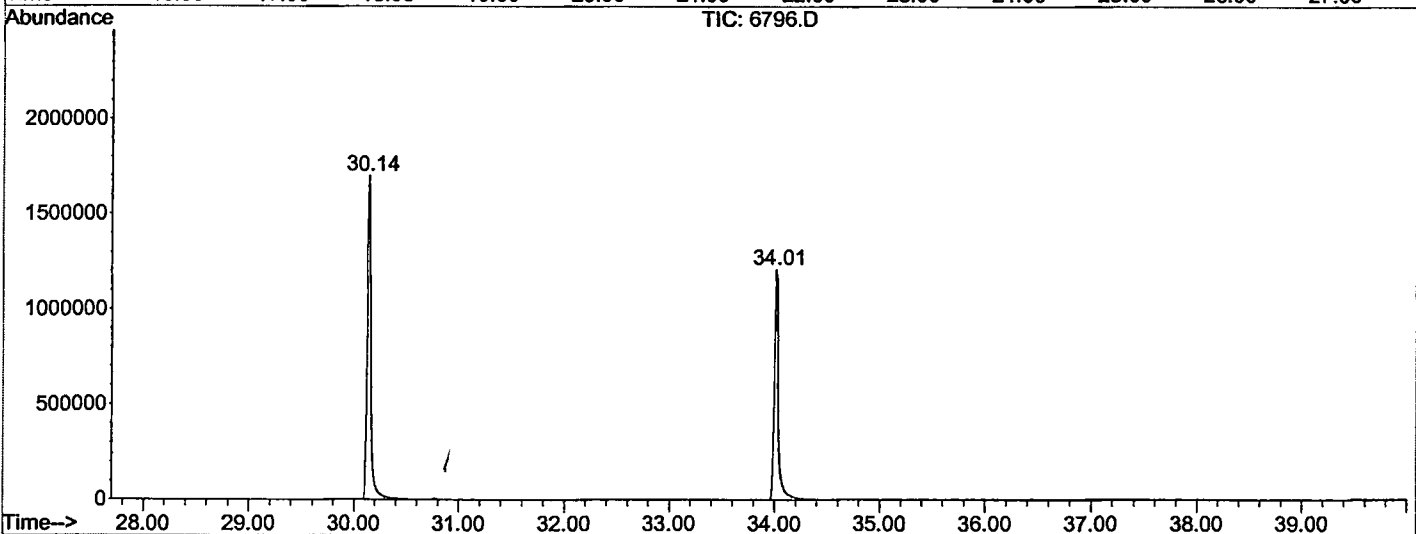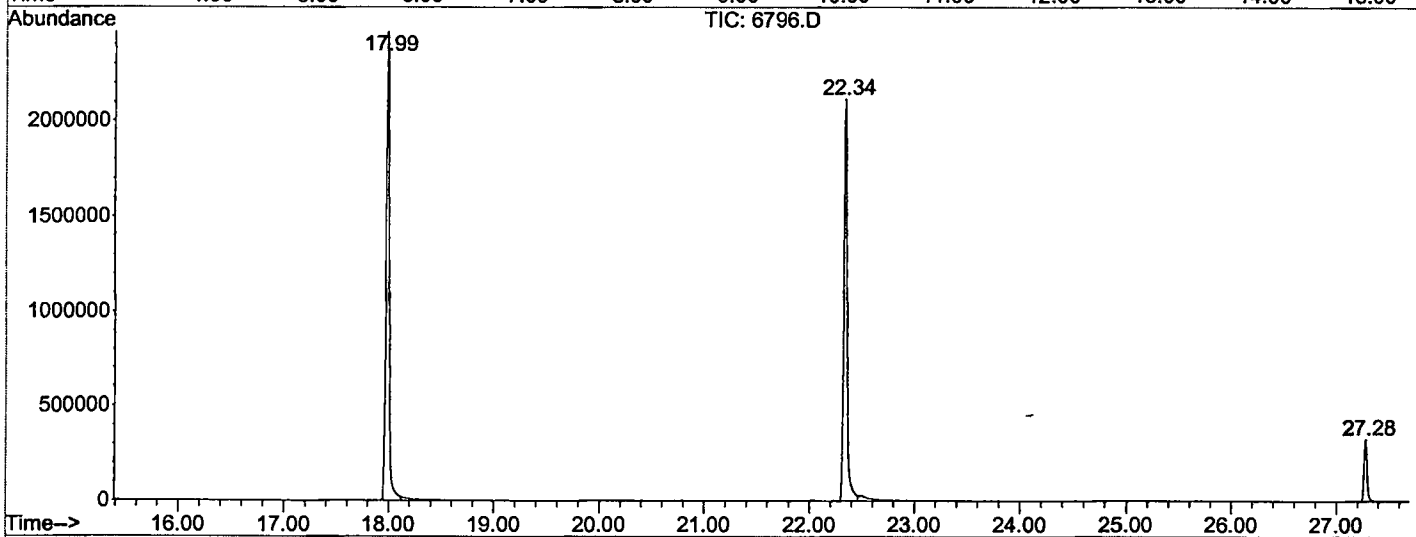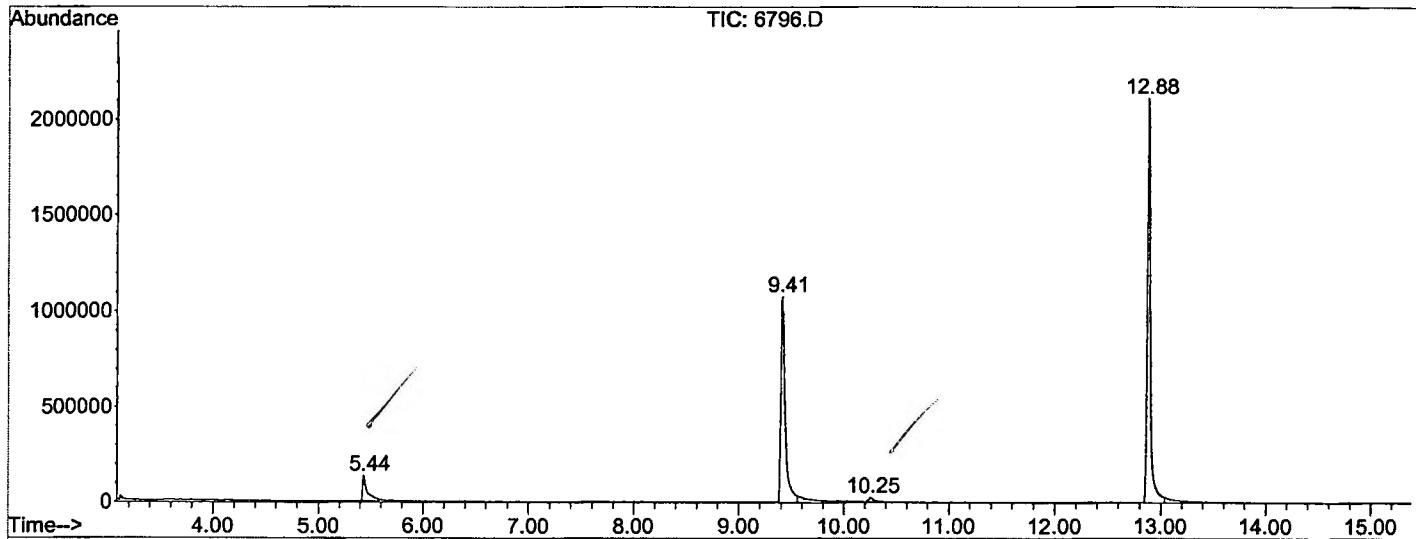

-----, Report

Data File : C:\MSDCHEM\1\DATA\041602\6796.D
 Acq On : 16 Apr 2002 7:21 pm
 Sample : SAMPLE 6796 3/21/02
 Misc :
 MS Integration Params: LSCINT.P










Vial: 14
 Operator: Bohlk
 Inst : Instrumen
 Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
 Title : Quantitation For Method 508gcscan
 Library : C:\DATABASE\WILEY7N.L

 Peak Number 1 Butane, 2-methoxy-2-methyl-... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.44	5.30 ug/L	399390	1,4-Dichlorobenzene-d4	9.41

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl- \$\$ E...	102	C6H14O	000994-05-8	38
2	3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	36
3	N-Ethylformamide \$\$ N-Formylethy...	73	C3H7NO	000627-45-2	9
4	1,3-Dioxolane, 2-heptyl-	172	C10H20O2	004359-57-3	9

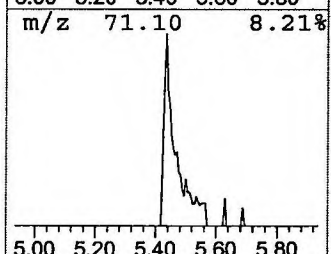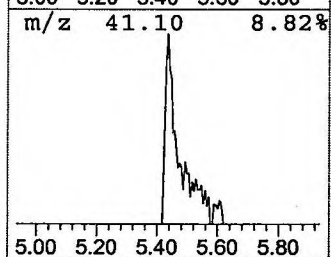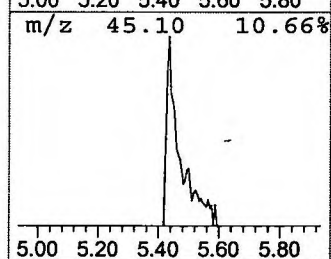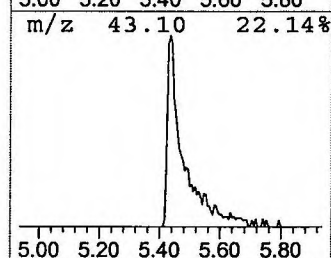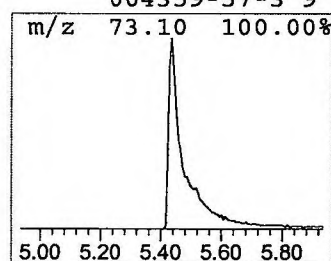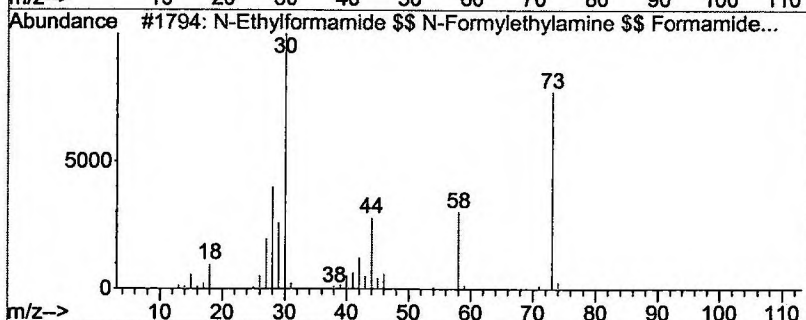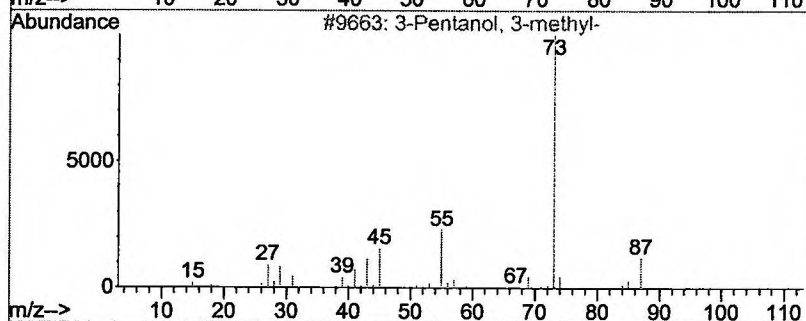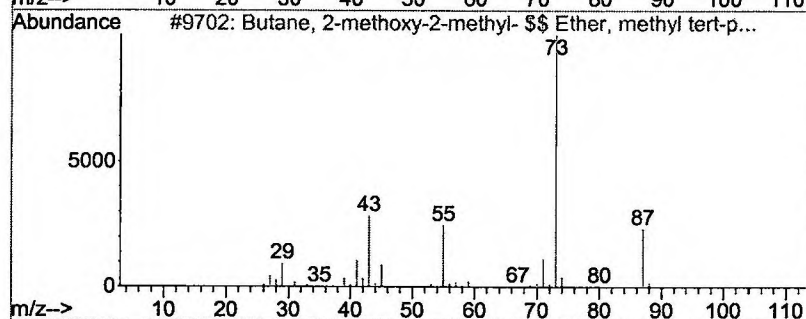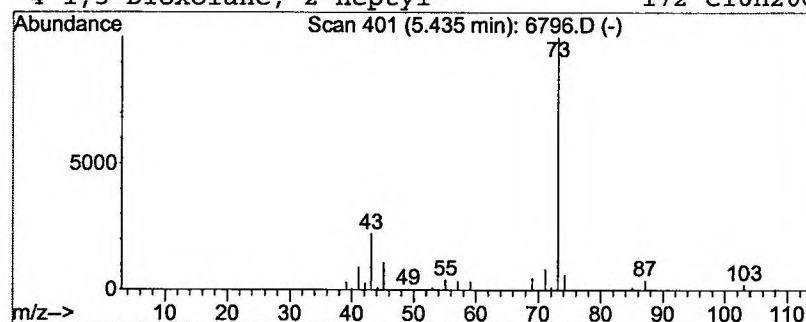

Operator ID: Bohlk Date Acquired: 16 Apr 2002 7:21 pm
 Data File: C:\MSDCHEM\1\DATA\041602\6796.D
 Name: SAMPLE 6796 3/21/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard---			
					#	RT	Resp	Conc
Butane, 2-methoxy...	5.44	5.3	ug/L	399390	1	9.41	3016410	40.0