

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/19/2002 Time: 10:00:57

Sample: AE06762
Analysis: \$GCMS GCMS Scan For Unknowns .
Units: ug
Started: 4/19/02 10:00 Ended: 4/19/02 10:00 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		94		5.0

Comments for Sample AE06762 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-19-2002 Time: 10:01:20

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Data File : C:\MSDCHEM\1\DATA\041602\6762.D

Vial: 10

Acq On : 16 Apr 2002 4:02 pm

Operator: Bohlk

Sample : SAMPLE 6762 3/21/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 18 16:06:11 2002

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	9.41	152	422555	40.00	ug/L	0.00
10) Naphthalene-d8	12.88	136	1965348	40.00	ug/L	0.00
17) Acenaphthene-d10	17.99	164	1106074	40.00	ug/L	0.00
30) Phenanthrene-d10	22.34	188	1567790	40.00	ug/L	0.00
39) Chrysene-d12	30.14	240	1187129	40.00	ug/L	-0.01
45) Perylene-d12	34.01	264	719103	40.00	ug/L	0.00

System Monitoring Compounds

28) TCMX (SURR)	0.00	244	0	0.00	ug/L	
Spiked Amount	10.000		Recovery	=	0.00%	
38) 2,4-DDD (SURR)	27.28	235	109496	9.38	ug/L	0.01
Spiked Amount	10.000		Recovery	=	93.80%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	d	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.		
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.		
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2 ' - oxybis (1-Chloropr	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	0.00	128	0	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
25) Diethylphthalate	0.00	149	0	N.D.		
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
31) N-Nitrosodiphenylamine	0.00	169	0	N.D.		
32) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.		
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	0.00	178	0	N.D.		
35) Anthracene	0.00	178	0	N.D.		
36) Di-n-butylphthalate	24.50	149	75875	1.53	ug/L	97
37) Fluoranthene	0.00	202	0	N.D.		
40) Pyrene	0.00	202	0	N.D.		
41) Butylbenzylphthalate	0.00	149	0	N.D.		
42) Benzo (a) anthracene	0.00	228	0	N.D.		
43) Bis (2-ethylhexyl) phthala	0.00	149	0	N.D.	d	
44) Chrysene	0.00	228	0	N.D.		

(#) = qualifier out of range (m) = manual integration

6762.D 5080402BBC.M Thu Apr 18 16:07:52 2002

Page 1

Data File : C:\MSDCHEM\1\DATA\041602\6762.D

Vial: 10

Acq On : 16 Apr 2002 4:02 pm

Operator: Bohlk

Sample : SAMPLE 6762 3/21/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 18 16:06:11 2002

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo (b) fluoranthene	0.00	252	0	N.D.		
48) Benzo (k) fluoranthene	0.00	252	0	N.D.		
49) Benzo (a) pyrene	0.00	252	0	N.D.	d	
50) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
51) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
52) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

6762.D 5080402BBC.M Thu Apr 18 16:07:52 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\041602\6762.D

Acq On : 16 Apr 2002 4:02 pm

Sample : SAMPLE 6762 3/21/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 18 16:07 2002

Vial: 10

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00


Quant Results File: 5080402BBC.RES

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

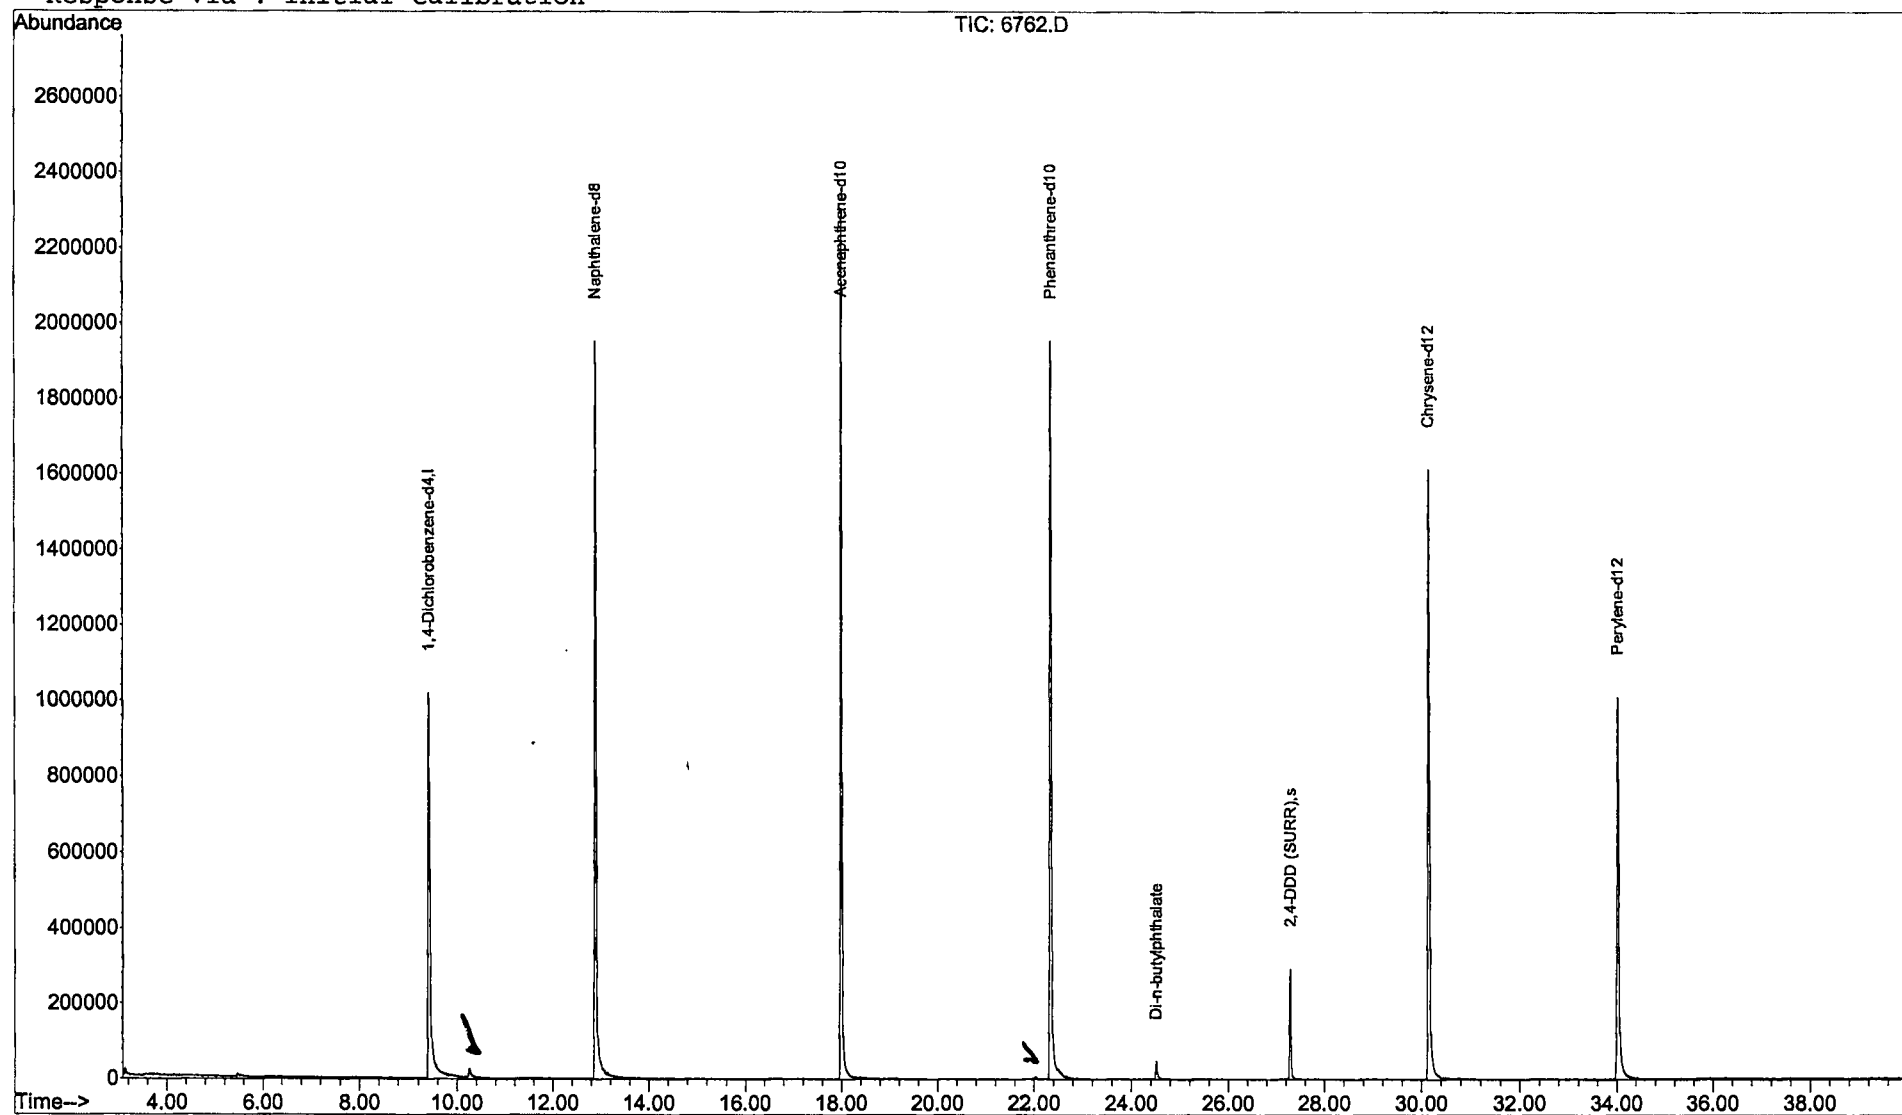

Data File : C:\MSDCHEM\1\DATA\041602\6762.D
 Acq On : 16 Apr 2002 4:02 pm
 Sample : SAMPLE 6762 3/21/02
 Misc :
 MS Integration Params: LSCINT.P

Vial: 10
 Operator: Bohlk
 Inst : Instrumen
 Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
 Title : Quantitation For Method 508gcscan
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.407	1071	1077	1100	rBV	1015751	2787826	58.94%	12.047%
2	10.259	1214	1222	1229	rBV3	21840	56570	1.20%	0.244%
3	12.880	1661	1668	1694	rBV	1951872	4251002	89.87%	18.370%
4	17.986	2529	2537	2560	rBV	2300612	4729940	100.00%	20.439%
5	22.339	3269	3278	3301	rBV2	1953181	4491878	94.97%	19.410%
6	24.502	3639	3646	3665	rBV	46755	119092	2.52%	0.515%
7	27.281	4111	4119	4129	rBV	291148	568726	12.02%	2.458%
8	30.142	4596	4606	4621	rBV2	1613092	3655246	77.28%	15.795%
9	34.014	5255	5265	5278	rBV2	1008424	2481307	52.46%	10.722%

Sum of corrected areas: 23141587

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\041602\6762.D
 Operator : Bohlk
 Acquired : 16 Apr 2002 4:02 pm using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: SAMPLE 6762 3/21/02
 Misc Info :
 Vial Number: 10
 Quant File :5080402BBC.RES (RTE Integrator)

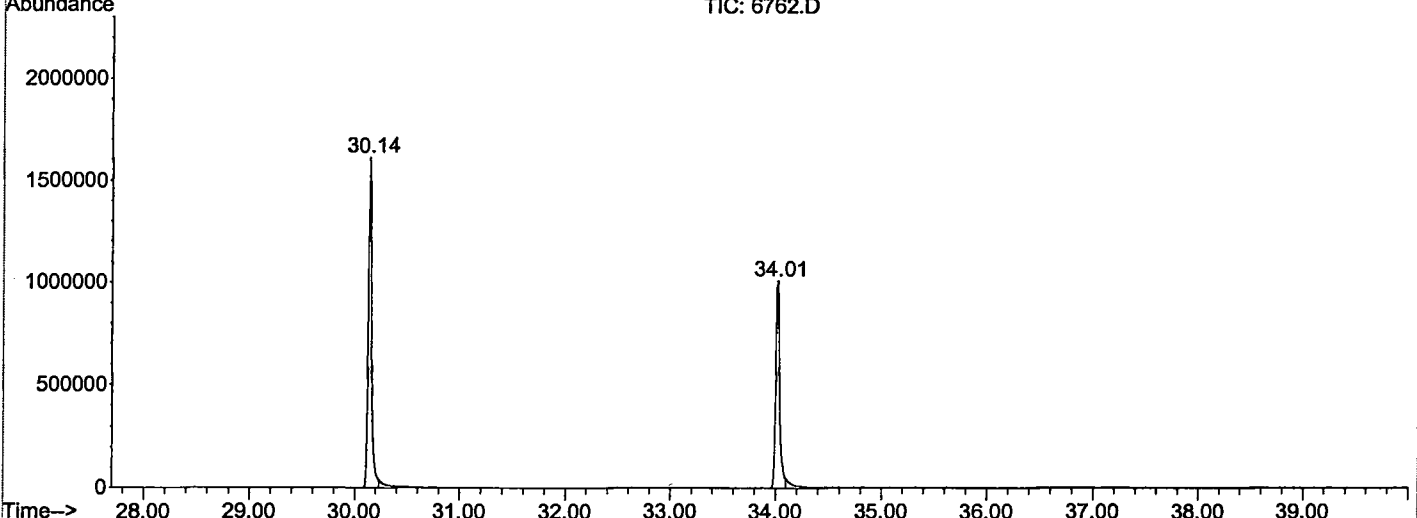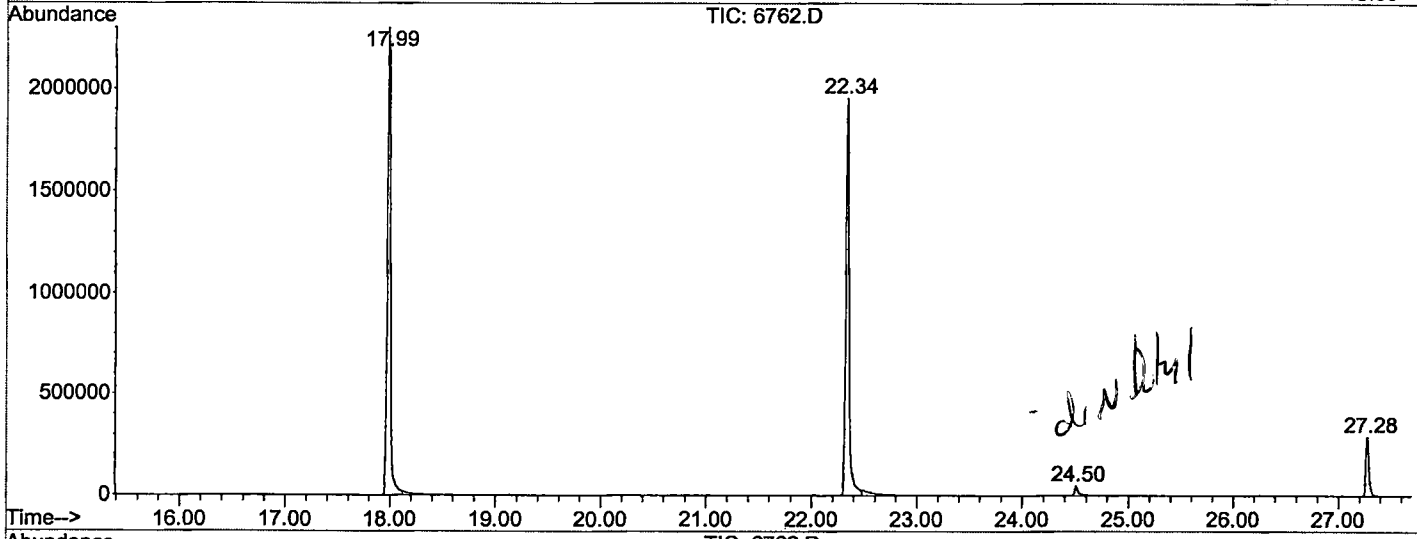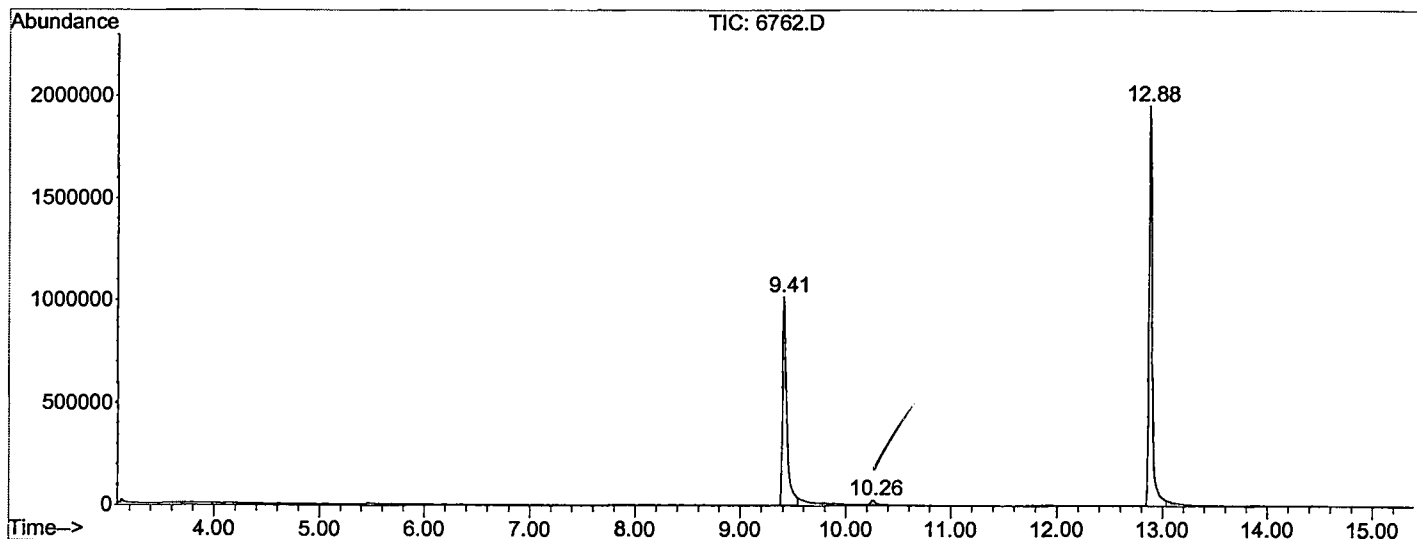

Data File : C:\MSDCHEM\1\DATA\041602\6762.D

Acq On : 16 Apr 2002 4:02 pm

Sample : SAMPLE 6762 3/21/02

Misc :

MS Integration Params: LSCINT.P

Vial: 10

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)










Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 Benzene-1,2,3,4-d4-, 5,6-di... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.26	0.81 ug/L	56570	1,4-Dichlorobenzene-d4	9.41

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Benzene-1,2,3,4-d4-, 5,6-dichlor...	150	C6D4Cl2	002199-69-1	91
2	1,4-Dichlorobenzene-d4	150	C6D4Cl2	003855-82-1	91
3	1,2-Dichlorobenzene-d4 \$\$ Benzen...	150	C6D4Cl2	002199-69-1	91
4	1,4-Dichlorobenzene-d4	150	C6D4Cl2	003855-82-1	64

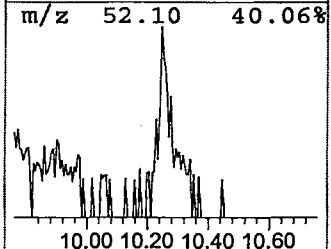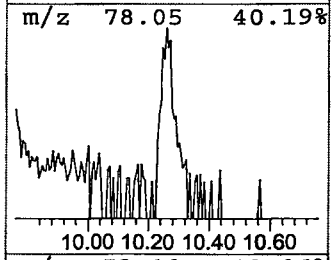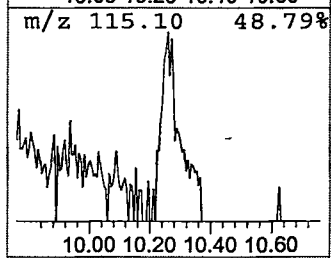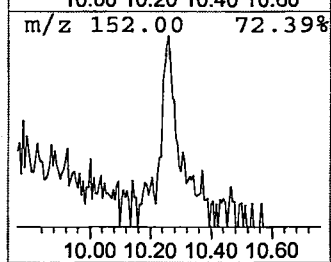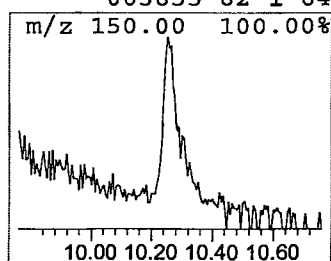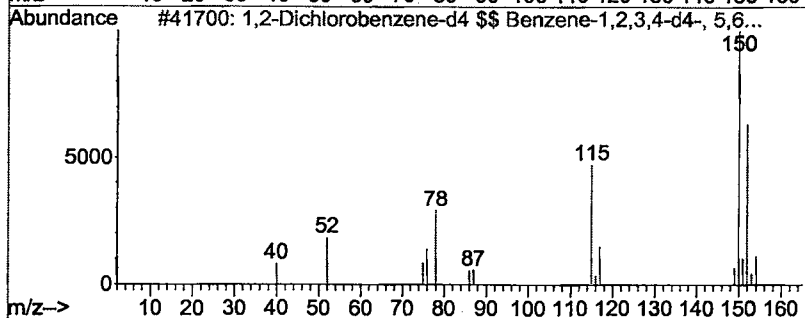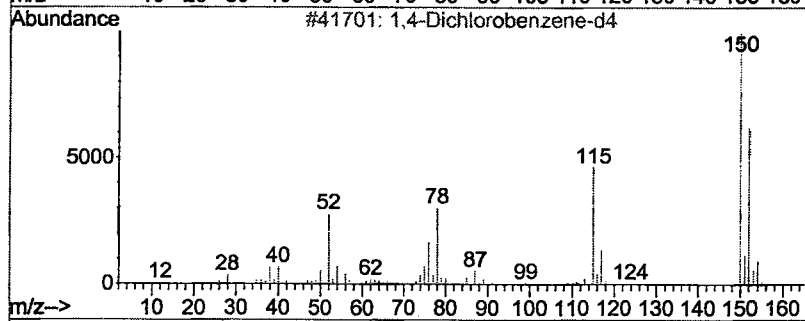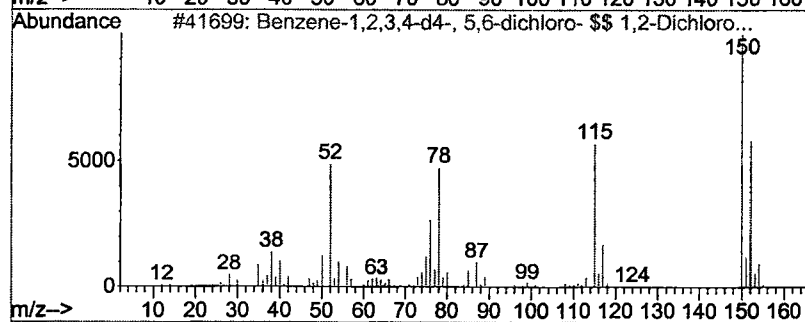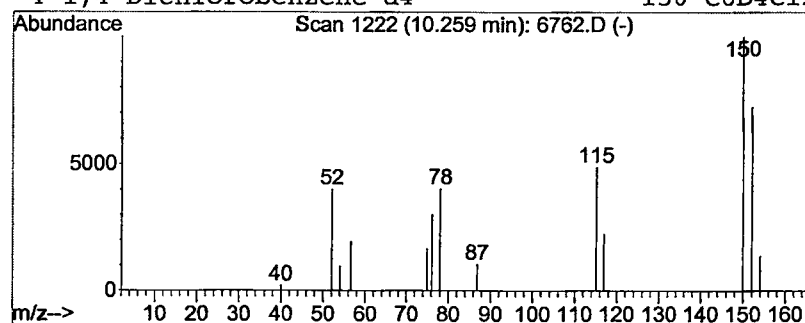

Operator ID: Bohlk Date Acquired: 16 Apr 2002 4:02 pm
 Data File: C:\MSDCHEM\1\DATA\041602\6762.D
 Name: SAMPLE 6762 3/21/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard---			
					#	RT	Resp	Conc
Benzene-1,2,3,4-d...	10.26	0.8	ug/L	56570	1	9.41	2787830	40.0