

Page 28

Reviewed by _____
Date _____

DFTPP

Data File : C:\HPCHEM\1\DATA\APR0405\DFTPP1.D

Acq On : 6 Apr 2002 5:45 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

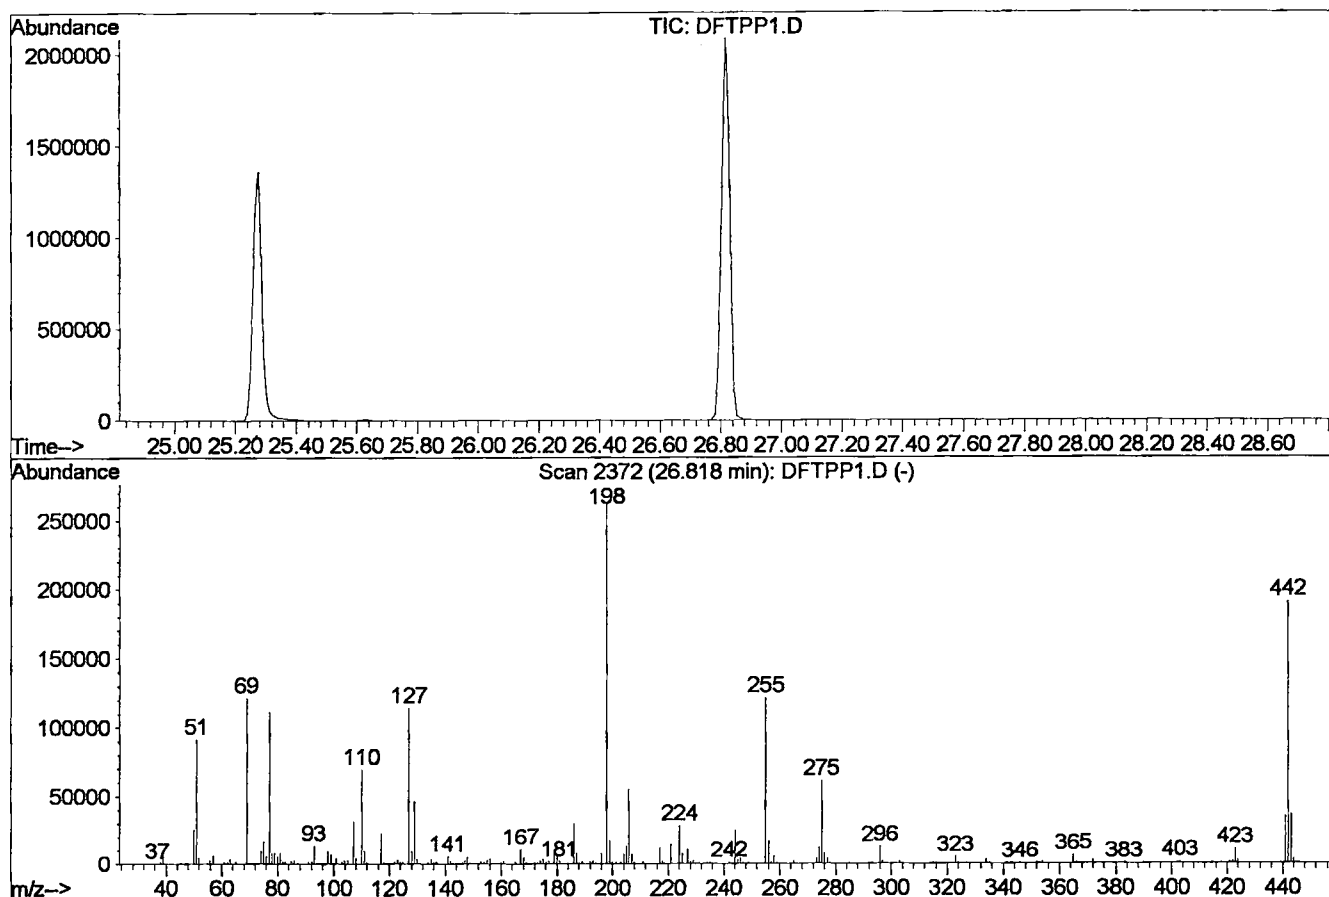

Spectrum Information: Scan 2372

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.8	91757	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.3	121963	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	43.5	114766	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	263542	PASS
199	198	5	9	6.7	17776	PASS
275	198	10	30	23.3	61387	PASS
365	198	1	100	2.5	6666	PASS
441	443	0.01	100	96.6	35632	PASS
442	198	40	110	72.5	191134	PASS
443	442	17	23	19.3	36880	PASS

DFTPP1.D GCMS0412.M

Mon Apr 15 13:18:02 2002