

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 04/16/2002 Time: 15:20:26

Sample: AE06997
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 4/16/02 15:19 Ended: 4/16/02 15:19 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		119		5.0

Comments for Sample AE06997 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-16-2002 Time: 15:20:41

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recoveries for 4 of the 43 compounds in the LCS Standard were high.

Data File : C:\HPCHEM\1\DATA\APR0405\6997.D

Vial: 26

Acq On : 6 Apr 2002 10:31 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: GOOFY.P

Quant Time: Apr 15 14:39 2002

Quant Results File: GCMS0408.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Apr 15 14:10:52 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0403

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.24	152	453626	20.00	ug/l	-0.02
10) Naphthalene-d8	15.88	136	1671831	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.18	164	933860	20.00	ug/l	-0.02
30) Phenanthrene-d10	25.63	188	1306388	20.00	ug/l	-0.03
39) Chrysene-d12	33.69	240	627534	20.00	ug/l	-0.03
45) Perylene-d12	37.93	264	338480	20.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	23.32	209	29895	11.88	ug/mL	0.00
Spiked Amount	10.000		Recovery	=	118.80%	
38) 2,4-DDD	0.00	235	0	0.00	ug/mL	
Spiked Amount	5.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D. d	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#)= qualifier out of range (m) = manual integration

6997.D GCMS0408.M

Mon Apr 15 14:39:48 2002

Page 1

Data File : C:\HPCHEM\1\DATA\APR0405\6997.D

Vial: 26

Acq On : 6 Apr 2002 10:31 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: GOOFY.P

Quant Time: Apr 15 14:39 2002

Quant Results File: GCMS0408.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Apr 15 14:10:52 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0403

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	25.63	178	402	N.D.		
35) Anthracene	25.63	178	402	N.D.		
36) Di-n-butylphthalate	27.60	149	1458	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
40) Pyrene	0.00	202	0	N.D.		
41) Butylbenzylphthalate	0.00	149	0	N.D.		
42) Benzo(a)anthracene	33.69	228	1380	N.D.		
43) Bis(2-ethylhexyl)phthalate	33.91	149	966	N.D.		
44) Chrysene	33.69	228	1380	N.D.		
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo(b)fluoranthene	0.00	252	0	N.D.		
48) Benzo(k)fluoranthene	0.00	252	0	N.D.		
49) Benzo(a)pyrene	37.94	252	1173	N.D.		
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

6997.D GCMS0408.M

Mon Apr 15 14:39:49 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR0405\6997.D
 Acq On : 6 Apr 2002 10:31 pm
 Sample : gc/ms scan 3/26
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 15 14:39 2002

Vial: 26
 Operator:
 Inst : GC/MS 209
 Multiplr: 2.00

Quant Results File: GCMS0408.RES

Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Mon Apr 15 14:10:52 2002
 Response via : Initial Calibration

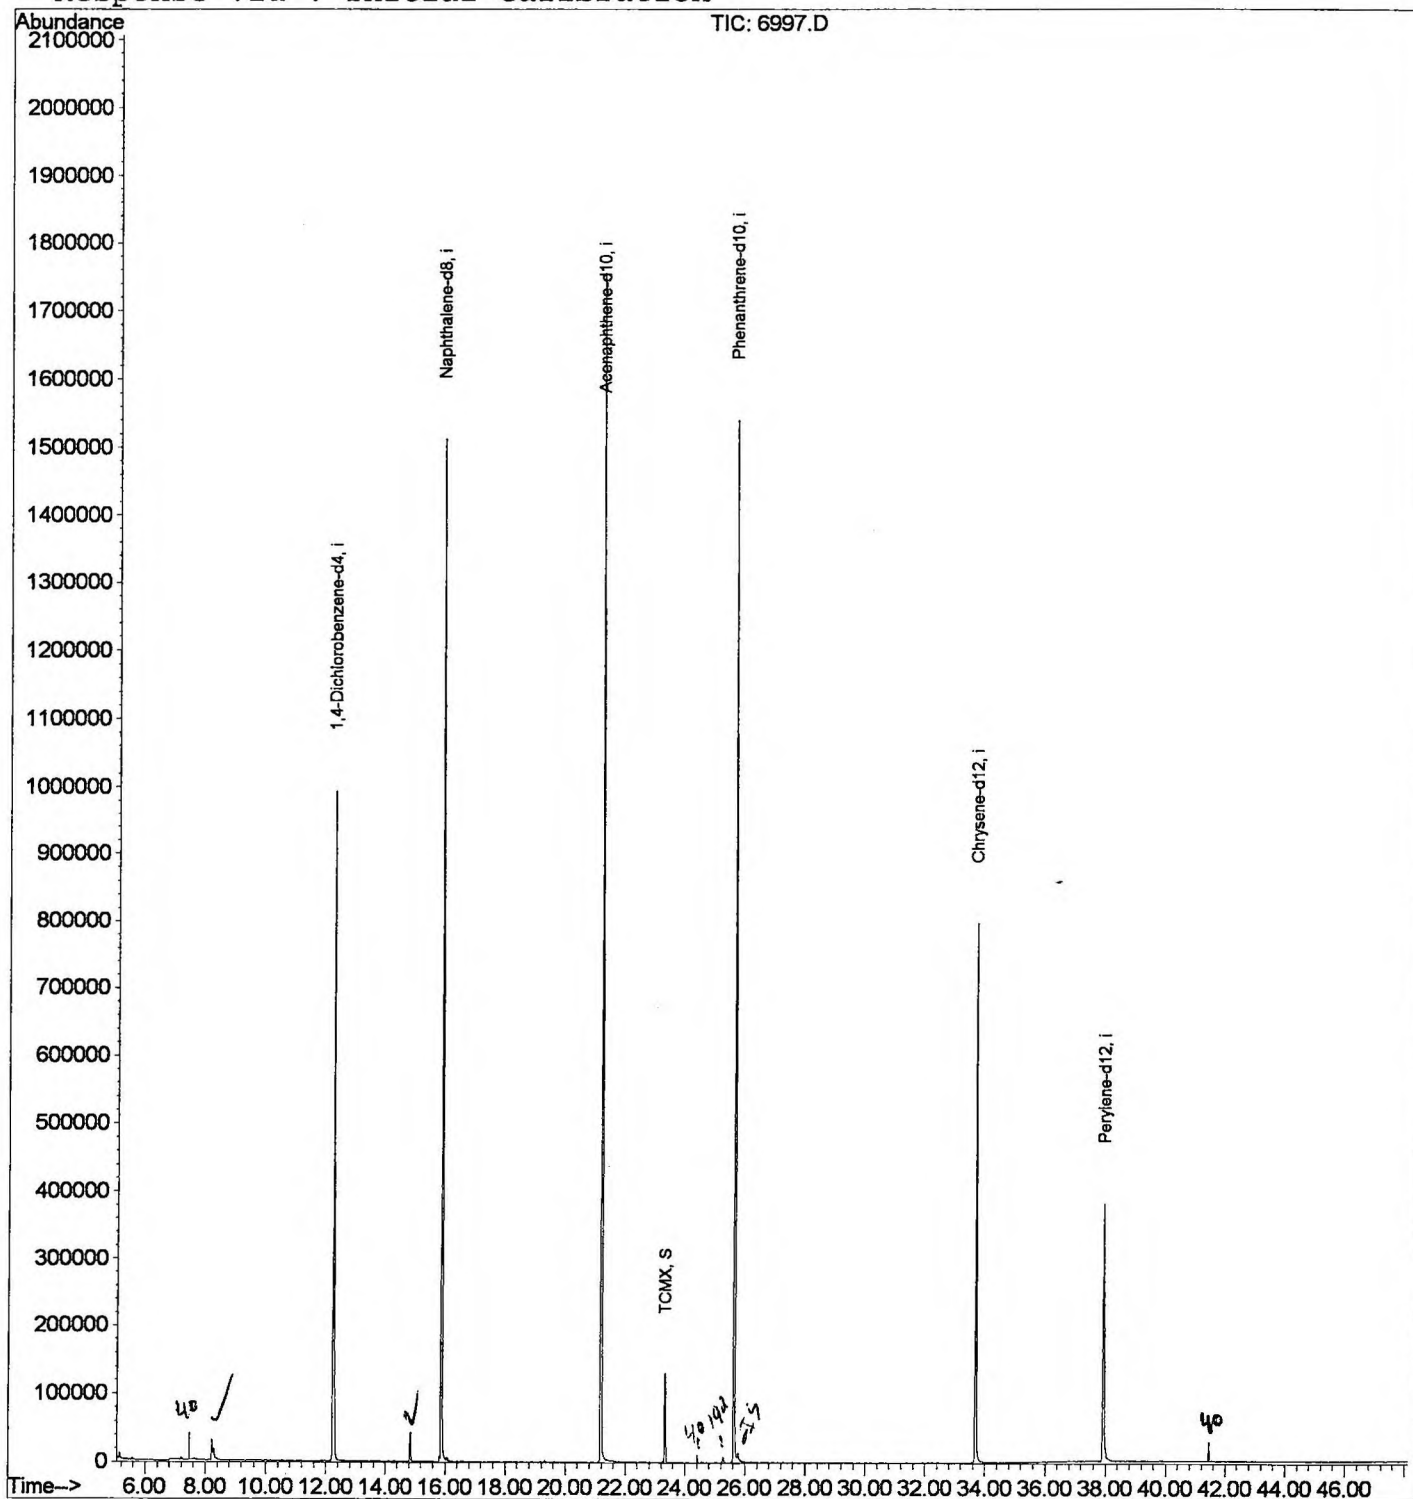

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR0405\6997.D

Vial: 26

Acq On : 6 Apr 2002 10:31 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.221	343	346	350	rBV	30594	64721	1.81%	0.409%
2	12.242	779	784	800	rBV	992201	2433342	67.89%	15.391%
3	14.840	1062	1067	1072	rBV	42740	82707	2.31%	0.523%
4	15.877	1175	1180	1197	rVB	1510588	3141067	87.64%	19.868%
5	21.183	1752	1758	1770	rBV	1754922	3584247	100.00%	22.671%
6	23.322	1985	1991	2000	rVB	129642	266094	7.42%	1.683%
7	25.627	2236	2242	2253	rBV2	1539405	3282485	91.58%	20.762%
8	33.687	3113	3120	3142	rBV2	796905	1819658	50.77%	11.510%
9	37.928	3574	3582	3596	rBV2	380697	1135601	31.68%	7.183%




Sum of corrected areas: 15809922

6997.D GCMS0408.M

Mon Apr 15 14:44:51 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR0405\6997.D
 Operator :
 Acquired : 6 Apr 2002 10:31 pm using AcqMethod GCMS0403
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 3/26
 Misc Info :
 Vial Number: 26
 Quant File :GCMS0408.RES (RTE Integrator)

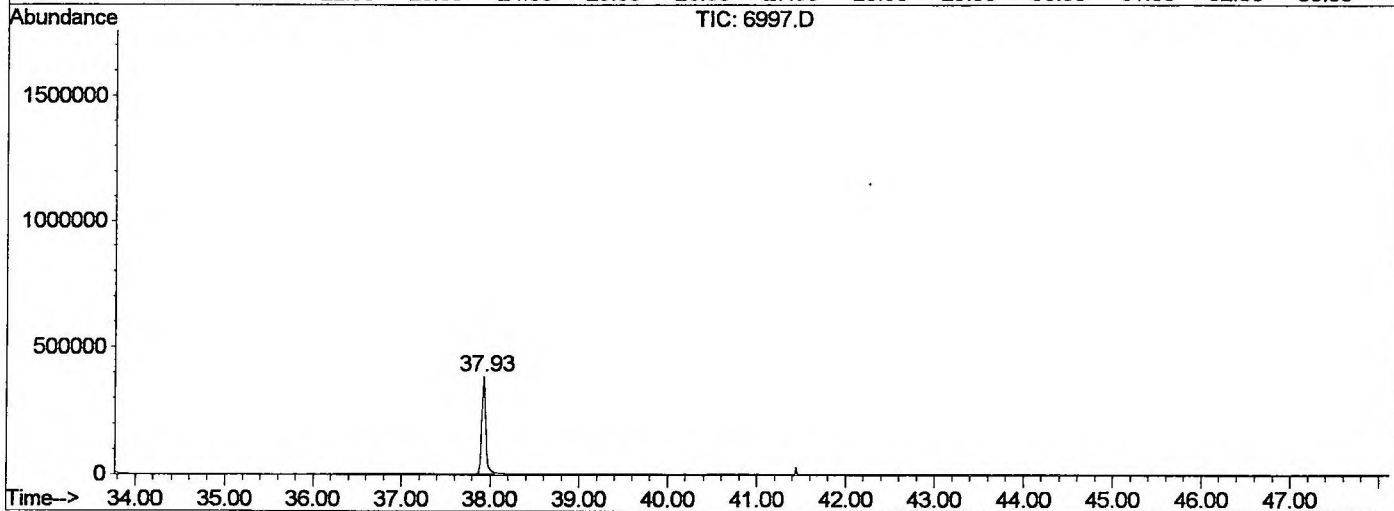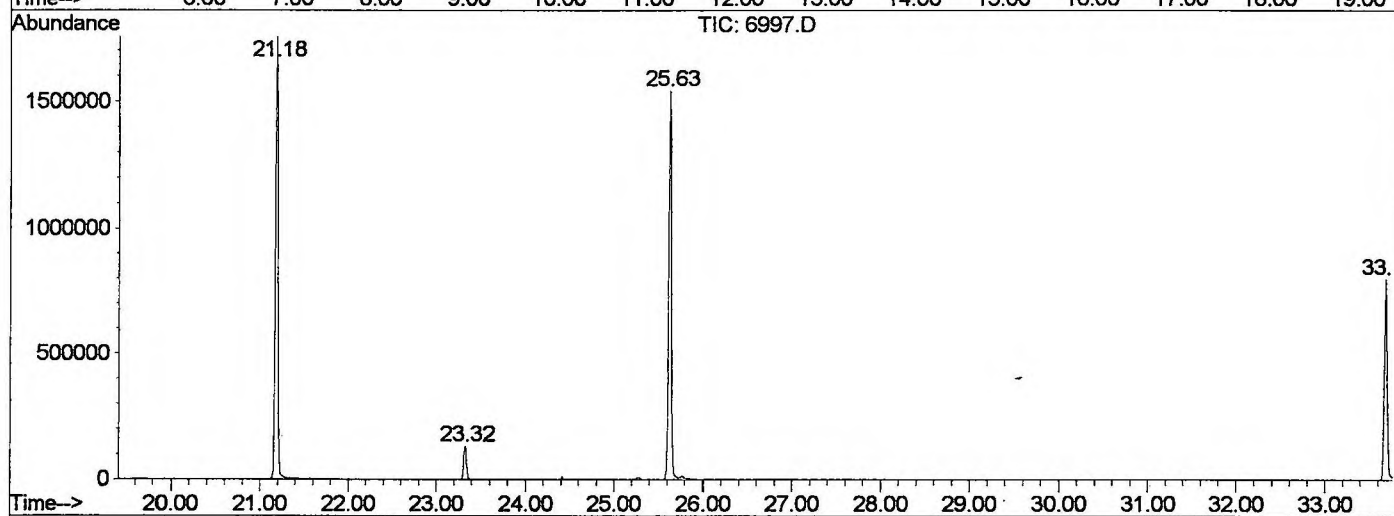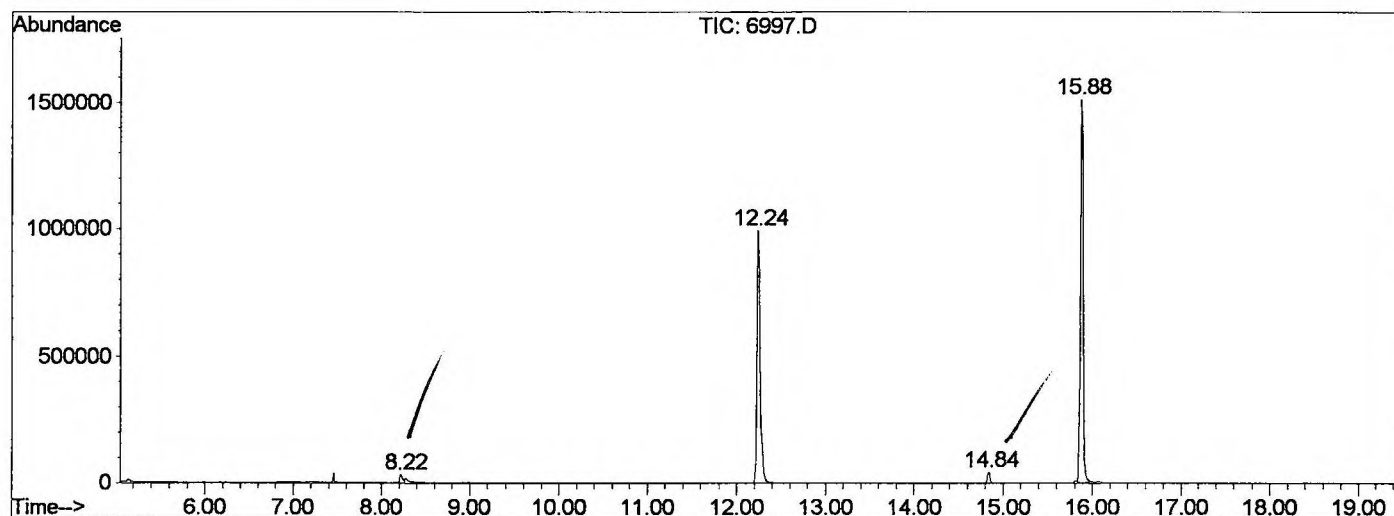

6997.D GCMS0408.M Mon Apr 15 14:44:52 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR0405\6997.D
Acq On : 6 Apr 2002 10:31 pm
Sample : gc/ms scan 3/26
Misc :
MS Integration Params: LSCINT.P


Vial: 26
Operator:
Inst : GC/MS 209
Multiplr: 2.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-methyl Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.22	1.06 ug/l	64721	1,4-Dichlorobenzene-d4	12.24

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	40
2			3-Hydroxy-2-pentanone	102	C5H10O2	003142-66-3	9
3			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
4			5-Hexen-2-one	98	C6H10O	000109-49-9	9

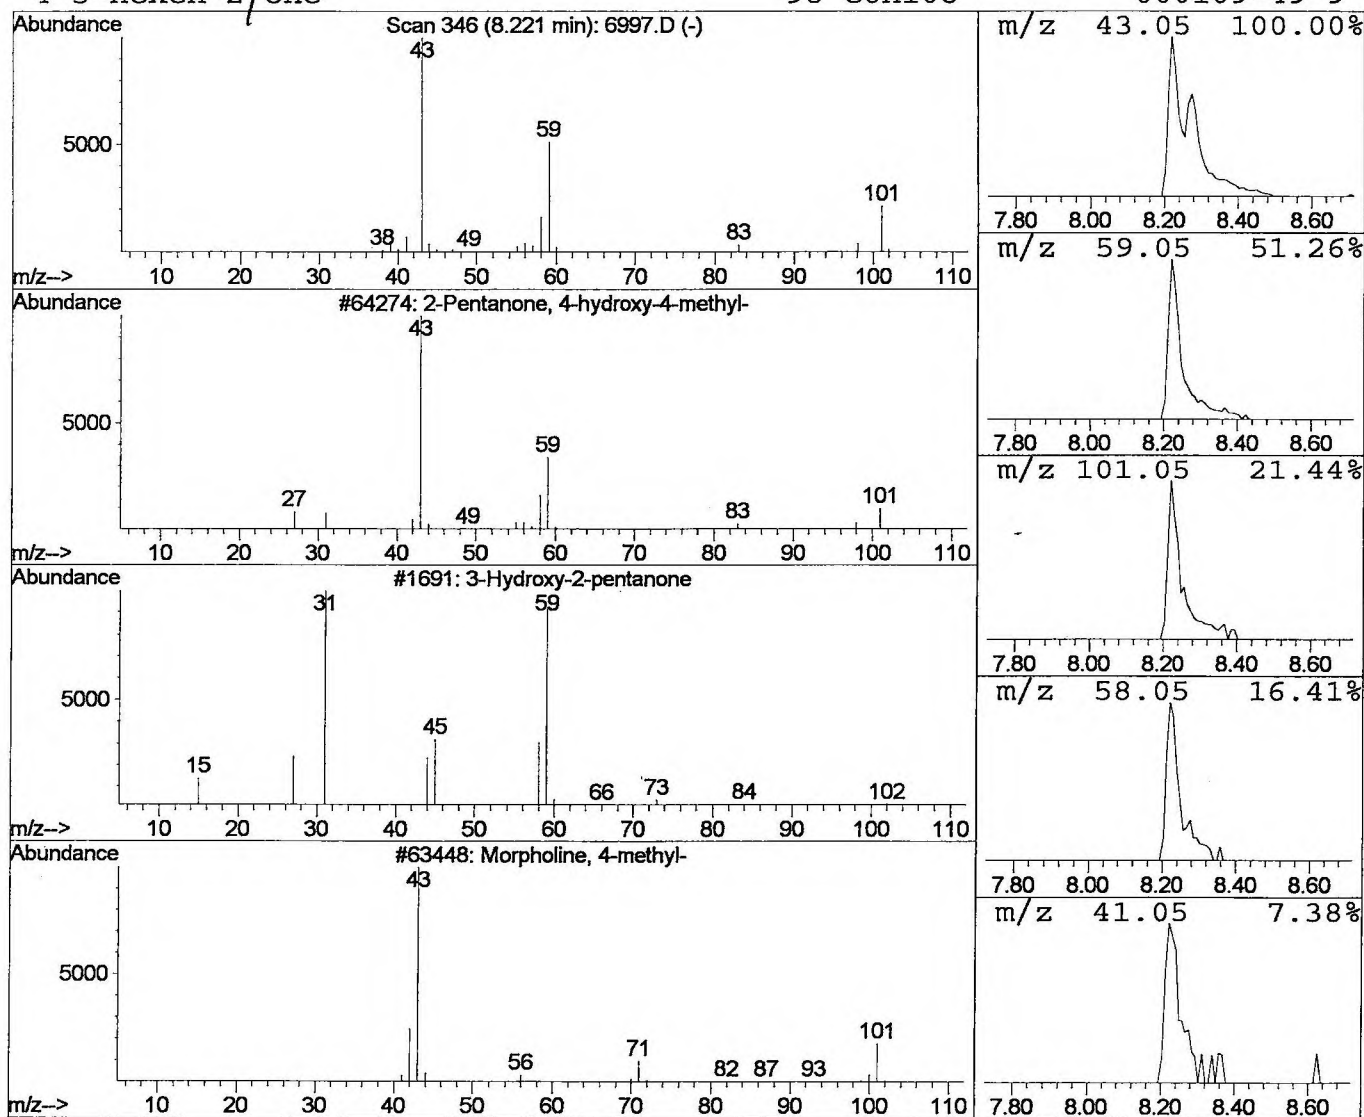

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR0405\6997.D

Acq On : 6 Apr 2002 10:31 pm

Sample : gc/ms scan 3/26

Misc :

MS Integration Params: LSCINT.P

Vial: 26

Operator:

Inst : GC/MS 209

Multiplr: 2.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Library : C:\DATABASE\NBS75K.L

Peak Number 2 Cyclopentasiloxane, decamethyl Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.84	1.05 ug/l	82707	Naphthalene-d8	15.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	87
2		N-(Trifluoroacetyl)-N,O,O',O''-tetr	553	C22H42F3NO4Si4	000000-00-0	47
3		Benzoic acid, 2,4-bis[(trimethylsil	370	C16H30O4Si3	010586-16-0	38
4		Phenethylamine, N-methyl-.beta.,3,4	399	C18H37NO3Si3	010538-85-9	38

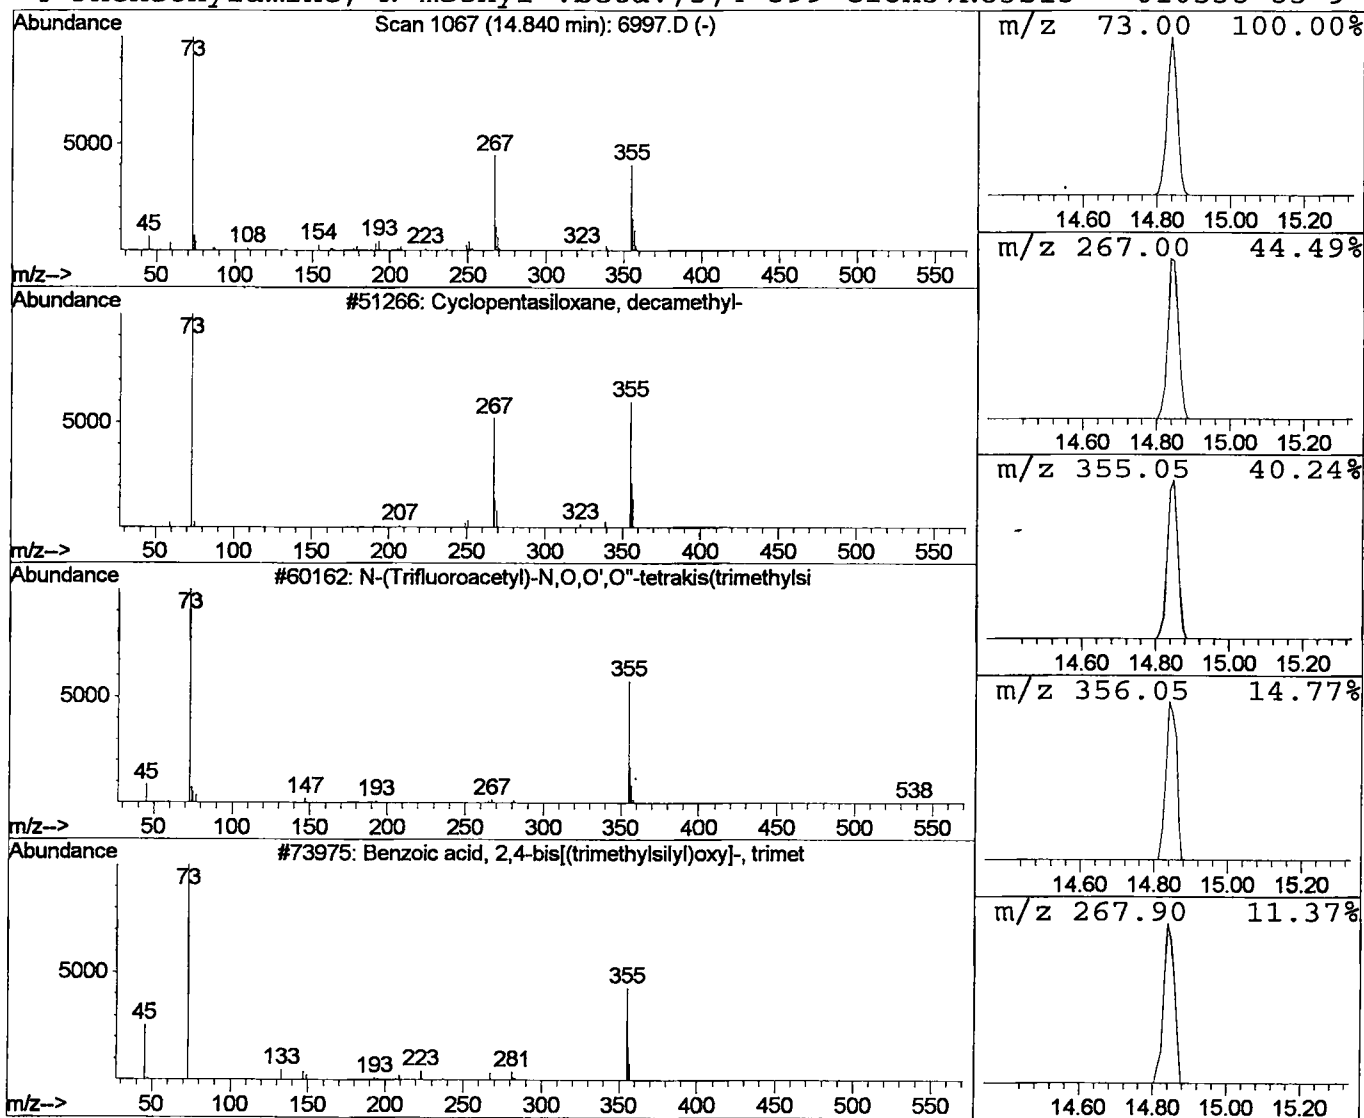

Tentatively Identified Compound (LSC) summary

* Operator ID: Date Acquired: 6 Apr 2002 10:31 pm
Data File: C:\HPCHEM\1\DATA\APR0405\6997.D
Name: gc/ms scan 3/26
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
2-Pentanone, 4-hydro	8.22	1.1	ug/l	64721	ISTD01	12.24	2433340	20.0
Cyclopentasiloxane,	14.84	1.1	ug/l	82707	ISTD02	15.88	3141070	20.0

6997.D GCMS0408.M Mon Apr 15 14:44:54 2002