



User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 04/16/2002 Time: 15:10:01

Sample: AE06995
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 4/16/02 15:09 Ended: 4/16/02 15:09 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		96		5.0

Comments for Sample AE06995 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-16-2002 Time: 15:10:19

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recoveries for 4 of the 43 compounds in the LCS Standard were high.

Data File : C:\HPCHEM\1\DATA\APR0405\6995.D

Vial: 24

Acq On : 6 Apr 2002 7:34 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: GOOFY.P

Quant Time: Apr 15 14:37 2002

Quant Results File: GCMS0408.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Apr 15 14:10:52 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0403

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.25	152	442059	20.00	ug/l	-0.02
10) Naphthalene-d8	15.88	136	1613643	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.19	164	899361	20.00	ug/l	-0.02
30) Phenanthrene-d10	25.63	188	1247111	20.00	ug/l	-0.03
39) Chrysene-d12	33.69	240	579880	20.00	ug/l	-0.03
45) Perylene-d12	37.93	264	309386	20.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	23.33	209	23194	9.57	ug/mL	0.00
Spiked Amount	10.000		Recovery	=	95.70%	
38) 2,4-DDD	0.00	235	0	0.00	ug/mL	
Spiked Amount	5.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.67	149	605	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#)=qualifier out of range (m)=manual integration

6995.D GCMS0408.M Mon Apr 15 14:37:26 2002

Page 1

Data File : C:\HPCHEM\1\DATA\APR0405\6995.D

Vial: 24

Acq On : 6 Apr 2002 7:34 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: GOOFY.P

Quant Time: Apr 15 14:37 2002

Quant Results File: GCMS0408.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Apr 15 14:10:52 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0403

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	0.00	178	0	N.D.		
35) Anthracene	25.63	178	108	N.D.		
36) Di-n-butylphthalate	27.60	149	4920	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
40) Pyrene	0.00	202	0	N.D.		
41) Butylbenzylphthalate	0.00	149	0	N.D.		
42) Benzo(a)anthracene	33.69	228	1248	N.D.		
43) Bis(2-ethylhexyl)phthalate	33.91	149	5083m	0.59	ug/l	
44) Chrysene	33.69	228	1248	N.D.		
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo(b)fluoranthene	0.00	252	0	N.D.		
48) Benzo(k)fluoranthene	0.00	252	0	N.D.		
49) Benzo(a)pyrene	37.92	252	1223	N.D.		
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

6995.D GCMS0408.M Mon Apr 15 14:37:27 2002

Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR0405\6995.D

Vial: 24

Acq On : 6 Apr 2002 7:34 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: GOOFY.P

Quant Time: Apr 15 14:37 2002


Quant Results File: GCMS0408.RES

Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Apr 15 14:10:52 2002

Response via : Initial Calibration

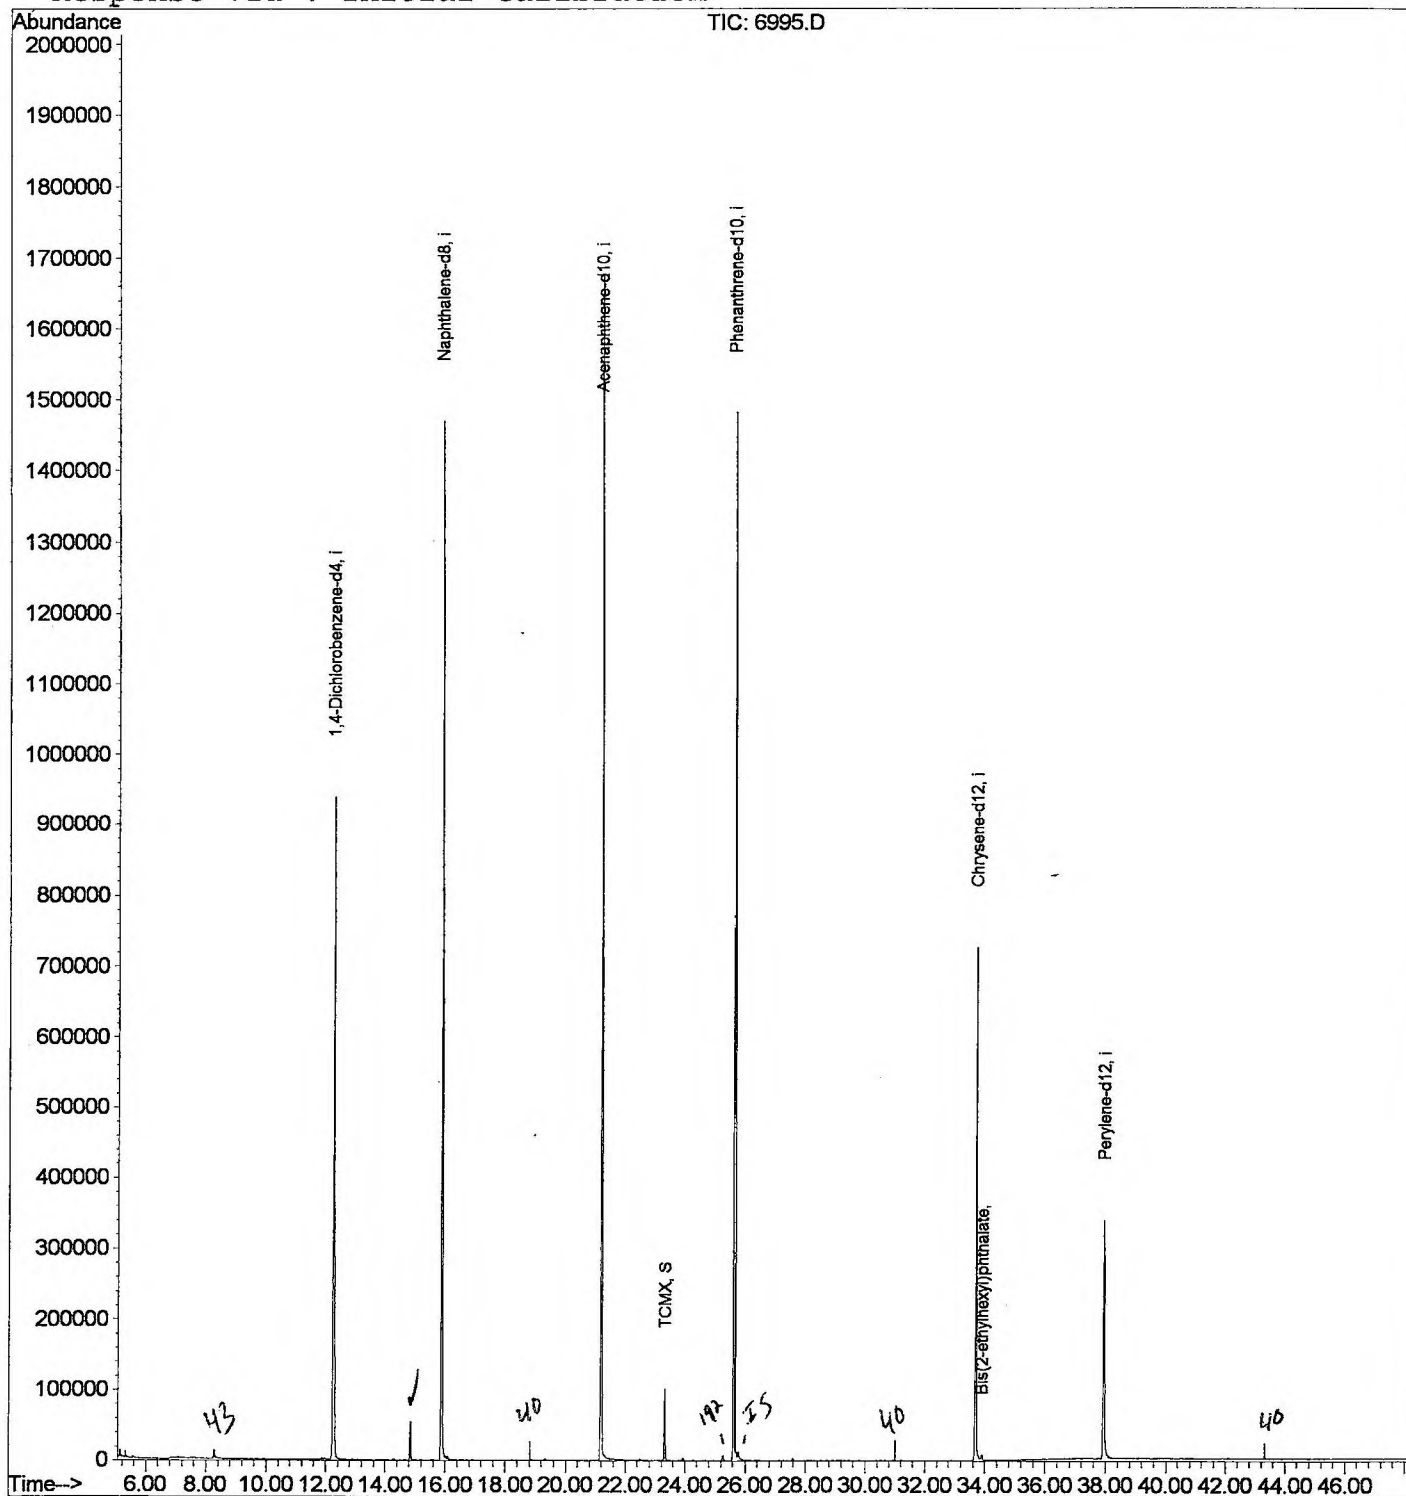

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR0405\6995.D

Vial: 24

Acq On : 6 Apr 2002 7:34 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	12.246	778	784	799	rVB	936429	2364740	68.16%	15.798%
2	14.844	1062	1067	1074	rBV	54265	105100	3.03%	0.702%
3	15.881	1174	1180	1197	rBV	1469422	3043852	87.74%	20.334%
4	21.187	1751	1758	1780	rBV	1677659	3469255	100.00%	23.176%
5	23.326	1984	1991	1998	rVB	102274	203797	5.87%	1.361%
6	25.631	2235	2242	2253	rBV	1481467	3101535	89.40%	20.720%
7	33.691	3113	3120	3132	rBV	725012	1658884	47.82%	11.082%
8	37.932	3574	3582	3595	rBV2	336117	1021874	29.46%	6.827%




Sum of corrected areas: 14969037

6995.D GCMS0408.M

Mon Apr 15 14:44:29 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR0405\6995.D
 Operator :
 Acquired : 6 Apr 2002 7:34 pm using AcqMethod GCMS0403
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 3/26
 Misc Info :
 Vial Number: 24
 Quant File :GCMS0408.RES (RTE Integrator)

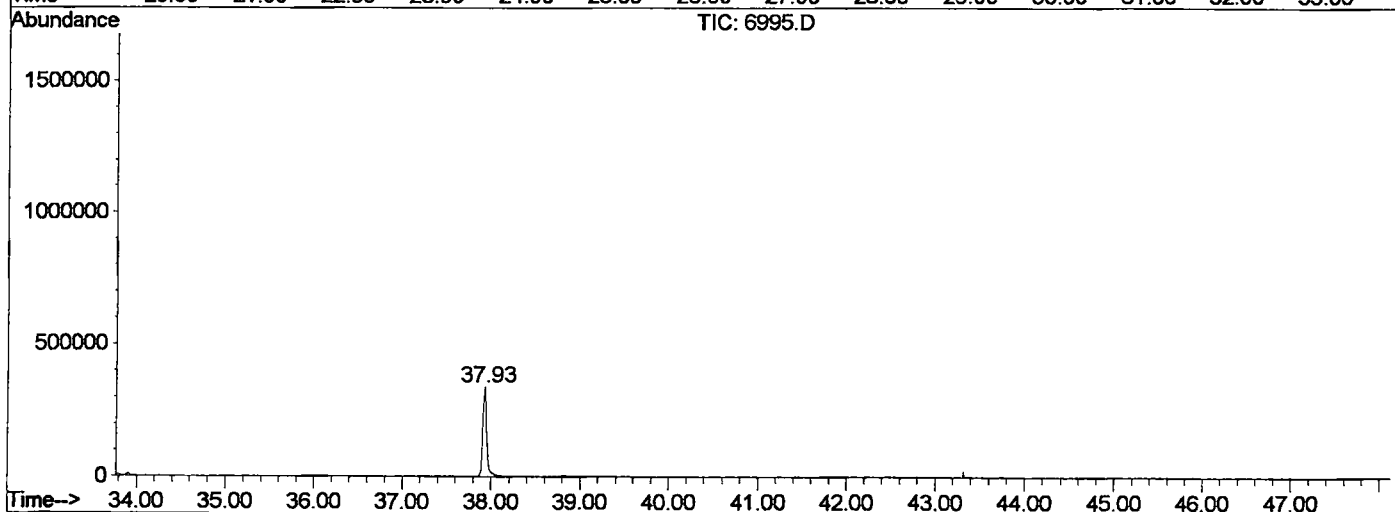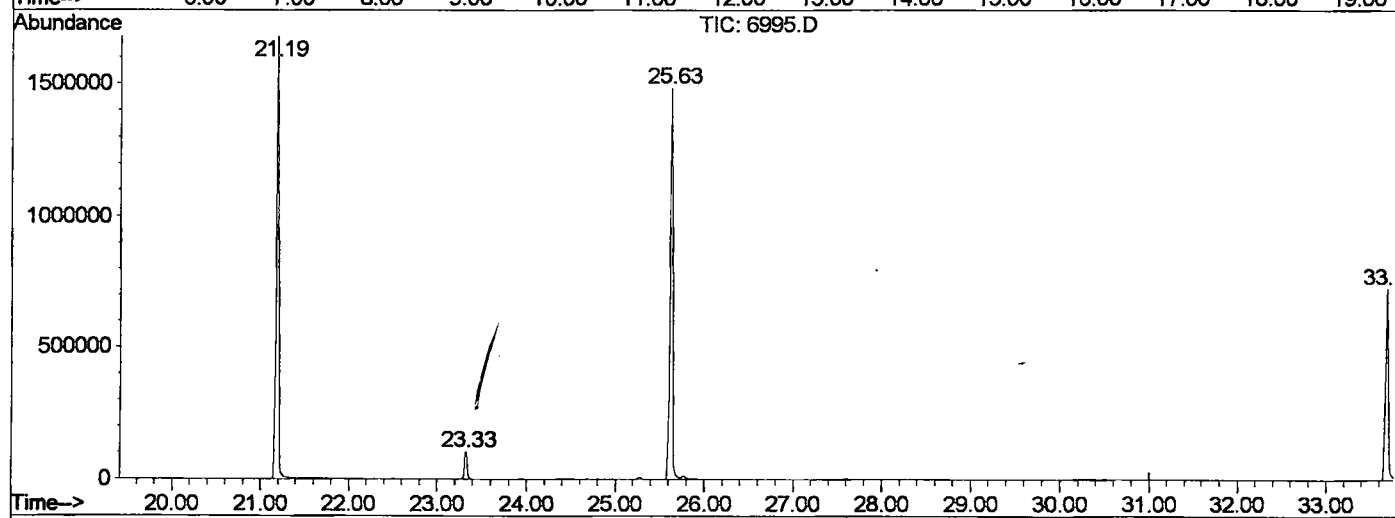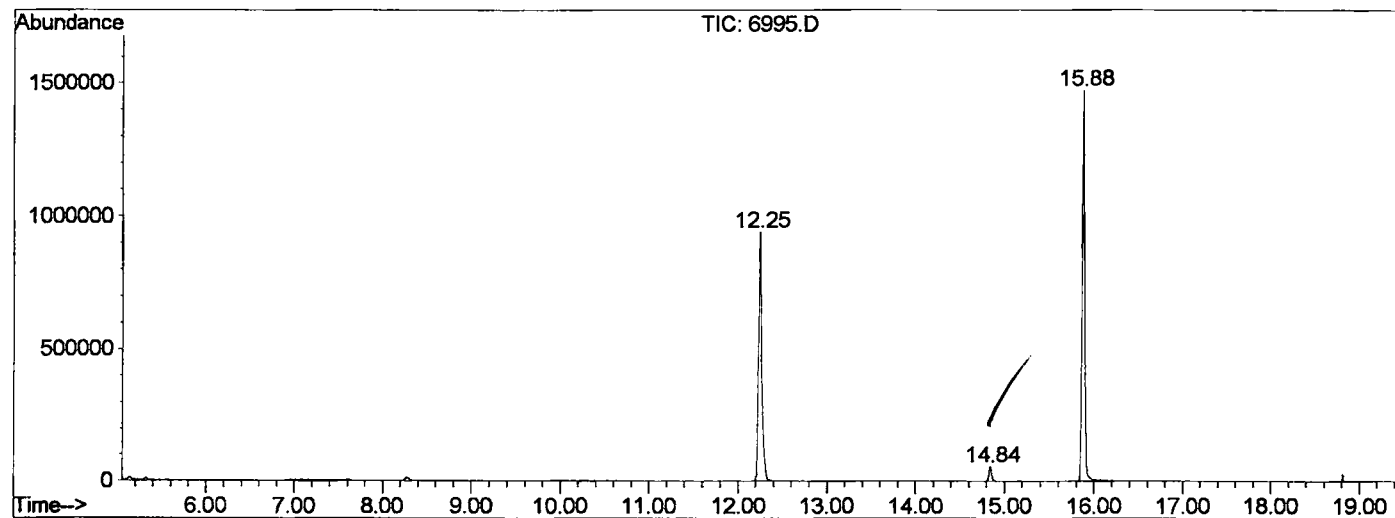

6995.D GCMS0408.M Mon Apr 15 14:44:30 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR0405\6995.D
Acq On : 6 Apr 2002 7:34 pm
Sample : gc/ms scan 3/26
Misc :
MS Integration Params: LSCINT.P










Vial: 24
Operator:
Inst : GC/MS 209
Multiplr: 2.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 Cyclopentasiloxane, decamethyl Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.84	1.38 ug/l	105100	Naphthalene-d8	15.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	90
2		Phenethylamine, N-methyl-.beta.,3,4	399	C18H37NO3Si3	010538-85-9	38
3		Noradrenaline, tetra-TMS	457	C20H43NO3Si4	000000-00-0	37
4		3,4-Dihydroxybenzyl alcohol, tris(tr	356	C16H32O3Si3	068595-79-9	37

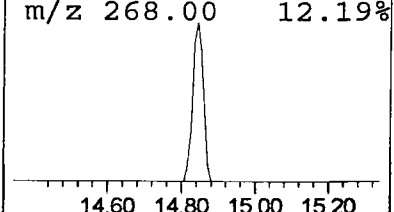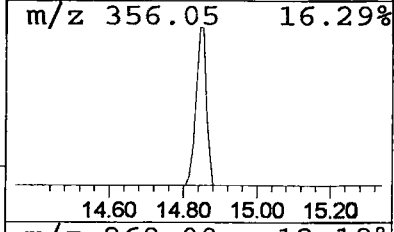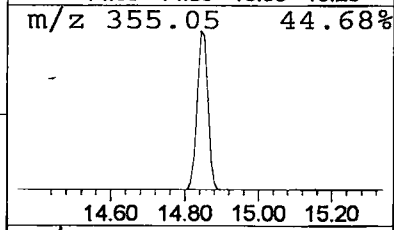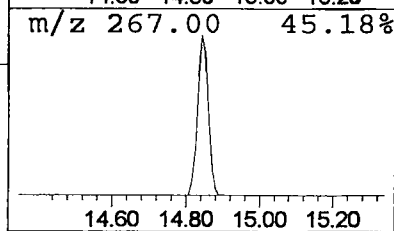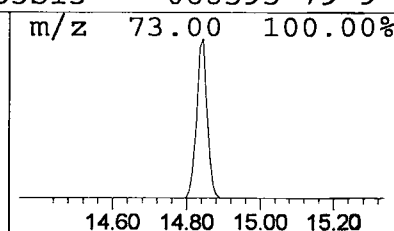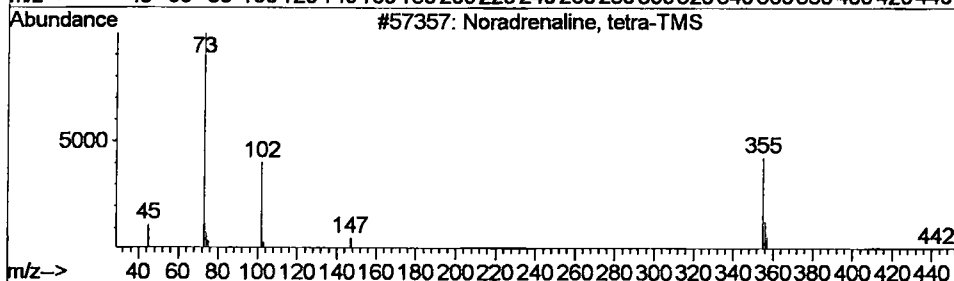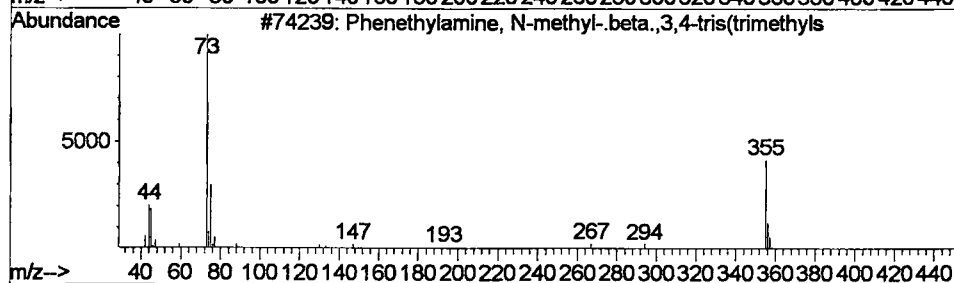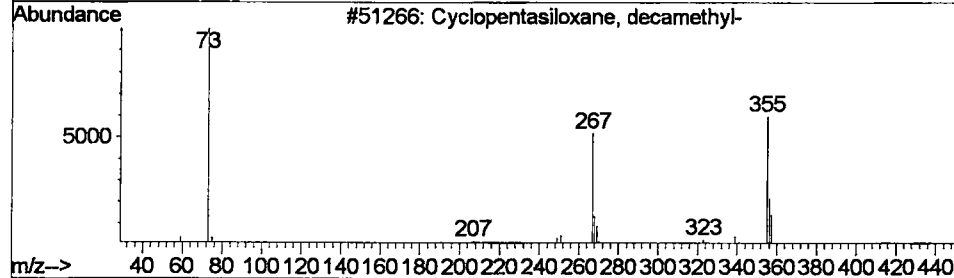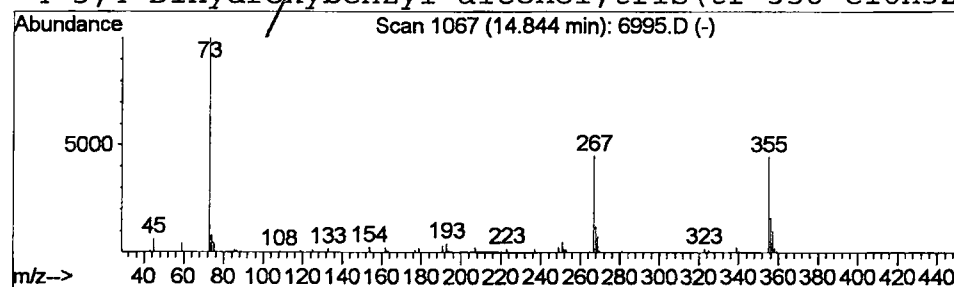

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 6 Apr 2002 7:34 pm
 Data File: C:\HPCHEM\1\DATA\APR0405\6995.D
 Name: gc/ms scan 3/26
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Cyclopentasiloxane,	14.84	1.4	ug/l	105100	ISTD02	15.88	3043850	20.0
6995.D GCMS0408.M	Mon Apr 15 14:44:31 2002							