

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/16/2002 Time: 15:07:18

Sample: AE06993
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/16/02 15:07 Ended: 4/16/02 15:07 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		100		5.0

Comments for Sample AE06993 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-16-2002 Time: 15:07:36

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recoveries for 4 of the 43 compounds in the LCS Standard were high.

Data File : C:\HPCHEM\1\DATA\APR0405\6993.D

Vial: 22

Acq On : 6 Apr 2002 4:36 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: GOOFY.P

Quant Time: Apr 15 14:34 2002

Quant Results File: GCMS0408.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Apr 15 14:10:52 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0403

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.25	152	458863	20.00	ug/l	-0.02
10) Naphthalene-d8	15.88	136	1657697	20.00	ug/l	-0.02
17) Acenaphthene-d10	21.19	164	945898	20.00	ug/l	-0.02
30) Phenanthrene-d10	25.63	188	1300882	20.00	ug/l	-0.02
39) Chrysene-d12	33.68	240	611481	20.00	ug/l	-0.03
45) Perylene-d12	37.93	264	328249	20.00	ug/l	-0.02

System Monitoring Compounds

28) TCMX	23.33	209	25633	10.05	ug/mL	0.00
Spiked Amount	10.000		Recovery	=	100.50%	
38) 2,4-DDD	0.00	235	0	0.00	ug/mL	
Spiked Amount	5.000		Recovery	=	0.00%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	0.00	128	0	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D. d
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.
25) Diethylphthalate	22.67	149	299	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.

(#)= qualifier out of range (m) = manual integration

6993.D GCMS0408.M

Mon Apr 15 14:34:51 2002

Page 1

Data File : C:\HPCHEM\1\DATA\APR0405\6993.D

Vial: 22

Acq On : 6 Apr 2002 4:36 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: GOOFY.P

Quant Time: Apr 15 14:34 2002

Quant Results File: GCMS0408.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Mon Apr 15 14:10:52 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0403

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	25.63	178	346	N.D.		
35) Anthracene	25.63	178	347	N.D.		
36) Di-n-butylphthalate	27.60	149	2690	N.D.		
37) Fluoranthene	0.00	202	0	N.D.		
40) Pyrene	0.00	202	0	N.D.		
41) Butylbenzylphthalate	0.00	149	0	N.D.		
42) Benzo(a)anthracene	33.69	228	1255	N.D.		
43) Bis(2-ethylhexyl)phthalate	33.91	149	1959	N.D.		
44) Chrysene	33.69	228	1255	N.D.		
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo(b)fluoranthene	0.00	252	0	N.D.		
48) Benzo(k)fluoranthene	0.00	252	0	N.D.		
49) Benzo(a)pyrene	37.94	252	928	N.D.		
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

6993.D GCMS0408.M

Mon Apr 15 14:34:52 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR0405\6993.D
Acq On : 6 Apr 2002 4:36 pm
Sample : gc/ms scan 3/26
Misc :
MS Integration Params: GOOFY.P
Quant Time: Apr 15 14:34 2002

Vial: 22
Operator:
Inst : GC/MS 209
Multiplr: 2.00

Quant Results File: GCMS0408.RES

Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Mon Apr 15 14:10:52 2002
Response via : Initial Calibration

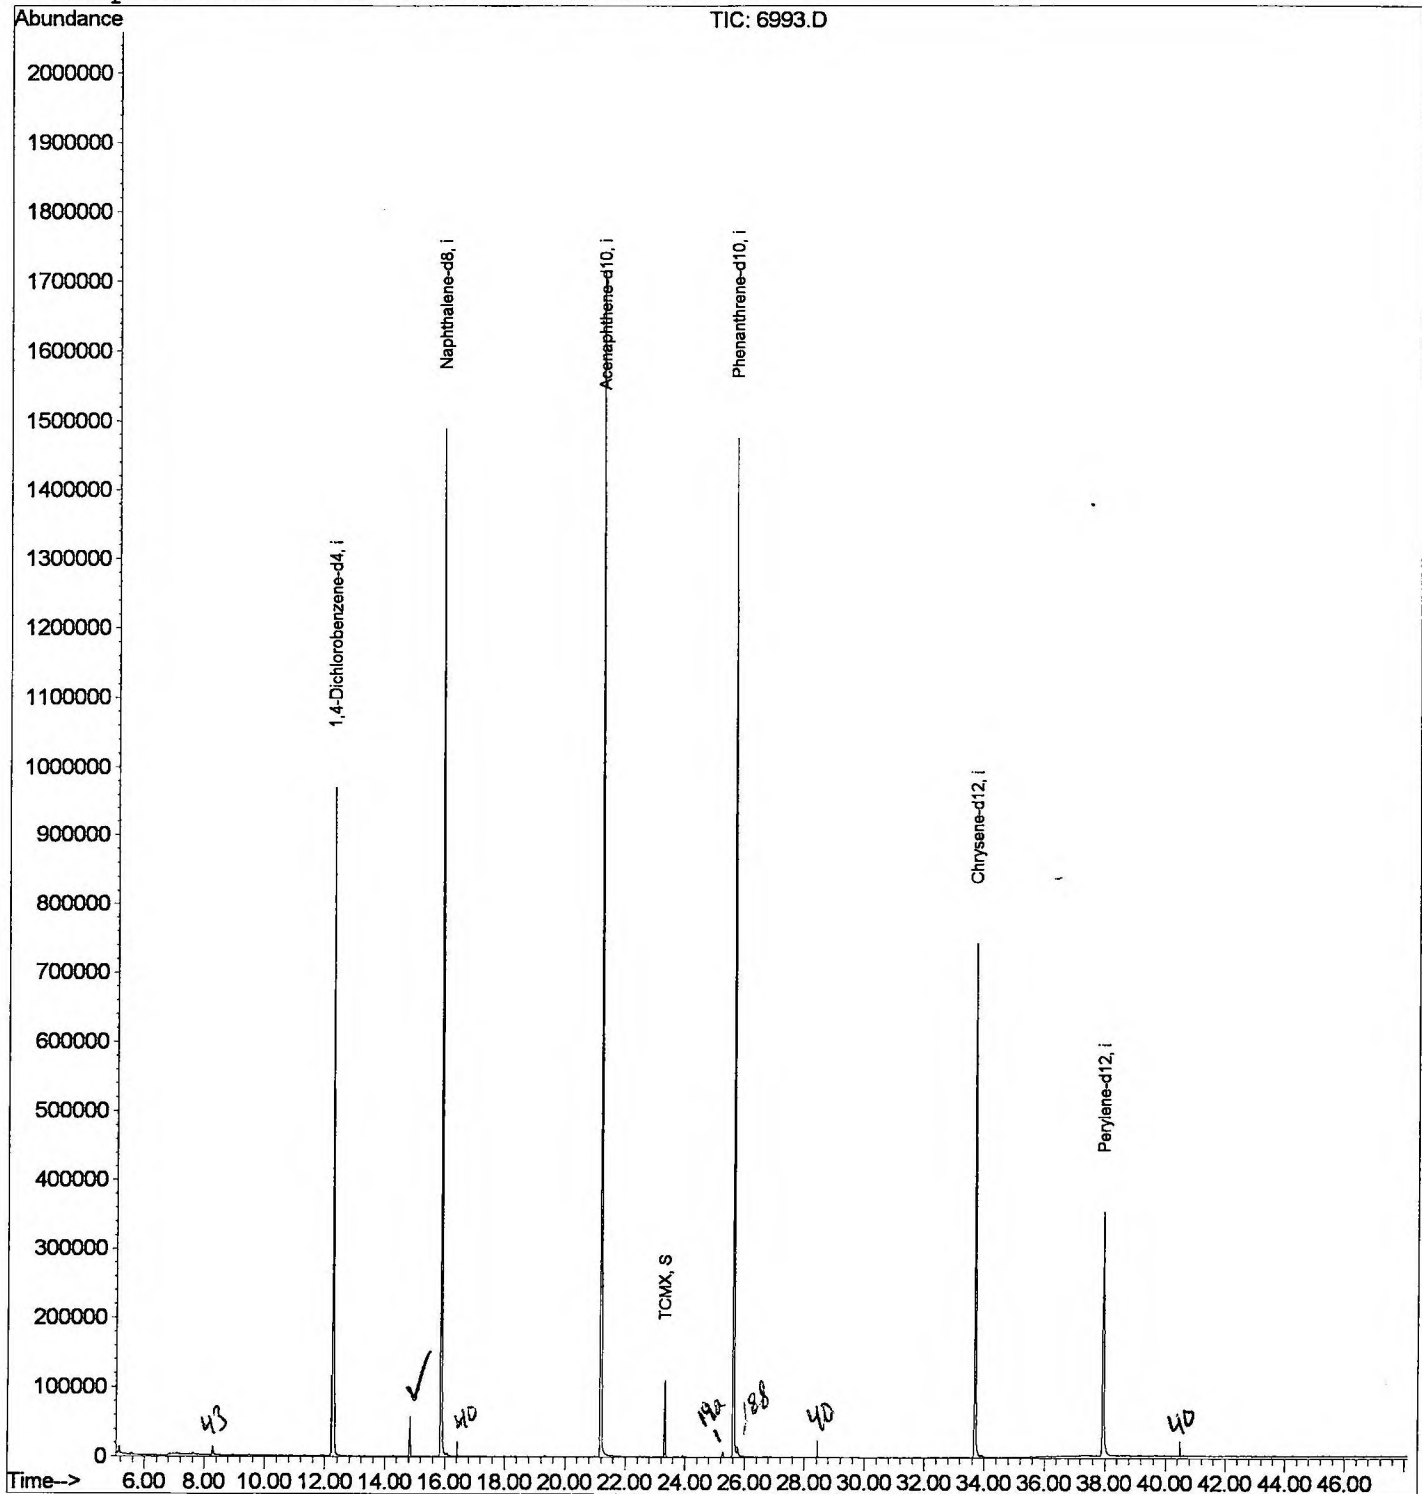

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR0405\6993.D

Vial: 22

Acq On : 6 Apr 2002 4:36 pm

Operator:

Sample : gc/ms scan 3/26

Inst : GC/MS 209

Misc :

Multiplr: 2.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	12.249	779	785	804	rVB	967836	2445379	67.79%	15.646%
2	14.847	1063	1068	1073	rVB	56618	110450	3.06%	0.707%
3	15.884	1175	1181	1199	rBV	1487528	3146749	87.23%	20.133%
4	21.190	1752	1759	1779	rBV	1715951	3607235	100.00%	23.079%
5	23.329	1986	1992	1998	rVB	109678	220869	6.12%	1.413%
6	25.634	2236	2243	2254	rBV2	1474677	3269431	90.64%	20.918%
7	33.685	3114	3120	3135	rBV2	742668	1746488	48.42%	11.174%
8	37.935	3575	3583	3598	rBV2	350857	1083080	30.03%	6.930%


Sum of corrected areas: 15629681

6993.D GCMS0408.M

Mon Apr 15 14:44:00 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR0405\6993.D
 Operator :
 Acquired : 6 Apr 2002 4:36 pm using AcqMethod GCMS0403
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 3/26
 Misc Info :
 Vial Number: 22
 Quant File :GCMS0408.RES (RTE Integrator)

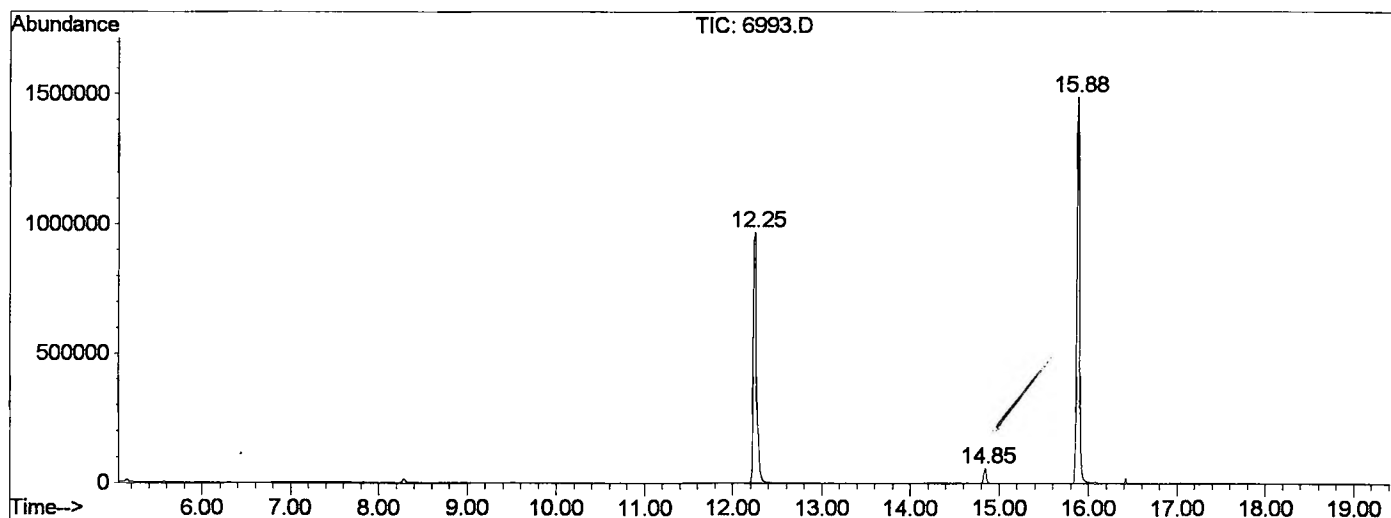

6993.D GCMS0408.M Mon Apr 15 14:44:01 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR0405\6993.D
 Acq On : 6 Apr 2002 4:36 pm
 Sample : gc/ms scan 3/26
 Misc :
 MS Integration Params: LSCINT.P


Vial: 22
 Operator:
 Inst : GC/MS 209
 Multiplr: 2.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 Cyclopentasiloxane, decamethyl Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.85	1.40 ug/l	110450	Naphthalene-d8	15.88

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	74
2		3,4-Dihydroxybenzyl alcohol, tris(tri	356	C16H32O3Si3	068595-79-9	58
3		p-Trimethylsilyloxyphenyl-bis(trimeth	370	C17H34O3Si3	000000-00-0	38
4		N-(Trifluoroacetyl)-O,O',O"-tris(tri	495	C20H36F3NO4Si3	000000-00-0	37

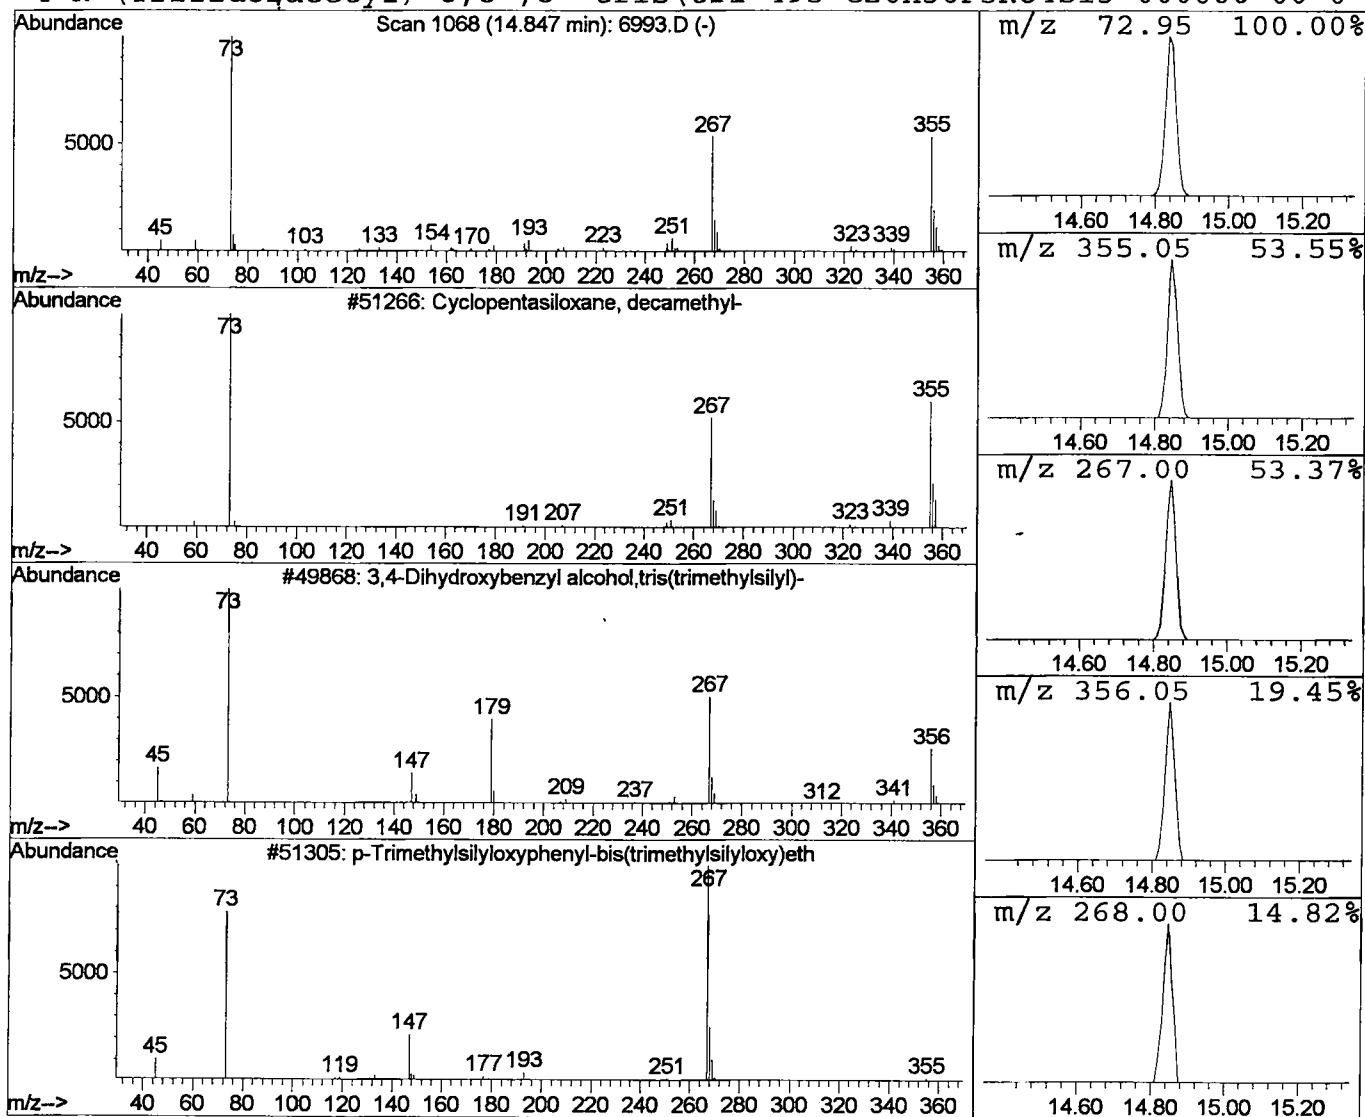

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 6 Apr 2002 4:36 pm
Data File: C:\HPCHEM\1\DATA\APR0405\6993.D
Name: gc/ms scan 3/26
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Cyclopentasiloxane,	14.85	1.4	ug/l	110450	ISTD02	15.88	3146750	20.0
6993.D GCMS0408.M	Mon Apr 15 14:44:03 2002							